

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122122\
 Data File : PS021505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 08:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 21:25:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.379	6.810	1320.5E6	956.6E6	454.468	554.882
Target Compounds							
1) T	Dalapon	2.445	0.000	114639	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.730	0.000	3267927	0	<MDL	N.D. #
3) T	4-Nitroph...	6.224	0.000	6023504	0	3.350	N.D. #
6) T	MCP	0.000	7.122f	0	3303106	N.D.	<MDL
7) T	MCPA	6.764	7.218f	4249220	18589743	<MDL	2.102 #
8) T	DICHLORPROP	0.000	7.652f	0	4386004	N.D.	2.227
9) T	2,4-D	7.310	7.950f	544554	2207761	<MDL	<MDL #
10) T	Pentachlo...	7.553	0.000	1073881	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.089	8.687	3647423	1457439	<MDL	<MDL #
12) T	2,4,5-T	8.322	9.088	46366280	2064360	2.457	<MDL #
13) T	2,4-DB	8.847	9.637f	1566656	1869154	<MDL	1.300 #
15) T	Picloram	9.734	10.904	10065347	61995257	<MDL	3.812 #
16) T	DCPA	10.165	10.817	2021834	1193790	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122122\
Data File : PS021505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 08:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 21:25:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

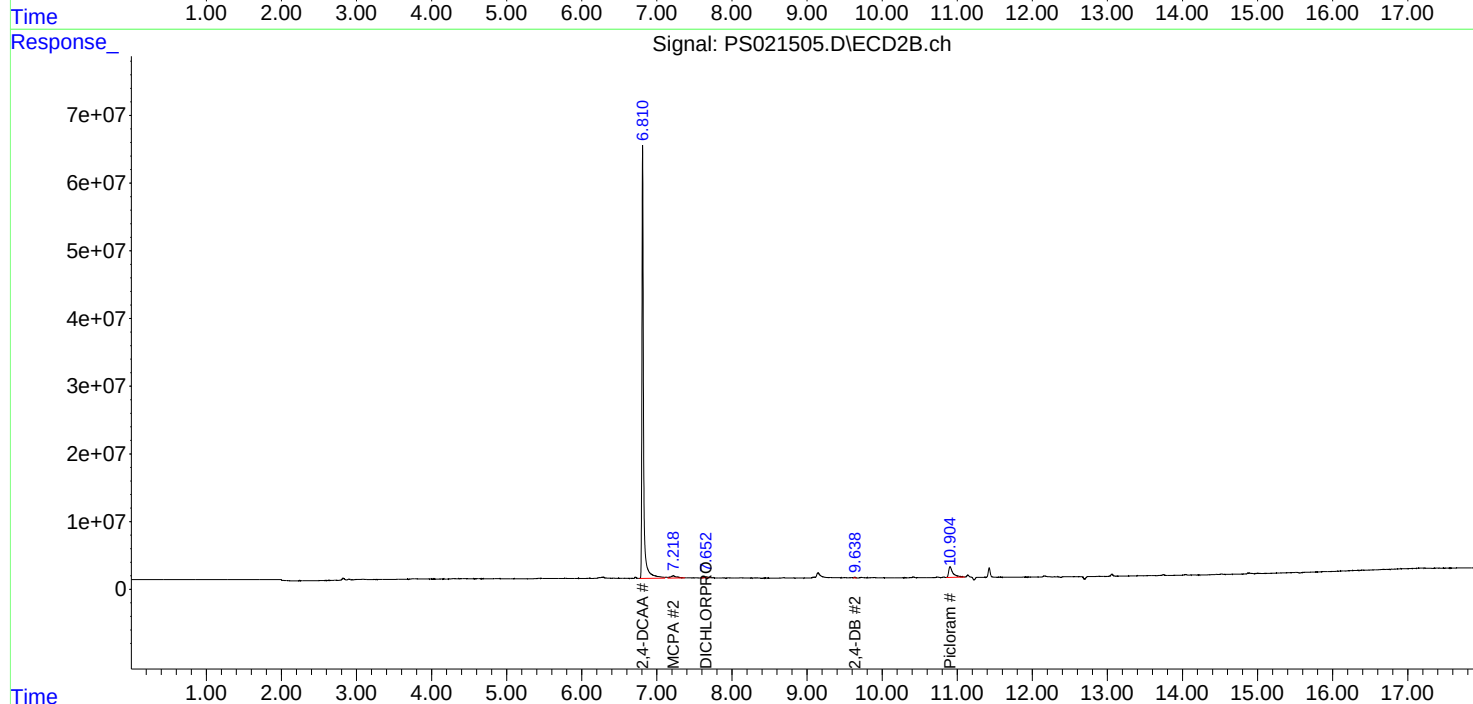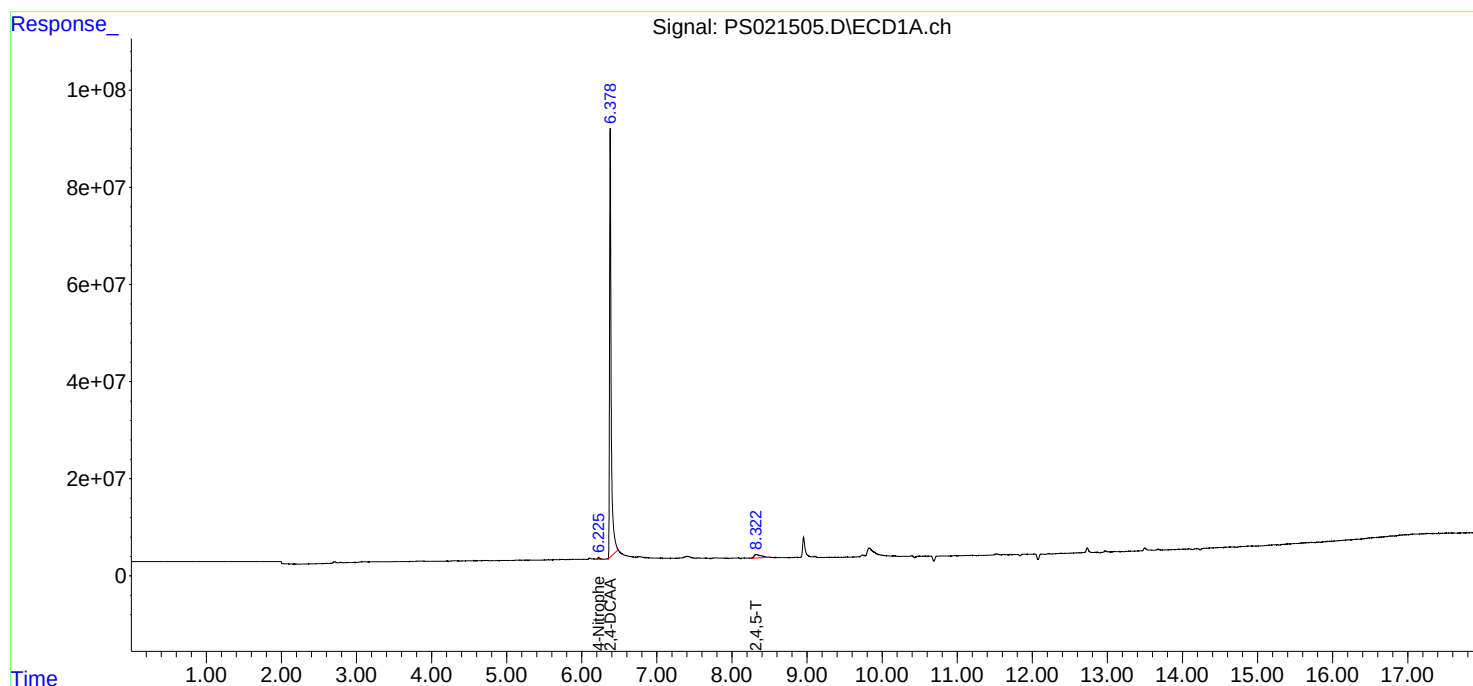


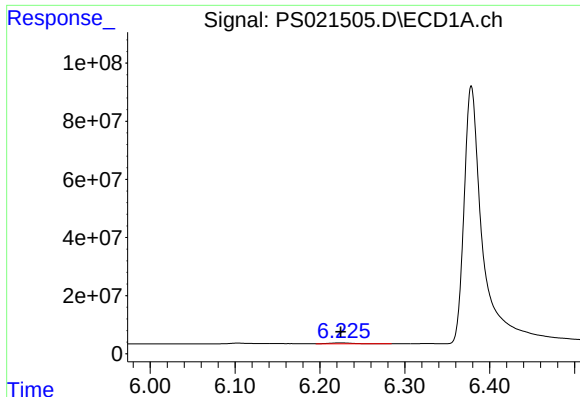

#3 4-Nitrophenol


R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 6023504
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

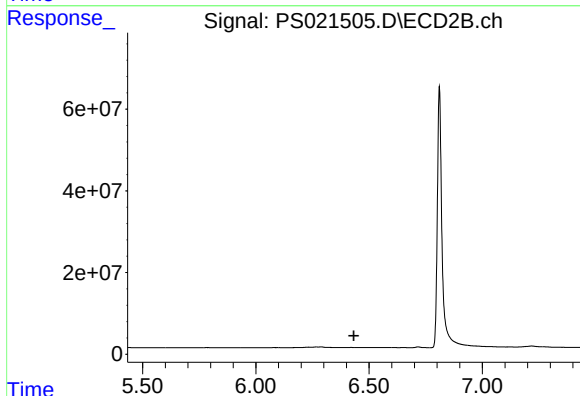


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

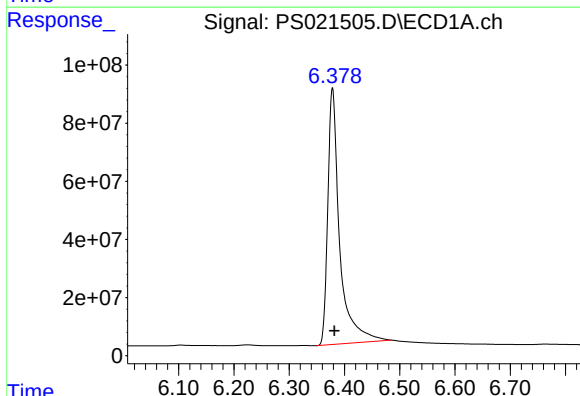


#4 2,4-DCAA

R.T.: 6.379 min
Delta R.T.: -0.003 min
Response: 1320453624
Conc: 454.47 ng/ml

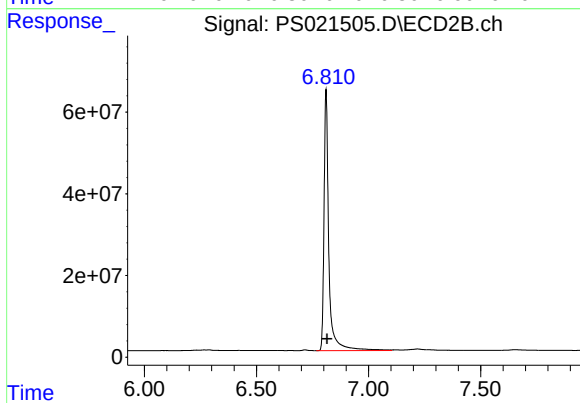

#4 2,4-DCAA


R.T.: 6.810 min
Delta R.T.: -0.005 min
Response: 956612162
Conc: 554.88 ng/ml

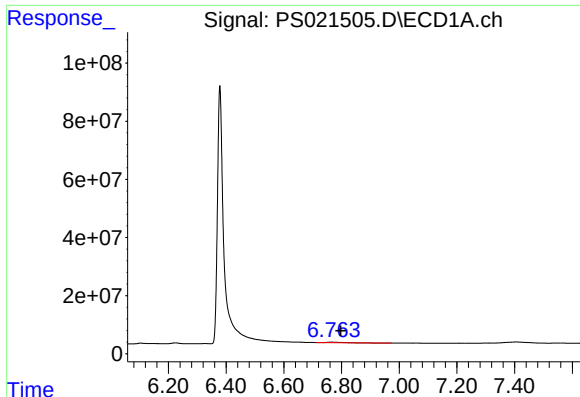

#7 MCPA


R.T.: 6.764 min
Delta R.T.: -0.034 min
Response: 4249220
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

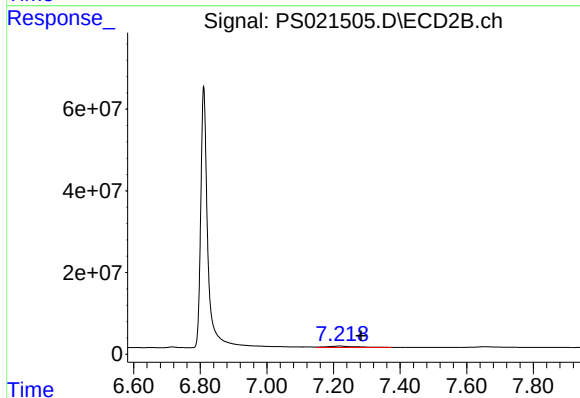


#7 MCPA

R.T.: 7.218 min
Delta R.T.: -0.064 min
Response: 18589743
Conc: 2.10 ug/ml

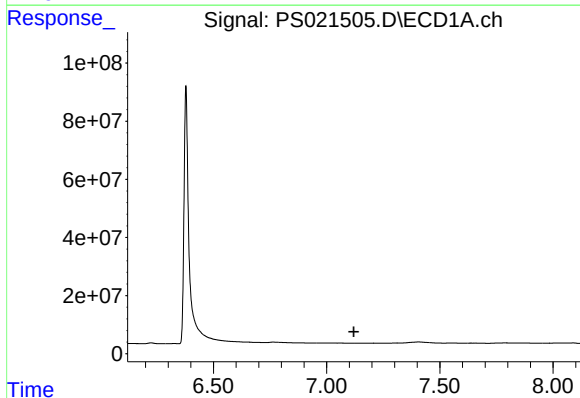


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.120 min
Response: 0
Conc: N.D.

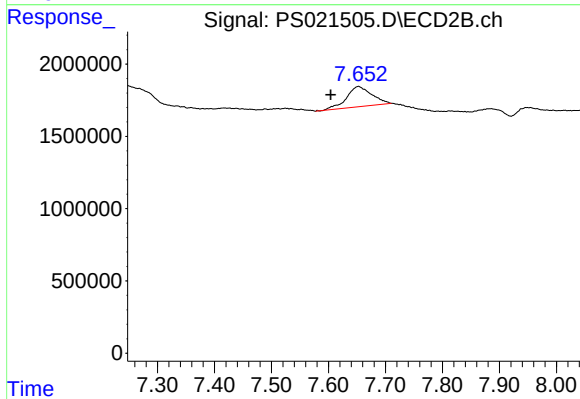

#8 DICHLORPROP


R.T.: 7.652 min
Delta R.T.: 0.049 min
Response: 4386004
Conc: 2.23 ng/ml

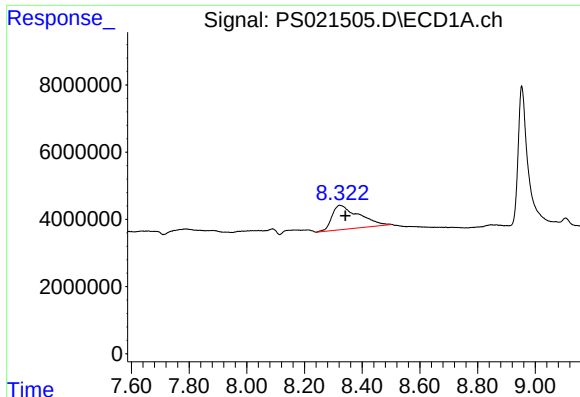

#12 2,4,5-T


R.T.: 8.322 min
Delta R.T.: -0.020 min
Response: 46366280
Conc: 2.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

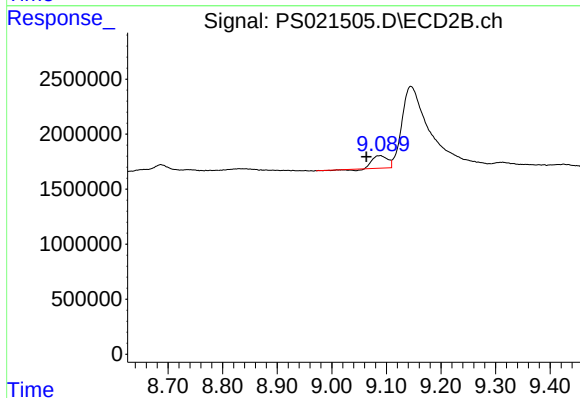


#12 2,4,5-T

R.T.: 9.088 min
Delta R.T.: 0.024 min
Response: 2064360
Conc: N.D.

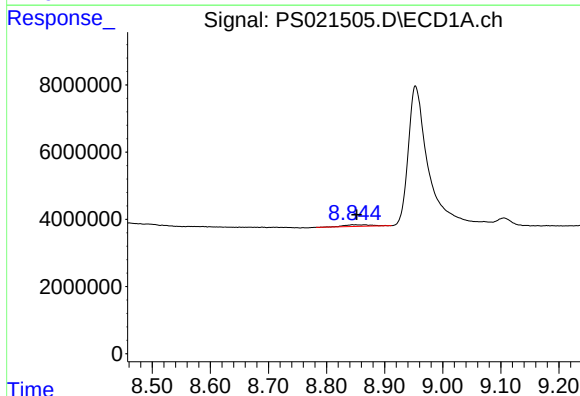


#13 2,4-DB

R.T.: 8.847 min
Delta R.T.: -0.005 min
Response: 1566656
Conc: N.D.

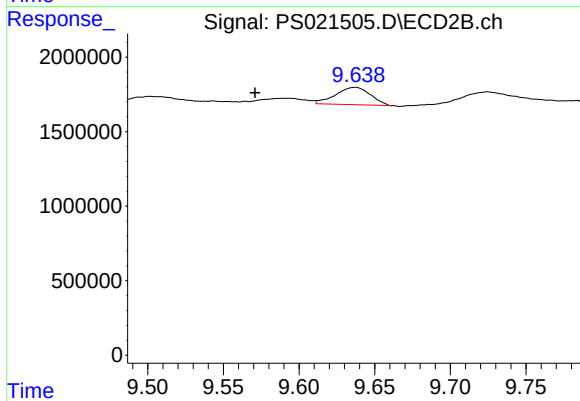

#13 2,4-DB


R.T.: 9.637 min
Delta R.T.: 0.066 min
Response: 1869154
Conc: 1.30 ng/ml

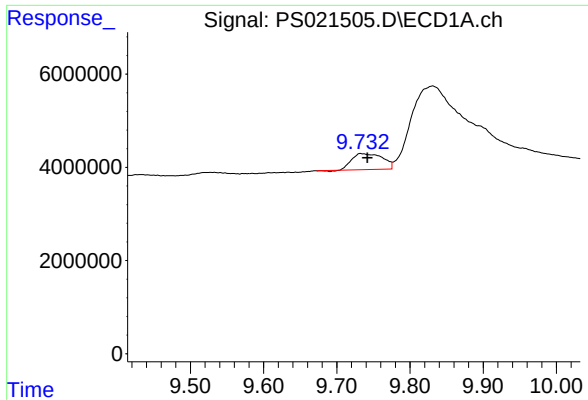

#15 Picloram

R.T.: 9.734 min
Delta R.T.: -0.008 min
Response: 10065347
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

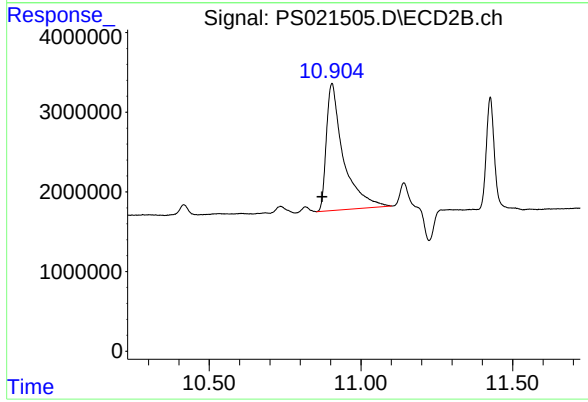

#15 Picloram

R.T.: 10.904 min
Delta R.T.: 0.032 min
Response: 61995257
Conc: 3.81 ng/ml