

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122122\
 Data File : PS021508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 11:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 21:29:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.378	6.810	1334.9E6	958.9E6	459.454	556.197
Target Compounds							
1) T	Dalapon	2.537f	0.000	399390	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.772	0.000	782511	0	<MDL	N.D. #
3) T	4-Nitroph...	6.224	0.000	6024466	0	3.350	N.D. #
6) T	MCP	6.703	7.097	-1231002	1984314	N.D.	<MDL
7) T	MCPA	6.762	7.216f	8640009	31893807	<MDL	3.607 #
8) T	DICHLORPROP	7.137	7.649f	524685	6004876	<MDL	3.049 #
9) T	2,4-D	0.000	7.944f	0	1431995	N.D.	<MDL
10) T	Pentachlo...	7.551	8.320	3932773	4935140	<MDL	<MDL #
11) T	2,4,5-TP ...	8.089	8.688	4559993	2343527	<MDL	<MDL #
12) T	2,4,5-T	8.314	9.084	43372145	3820661	2.299	<MDL #
13) T	2,4-DB	8.844	9.638f	1879104	1720140	<MDL	1.197 #
14) T	DINOSEB	0.000	9.893	0	2547474	N.D.	<MDL
15) T	Picloram	9.729	10.900	10231280	79727991	<MDL	4.903 #
16) T	DCPA	10.164	10.818	5670857	2919387	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122122\
Data File : PS021508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 11:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 21:29:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

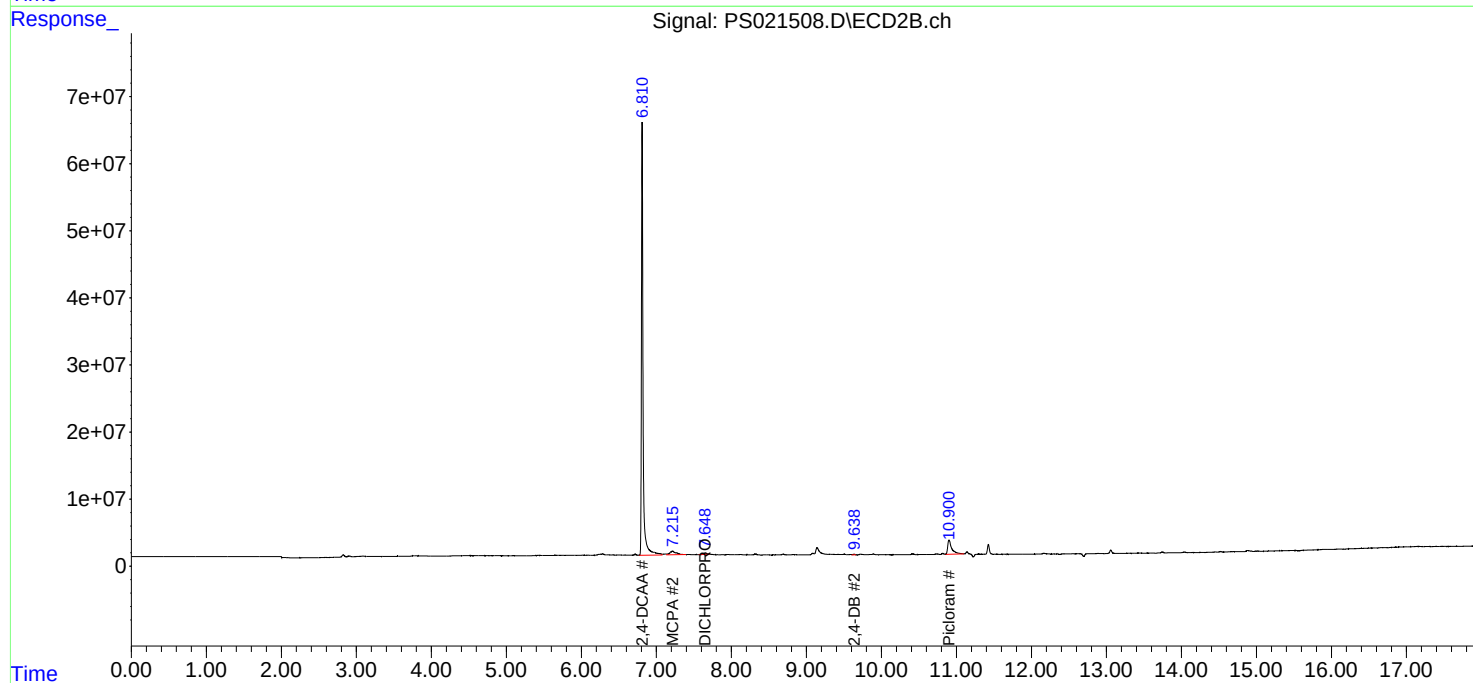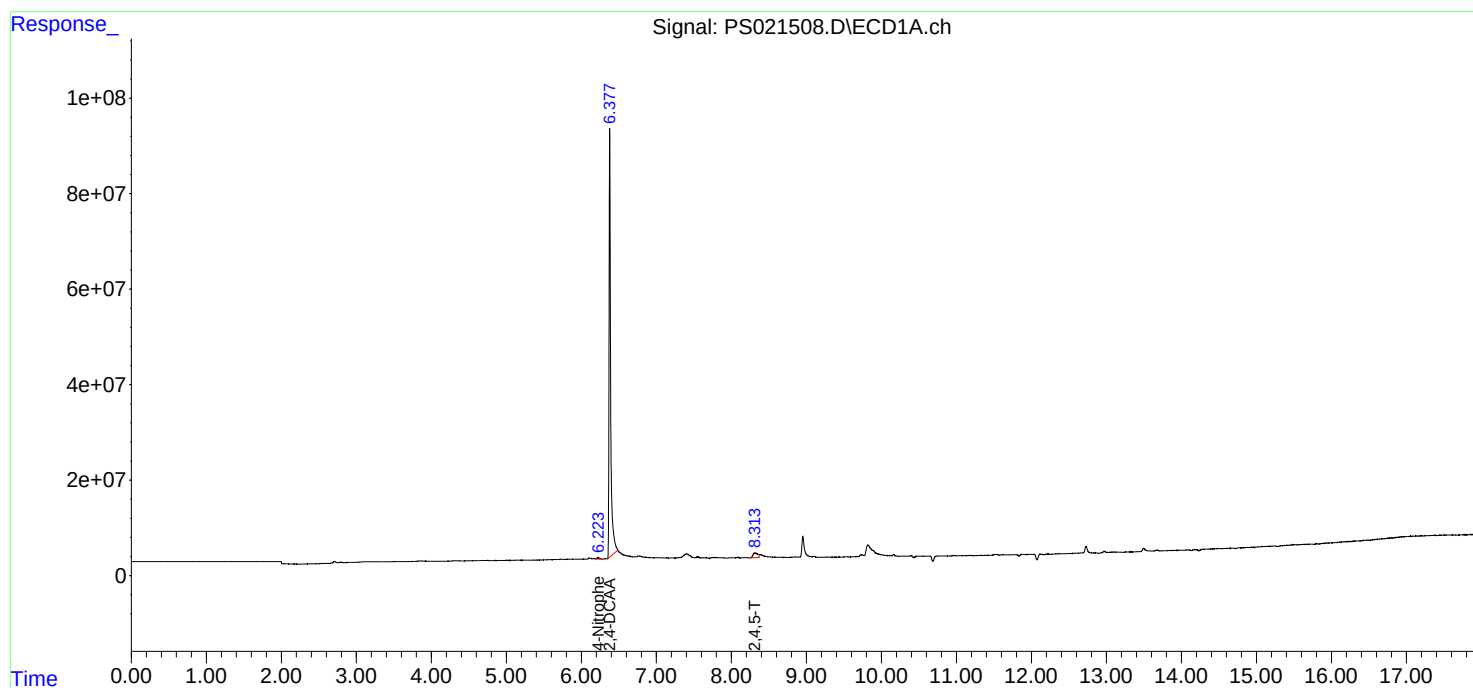


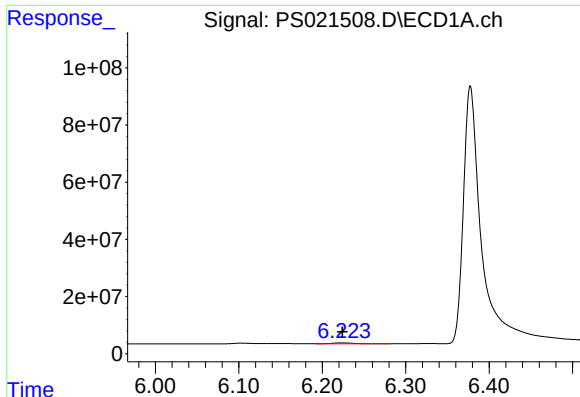

#3 4-Nitrophenol


R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 6024466
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

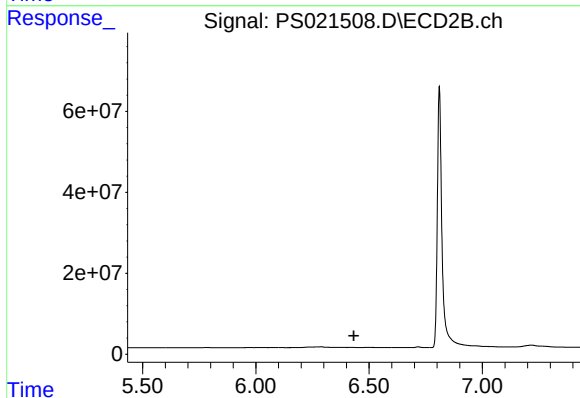


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

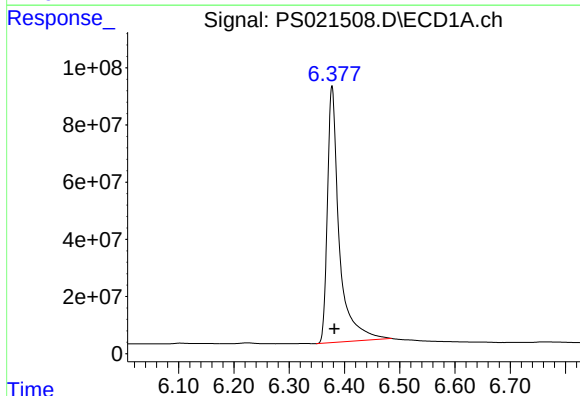


#4 2,4-DCAA

R.T.: 6.378 min
Delta R.T.: -0.004 min
Response: 1334940415
Conc: 459.45 ng/ml

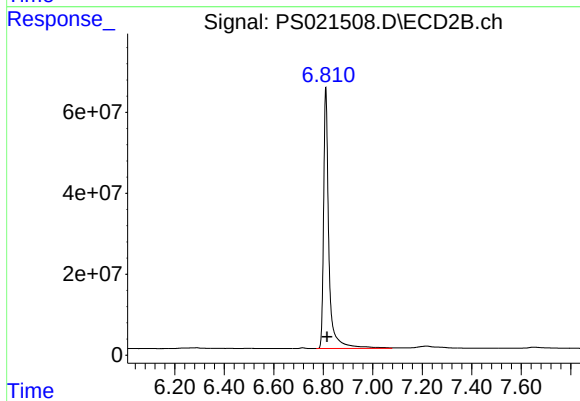

#4 2,4-DCAA


R.T.: 6.810 min
Delta R.T.: -0.005 min
Response: 958879712
Conc: 556.20 ng/ml

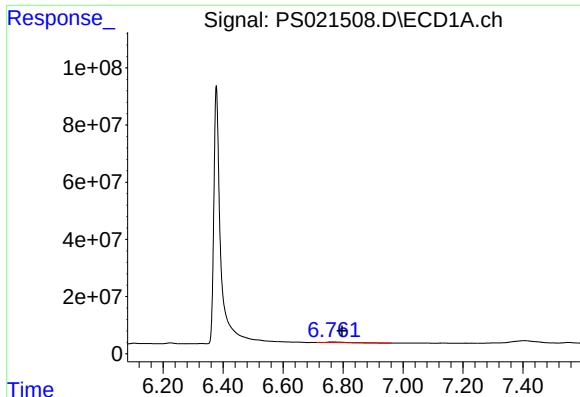

#7 MCPA


R.T.: 6.762 min
Delta R.T.: -0.036 min
Response: 8640009
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

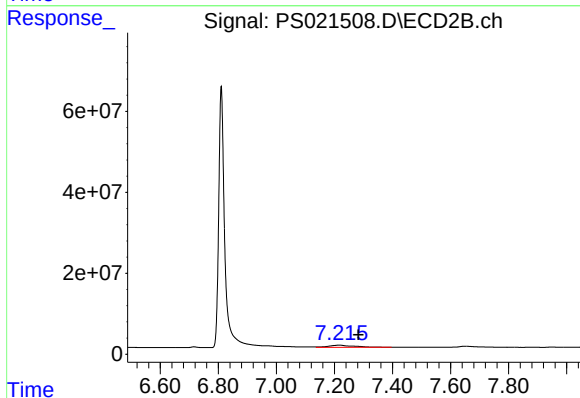


#7 MCPA

R.T.: 7.216 min
Delta R.T.: -0.066 min
Response: 31893807
Conc: 3.61 ug/ml

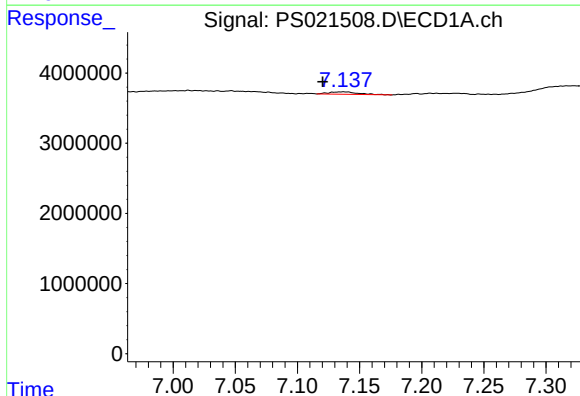


#8 DICHLORPROP

R.T.: 7.137 min
Delta R.T.: 0.016 min
Response: 524685
Conc: N.D.

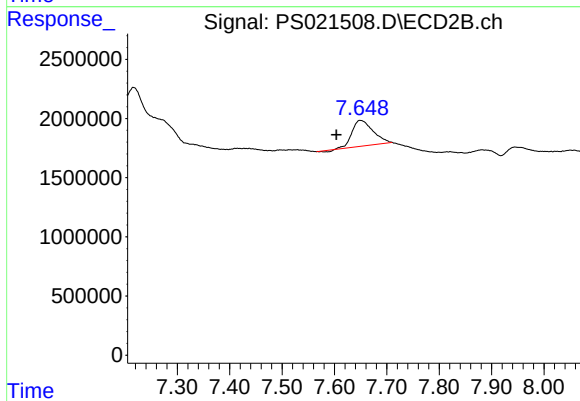

#8 DICHLORPROP


R.T.: 7.649 min
Delta R.T.: 0.045 min
Response: 6004876
Conc: 3.05 ng/ml

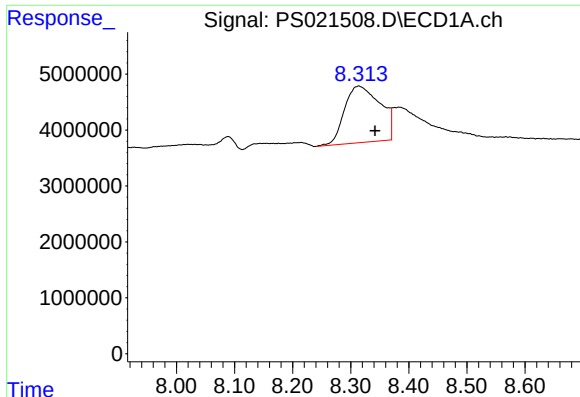

#12 2,4,5-T


R.T.: 8.314 min
Delta R.T.: -0.028 min
Response: 43372145
Conc: 2.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

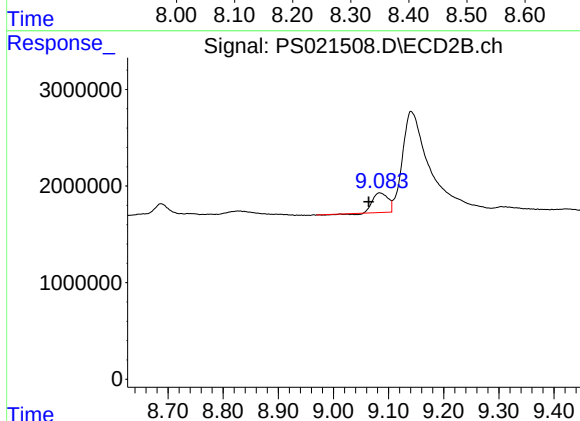


#12 2,4,5-T

R.T.: 9.084 min
Delta R.T.: 0.021 min
Response: 3820661
Conc: N.D.

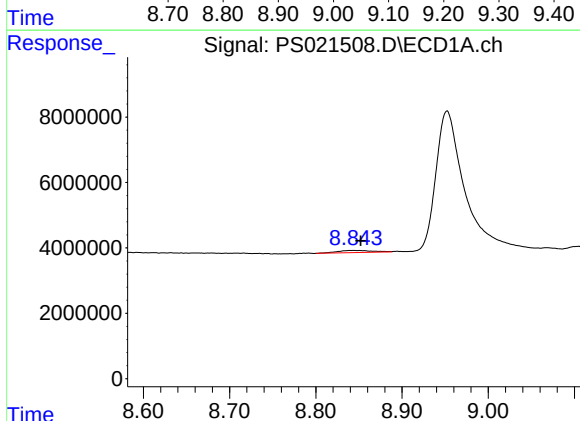


#13 2,4-DB

R.T.: 8.844 min
Delta R.T.: -0.009 min
Response: 1879104
Conc: N.D.

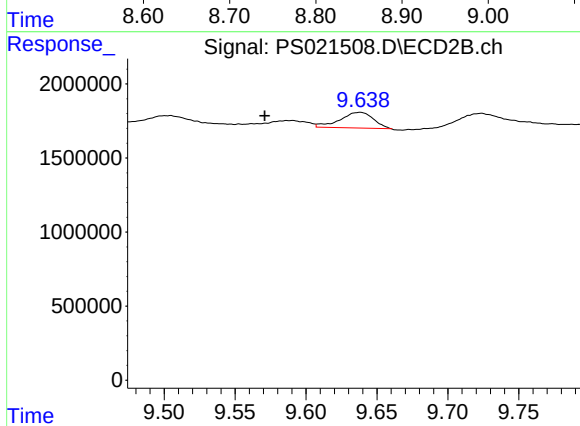

#13 2,4-DB


R.T.: 9.638 min
Delta R.T.: 0.067 min
Response: 1720140
Conc: 1.20 ng/ml

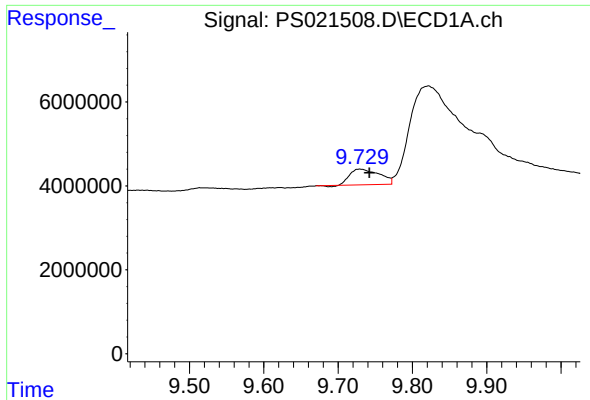

#15 Picloram

R.T.: 9.729 min
Delta R.T.: -0.013 min
Response: 10231280
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

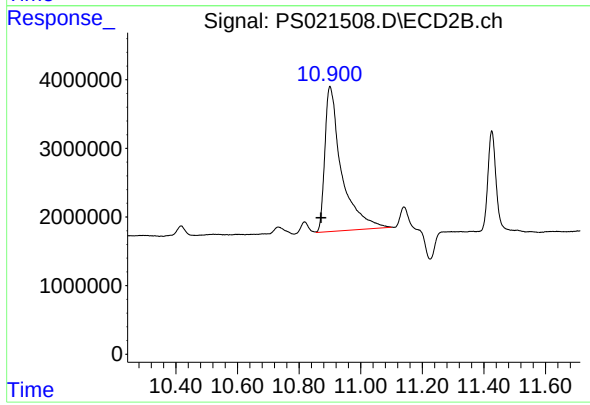

#15 Picloram

R.T.: 10.900 min
Delta R.T.: 0.028 min
Response: 79727991
Conc: 4.90 ng/ml