

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122123\
 Data File : PS025144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 10:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 22:31:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	2.511	2.556	5818392	3334589	2.018	2.907 #
2) T	3,5-DICHL...	5.697	0.000	1203278	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.965	0	1145105	N.D.	<MDL
6) T	MCPP	0.000	6.965f	0	1145105	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.550	0	997672	N.D.	1.268
9) T	2,4-D	7.247	7.764f	7720441	763816	2.542	<MDL #
10) T	Pentachlo...	0.000	8.243	0	727505	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.604	0	372777	N.D.	<MDL
12) T	2,4,5-T	0.000	8.972	0	789032	N.D.	<MDL
14) T	DINOSEB	0.000	9.802	0	939793	N.D.	<MDL
15) T	Picloram	9.683	10.754	22854354	9181912	1.173	1.403
16) T	DCPA	0.000	10.754	0	9181912	N.D.	1.694



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122123\
Data File : PS025144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 10:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 22:31:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

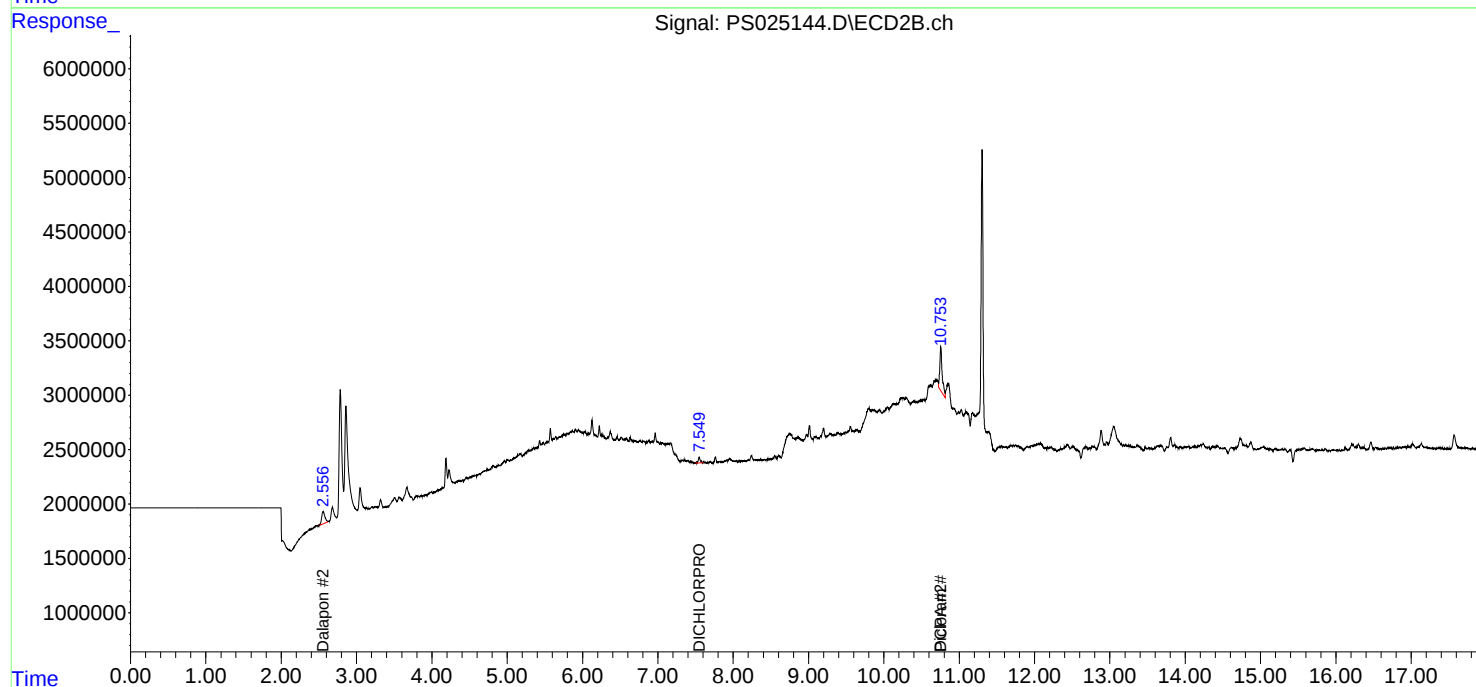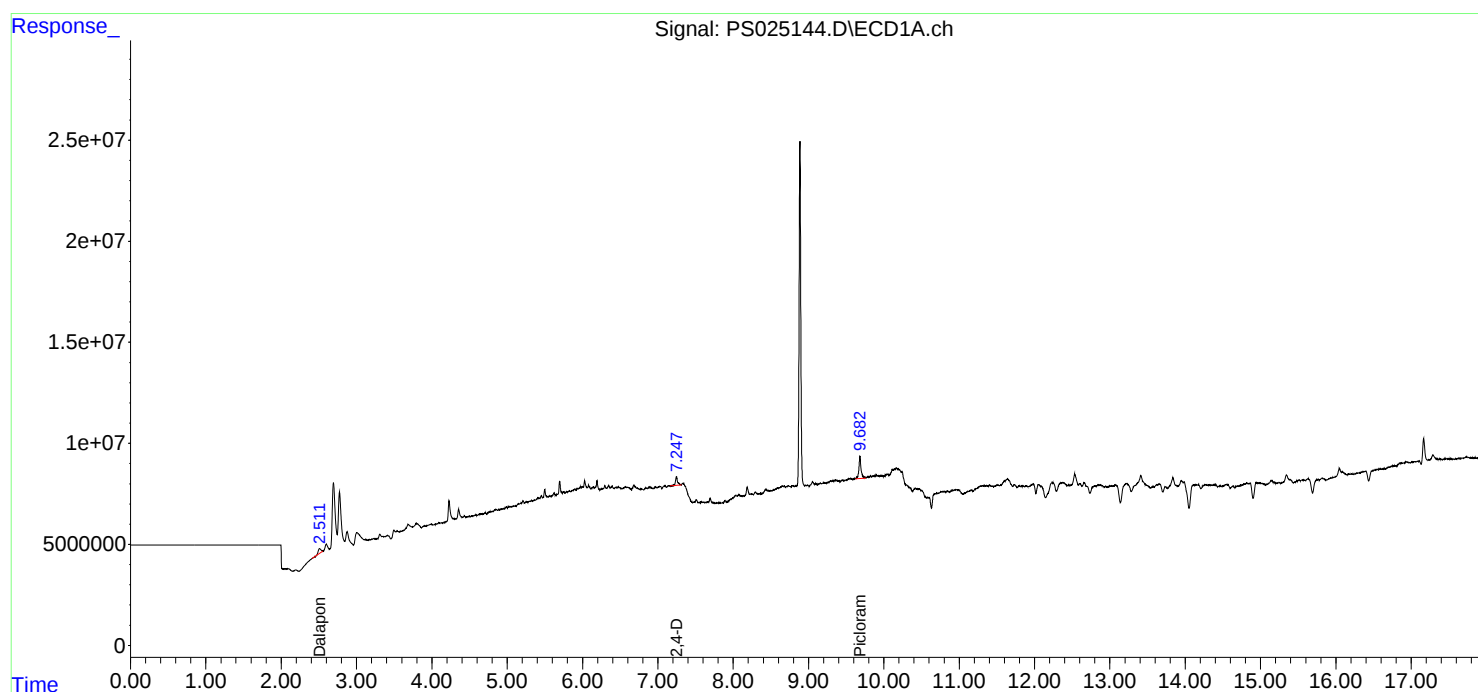


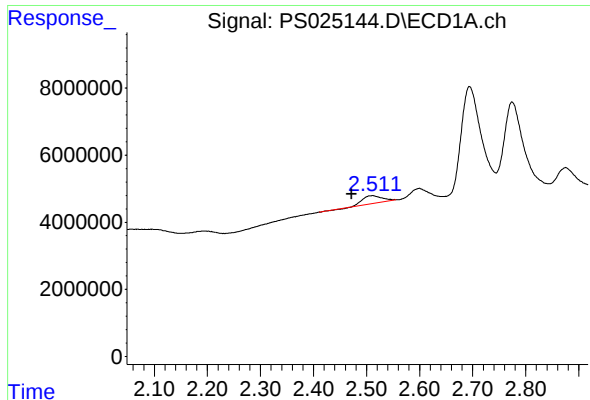

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: 0.039 min
Response: 5818392
Conc: 2.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

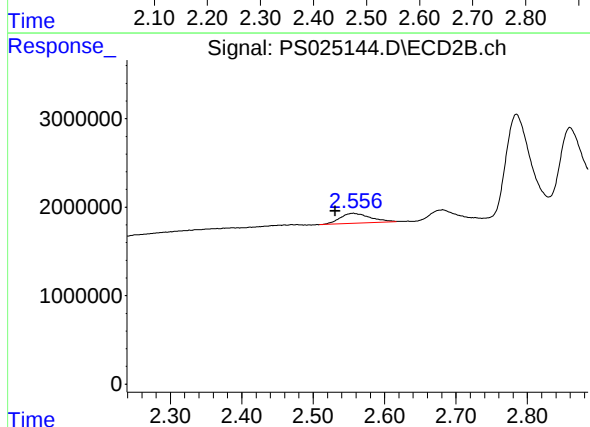


#1 Dalapon

R.T.: 2.556 min
Delta R.T.: 0.025 min
Response: 3334589
Conc: 2.91 ng/ml

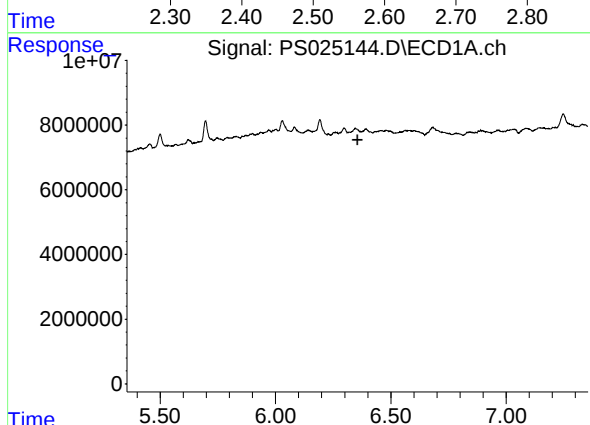


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.355 min
Response: 0
Conc: N.D.

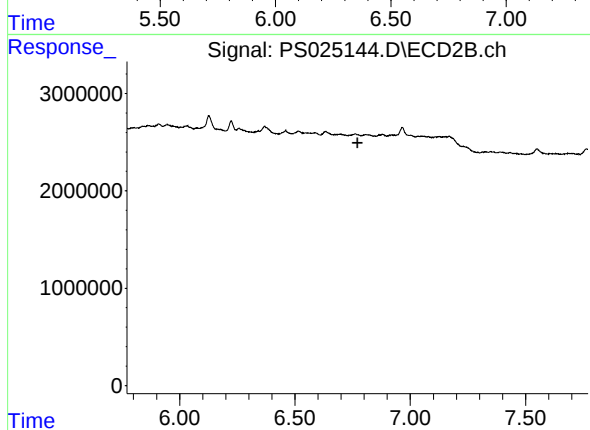

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

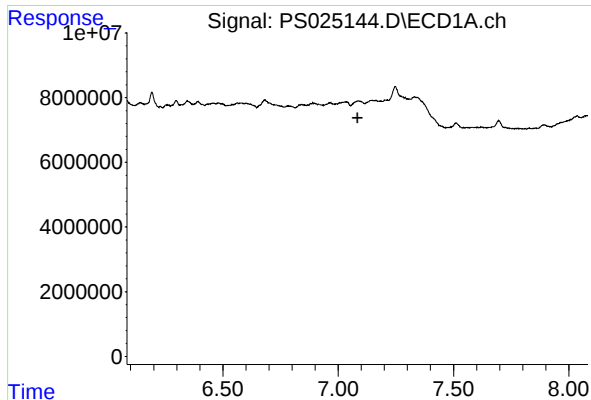

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

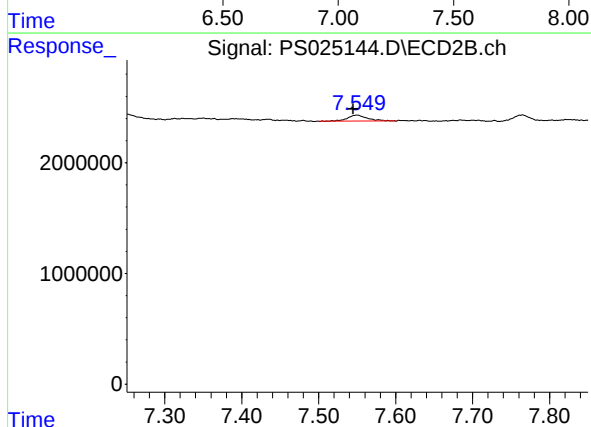


#8 DICHLORPROP

R.T.: 7.550 min
Delta R.T.: 0.004 min
Response: 997672
Conc: 1.27 ng/ml

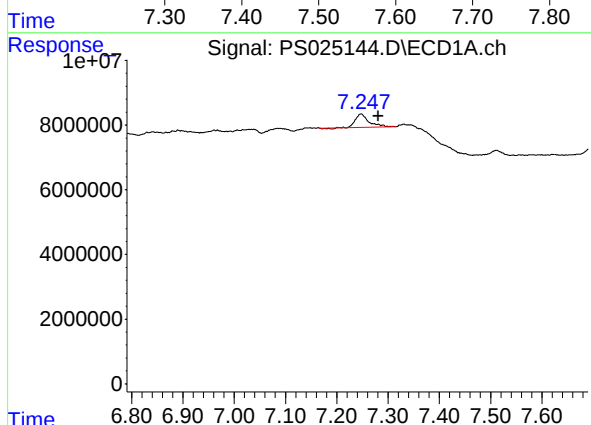


#9 2,4-D

R.T.: 7.247 min
Delta R.T.: -0.034 min
Response: 7720441
Conc: 2.54 ng/ml

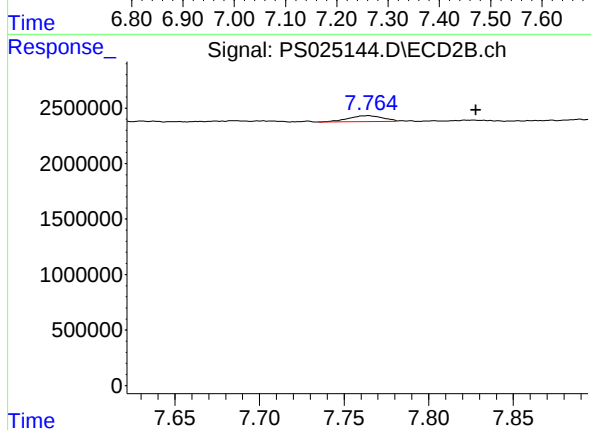

#9 2,4-D


R.T.: 7.764 min
Delta R.T.: -0.064 min
Response: 763816
Conc: N.D.

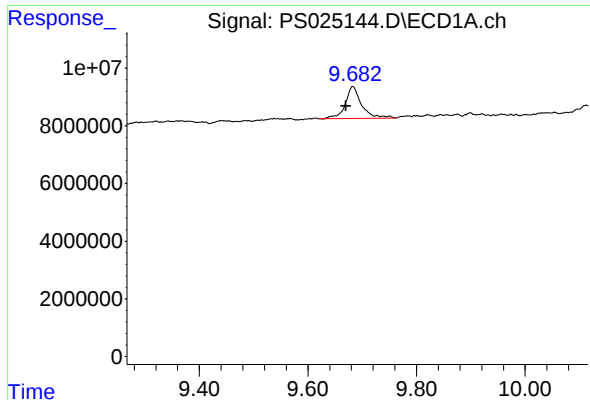

#15 Picloram


R.T.: 9.683 min
Delta R.T.: 0.013 min
Response: 22854354
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

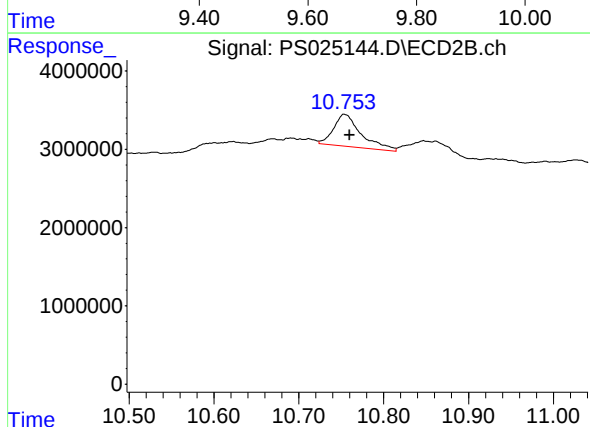


#15 Picloram

R.T.: 10.754 min
Delta R.T.: -0.006 min
Response: 9181912
Conc: 1.40 ng/ml

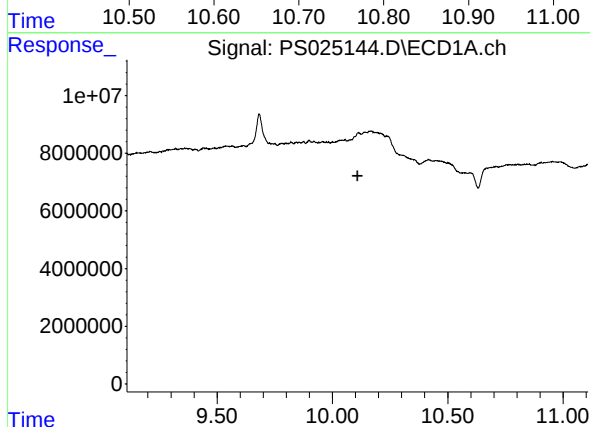

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

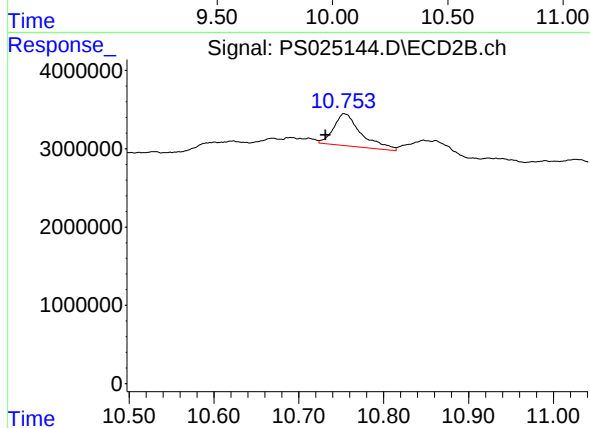

#16 DCPA

R.T.: 10.754 min
Delta R.T.: 0.022 min
Response: 9181912
Conc: 1.69 ng/ml