

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122221\
 Data File : PS017799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2021 10:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 12:59:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.128	6.716	864.9E6	367.1E6	553.409	615.836
Target Compounds							
2) T	3,5-DICHL...	6.392	0.000	210.9E6	0	94.396	N.D. #
5) T	DICAMBA	7.317	6.932f	9257592	57276059	1.464	21.500 #
6) T	MCP	0.000	6.932	0	57276059	N.D.	26.314
9) T	2,4-D	8.300f	0.000	316.8E6	0	179.197	N.D. #
12) T	2,4,5-T	9.343	0.000	34564335	0	3.973	N.D. #
14) T	DINOSEB	11.062	0.000	28027237	0	4.099	N.D. #
15) T	Picloram	10.886	10.797f	24872547	82376989	2.292	16.772 #
16) T	DCPA	11.334	0.000	6533648	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122221\
Data File : PS017799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2021 10:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 12:59:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

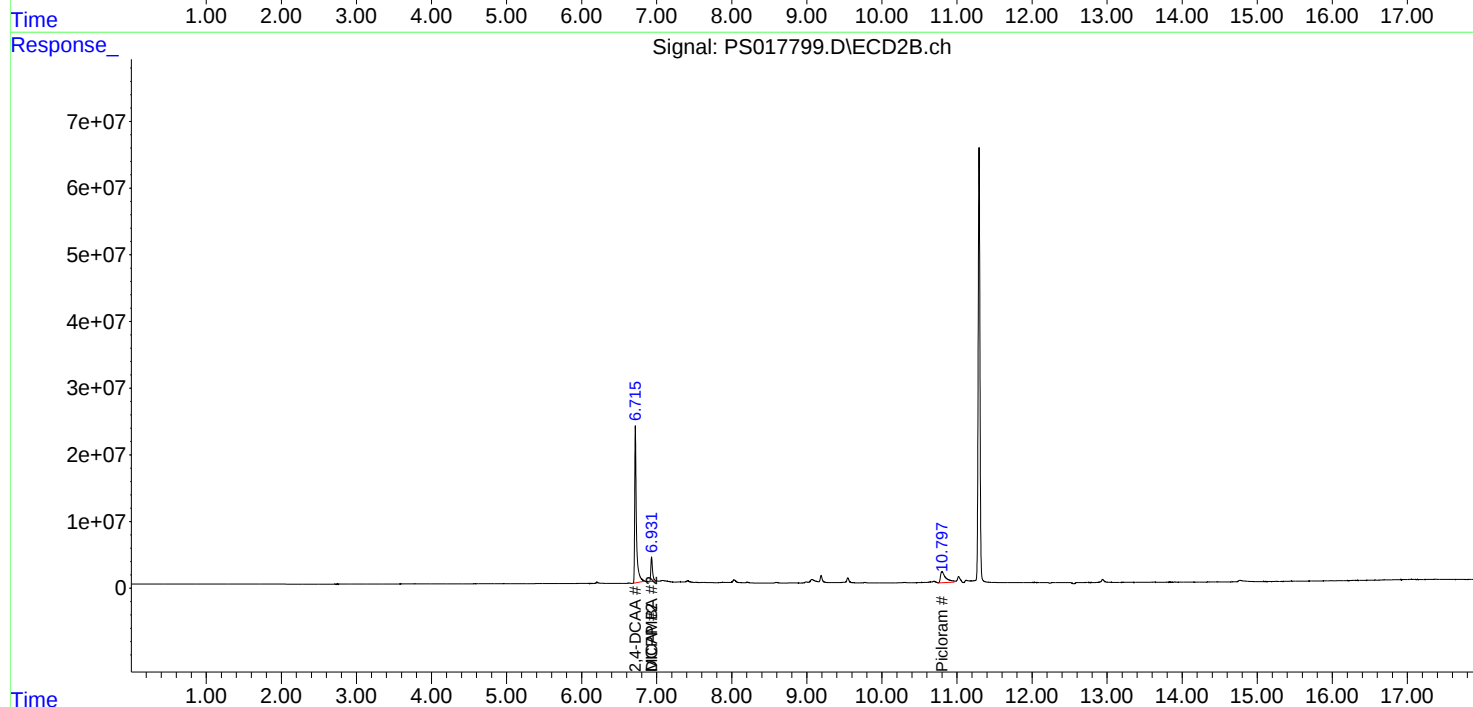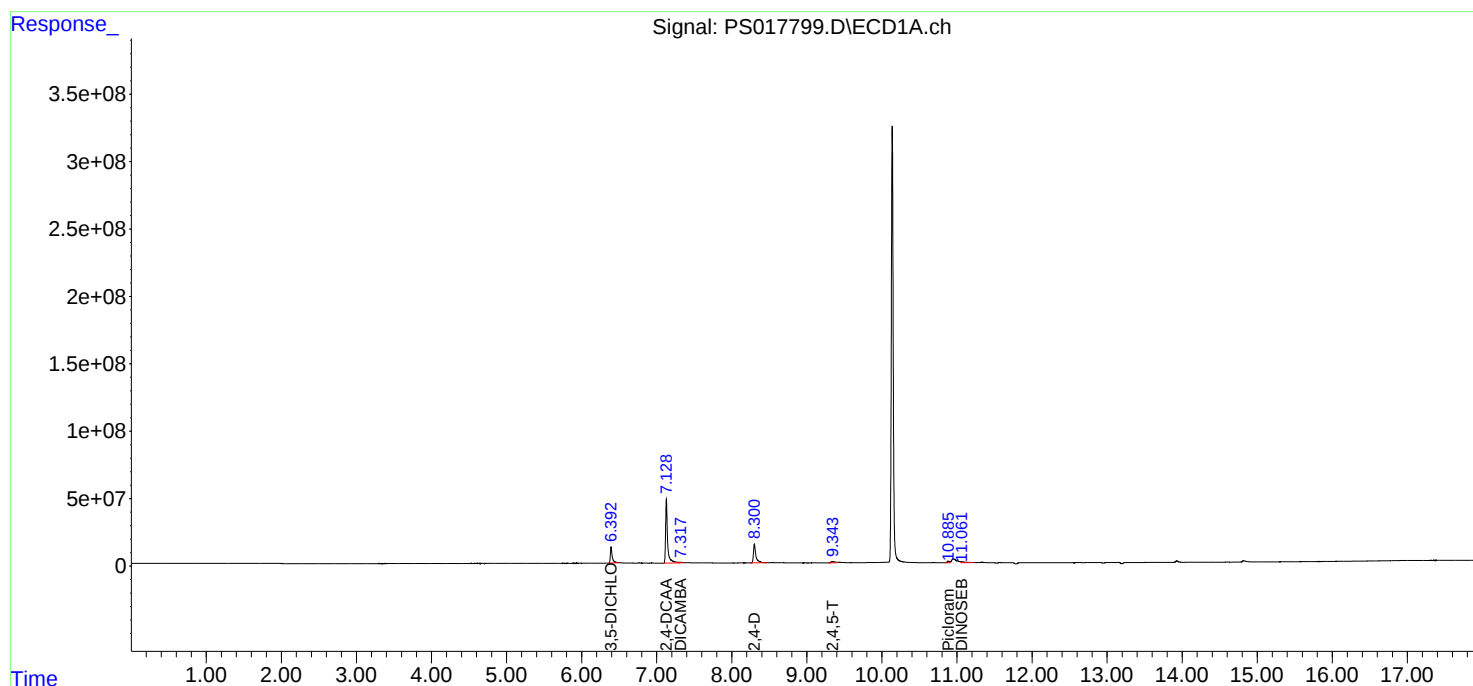


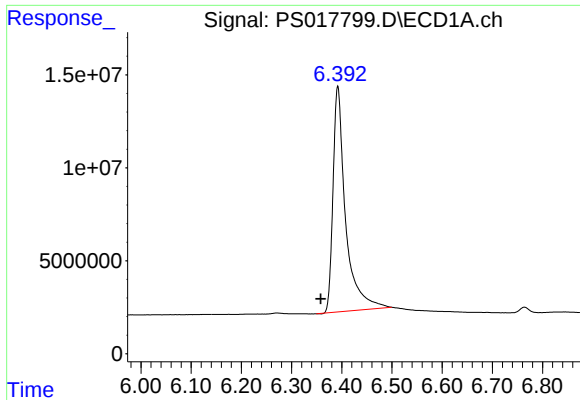

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.392 min
Delta R.T.: 0.034 min
Response: 210894254
Conc: 94.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

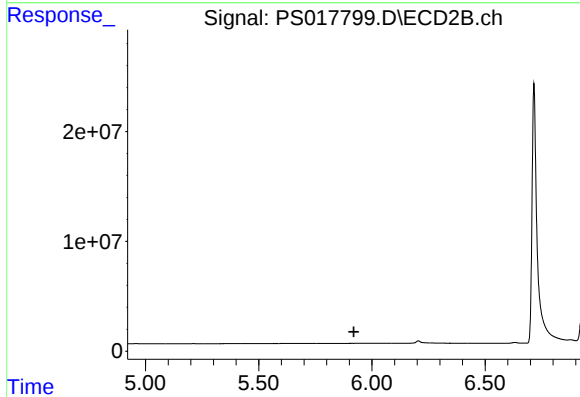


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

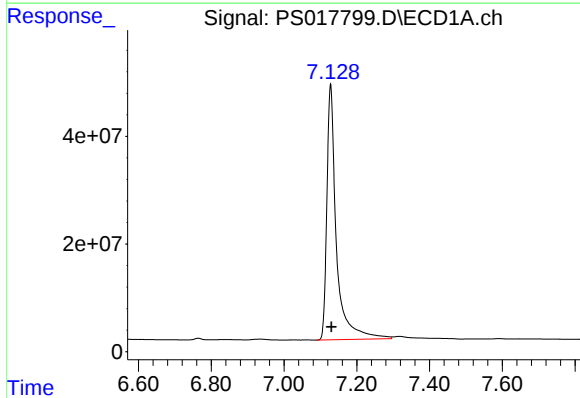


#4 2,4-DCAA

R.T.: 7.128 min
Delta R.T.: -0.002 min
Response: 864947819
Conc: 553.41 ng/ml

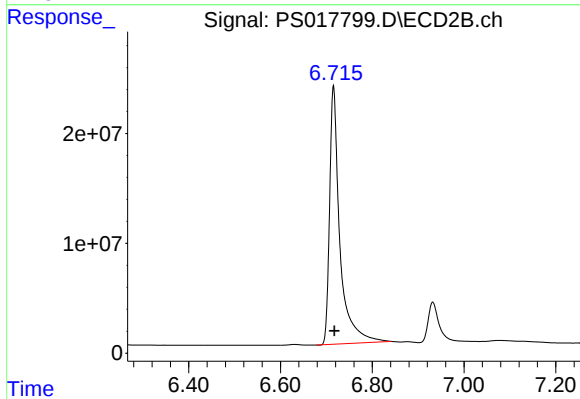

#4 2,4-DCAA


R.T.: 6.716 min
Delta R.T.: -0.002 min
Response: 367100513
Conc: 615.84 ng/ml

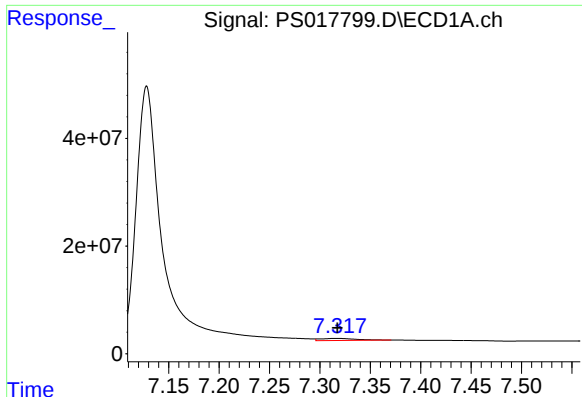

#5 DICAMBA


R.T.: 7.317 min
Delta R.T.: 0.000 min
Response: 9257592
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

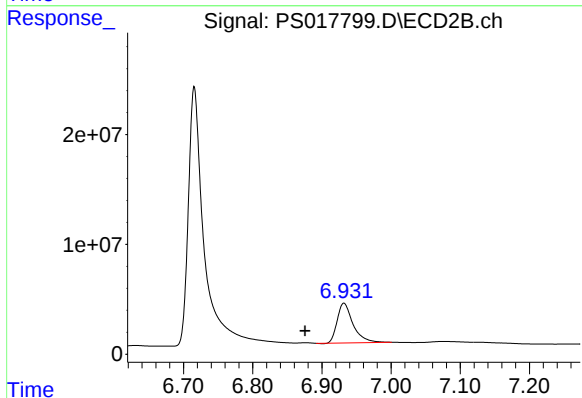


#5 DICAMBA

R.T.: 6.932 min
Delta R.T.: 0.056 min
Response: 57276059
Conc: 21.50 ng/ml

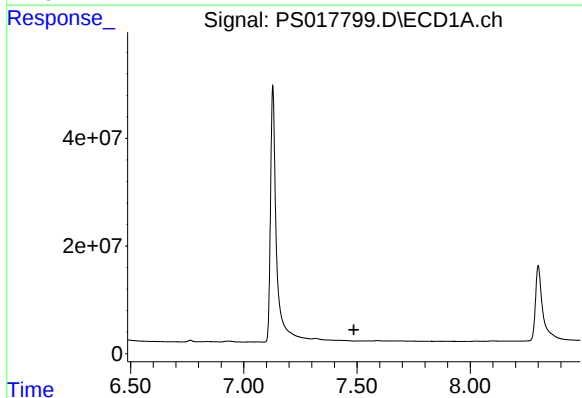


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

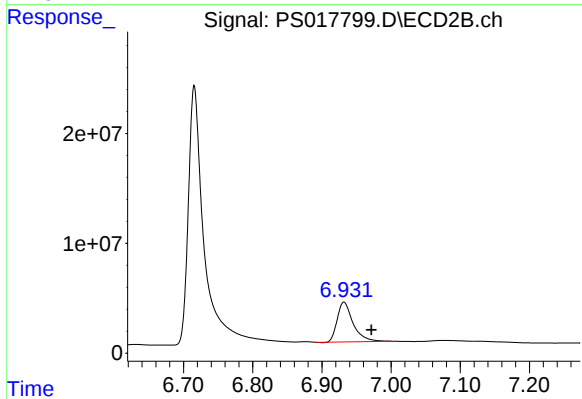

#6 MCP


R.T.: 6.932 min
Delta R.T.: -0.040 min
Response: 57276059
Conc: 26.31 ug/ml

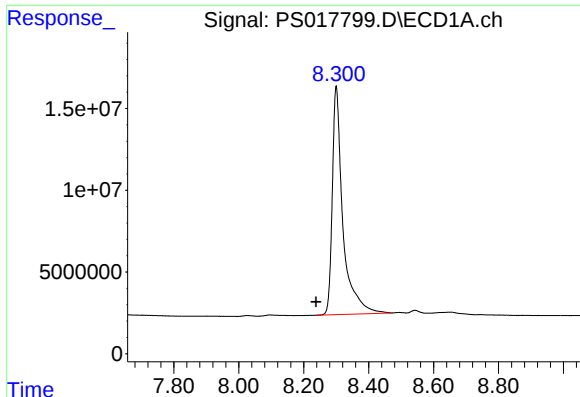

#9 2,4-D


R.T.: 8.300 min
Delta R.T.: 0.062 min
Response: 316798683
Conc: 179.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

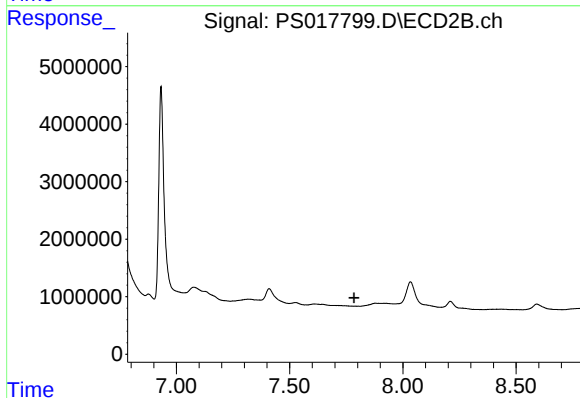


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

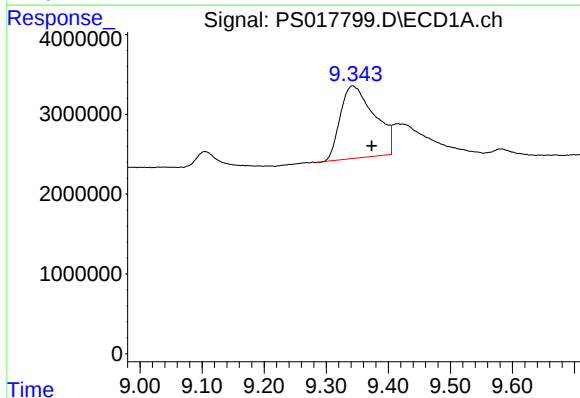


#12 2,4,5-T

R.T.: 9.343 min
Delta R.T.: -0.031 min
Response: 34564335
Conc: 3.97 ng/ml

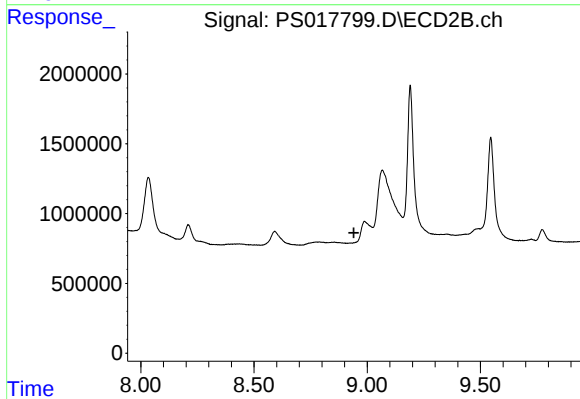

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.941 min
Response: 0
Conc: N.D.

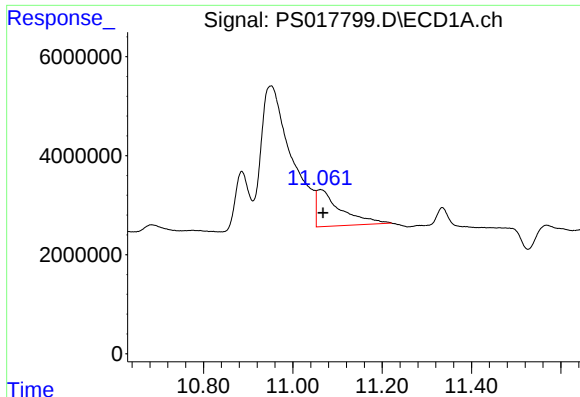

#14 DINoseb


R.T.: 11.062 min
Delta R.T.: -0.006 min
Response: 28027237
Conc: 4.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

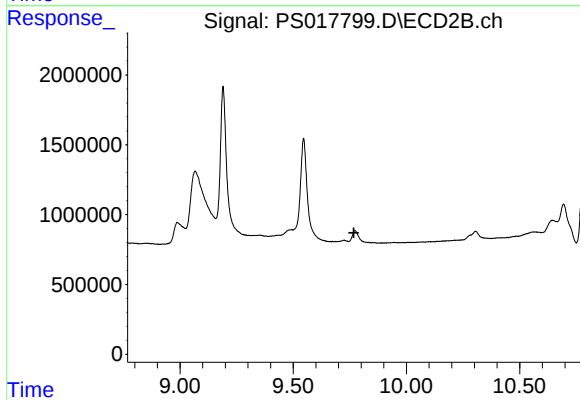


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

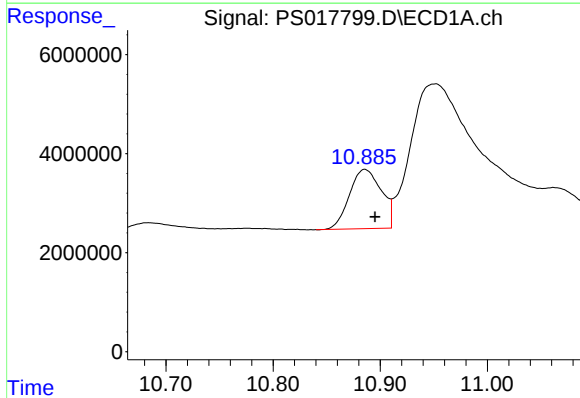

#15 Picloram

R.T.: 10.886 min
Delta R.T.: -0.010 min
Response: 24872547
Conc: 2.29 ng/ml

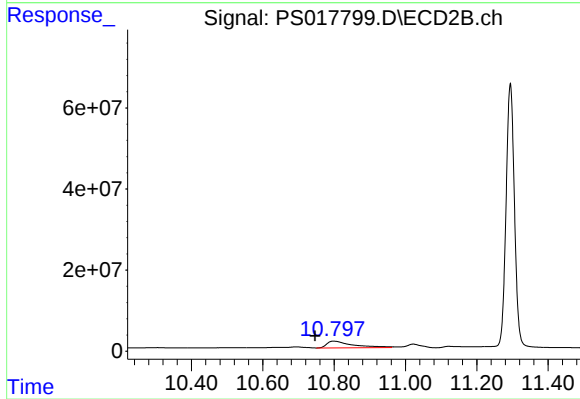

#15 Picloram

R.T.: 10.797 min
Delta R.T.: 0.051 min
Response: 82376989
Conc: 16.77 ng/ml