

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122221\
 Data File : PS017802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2021 13:49
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 14:31:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.129	6.711	871.5E6	392.1E6	557.582	657.855
Target Compounds							
2) T	3,5-DICHL...	6.392	0.000	232.6E6	0	104.108	N.D. #
5) T	DICAMBA	7.319	6.926f	19681791	62261419	3.113	23.372 #
6) T	MCP	0.000	6.926f	0	62261419	N.D.	28.605
7) T	MCPA	7.585f	0.000	8101149	0	1.225	N.D. #
9) T	2,4-D	8.298f	0.000	333.7E6	0	188.768	N.D. #
10) T	Pentachlo...	8.542	8.203	17739285	7597749	<MDL	<MDL #
11) T	2,4,5-TP ...	9.097	0.000	15375308	0	1.807	N.D. #
12) T	2,4,5-T	9.412	0.000	30156155	0	3.467	N.D. #
14) T	DINOSEB	11.069	0.000	24655740	0	3.606	N.D. #
15) T	Picloram	10.881	10.801f	34361140	16849650	3.167	3.431
16) T	DCPA	11.336	10.688	20983323	16213568	1.932	3.620 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122221\
Data File : PS017802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2021 13:49
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 14:31:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

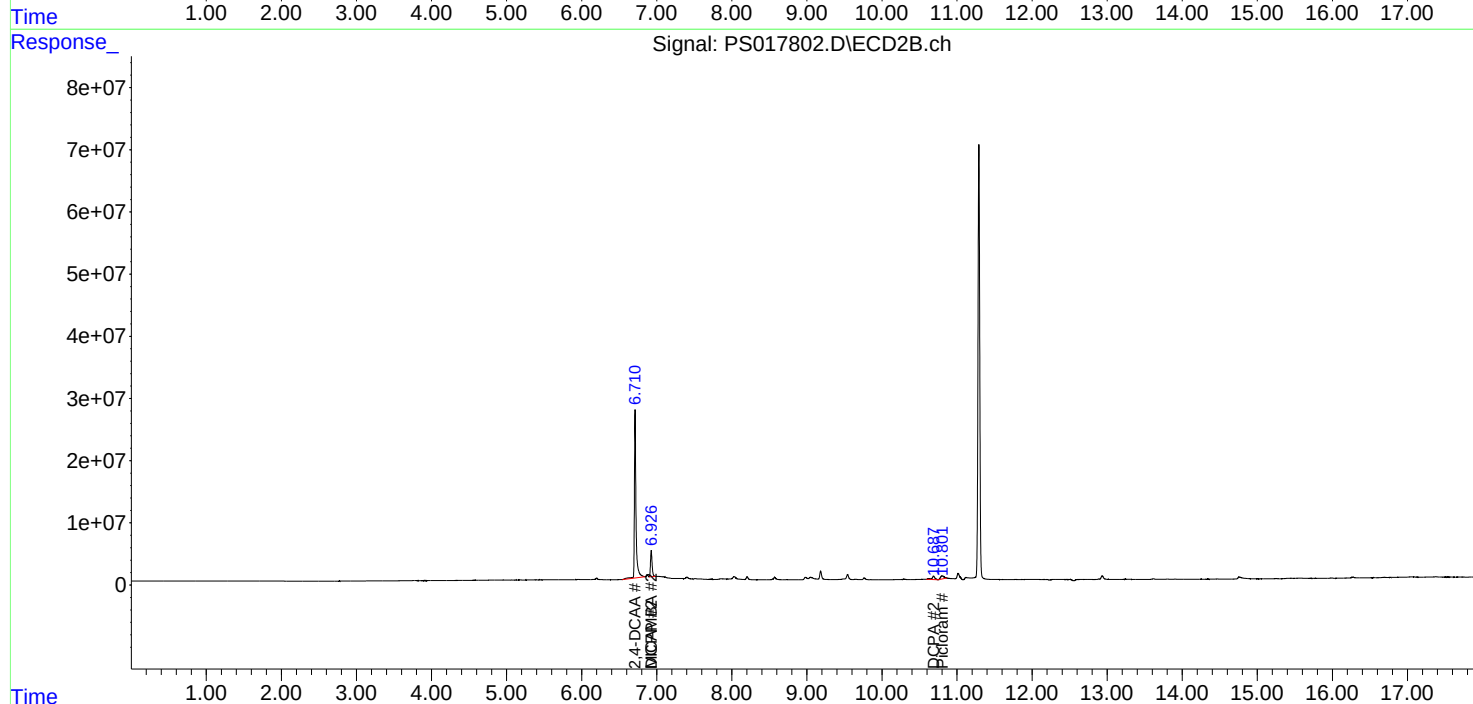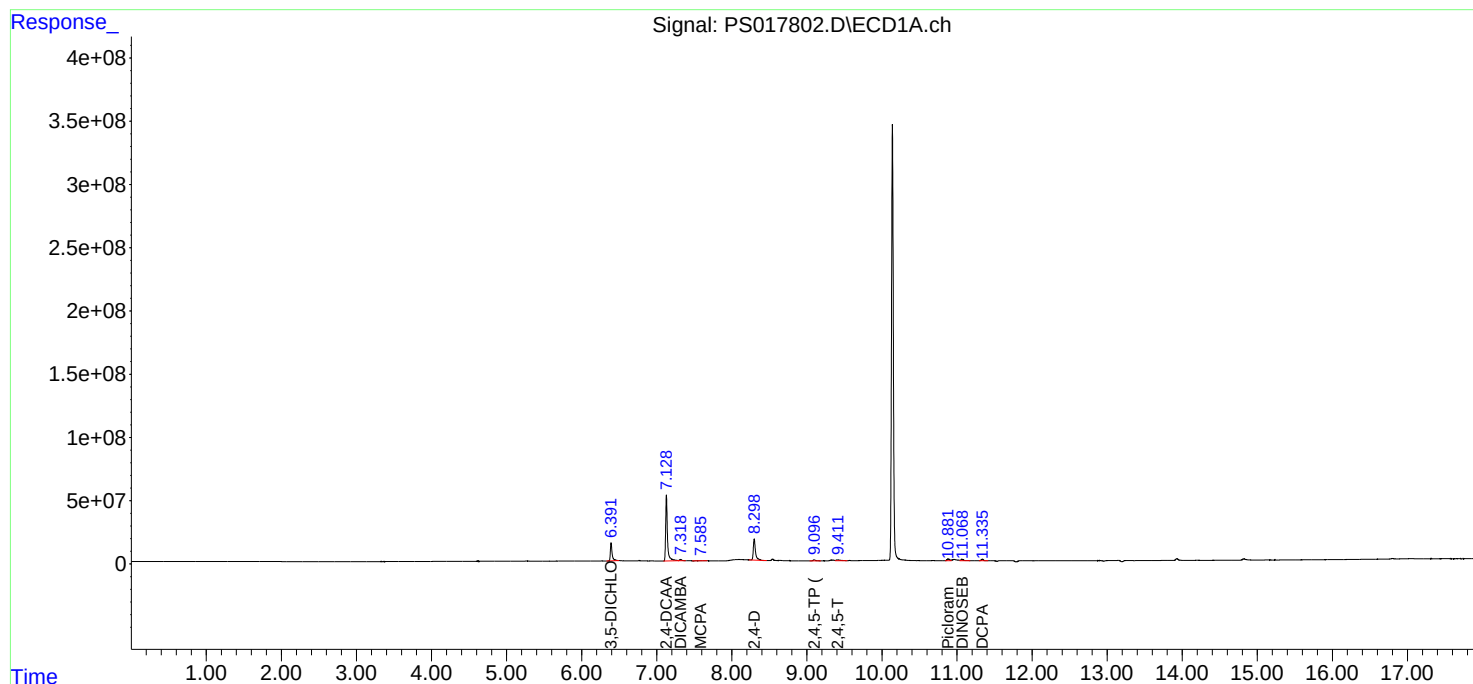


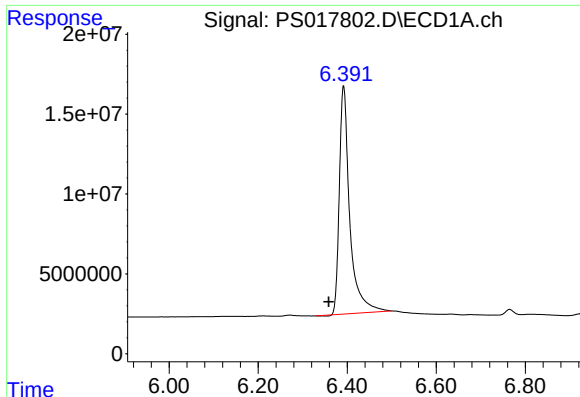

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.392 min
Delta R.T.: 0.034 min
Response: 232591411
Conc: 104.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

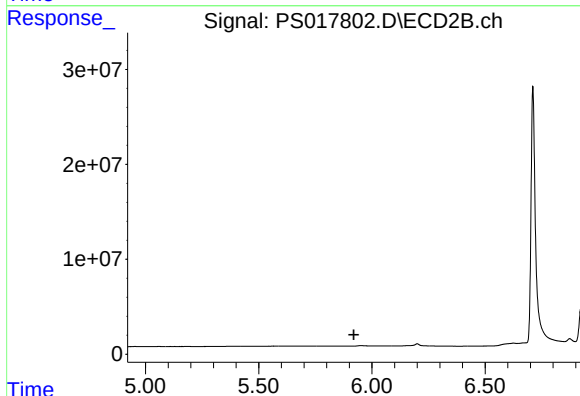


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

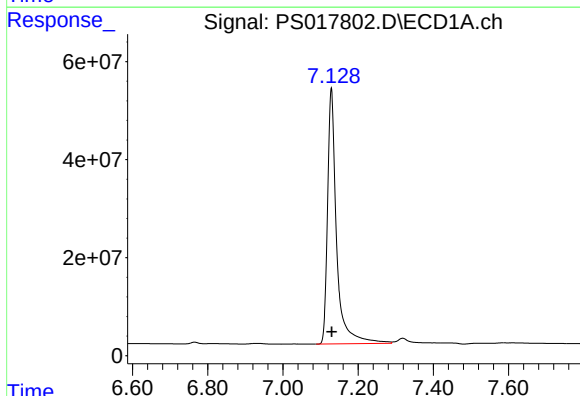


#4 2,4-DCAA

R.T.: 7.129 min
Delta R.T.: -0.001 min
Response: 871471066
Conc: 557.58 ng/ml

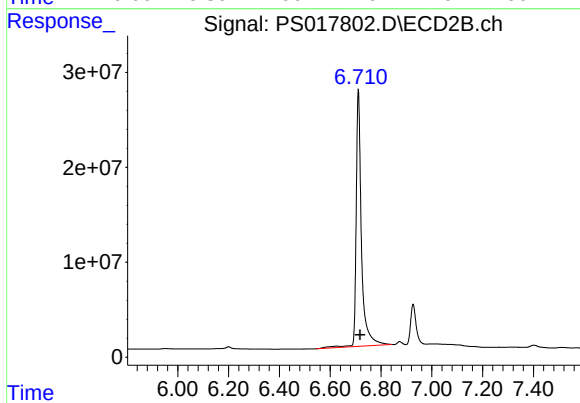

#4 2,4-DCAA


R.T.: 6.711 min
Delta R.T.: -0.007 min
Response: 392148446
Conc: 657.86 ng/ml

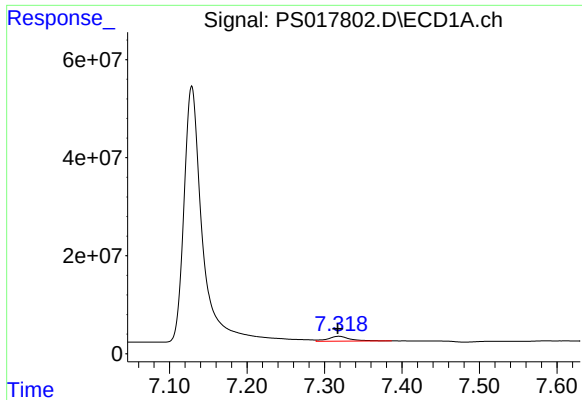

#5 DICAMBA


R.T.: 7.319 min
Delta R.T.: 0.001 min
Response: 19681791
Conc: 3.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

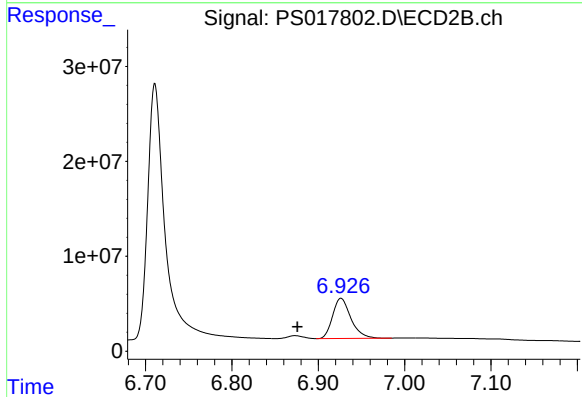


#5 DICAMBA

R.T.: 6.926 min
Delta R.T.: 0.051 min
Response: 62261419
Conc: 23.37 ng/ml

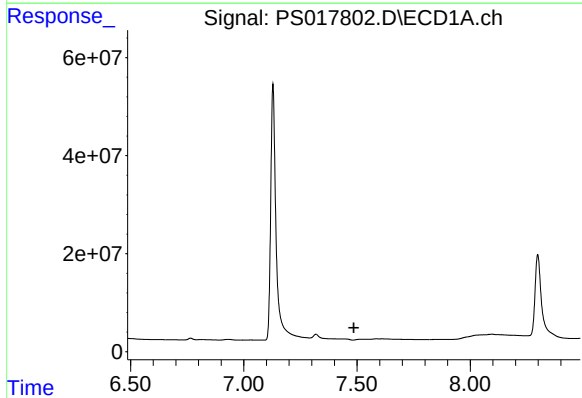


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

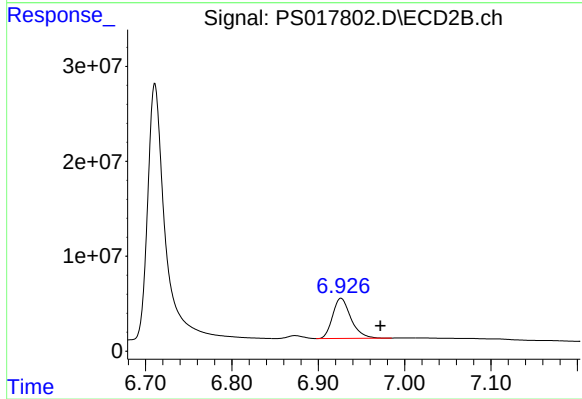

#6 MCP


R.T.: 6.926 min
Delta R.T.: -0.045 min
Response: 62261419
Conc: 28.60 ug/ml

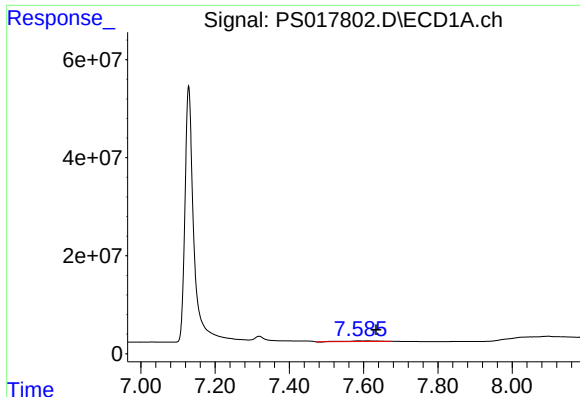

#7 MCPA


R.T.: 7.585 min
Delta R.T.: -0.048 min
Response: 8101149
Conc: 1.22 ug/ml

Instrument :
ECD_S
ClientSampleId :

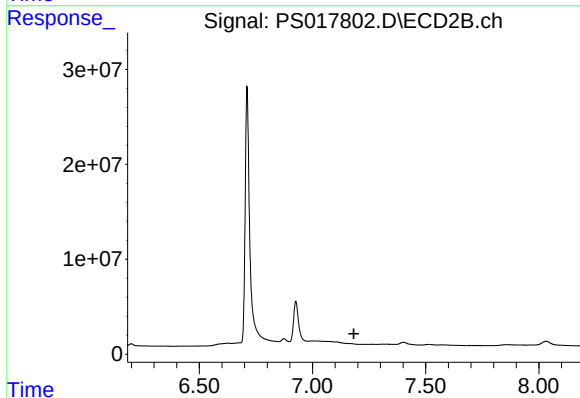


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.183 min
Response: 0
Conc: N.D.

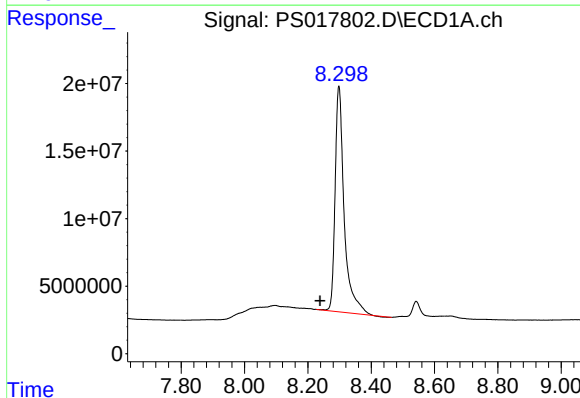


#9 2,4-D

R.T.: 8.298 min
Delta R.T.: 0.060 min
Response: 333717976
Conc: 188.77 ng/ml

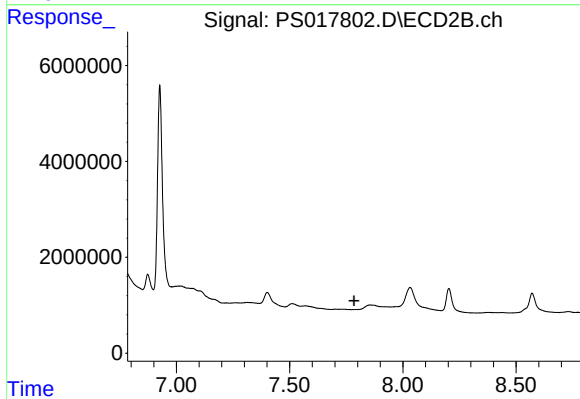

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

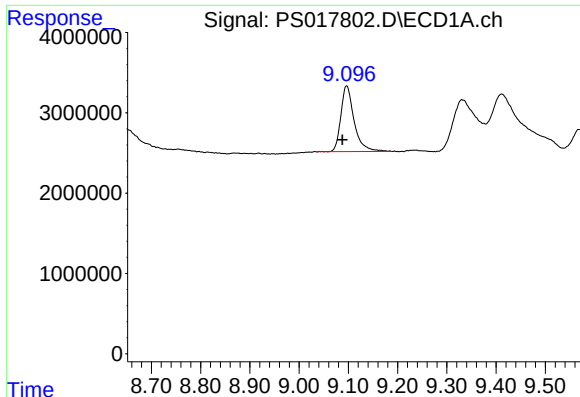

#11 2,4,5-TP (SILVEX)


R.T.: 9.097 min
Delta R.T.: 0.008 min
Response: 15375308
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

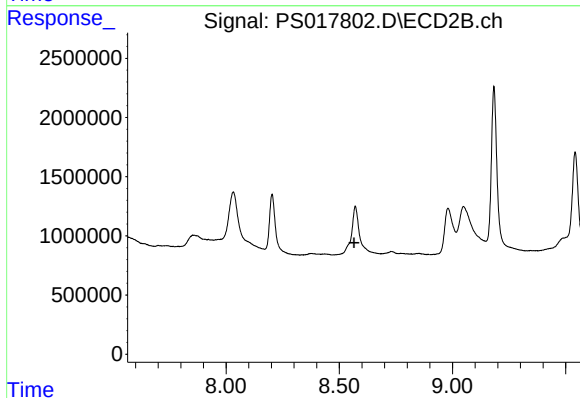


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.565 min
Response: 0
Conc: N.D.

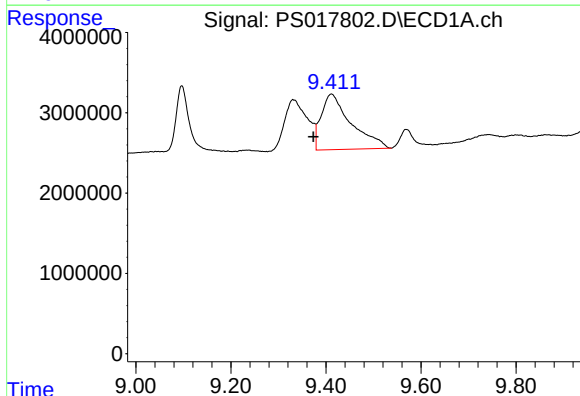


#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: 0.038 min
Response: 30156155
Conc: 3.47 ng/ml

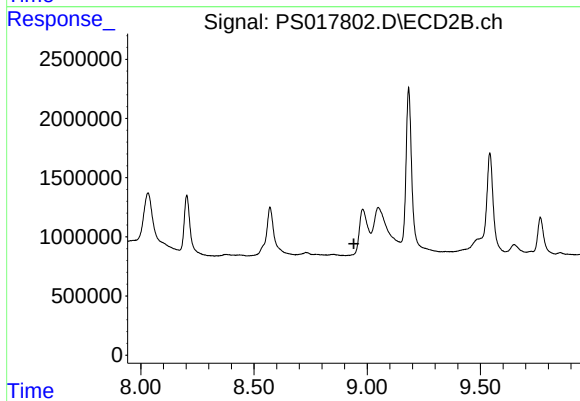

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.941 min
Response: 0
Conc: N.D.

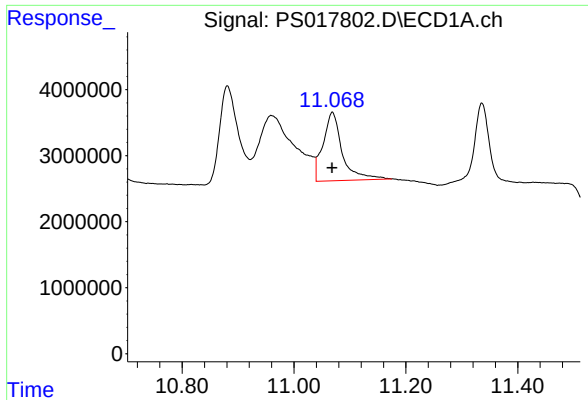

#14 DINOSEB


R.T.: 11.069 min
Delta R.T.: 0.000 min
Response: 24655740
Conc: 3.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

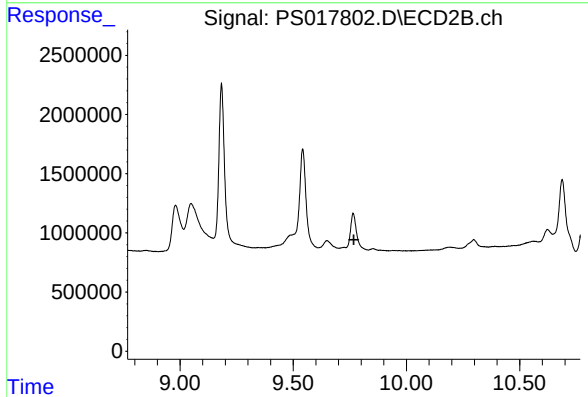


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

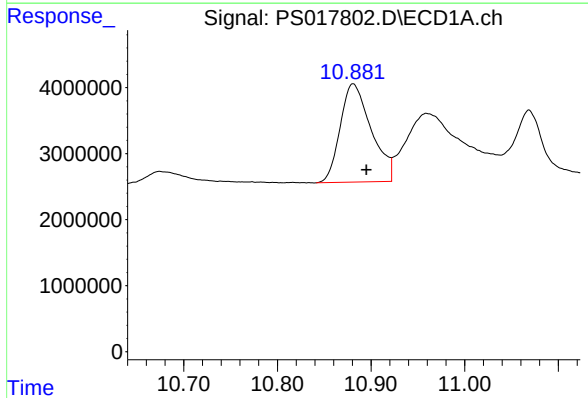


#15 Picloram

R.T.: 10.881 min
Delta R.T.: -0.014 min
Response: 34361140
Conc: 3.17 ng/ml

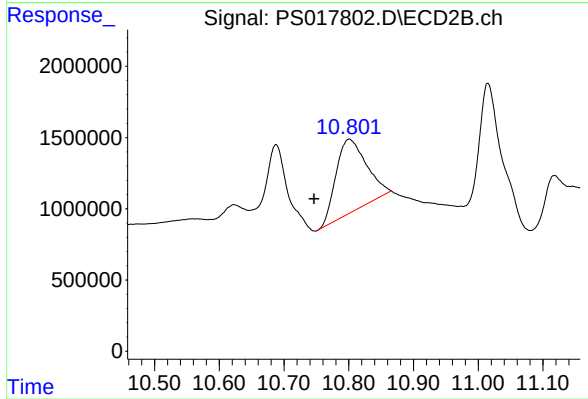

#15 Picloram


R.T.: 10.801 min
Delta R.T.: 0.054 min
Response: 16849650
Conc: 3.43 ng/ml

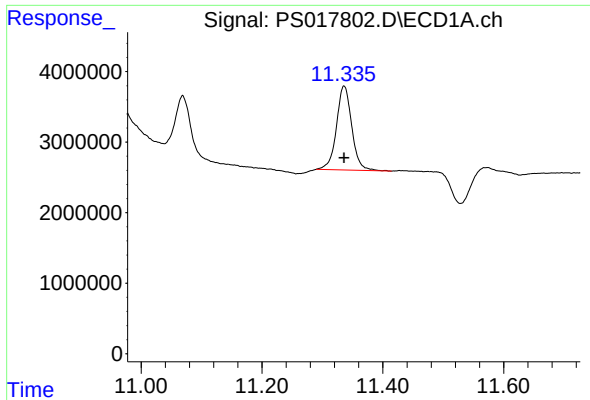

#16 DCPA

R.T.: 11.336 min
Delta R.T.: 0.000 min
Response: 20983323
Conc: 1.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

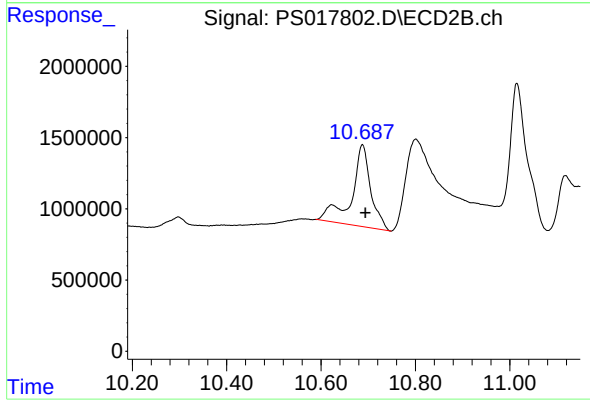

#16 DCPA

R.T.: 10.688 min
Delta R.T.: -0.006 min
Response: 16213568
Conc: 3.62 ng/ml