

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122222\
 Data File : PS021535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 01:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 02:58:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.375	6.808	1451.1E6	1006.0E6	499.441	583.531
Target Compounds							
2) T	3,5-DICHL...	5.755	0.000	1024149	0	<MDL	N.D. #
3) T	4-Nitroph...	6.219	0.000	6569472	0	3.654	N.D. #
7) T	MCPA	6.748f	0.000	7173307	0	<MDL	N.D. #
8) T	DICHLORPROP	7.116	7.638	279843	6402634	<MDL	3.251 #
9) T	2,4-D	0.000	7.941f	0	539968	N.D.	<MDL
10) T	Pentachlo...	7.543	0.000	694768	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.080	8.684	6888923	5772735	<MDL	<MDL #
12) T	2,4,5-T	8.364	9.073	8138489	13633053	<MDL	1.258 #
13) T	2,4-DB	8.868	9.583	553665	921203	<MDL	<MDL #
14) T	DINOSEB	9.901	9.892	3030033	1047722	<MDL	<MDL #
15) T	Picloram	9.717	10.866	20619476	2581552	<MDL	<MDL #
16) T	DCPA	10.162	10.817	2398000	8322397	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122222\
Data File : PS021535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 01:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 02:58:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

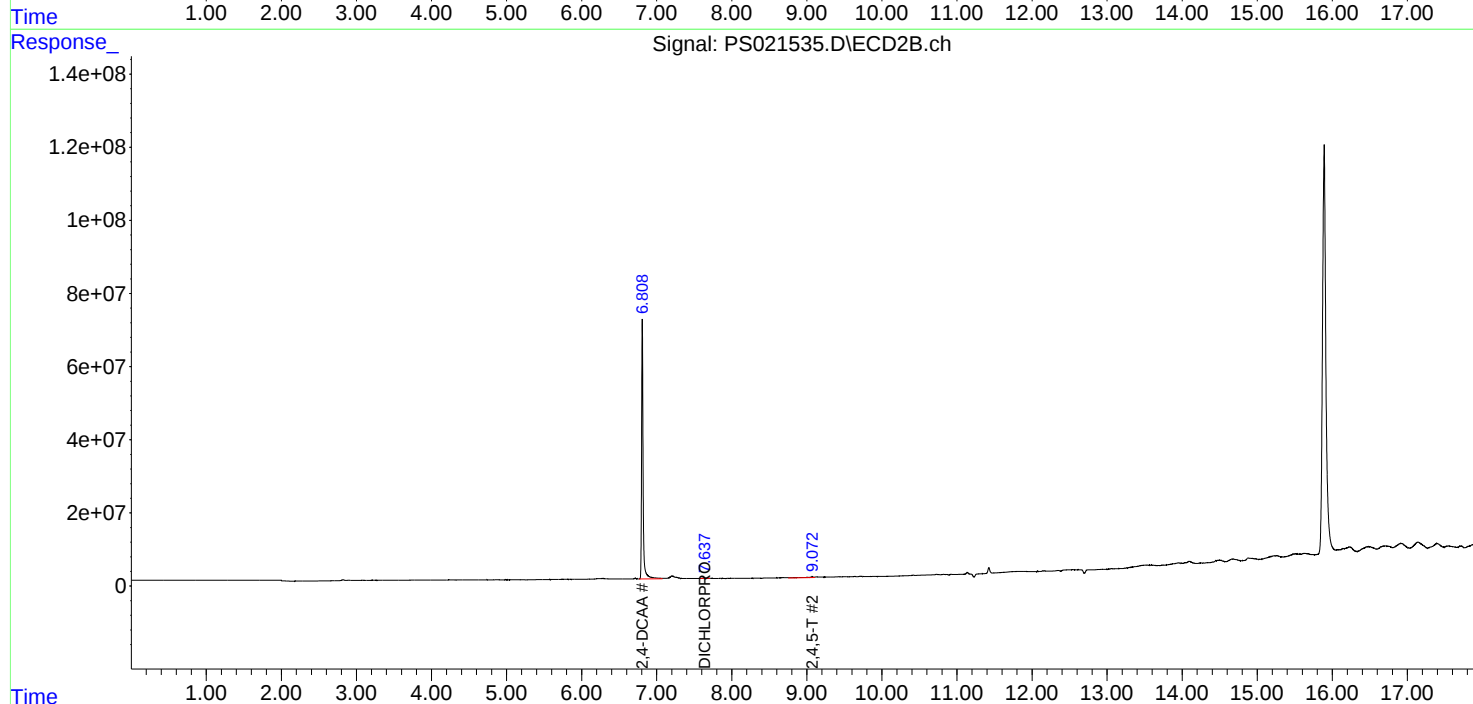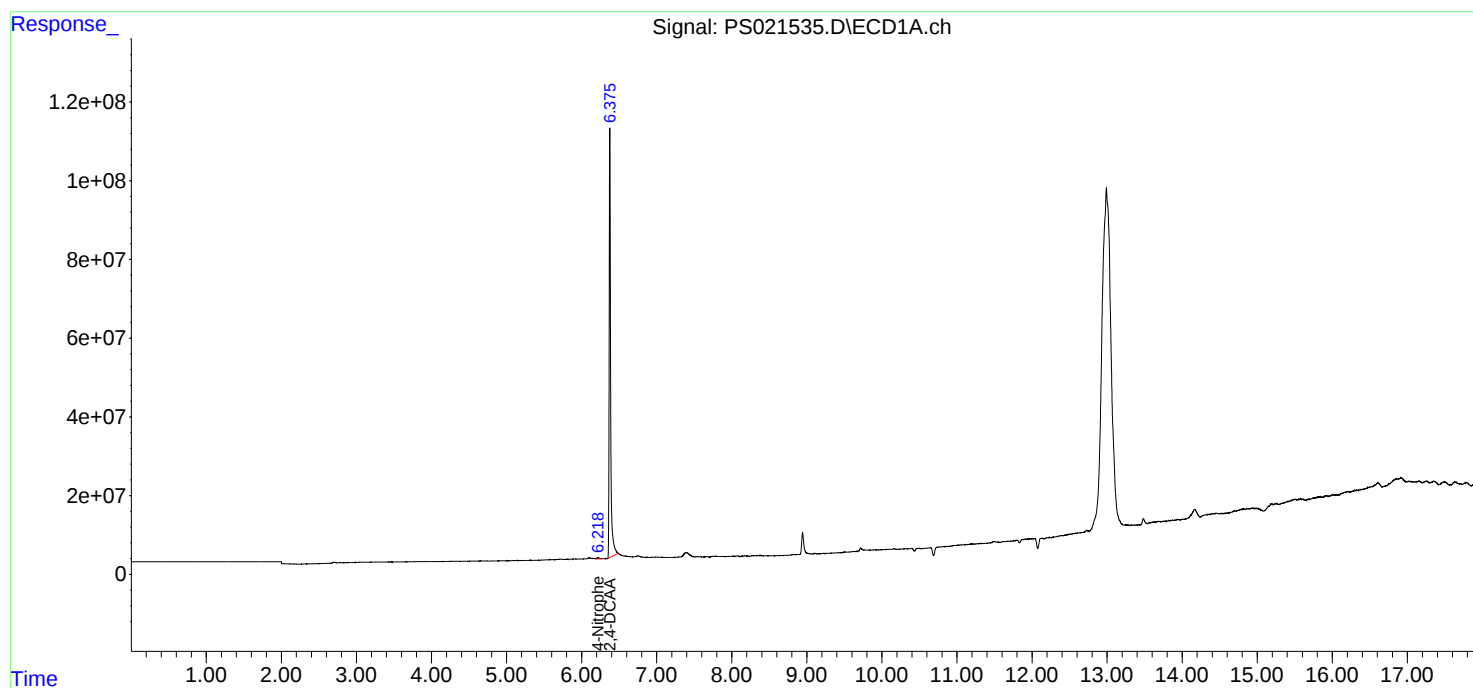


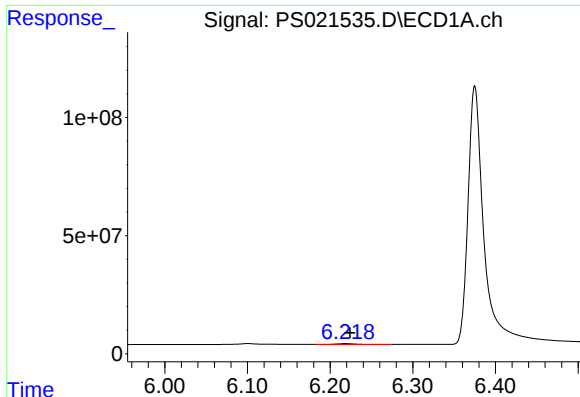

#3 4-Nitrophenol


R.T.: 6.219 min
Delta R.T.: -0.006 min
Response: 6569472
Conc: 3.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

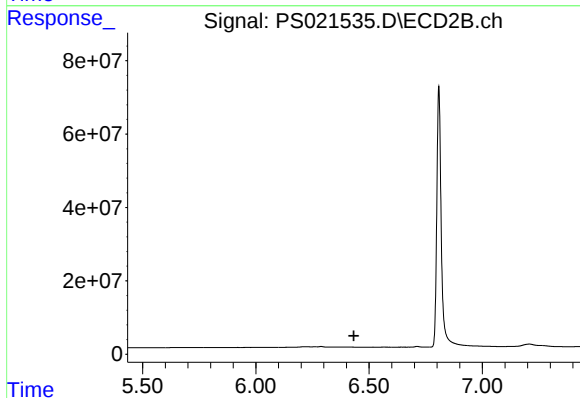


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

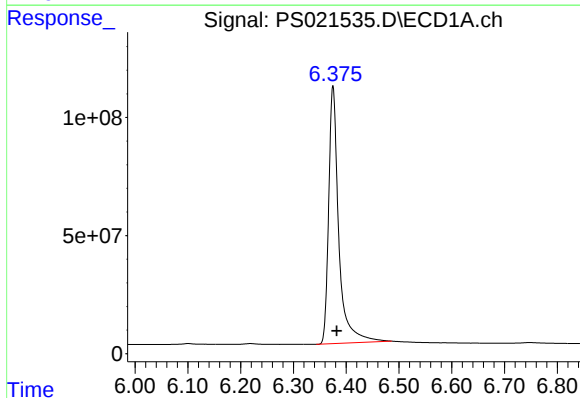


#4 2,4-DCAA

R.T.: 6.375 min
Delta R.T.: -0.007 min
Response: 1451123555
Conc: 499.44 ng/ml

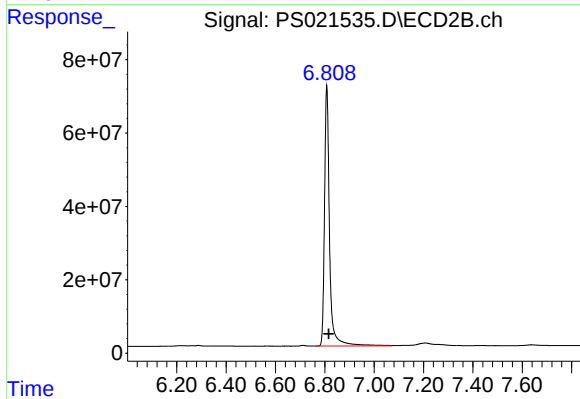

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: -0.008 min
Response: 1006003574
Conc: 583.53 ng/ml

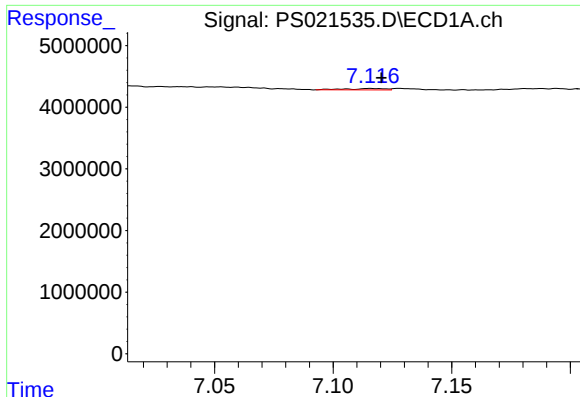

#8 DICHLORPROP


R.T.: 7.116 min
Delta R.T.: -0.004 min
Response: 279843
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

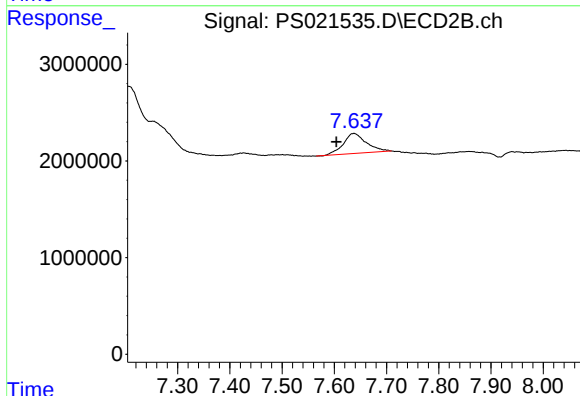


#8 DICHLORPROP

R.T.: 7.638 min
Delta R.T.: 0.034 min
Response: 6402634
Conc: 3.25 ng/ml

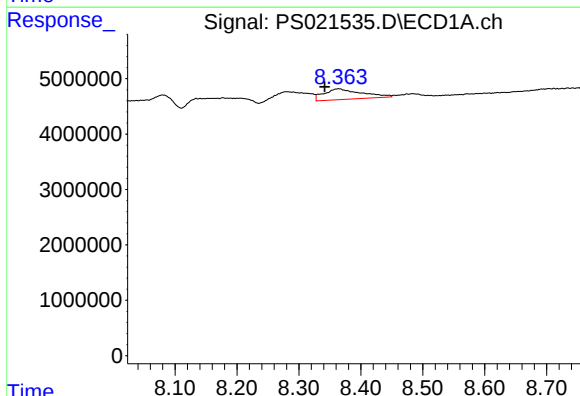

#12 2,4,5-T

R.T.: 8.364 min
Delta R.T.: 0.022 min
Response: 8138489
Conc: N.D.

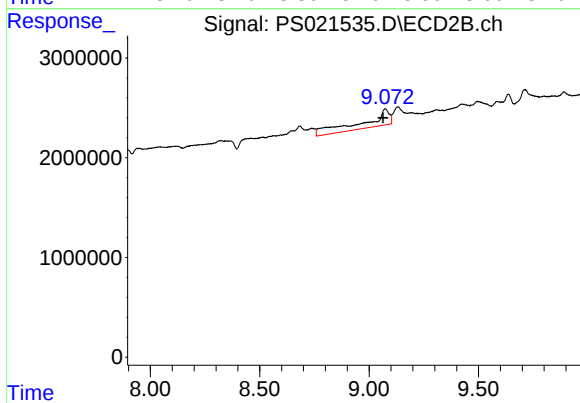

#12 2,4,5-T

R.T.: 9.073 min
Delta R.T.: 0.009 min
Response: 13633053
Conc: 1.26 ng/ml