

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122320\
 Data File : PS013586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2020 18:43
 Operator : DD\AJ
 Sample : PB133784BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:48:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.212	6.914	466.5E6	233.7E6	501.041	594.132
Target Compounds							
1) T	Dalapon	2.990f	2.586	67922111	84557461	63.230	160.899 #
2) T	3,5-DICHL...	0.000	6.096	0	34093876	N.D.	54.869
3) T	4-Nitroph...	6.986f	0.000	8288152	0	18.395	N.D. #
5) T	DICAMBA	0.000	7.047	0	7749968	N.D.	4.611
7) T	MCPA	7.697	7.370	18890188	25121691	4.833	12.080 #
8) T	DICHLORPROP	0.000	7.758f	0	9544772	N.D.	21.357
10) T	Pentachlo...	8.683f	0.000	22287118	0	1.663	N.D. #
11) T	2,4,5-TP ...	0.000	8.766	0	8106161	N.D.	3.453
12) T	2,4,5-T	9.399f	0.000	18683586	0	3.379	N.D. #
15) T	Picloram	11.063f	11.054f	20344101	38124786	2.954	10.950 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122320\
Data File : PS013586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2020 18:43
Operator : DD\AJ
Sample : PB133784BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:48:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

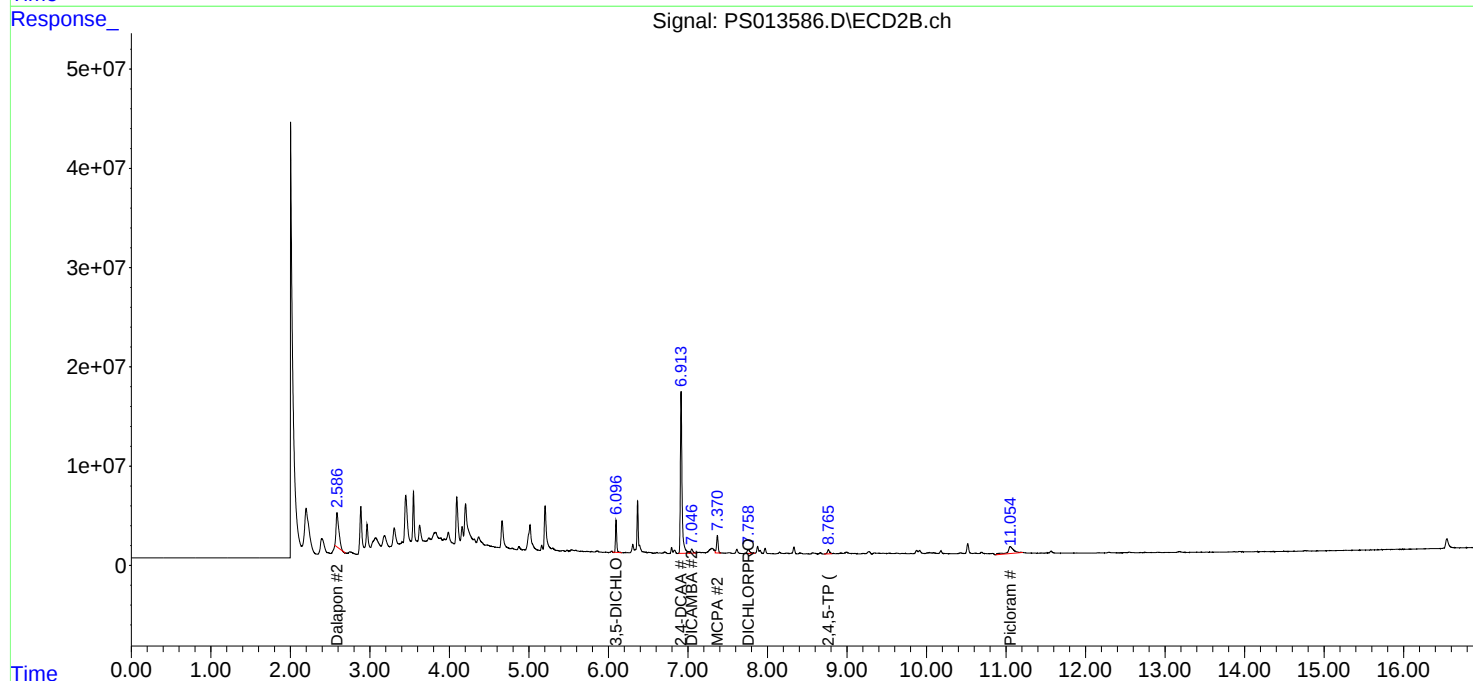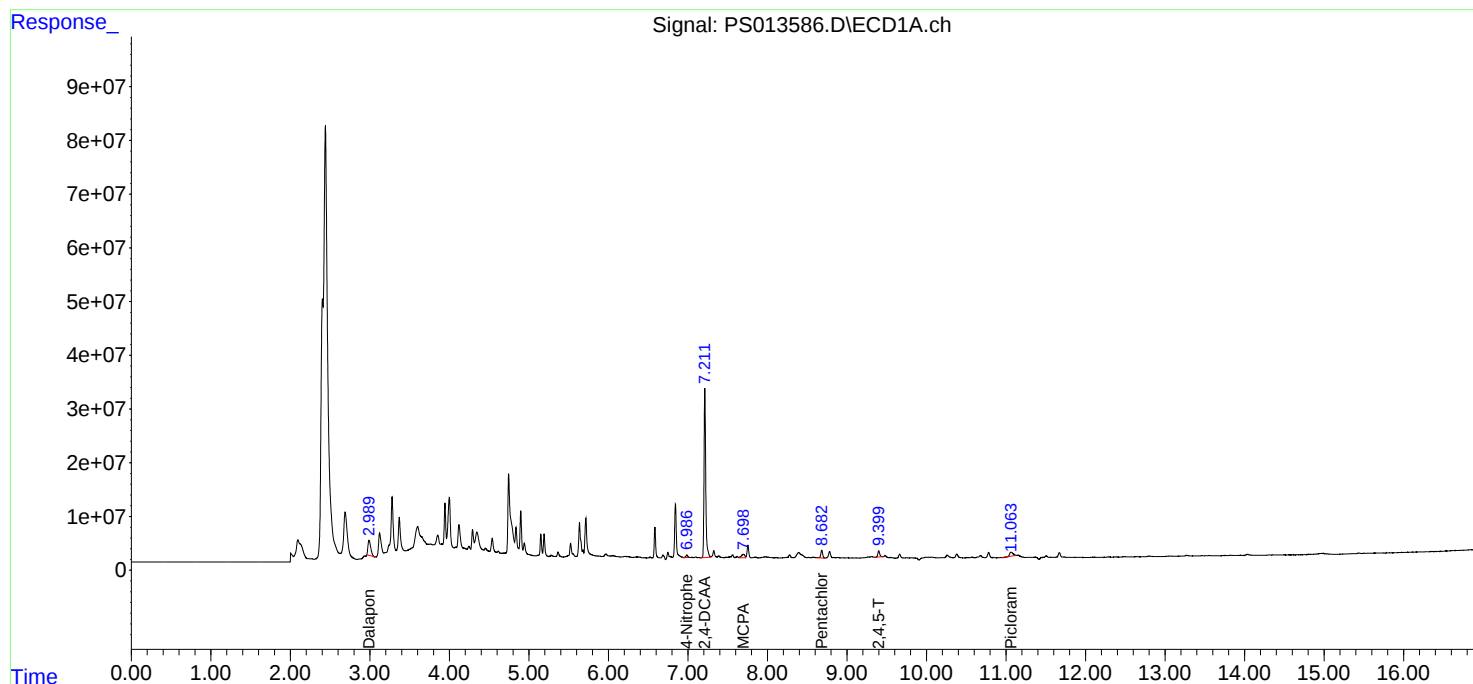


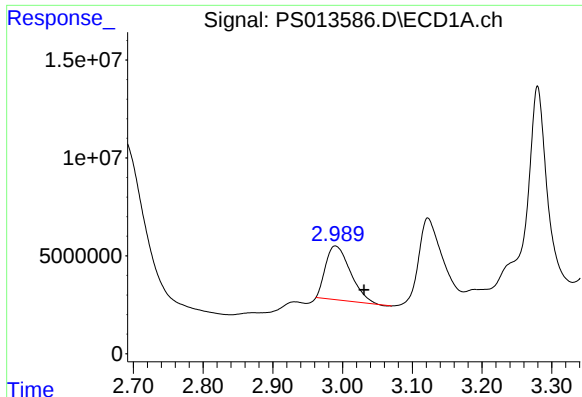

#1 Dalapon


R.T.: 2.990 min
Delta R.T.: -0.041 min
Response: 67922111
Conc: 63.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

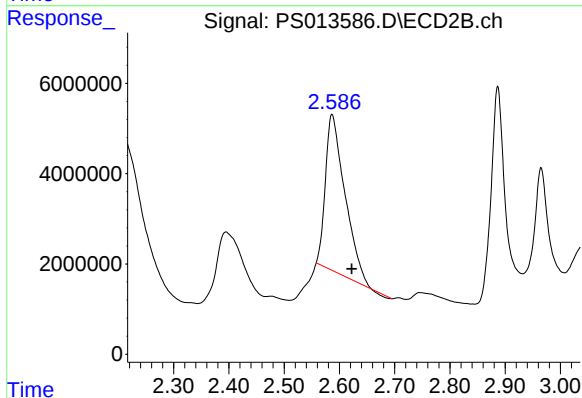


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 84557461
Conc: 160.90 ng/ml

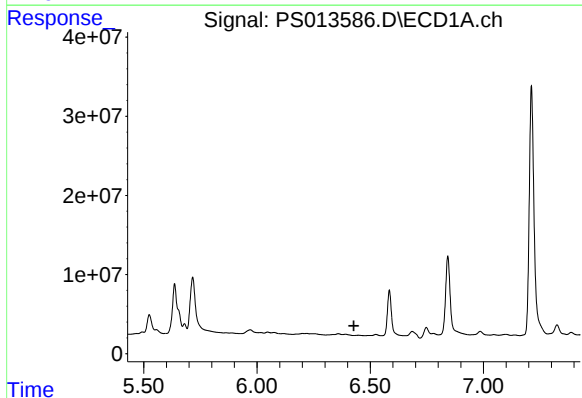


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

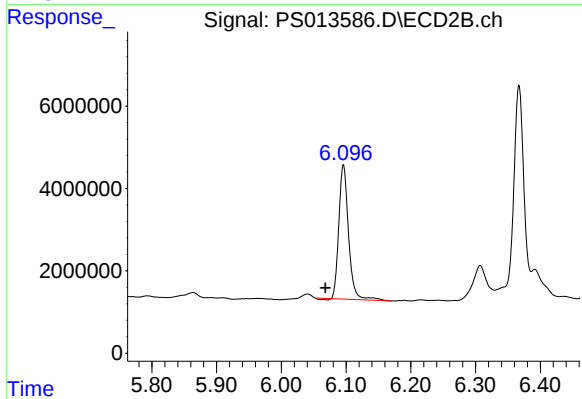

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.028 min
Response: 34093876
Conc: 54.87 ng/ml

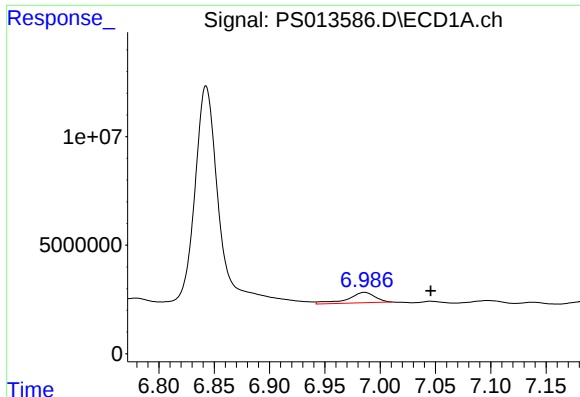

#3 4-Nitrophenol


R.T.: 6.986 min
Delta R.T.: -0.060 min
Response: 8288152
Conc: 18.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

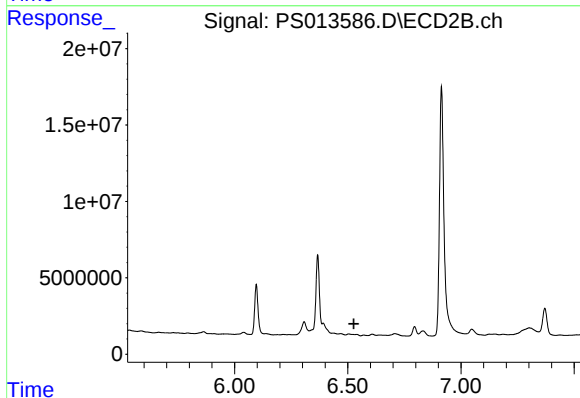


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

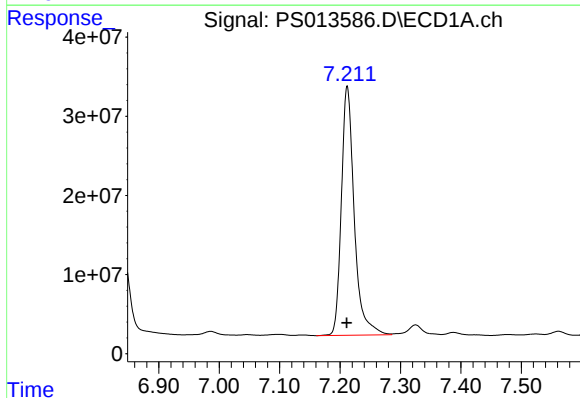


#4 2,4-DCAA

R.T.: 7.212 min
Delta R.T.: 0.001 min
Response: 466499091
Conc: 501.04 ng/ml

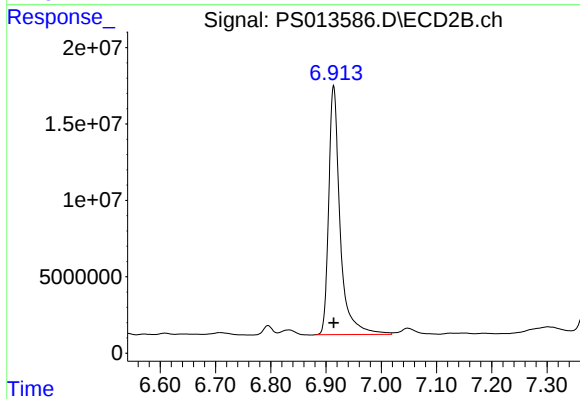

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 233708577
Conc: 594.13 ng/ml

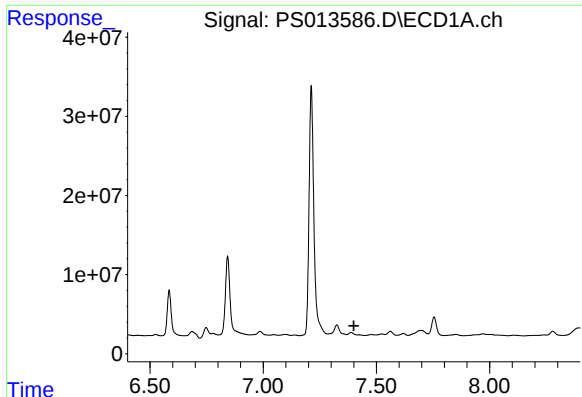

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.401 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

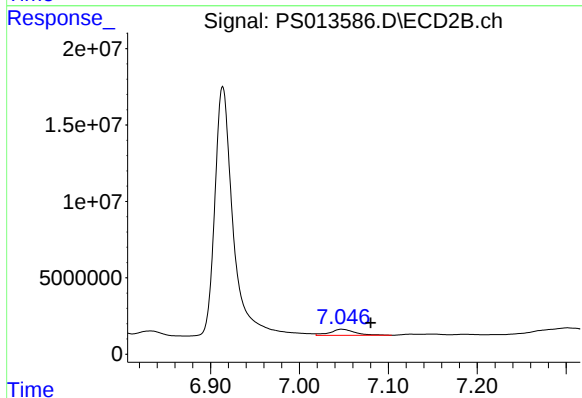


#5 DICAMBA

R.T.: 7.047 min
Delta R.T.: -0.033 min
Response: 7749968
Conc: 4.61 ng/ml

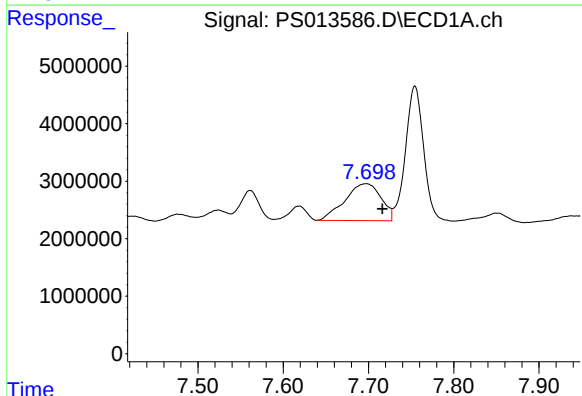


#7 MCPA

R.T.: 7.697 min
Delta R.T.: -0.020 min
Response: 18890188
Conc: 4.83 ug/ml

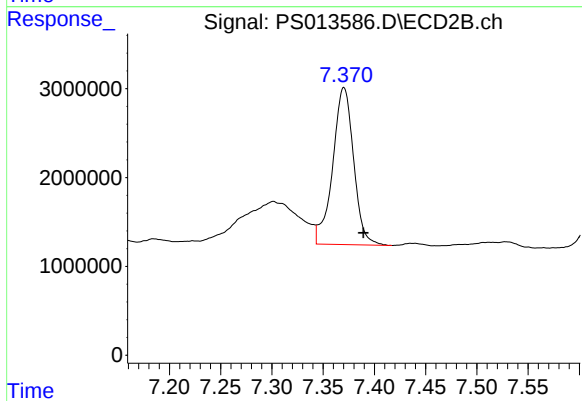

#7 MCPA


R.T.: 7.370 min
Delta R.T.: -0.019 min
Response: 25121691
Conc: 12.08 ug/ml

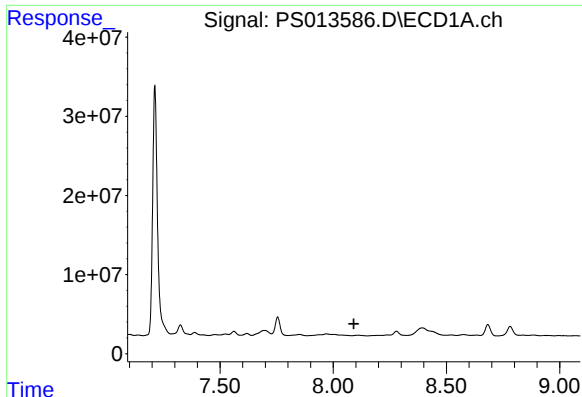

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

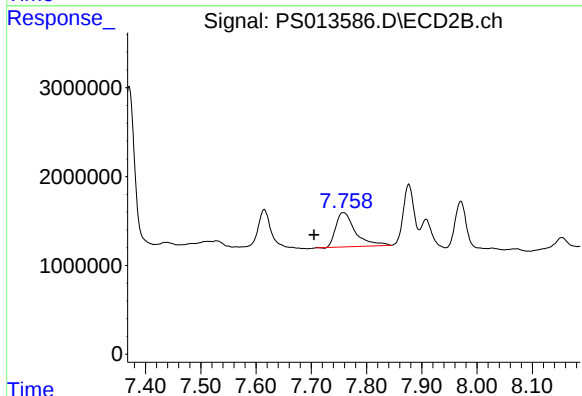


#8 DICHLORPROP

R.T.: 7.758 min
Delta R.T.: 0.053 min
Response: 9544772
Conc: 21.36 ng/ml

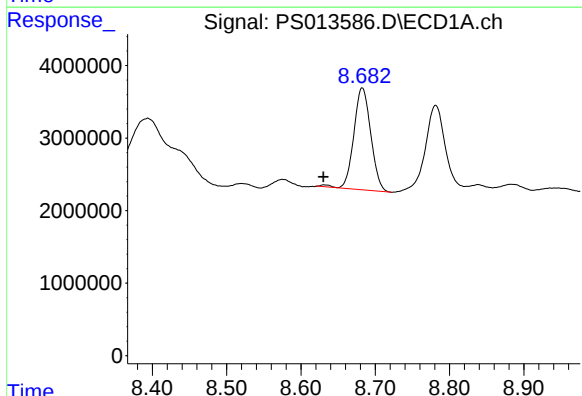


#10 Pentachlorophenol

R.T.: 8.683 min
Delta R.T.: 0.053 min
Response: 22287118
Conc: 1.66 ng/ml

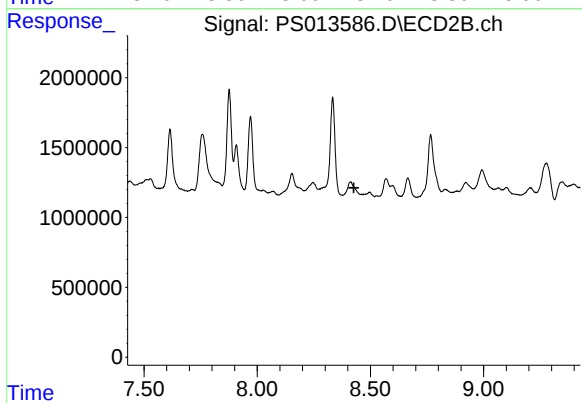

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.427 min
Response: 0
Conc: N.D.

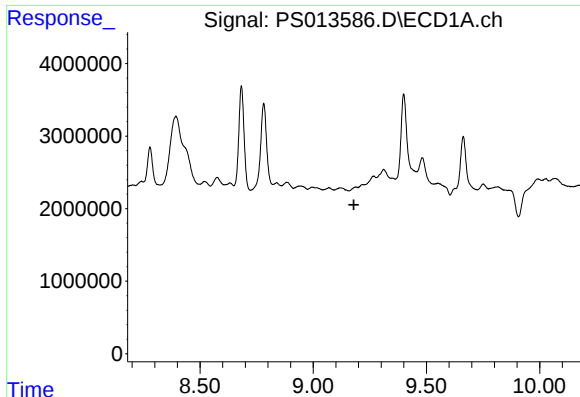

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

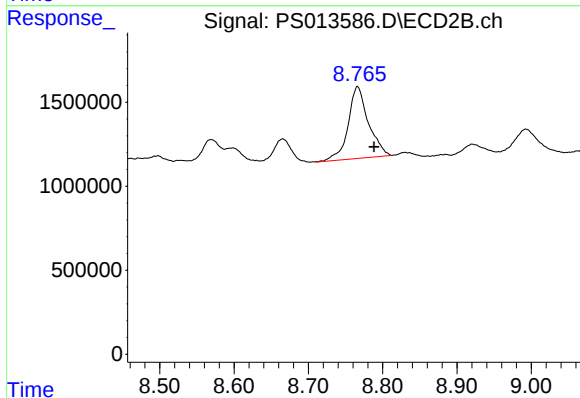


#11 2,4,5-TP (SILVEX)

R.T.: 8.766 min
Delta R.T.: -0.022 min
Response: 8106161
Conc: 3.45 ng/ml

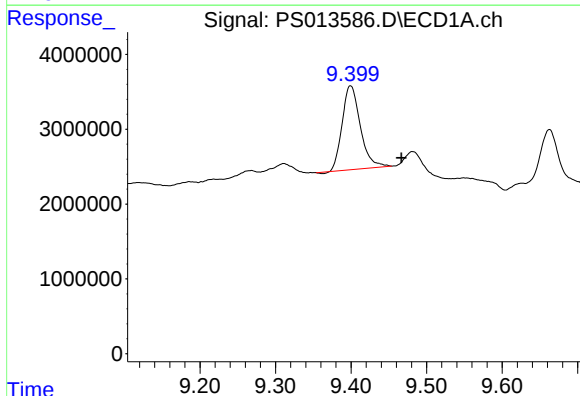


#12 2,4,5-T

R.T.: 9.399 min
Delta R.T.: -0.067 min
Response: 18683586
Conc: 3.38 ng/ml

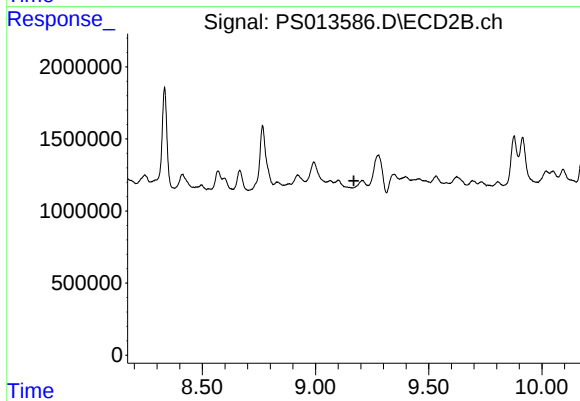

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

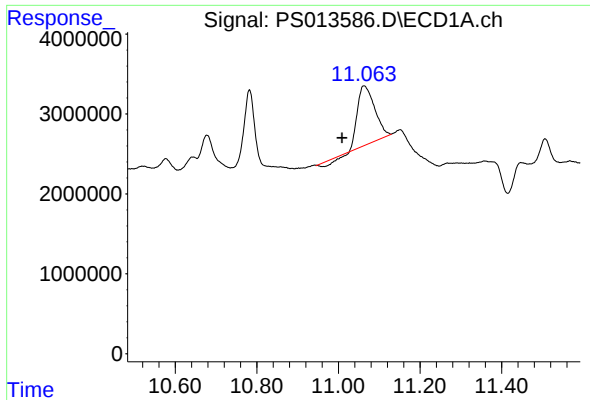

#15 Picloram

R.T.: 11.063 min
Delta R.T.: 0.054 min
Response: 20344101
Conc: 2.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

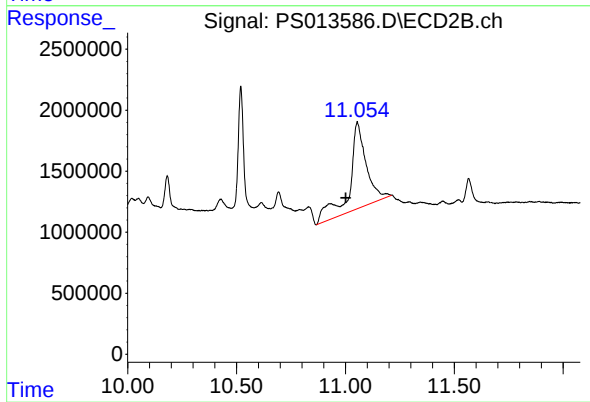

#15 Picloram

R.T.: 11.054 min
Delta R.T.: 0.053 min
Response: 38124786
Conc: 10.95 ng/ml