

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122320\
 Data File : PS013593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2020 21:24
 Operator : DD\AJ
 Sample : L5179-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:51:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	6.912	322.9E6	158.7E6	346.851	403.443
Target Compounds							
1) T	Dalapon	2.992	2.589	73529796	89457424	68.451	170.223 #
2) T	3,5-DICHL...	0.000	6.094	0	47383659	N.D.	76.257
5) T	DICAMBA	7.386	7.045	10193124	6762934	2.760	4.024 #
7) T	MCPA	7.713	0.000	74648609	0	19.099	N.D. #
8) T	DICHLORPROP	0.000	7.740	0	12064322	N.D.	26.995
10) T	Pentachlo...	8.682f	0.000	11065267	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.214	8.793	19970982	18984728	3.746	8.087 #
12) T	2,4,5-T	9.398f	9.238f	34779759	7084651	6.291	3.175 #
15) T	Picloram	11.010	0.000	11903779	0	1.728	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122320\
Data File : PS013593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2020 21:24
Operator : DD\AJ
Sample : L5179-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:51:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

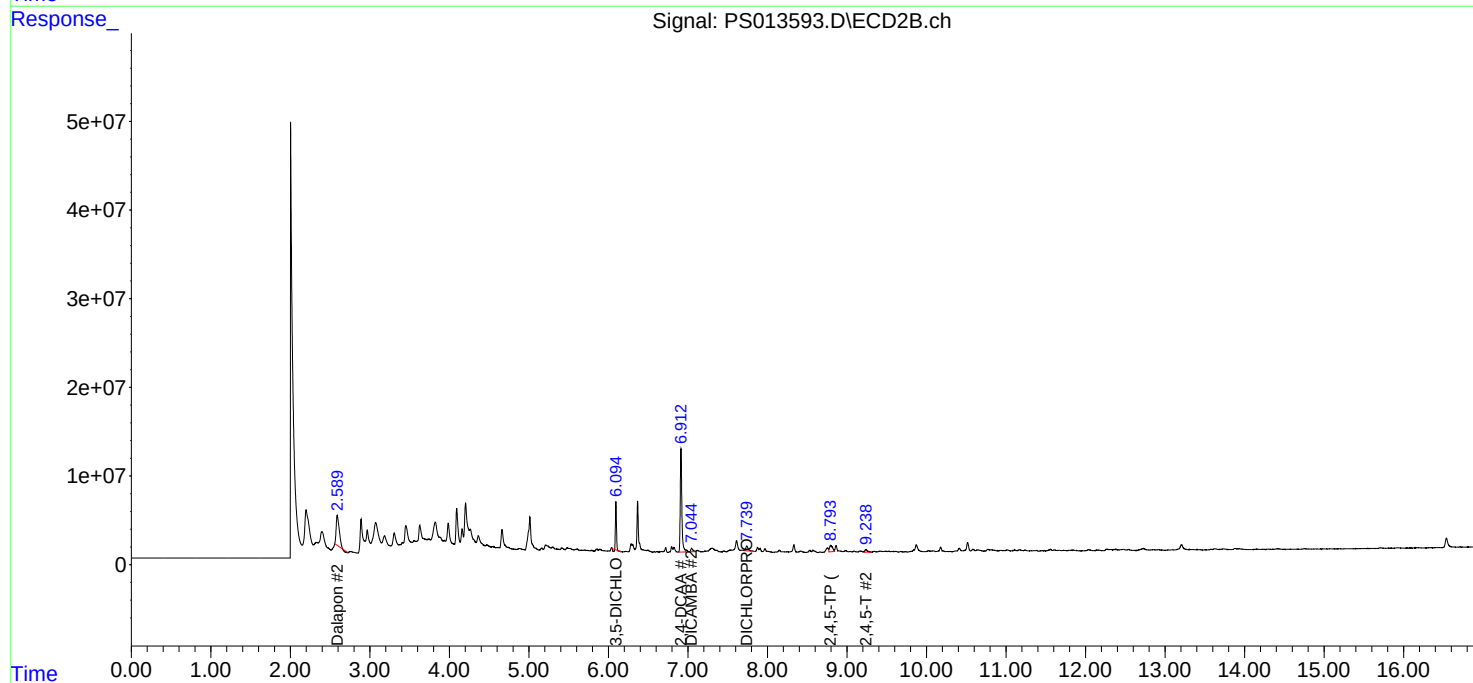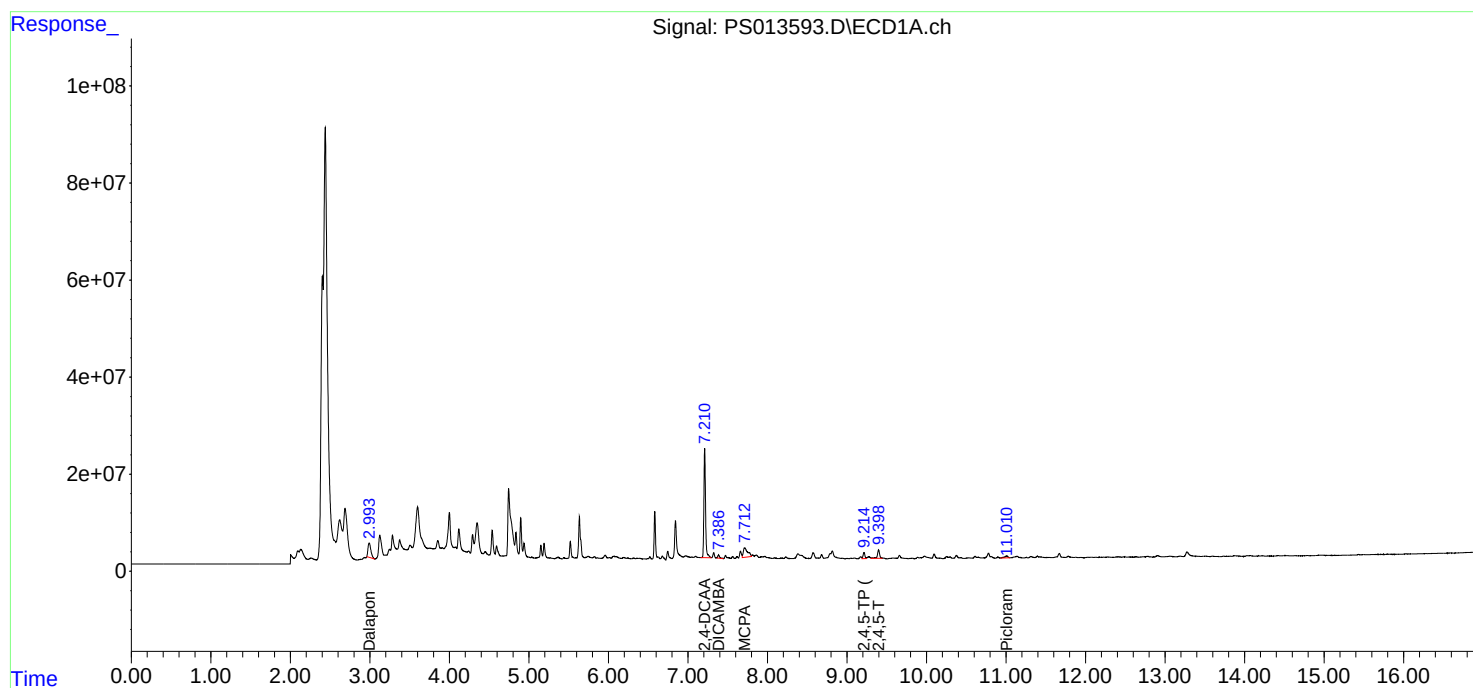


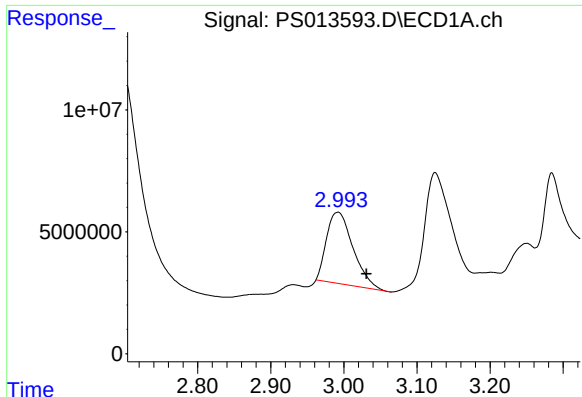

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.039 min
Response: 73529796
Conc: 68.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

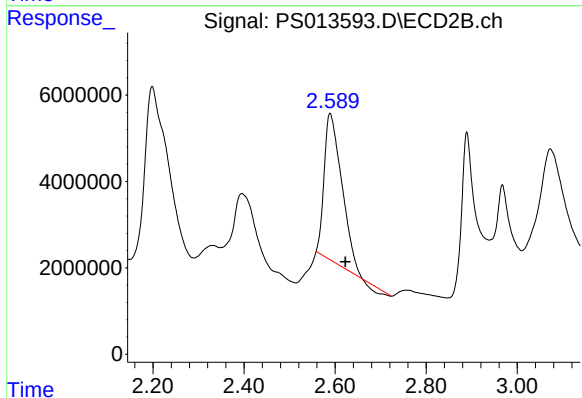


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.033 min
Response: 89457424
Conc: 170.22 ng/ml

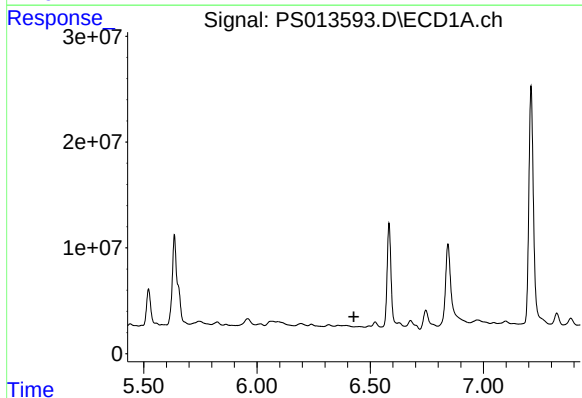


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

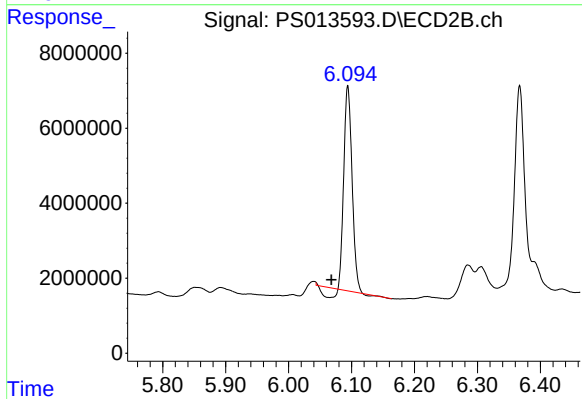

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.026 min
Response: 47383659
Conc: 76.26 ng/ml

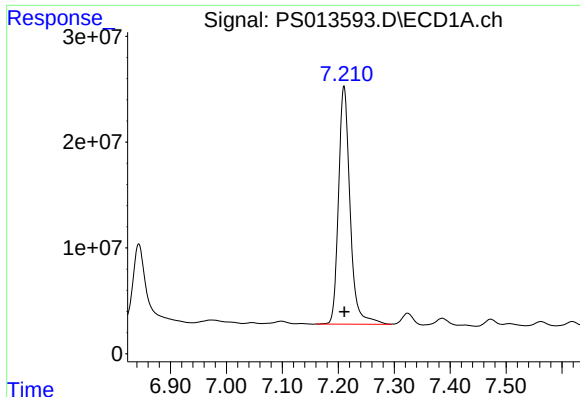

#4 2,4-DCAA


R.T.: 7.210 min
Delta R.T.: 0.000 min
Response: 322938602
Conc: 346.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

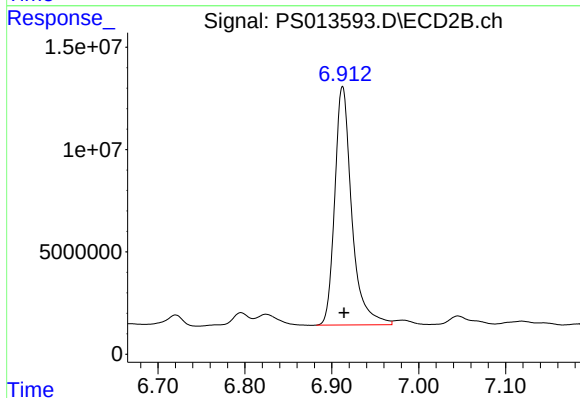


#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: -0.002 min
Response: 158698976
Conc: 403.44 ng/ml

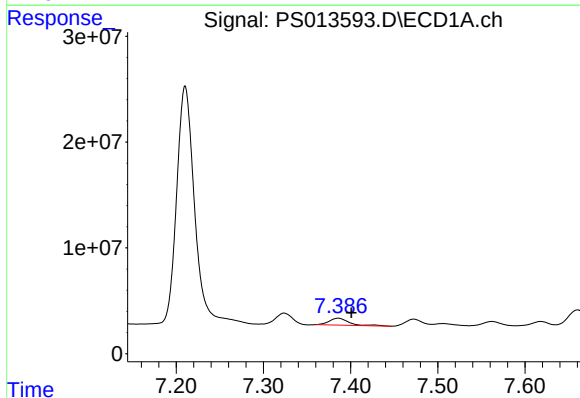


#5 DICAMBA

R.T.: 7.386 min
Delta R.T.: -0.015 min
Response: 10193124
Conc: 2.76 ng/ml

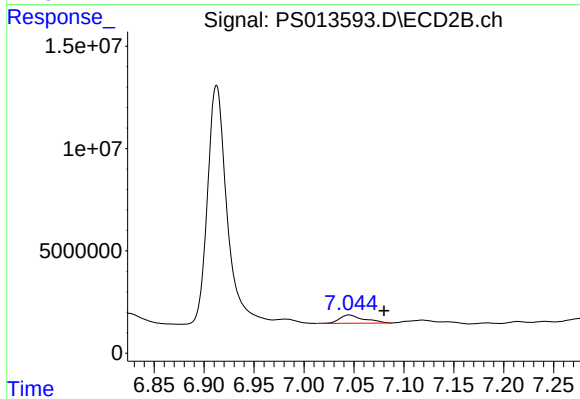

#5 DICAMBA


R.T.: 7.045 min
Delta R.T.: -0.035 min
Response: 6762934
Conc: 4.02 ng/ml

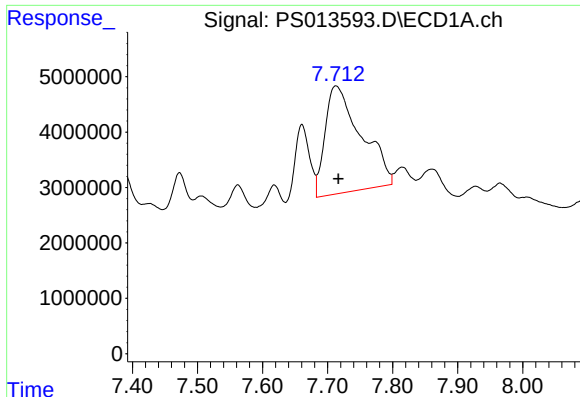

#7 MCPA


R.T.: 7.713 min
Delta R.T.: -0.004 min
Response: 74648609
Conc: 19.10 ug/ml

Instrument :
ECD_S
ClientSampleId :

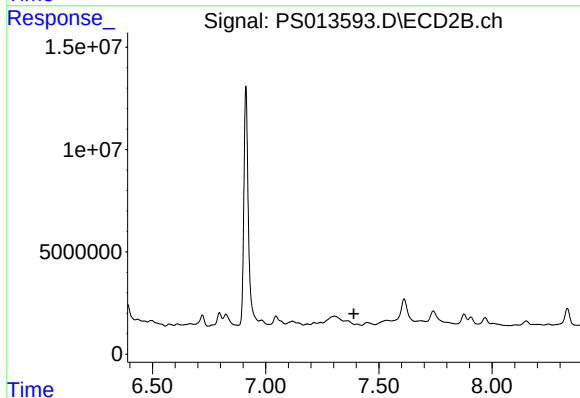


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

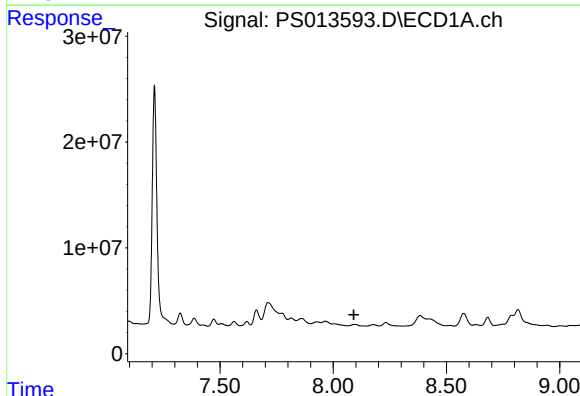


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

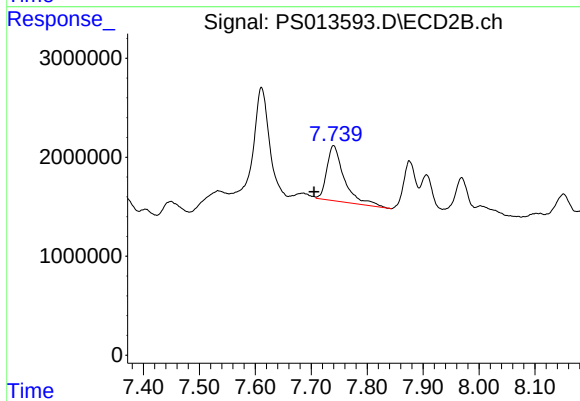

#8 DICHLORPROP


R.T.: 7.740 min
Delta R.T.: 0.035 min
Response: 12064322
Conc: 26.99 ng/ml

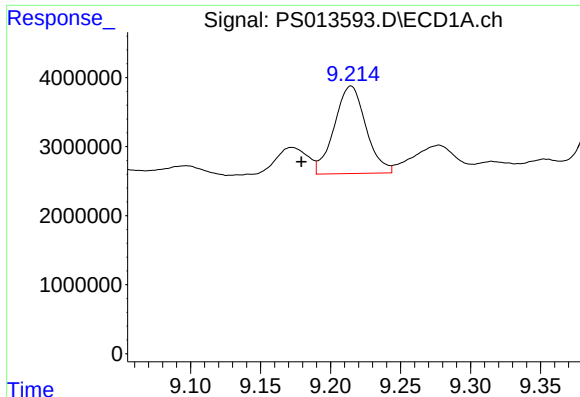

#11 2,4,5-TP (SILVEX)


R.T.: 9.214 min
Delta R.T.: 0.035 min
Response: 19970982
Conc: 3.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

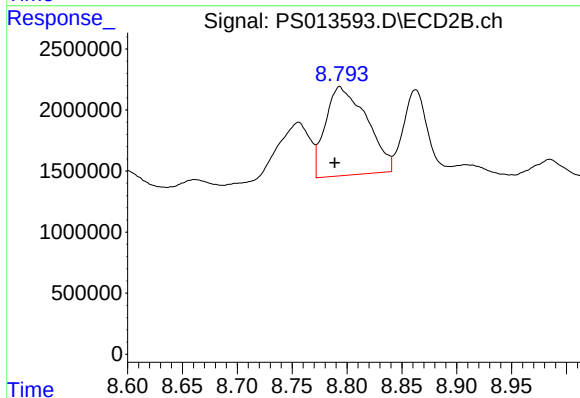


#11 2,4,5-TP (SILVEX)

R.T.: 8.793 min
Delta R.T.: 0.005 min
Response: 18984728
Conc: 8.09 ng/ml

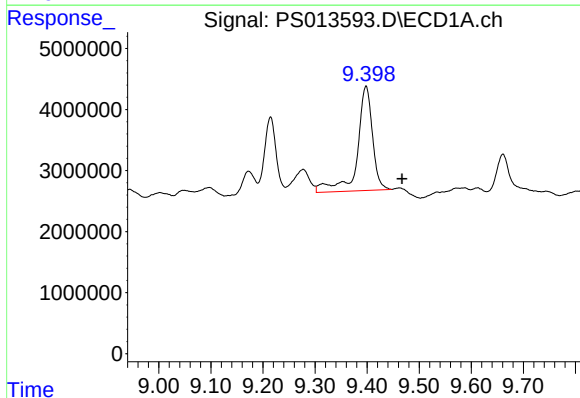


#12 2,4,5-T

R.T.: 9.398 min
Delta R.T.: -0.069 min
Response: 34779759
Conc: 6.29 ng/ml

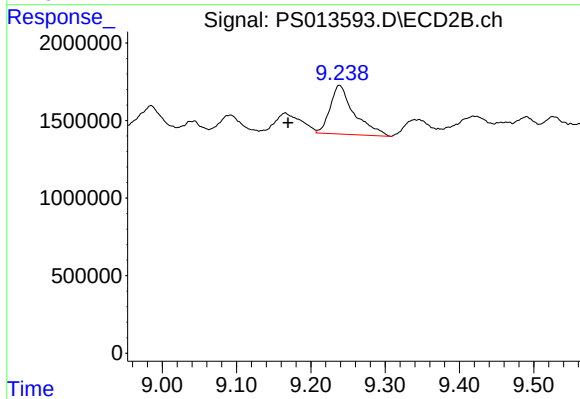

#12 2,4,5-T


R.T.: 9.238 min
Delta R.T.: 0.069 min
Response: 7084651
Conc: 3.18 ng/ml

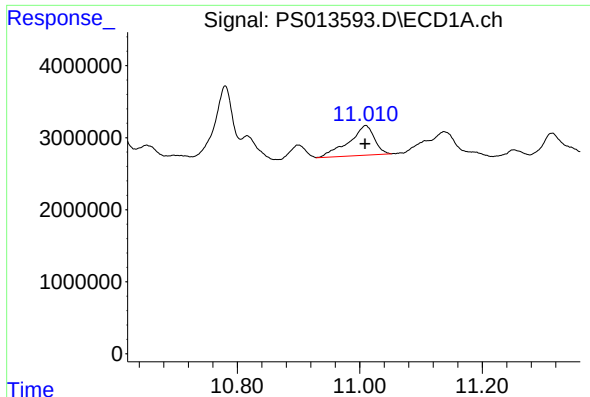

#15 Picloram

R.T.: 11.010 min
Delta R.T.: 0.000 min
Response: 11903779
Conc: 1.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

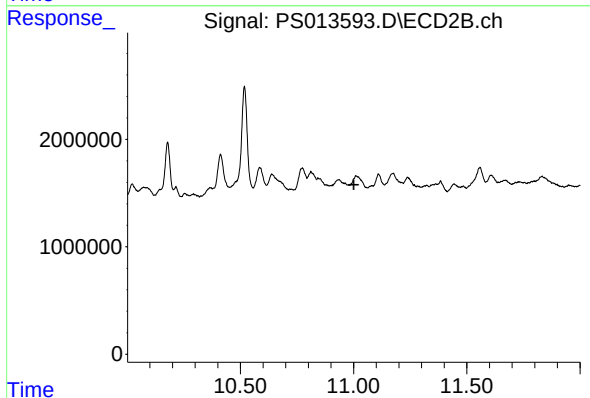

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.001 min
Response: 0
Conc: N.D.