

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122320\
 Data File : PS013595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2020 22:10
 Operator : DD\AJ
 Sample : L5189-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:51:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.913	306.6E6	150.7E6	329.272	383.051
Target Compounds							
1) T	Dalapon	2.992	2.589	78192158	114.5E6	72.791	217.949 #
2) T	3,5-DICHL...	0.000	6.094	0	53453098	N.D.	86.025
3) T	4-Nitroph...	6.979f	0.000	4739225	0	10.518	N.D. #
5) T	DICAMBA	7.386	7.046	10020106	6801748	2.713	4.047 #
6) T	MCPD	7.618f	0.000	5329809	0	1.963	N.D. #
7) T	MCPA	7.724	0.000	110.3E6	0	28.219	N.D. #
8) T	DICHLORPROP	0.000	7.752f	0	12425709	N.D.	27.803
10) T	Pentachlo...	8.682f	0.000	15010939	0	1.120	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	7066772	N.D.	3.010
12) T	2,4,5-T	9.398f	0.000	26363115	0	4.768	N.D. #
15) T	Picloram	10.999	0.000	9006353	0	1.308	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122320\
Data File : PS013595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2020 22:10
Operator : DD\AJ
Sample : L5189-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:51:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

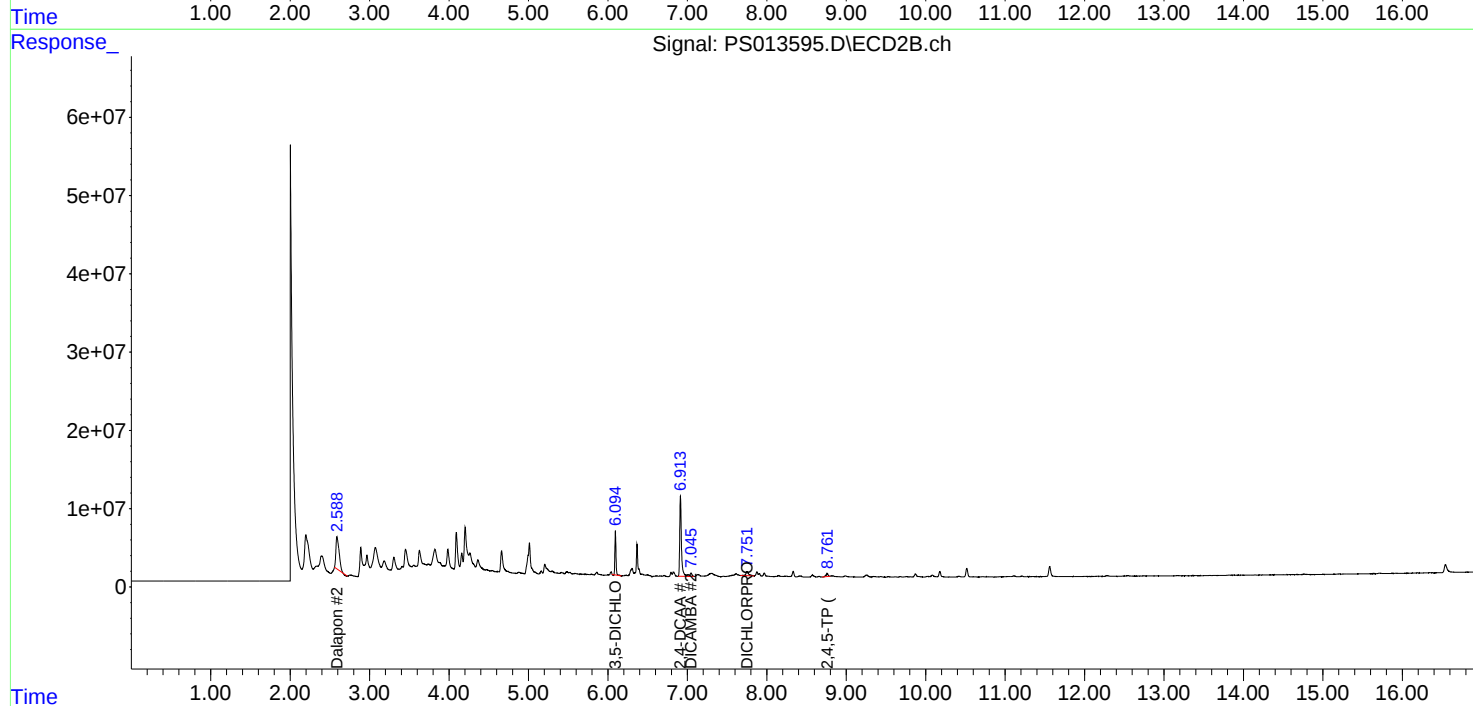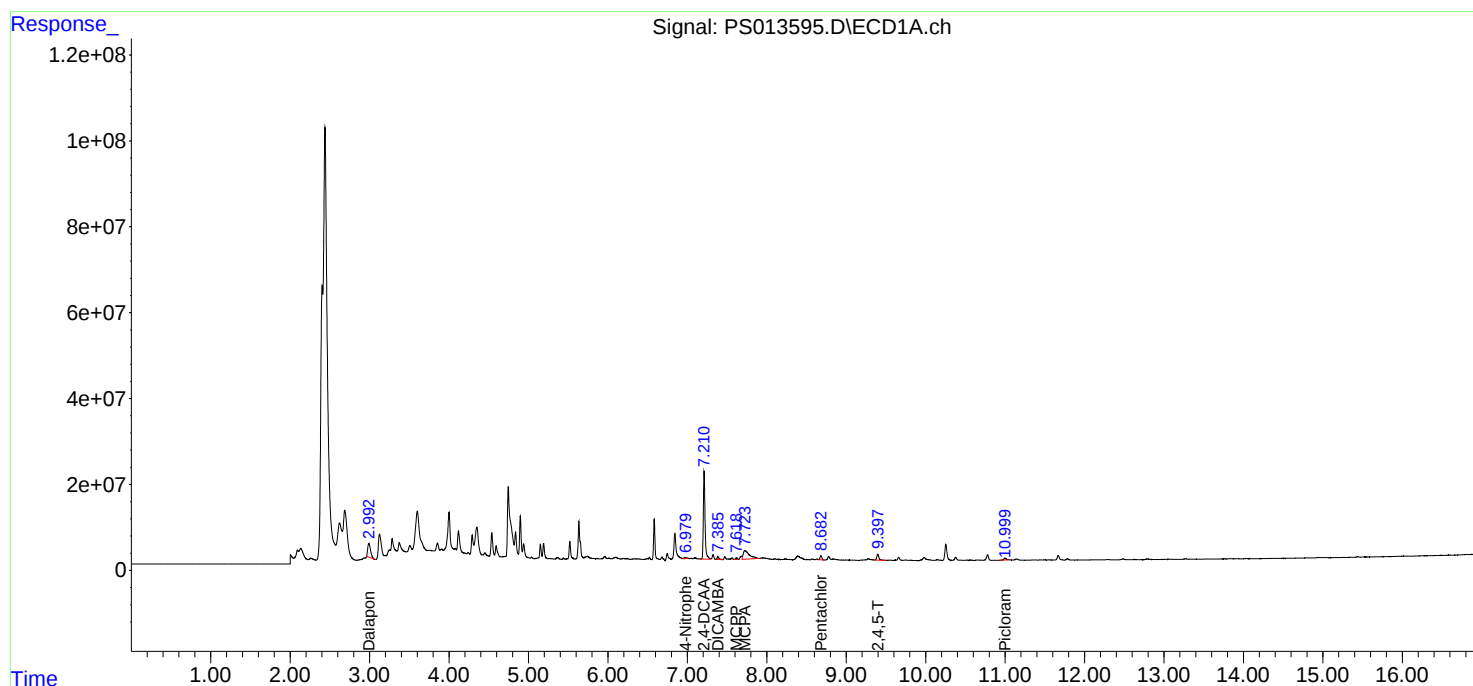


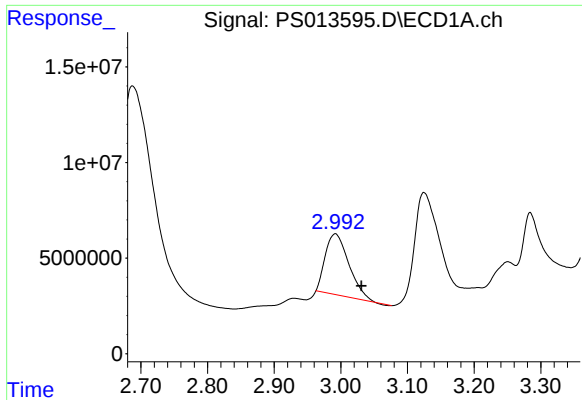

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.039 min
Response: 78192158
Conc: 72.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

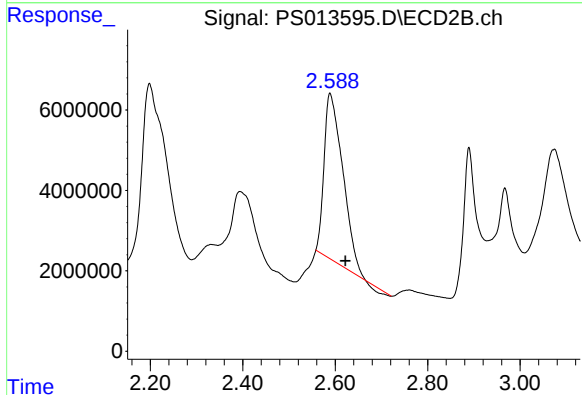


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.034 min
Response: 114539140
Conc: 217.95 ng/ml

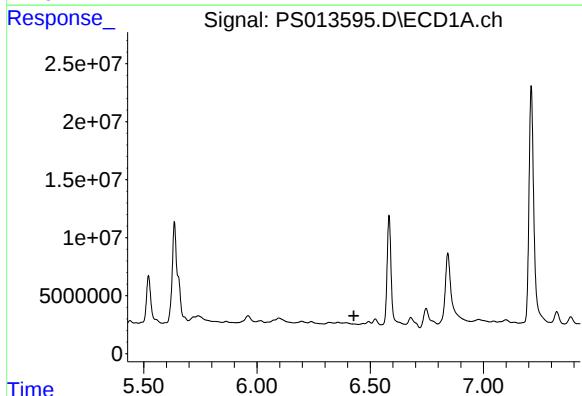


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

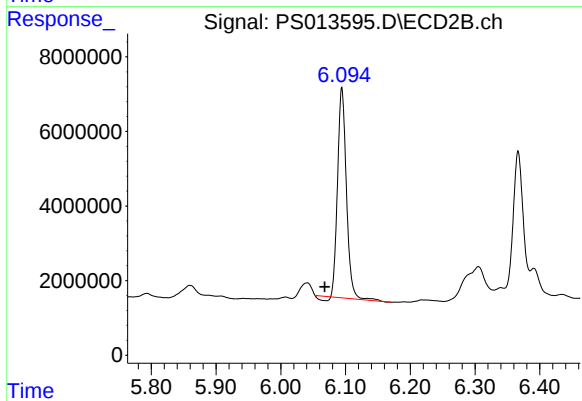

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.027 min
Response: 53453098
Conc: 86.02 ng/ml

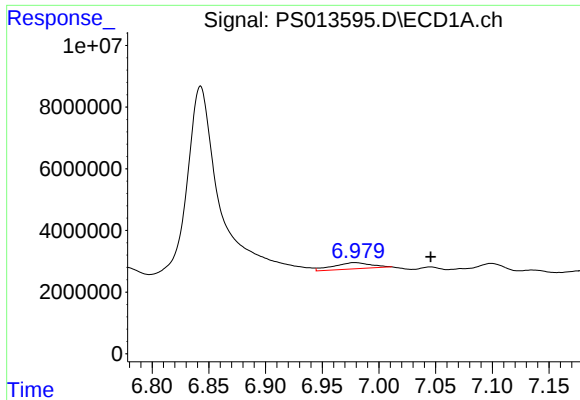

#3 4-Nitrophenol


R.T.: 6.979 min
Delta R.T.: -0.067 min
Response: 4739225
Conc: 10.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

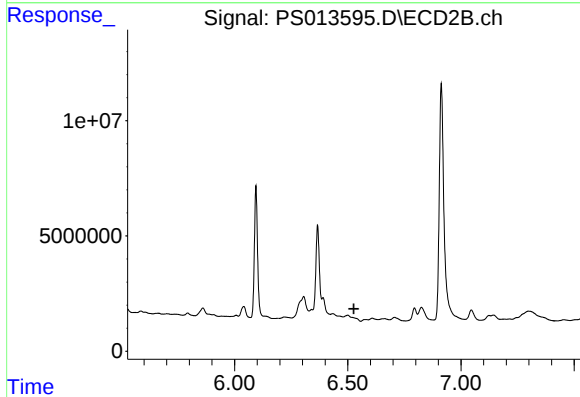


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

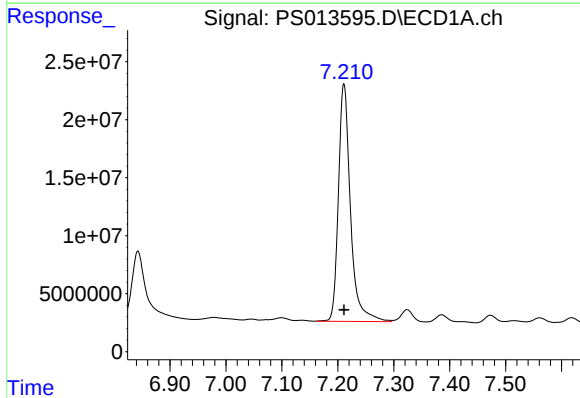


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 306571787
Conc: 329.27 ng/ml

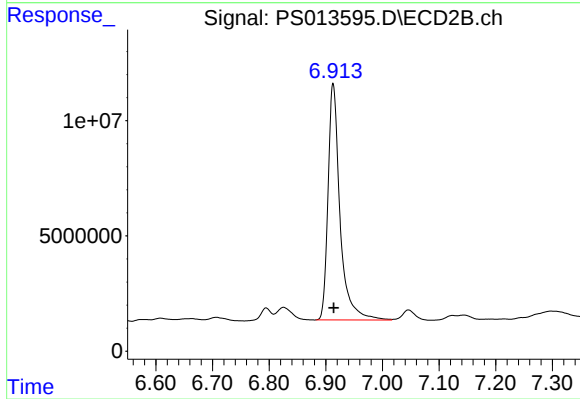

#4 2,4-DCAA


R.T.: 6.913 min
Delta R.T.: -0.001 min
Response: 150677585
Conc: 383.05 ng/ml

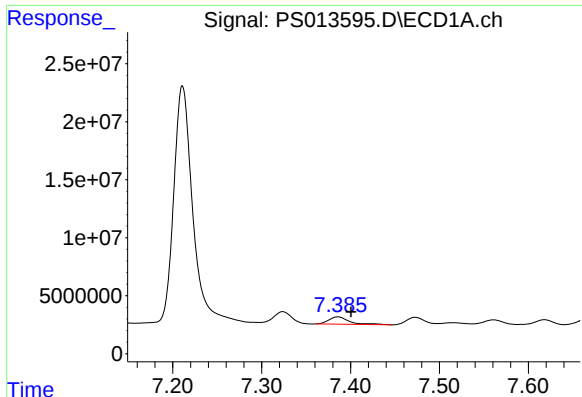

#5 DICAMBA


R.T.: 7.386 min
Delta R.T.: -0.015 min
Response: 10020106
Conc: 2.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

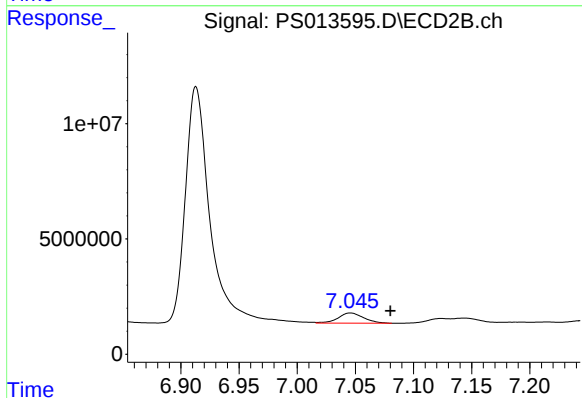


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 6801748
Conc: 4.05 ng/ml

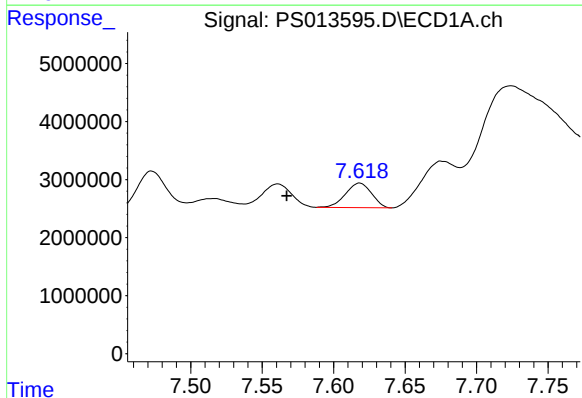


#6 MCP

R.T.: 7.618 min
Delta R.T.: 0.051 min
Response: 5329809
Conc: 1.96 ug/ml

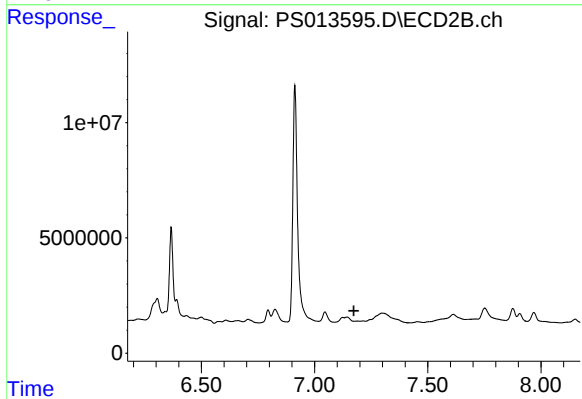

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.174 min
Response: 0
Conc: N.D.

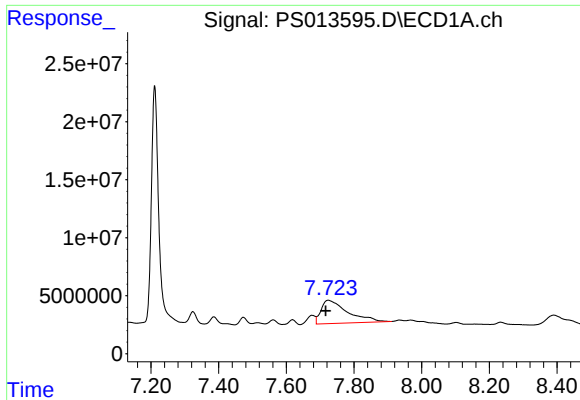

#7 MCPA


R.T.: 7.724 min
Delta R.T.: 0.007 min
Response: 110295686
Conc: 28.22 ug/ml

Instrument :
ECD_S
ClientSampleId :

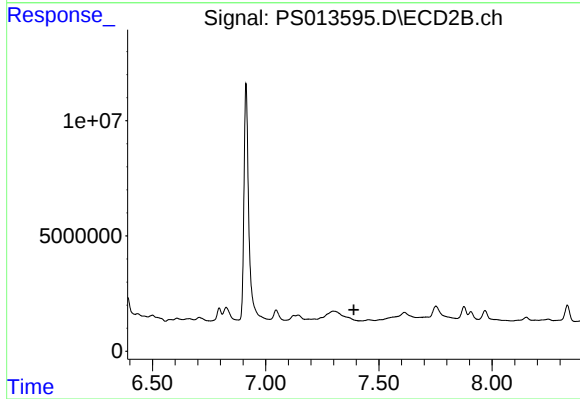


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

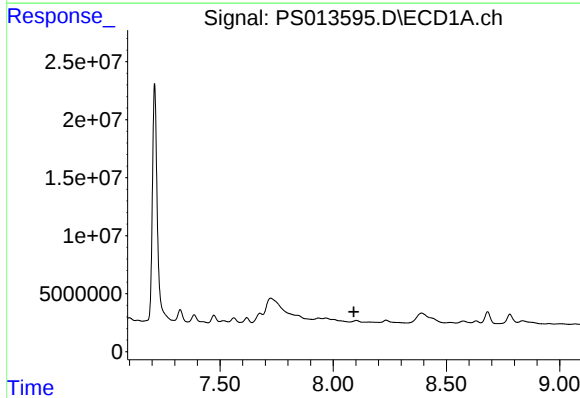


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

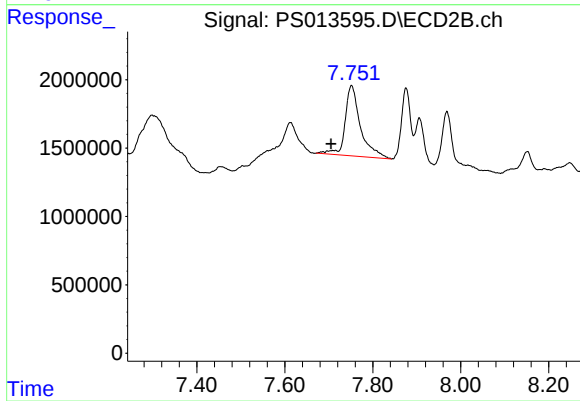

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.046 min
Response: 12425709
Conc: 27.80 ng/ml

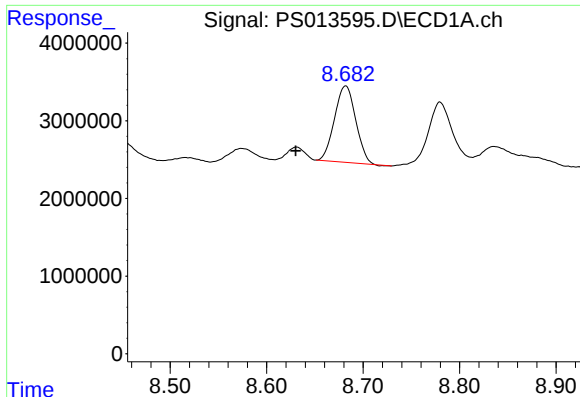

#10 Pentachlorophenol


R.T.: 8.682 min
Delta R.T.: 0.052 min
Response: 15010939
Conc: 1.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

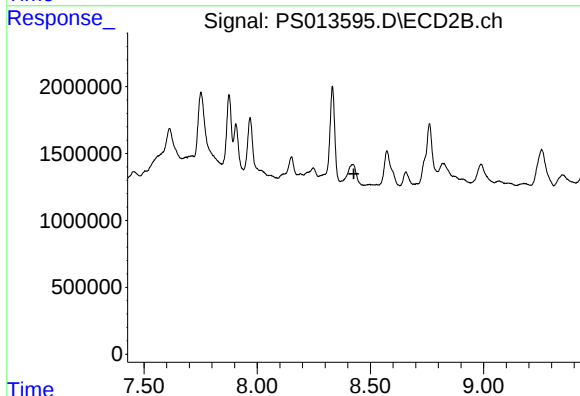


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.427 min
Response: 0
Conc: N.D.

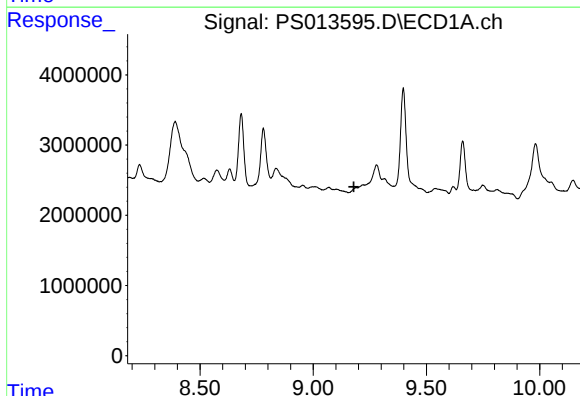


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

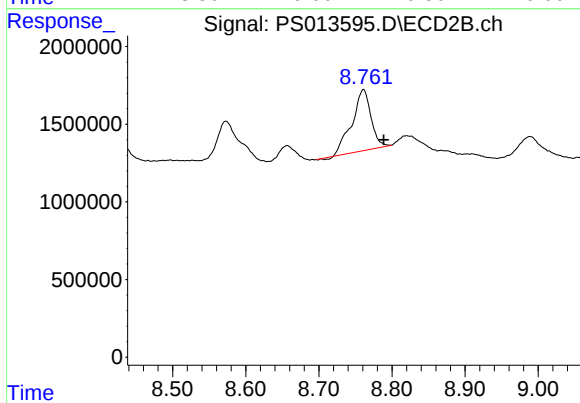

#11 2,4,5-TP (SILVEX)


R.T.: 8.761 min
Delta R.T.: -0.028 min
Response: 7066772
Conc: 3.01 ng/ml

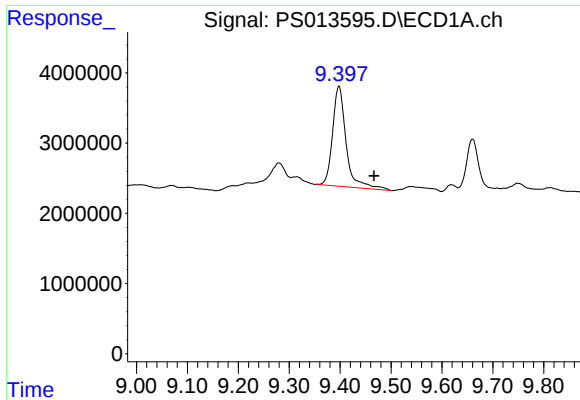

#12 2,4,5-T


R.T.: 9.398 min
Delta R.T.: -0.069 min
Response: 26363115
Conc: 4.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

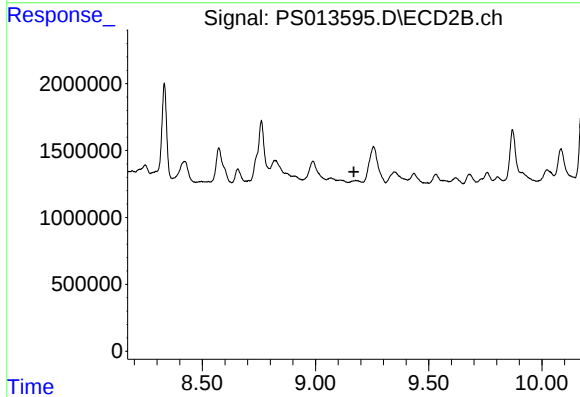


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

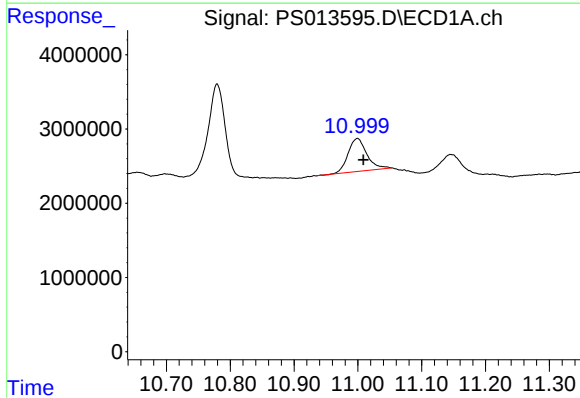

#15 Picloram

R.T.: 10.999 min
Delta R.T.: -0.010 min
Response: 9006353
Conc: 1.31 ng/ml

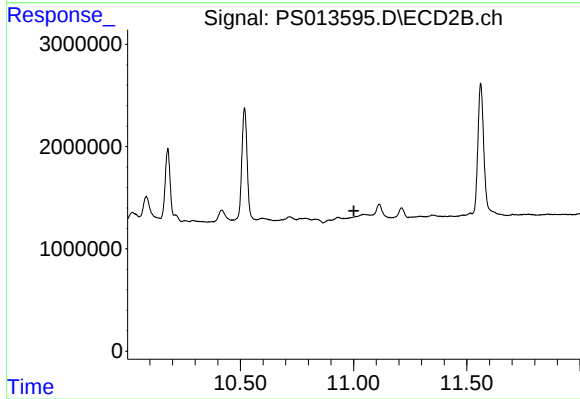

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.001 min
Response: 0
Conc: N.D.