

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122320\
 Data File : PS013599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2020 23:42
 Operator : DD\AJ
 Sample : L5189-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:53:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	305.0E6	149.9E6	327.625	381.009
Target Compounds							
1) T	Dalapon	2.991f	2.590	83409724	124.7E6	77.648	237.375 #
2) T	3,5-DICHL...	0.000	6.095	0	53107454	N.D.	85.469
3) T	4-Nitroph...	6.981f	0.000	5146684	0	11.423	N.D. #
5) T	DICAMBA	7.387	7.046	10840580	7351227	2.936	4.374 #
6) T	MCPD	7.619f	7.124f	5576265	484412	2.054	<MDL #
7) T	MCPA	7.720	0.000	109.2E6	0	27.948	N.D. #
8) T	DICHLORPROP	0.000	7.746f	0	27139109	N.D.	60.726
10) T	Pentachlo...	8.631	8.427	7970190	5845972	<MDL	1.037 #
11) T	2,4,5-TP ...	0.000	8.761	0	8659072	N.D.	3.688
12) T	2,4,5-T	9.398f	0.000	21640720	0	3.914	N.D. #
15) T	Picloram	11.000	0.000	15223043	0	2.210	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122320\
Data File : PS013599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2020 23:42
Operator : DD\AJ
Sample : L5189-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:53:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

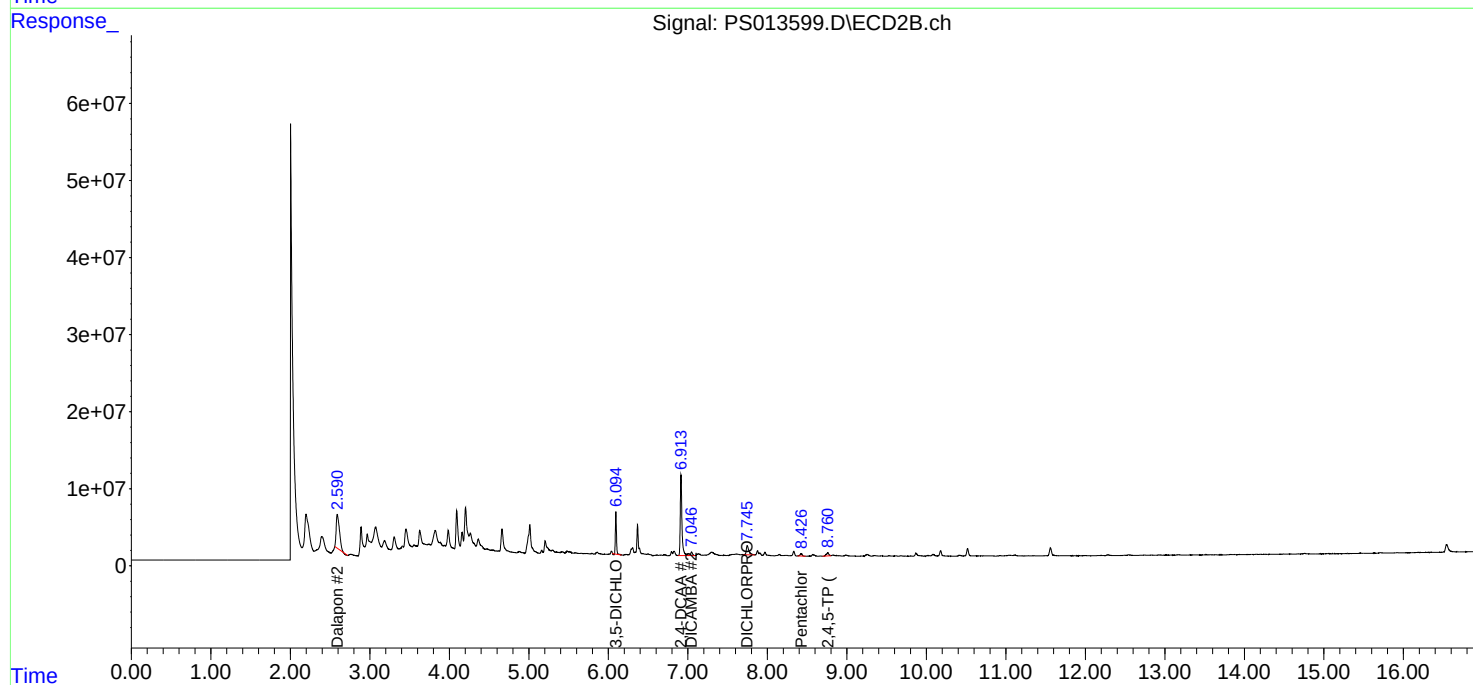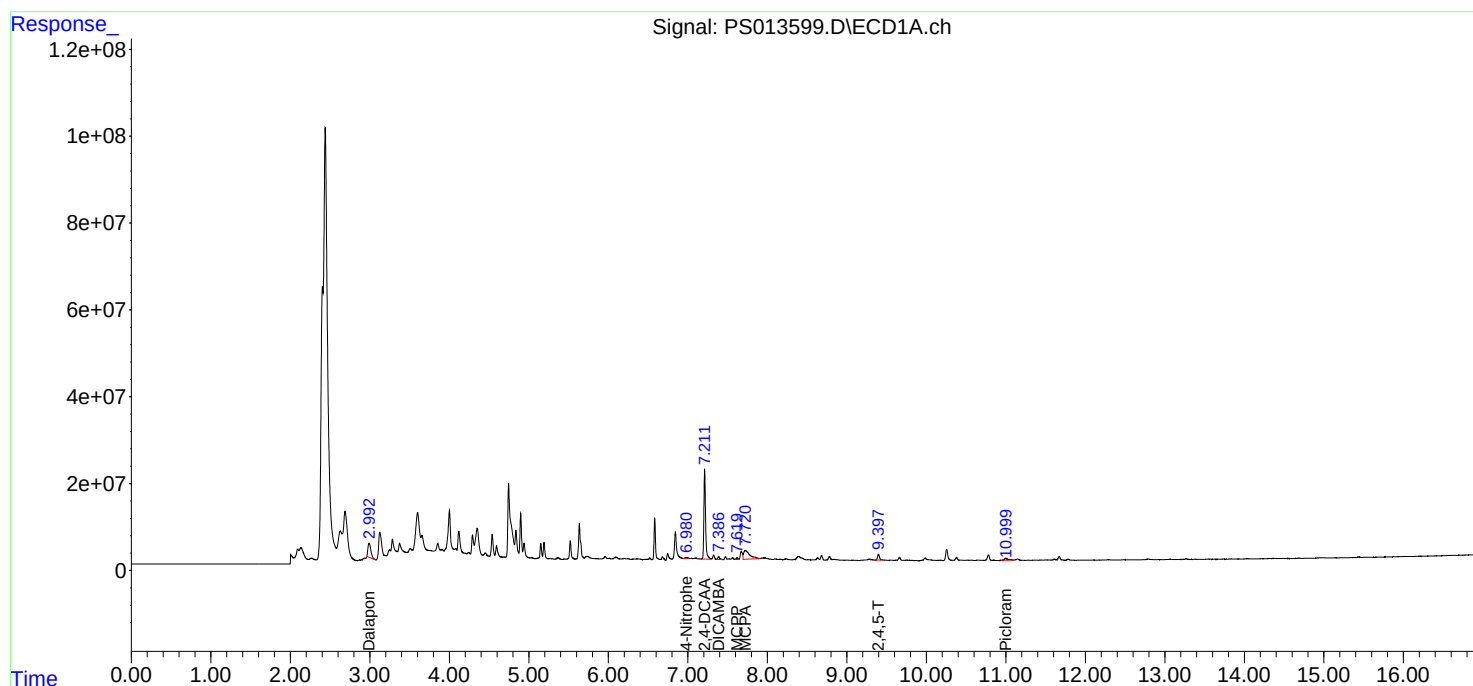


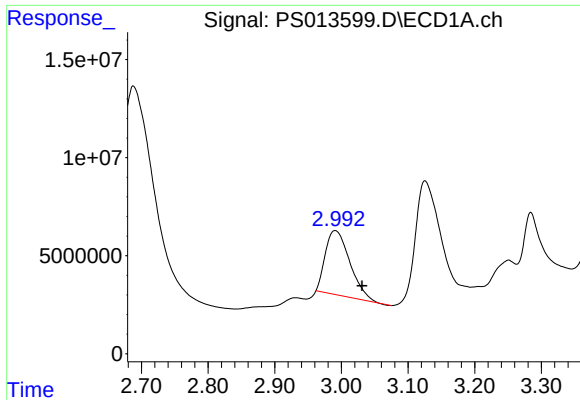

#1 Dalapon


R.T.: 2.991 min
Delta R.T.: -0.040 min
Response: 83409724
Conc: 77.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

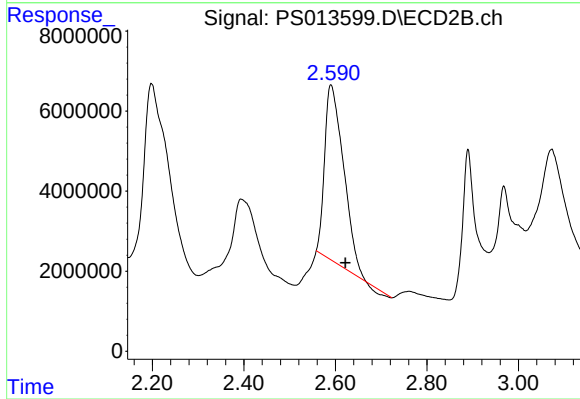


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.032 min
Response: 124747937
Conc: 237.38 ng/ml

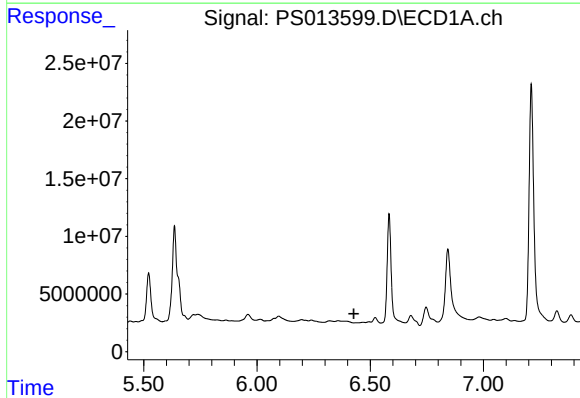


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

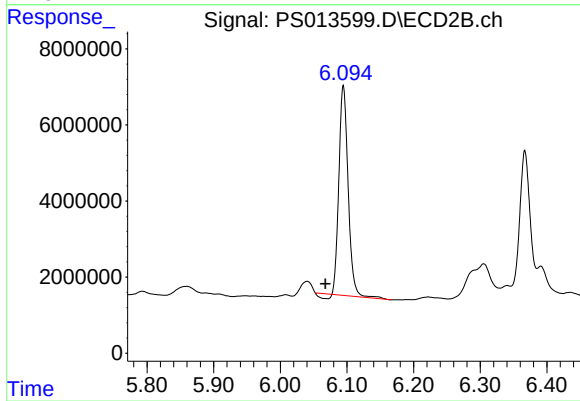

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.027 min
Response: 53107454
Conc: 85.47 ng/ml

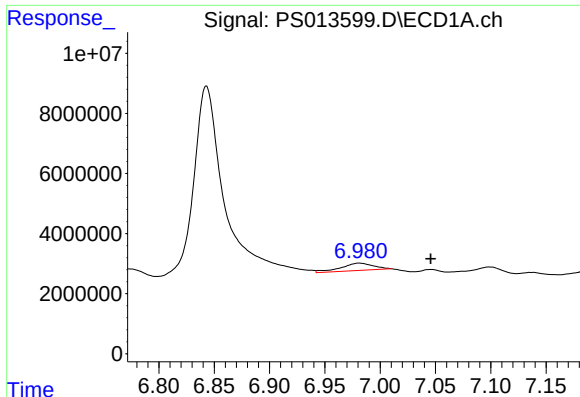

#3 4-Nitrophenol


R.T.: 6.981 min
Delta R.T.: -0.065 min
Response: 5146684
Conc: 11.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

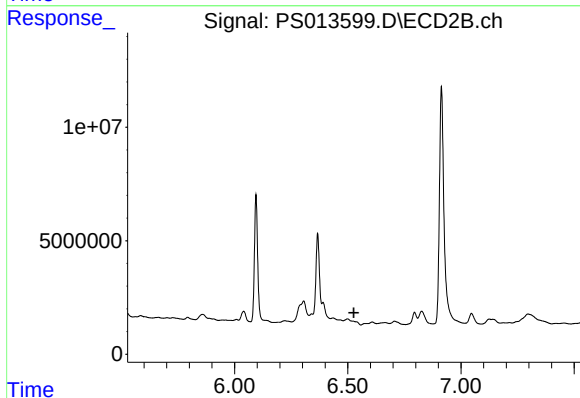


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

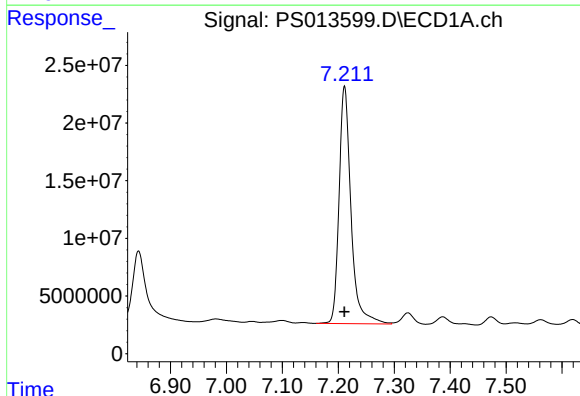


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 305038548
Conc: 327.63 ng/ml

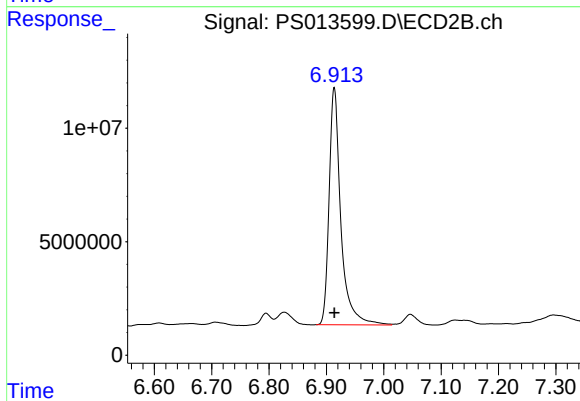

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 149874183
Conc: 381.01 ng/ml

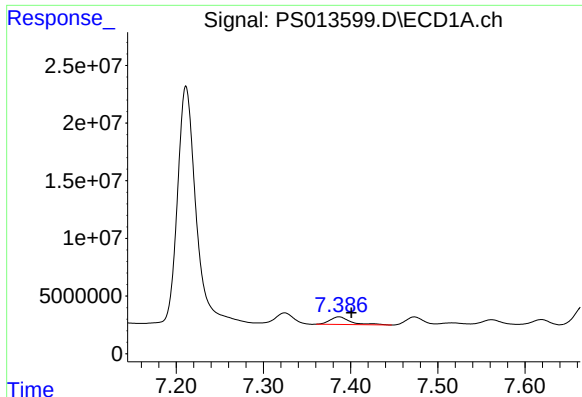

#5 DICAMBA


R.T.: 7.387 min
Delta R.T.: -0.014 min
Response: 10840580
Conc: 2.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

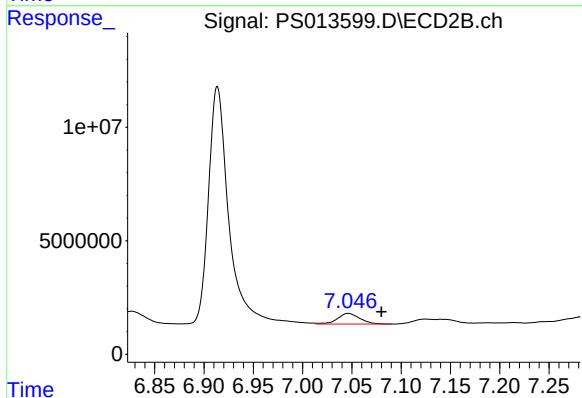


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 7351227
Conc: 4.37 ng/ml

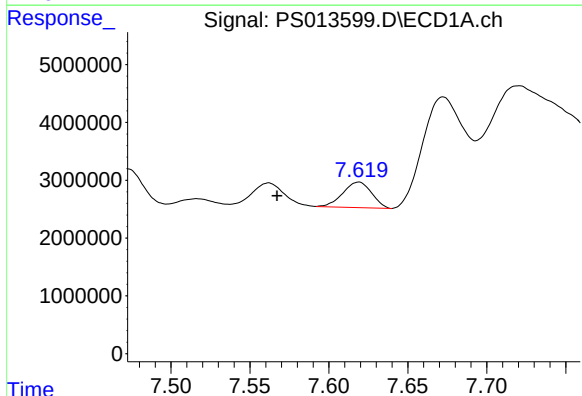


#6 MCP

R.T.: 7.619 min
Delta R.T.: 0.051 min
Response: 5576265
Conc: 2.05 ug/ml

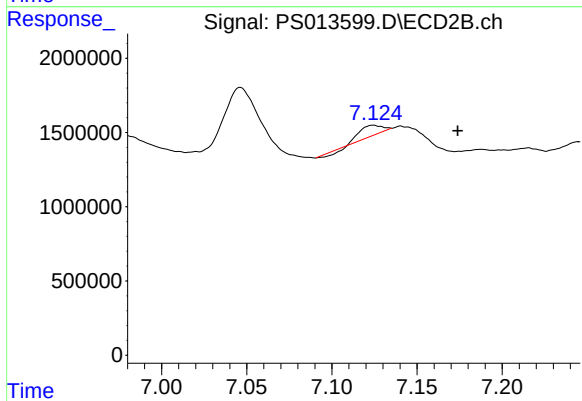

#6 MCP


R.T.: 7.124 min
Delta R.T.: -0.050 min
Response: 484412
Conc: N.D.

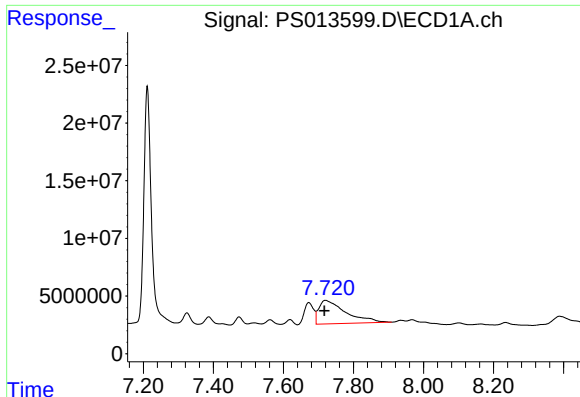

#7 MCPA


R.T.: 7.720 min
Delta R.T.: 0.004 min
Response: 109236355
Conc: 27.95 ug/ml

Instrument :
ECD_S
ClientSampleId :

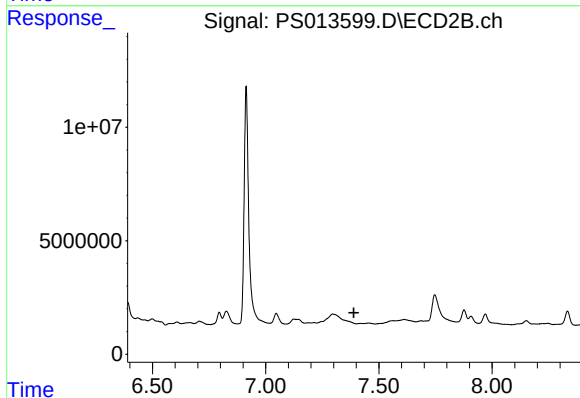


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

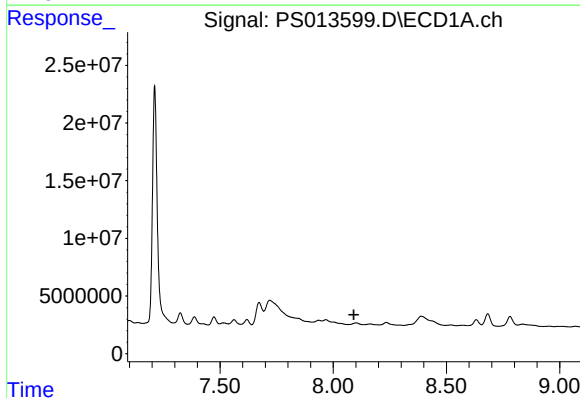


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

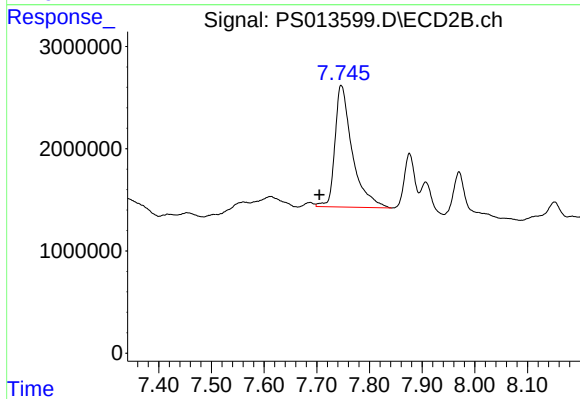

#8 DICHLORPROP


R.T.: 7.746 min
Delta R.T.: 0.041 min
Response: 27139109
Conc: 60.73 ng/ml

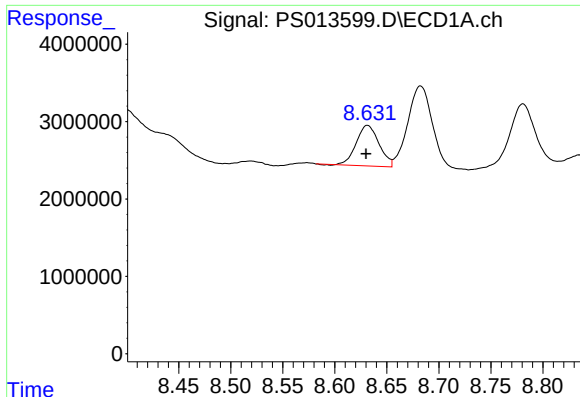

#10 Pentachlorophenol


R.T.: 8.631 min
Delta R.T.: 0.001 min
Response: 7970190
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

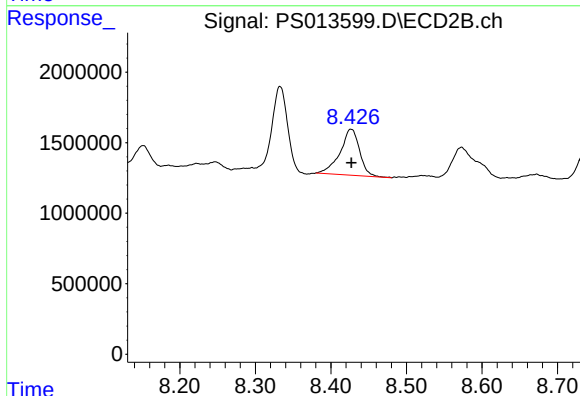


#10 Pentachlorophenol

R.T.: 8.427 min
Delta R.T.: 0.000 min
Response: 5845972
Conc: 1.04 ng/ml

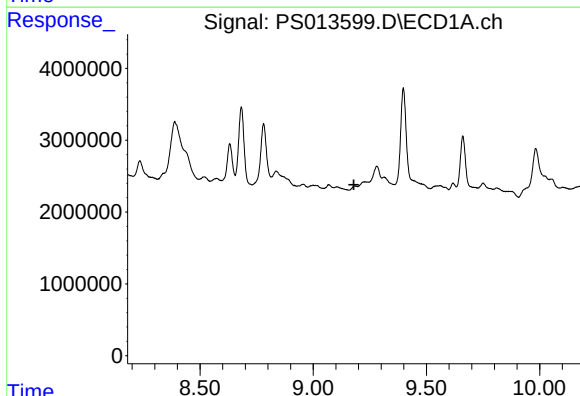


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

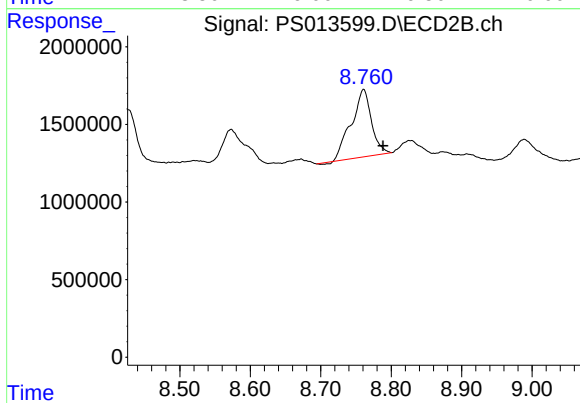

#11 2,4,5-TP (SILVEX)


R.T.: 8.761 min
Delta R.T.: -0.028 min
Response: 8659072
Conc: 3.69 ng/ml

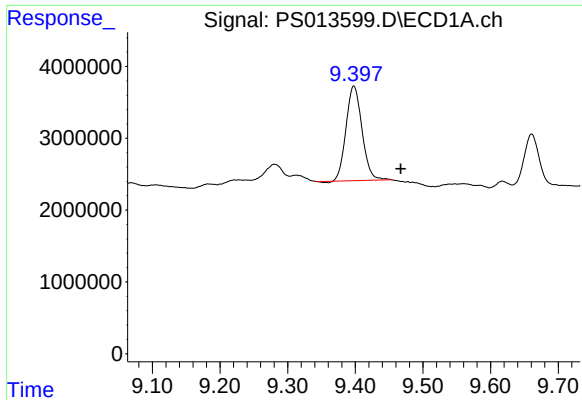

#12 2,4,5-T


R.T.: 9.398 min
Delta R.T.: -0.069 min
Response: 21640720
Conc: 3.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

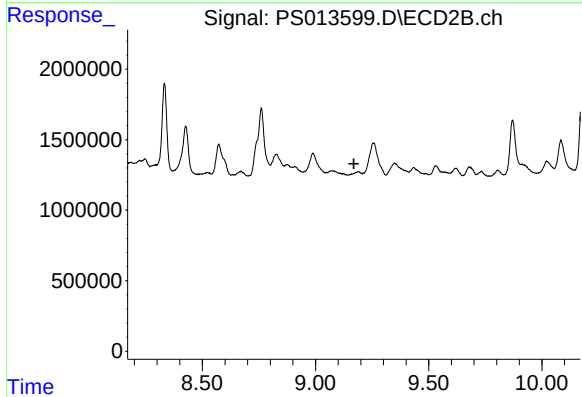


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

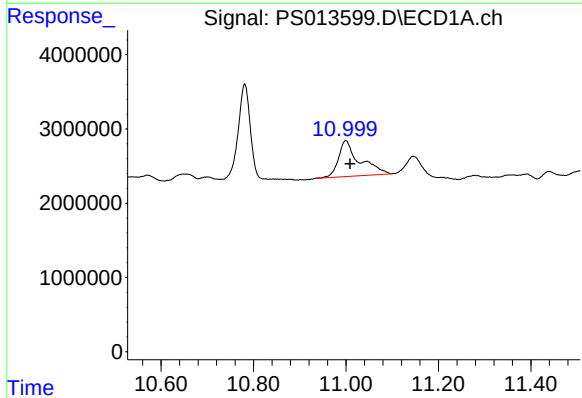

#15 Picloram

R.T.: 11.000 min
Delta R.T.: -0.009 min
Response: 15223043
Conc: 2.21 ng/ml

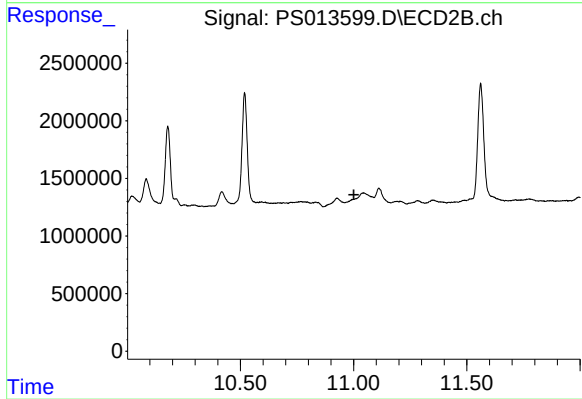

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.001 min
Response: 0
Conc: N.D.