

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122321\
 Data File : PS017804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2021 12:14
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:04:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.165	0.000	5294479	0	3.388	N.D. #
Target Compounds							
5) T	DICAMBA	7.326	6.886	16202620	6293607	2.562	2.363
8) T	DICHLORPROP	8.024	0.000	5655281	0	3.619	N.D. #
10) T	Pentachlo...	8.545	0.000	16857018	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.107	0.000	20511328	0	2.411	N.D. #
12) T	2,4,5-T	9.337	9.005f	79888300	8064139	9.183	2.358 #
14) T	DINOSEB	11.068	0.000	64209956	0	9.390	N.D. #
15) T	Picloram	10.889	10.694f	7189460	12551683	<MDL	2.556 #
16) T	DCPA	11.336	10.694	28942166	12551683	2.665	2.802



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122321\
Data File : PS017804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2021 12:14
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:04:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

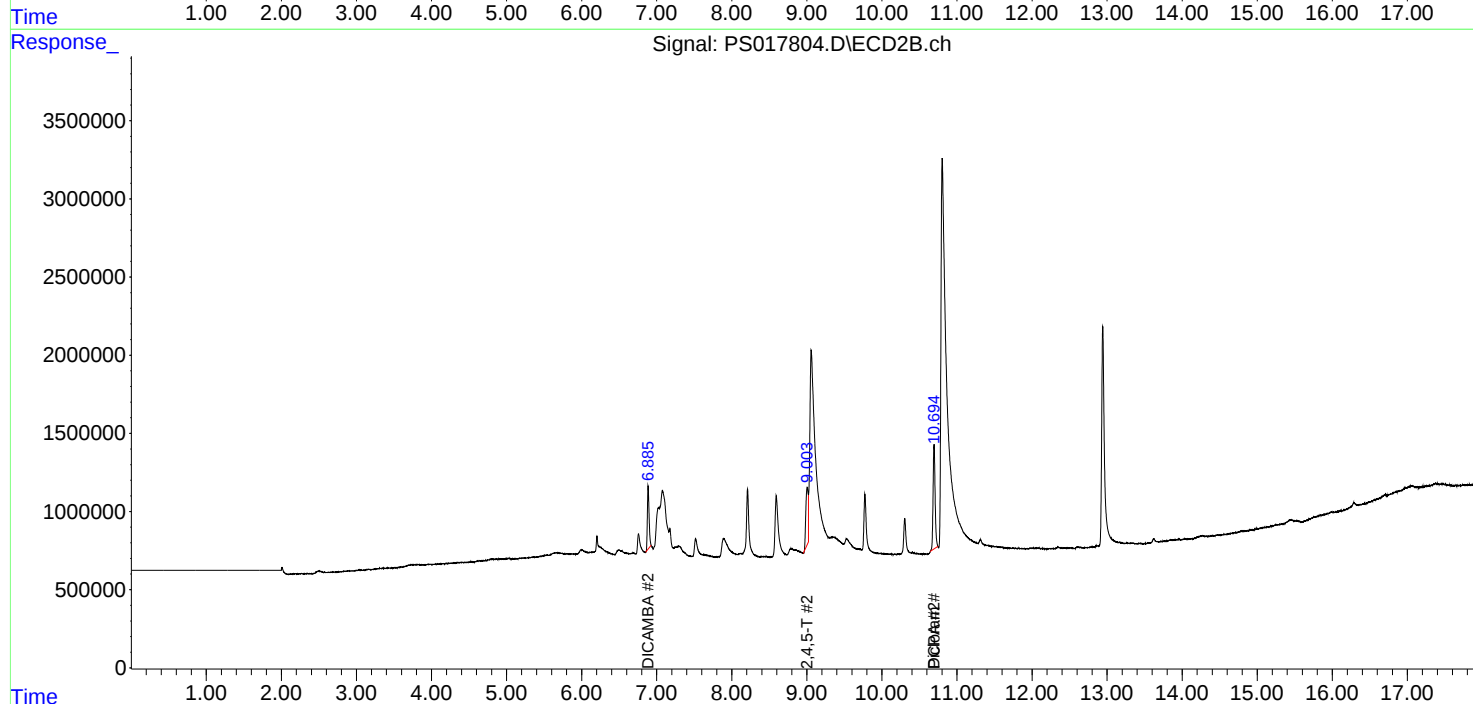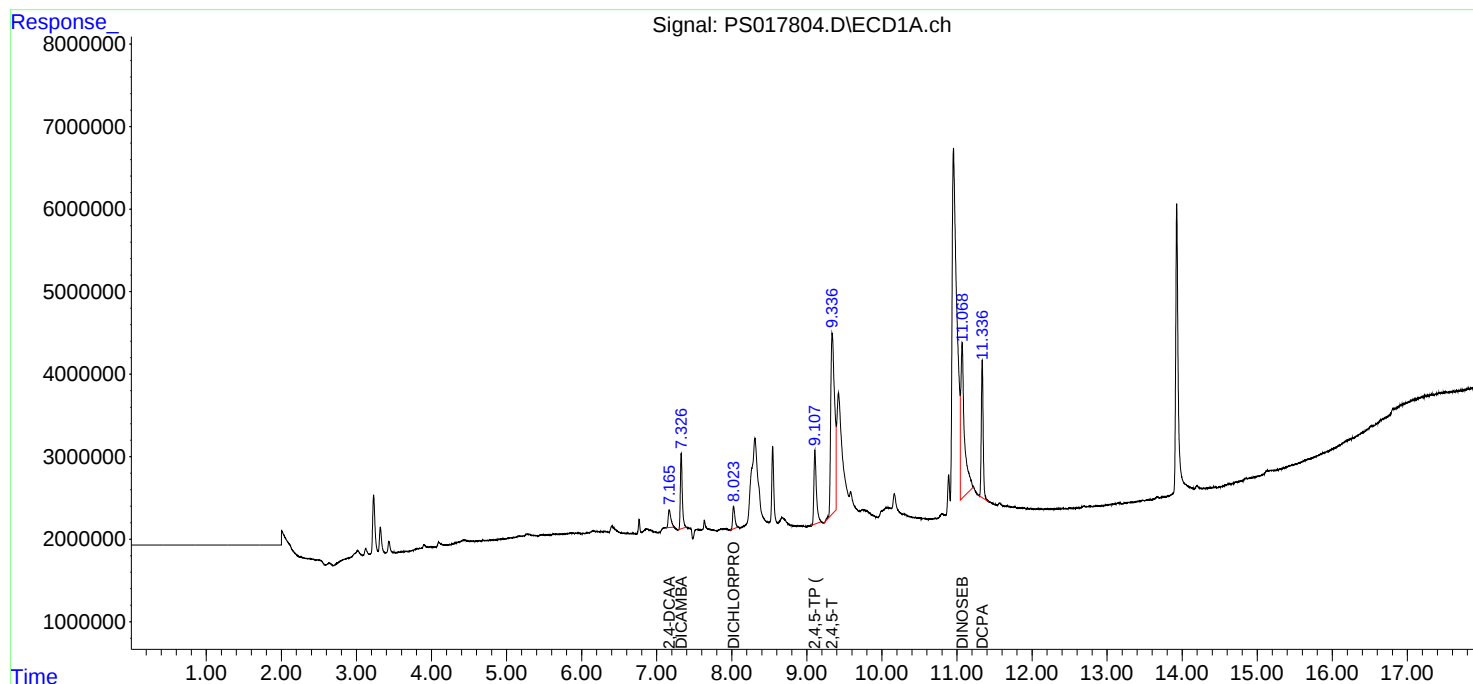


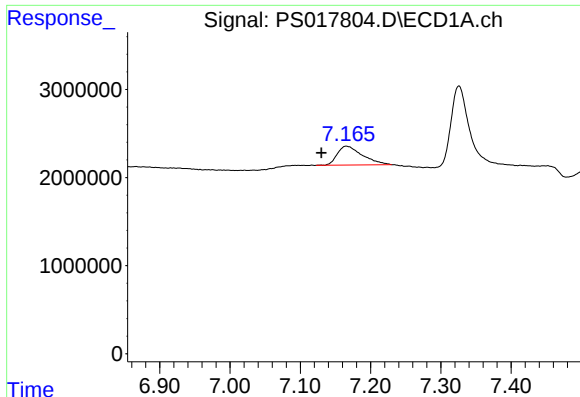

#4 2,4-DCAA


R.T.: 7.165 min
Delta R.T.: 0.035 min
Response: 5294479
Conc: 3.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

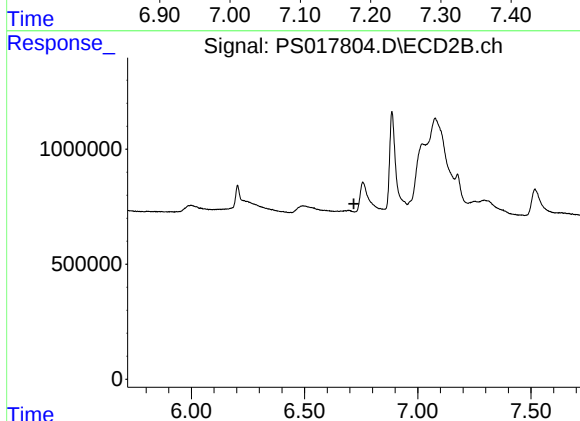


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.718 min
Response: 0
Conc: N.D.

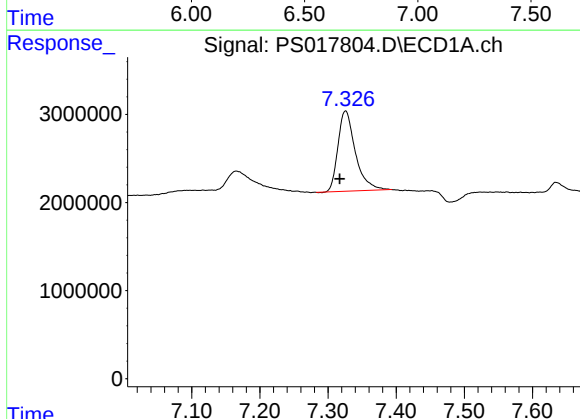


#5 DICAMBA

R.T.: 7.326 min
Delta R.T.: 0.008 min
Response: 16202620
Conc: 2.56 ng/ml

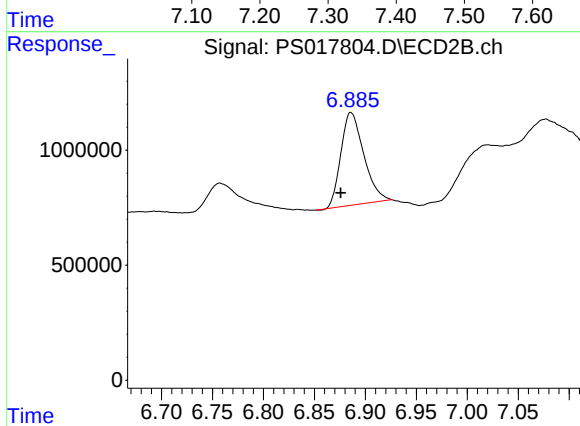

#5 DICAMBA


R.T.: 6.886 min
Delta R.T.: 0.010 min
Response: 6293607
Conc: 2.36 ng/ml

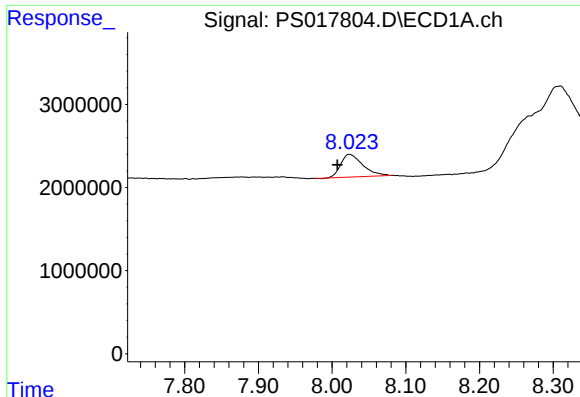

#8 DICHLORPROP


R.T.: 8.024 min
Delta R.T.: 0.016 min
Response: 5655281
Conc: 3.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

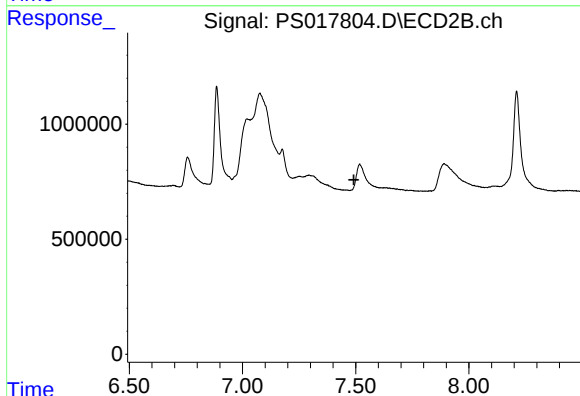


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.492 min
Response: 0
Conc: N.D.

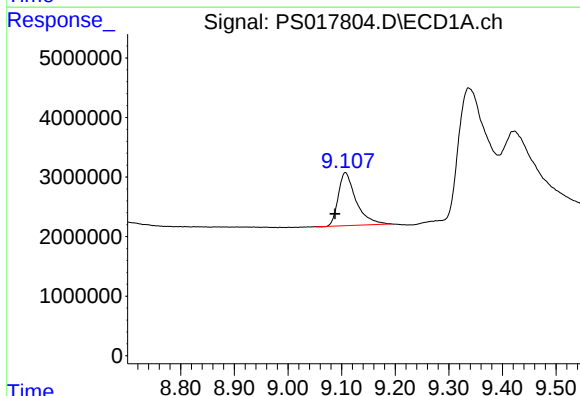


#11 2,4,5-TP (SILVEX)

R.T.: 9.107 min
Delta R.T.: 0.019 min
Response: 20511328
Conc: 2.41 ng/ml

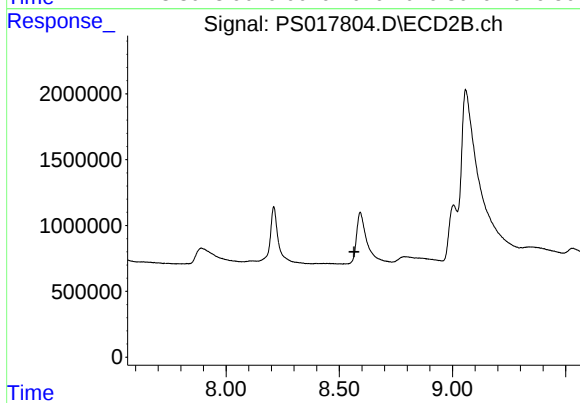

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.565 min
Response: 0
Conc: N.D.

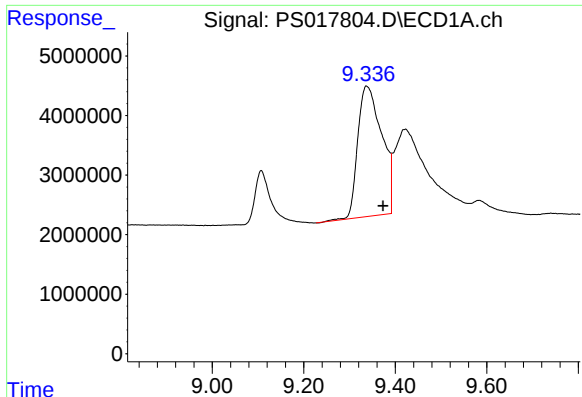

#12 2,4,5-T


R.T.: 9.337 min
Delta R.T.: -0.037 min
Response: 79888300
Conc: 9.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

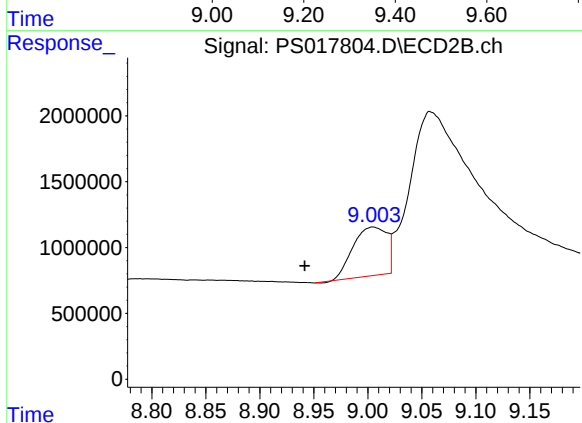


#12 2,4,5-T

R.T.: 9.005 min
Delta R.T.: 0.063 min
Response: 8064139
Conc: 2.36 ng/ml

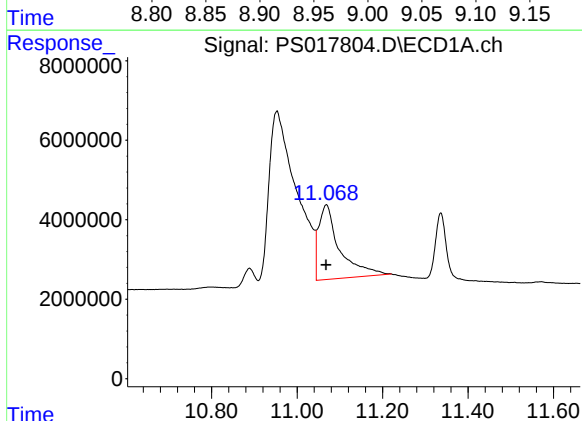


#14 DINOSEB

R.T.: 11.068 min
Delta R.T.: 0.000 min
Response: 64209956
Conc: 9.39 ng/ml

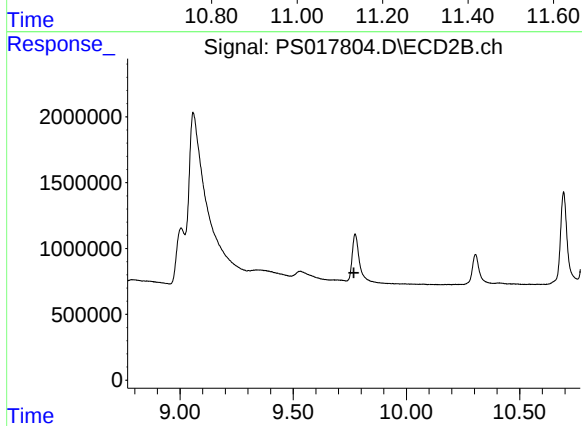

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

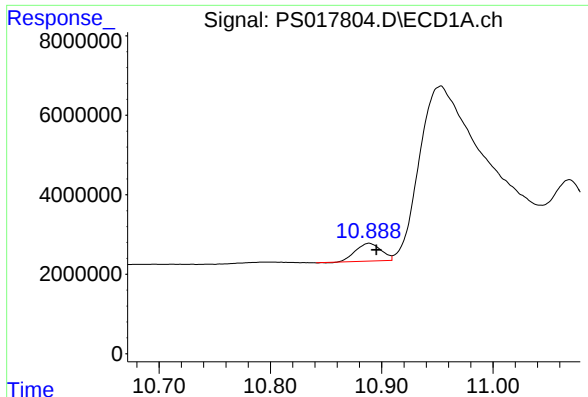

#15 Picloram


R.T.: 10.889 min
Delta R.T.: -0.007 min
Response: 7189460
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

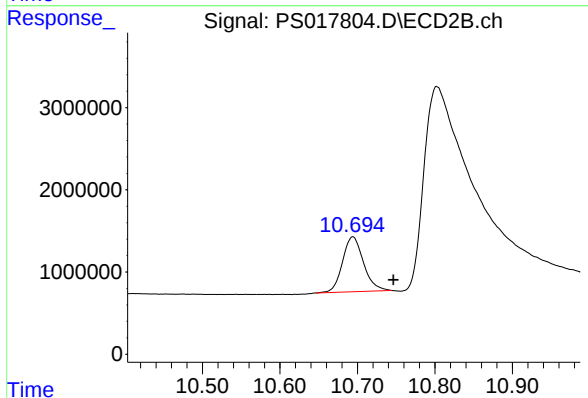


#15 Picloram

R.T.: 10.694 min
Delta R.T.: -0.053 min
Response: 12551683
Conc: 2.56 ng/ml

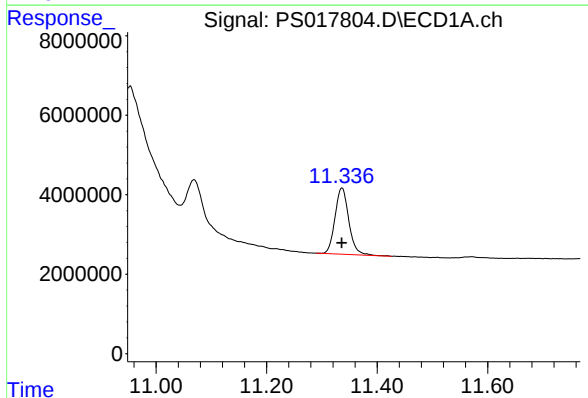

#16 DCPA

R.T.: 11.336 min
Delta R.T.: 0.000 min
Response: 28942166
Conc: 2.66 ng/ml

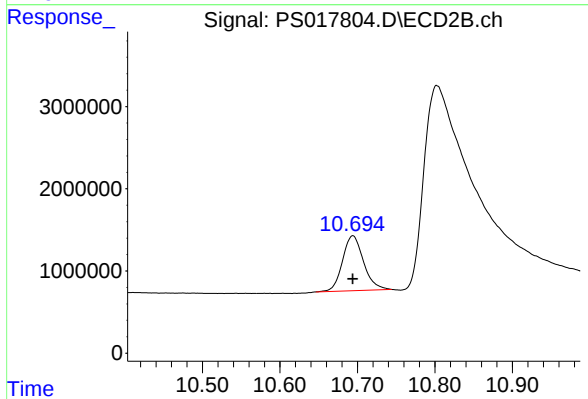

#16 DCPA

R.T.: 10.694 min
Delta R.T.: 0.000 min
Response: 12551683
Conc: 2.80 ng/ml