

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122322\
 Data File : PS021537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 08:25
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 01:14:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.375	0.000	960487	0	<MDL	N.D.	#
Target Compounds								
2) T	3,5-DICHL...	5.749	0.000	408422	0	<MDL	N.D.	#
3) T	4-Nitroph...	6.213	6.457	3326025	692227	1.850	<MDL	#
5) T	DICAMBA	6.527	6.979	746395	1198224	<MDL	<MDL	#
6) T	MCP	6.636	7.029f	209436	4295026	<MDL	<MDL	#
7) T	MCPA	6.823	0.000	1060924	0	<MDL	N.D.	#
8) T	DICHLORPROP	7.128	7.622	1810186	9208620	<MDL	4.675	#
9) T	2,4-D	7.342	0.000	19810616	0	5.184	N.D.	#
10) T	Pentachlo...	7.553	8.317	3204449	1682702	<MDL	<MDL	#
11) T	2,4,5-TP ...	8.086	8.678	6920373	1305311	<MDL	<MDL	#
12) T	2,4,5-T	8.353	9.064	8217884	5968575	<MDL	<MDL	#
13) T	2,4-DB	8.868	0.000	849149	0	<MDL	N.D.	#
14) T	DINOSEB	9.907	9.897	4335114	314760	<MDL	<MDL	#
15) T	Picloram	9.719	10.870	115.9E6	37479098	4.048	2.305	#
16) T	DCPA	10.168	10.820	3595877	9665364	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122322\
Data File : PS021537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 08:25
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 01:14:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

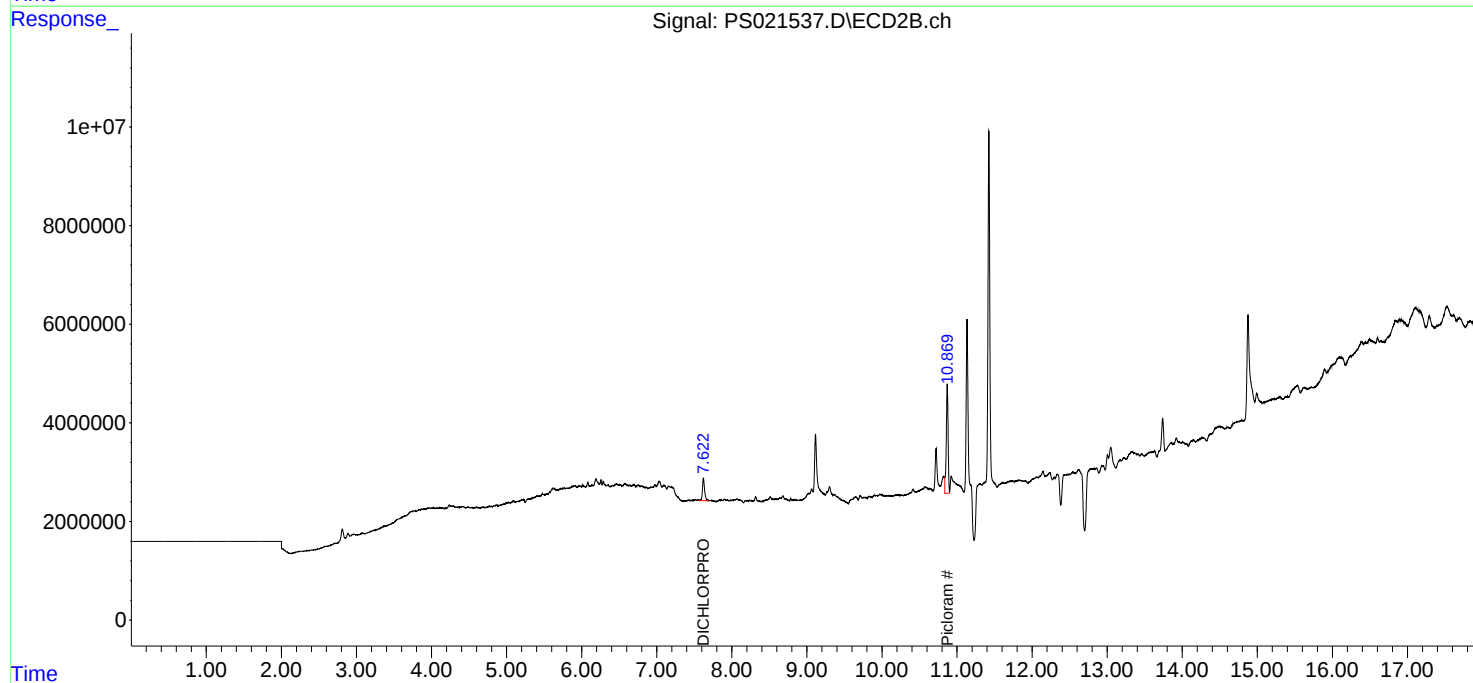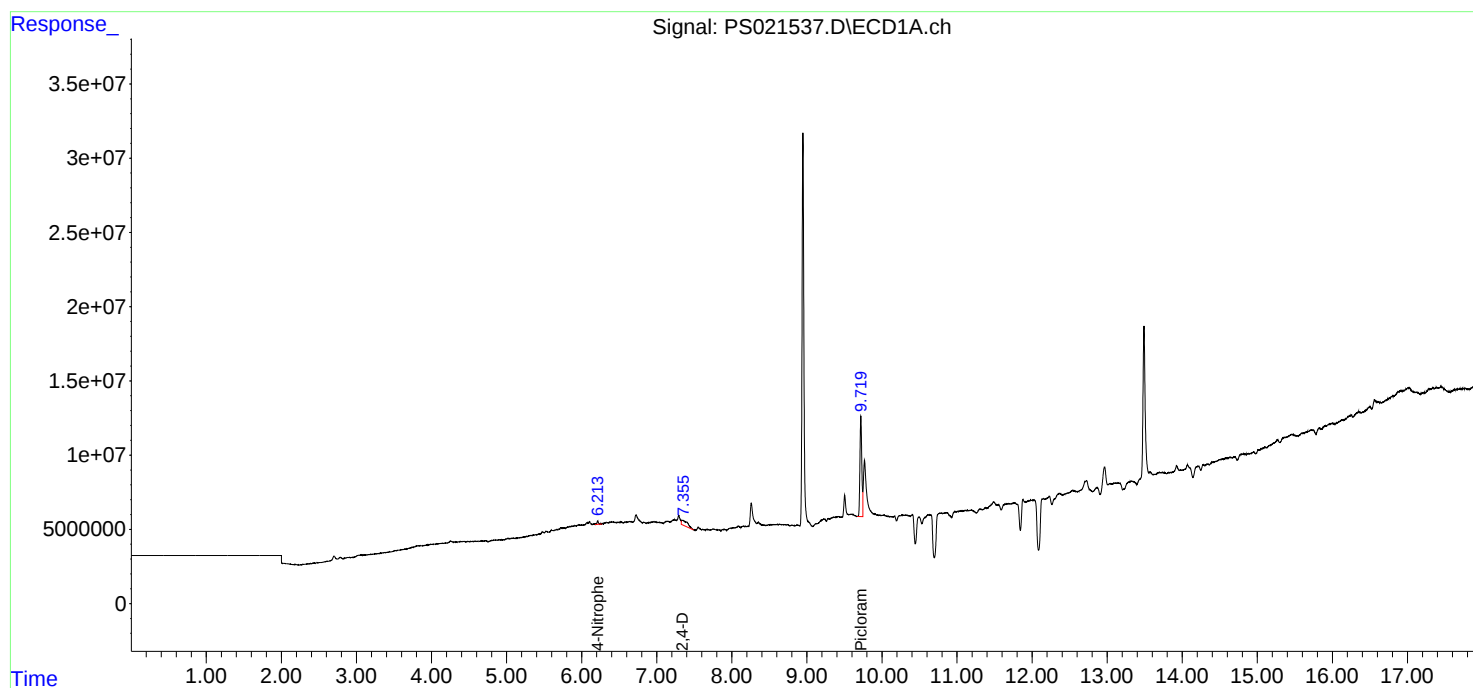


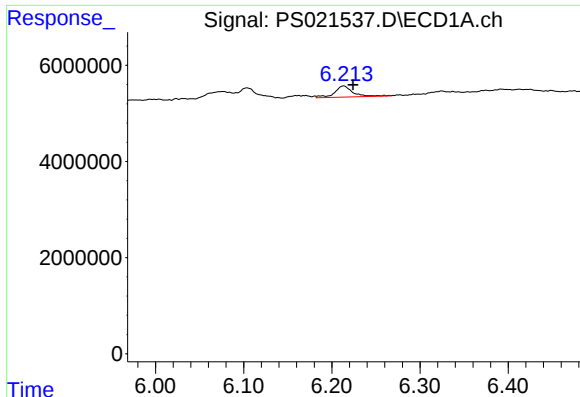

#3 4-Nitrophenol


R.T.: 6.213 min
Delta R.T.: -0.011 min
Response: 3326025
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

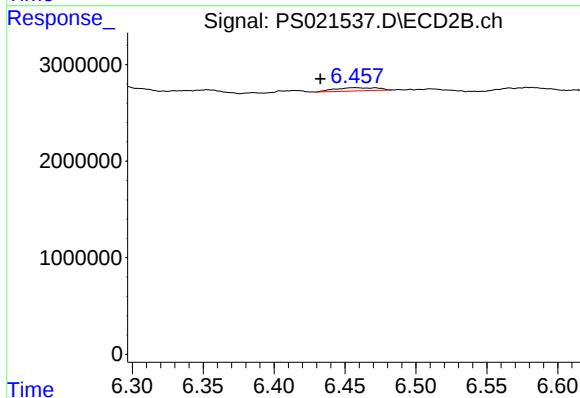


#3 4-Nitrophenol

R.T.: 6.457 min
Delta R.T.: 0.024 min
Response: 692227
Conc: N.D.

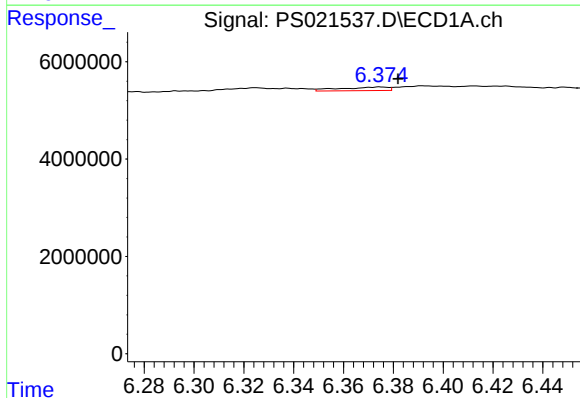


#4 2,4-DCAA

R.T.: 6.375 min
Delta R.T.: -0.007 min
Response: 960487
Conc: N.D.

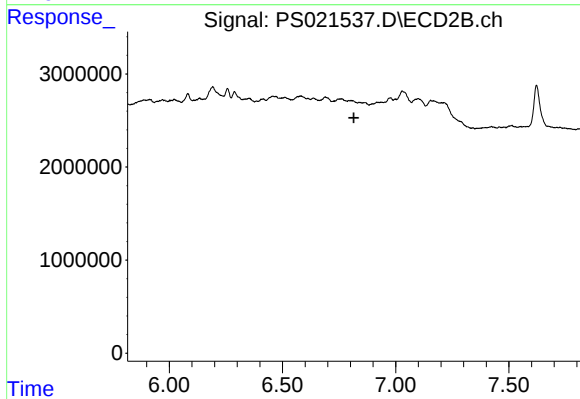

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.816 min
Response: 0
Conc: N.D.

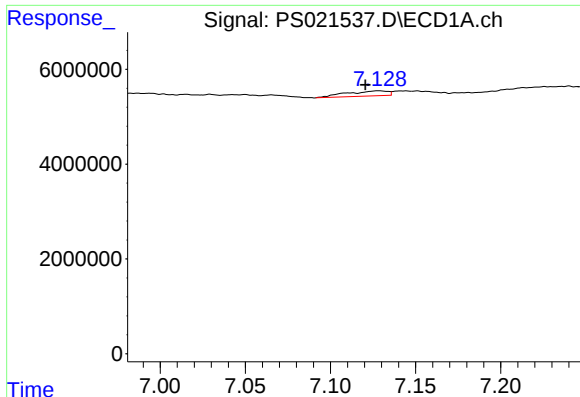

#8 DICHLORPROP


R.T.: 7.128 min
Delta R.T.: 0.008 min
Response: 1810186
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

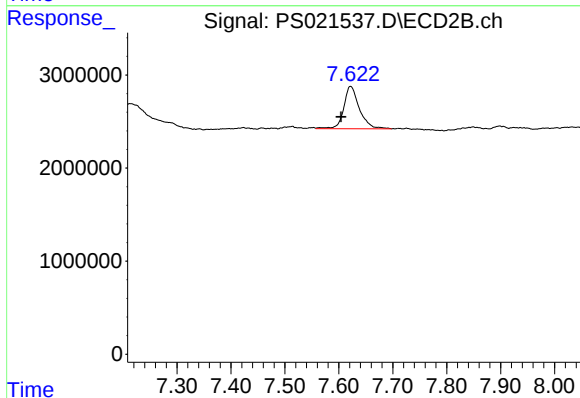


#8 DICHLORPROP

R.T.: 7.622 min
Delta R.T.: 0.018 min
Response: 9208620
Conc: 4.68 ng/ml

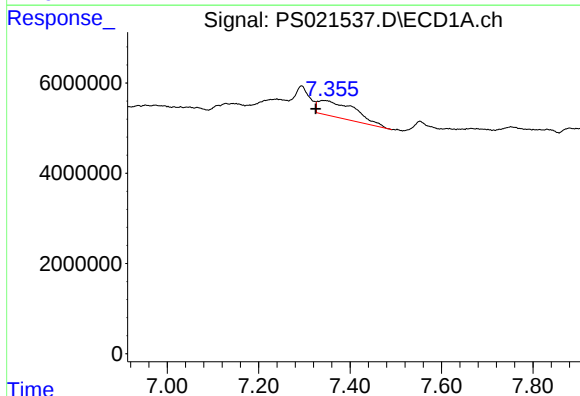


#9 2,4-D

R.T.: 7.342 min
Delta R.T.: 0.017 min
Response: 19810616
Conc: 5.18 ng/ml

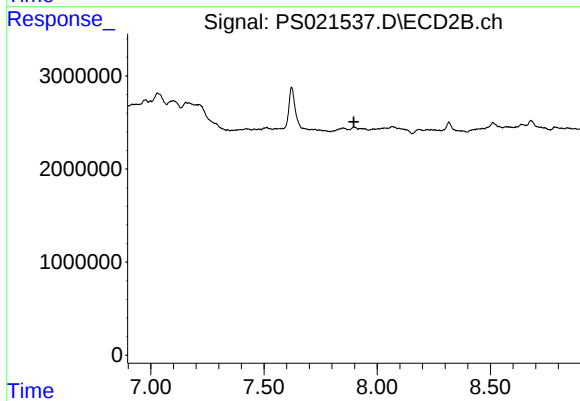

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.897 min
Response: 0
Conc: N.D.

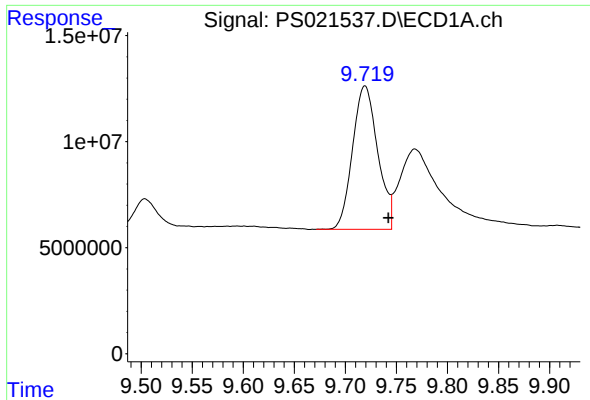

#15 Picloram

R.T.: 9.719 min
Delta R.T.: -0.023 min
Response: 115945447
Conc: 4.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

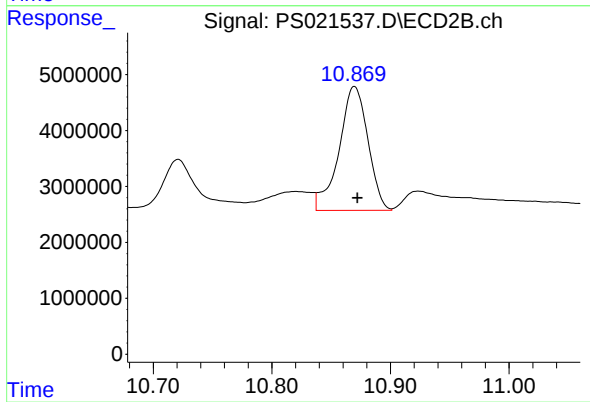

#15 Picloram

R.T.: 10.870 min
Delta R.T.: -0.002 min
Response: 37479098
Conc: 2.30 ng/ml