

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122322\
 Data File : PS021554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 20:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 01:21:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.376	6.809	1503.5E6	1045.0E6	517.467	606.173
Target Compounds							
1) T	Dalapon	2.514	0.000	309740	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.728	0.000	5687800	0	1.431	N.D. #
3) T	4-Nitroph...	6.221	0.000	7239324	0	4.026	N.D. #
5) T	DICAMBA	0.000	6.969	0	7678154	N.D.	1.005
6) T	MCP	0.000	7.026f	0	3230820	N.D.	<MDL
7) T	MCPA	6.756f	7.215f	6636029	25688496	<MDL	2.905 #
8) T	DICHLORPROP	7.132	7.644f	825054	5559670	<MDL	2.823 #
9) T	2,4-D	7.304	7.945f	3557513	340475	<MDL	<MDL #
10) T	Pentachlo...	7.549	8.320	1129295	1199709	<MDL	<MDL #
11) T	2,4,5-TP ...	8.087	8.688	11042955	3115043	<MDL	<MDL #
12) T	2,4,5-T	8.315	9.084	6896548	4535925	<MDL	<MDL #
13) T	2,4-DB	8.842	9.637f	2455255	1923242	<MDL	1.338 #
14) T	DINOSEB	9.898	9.894	13546125	1888674	<MDL	<MDL #
15) T	Picloram	9.725	10.921f	38273338	11645505	1.336	<MDL #
16) T	DCPA	10.164	10.819	5350369	13209974	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122322\
Data File : PS021554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 20:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 01:21:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

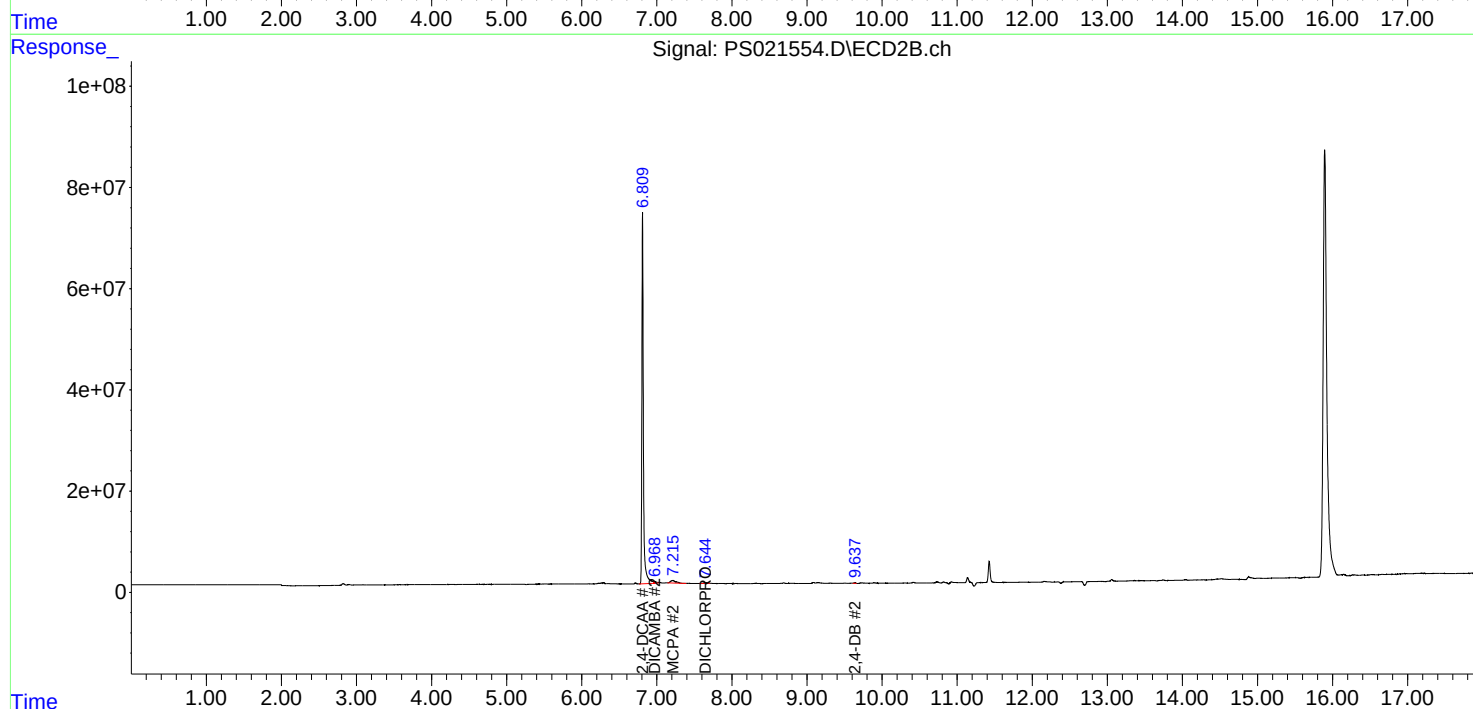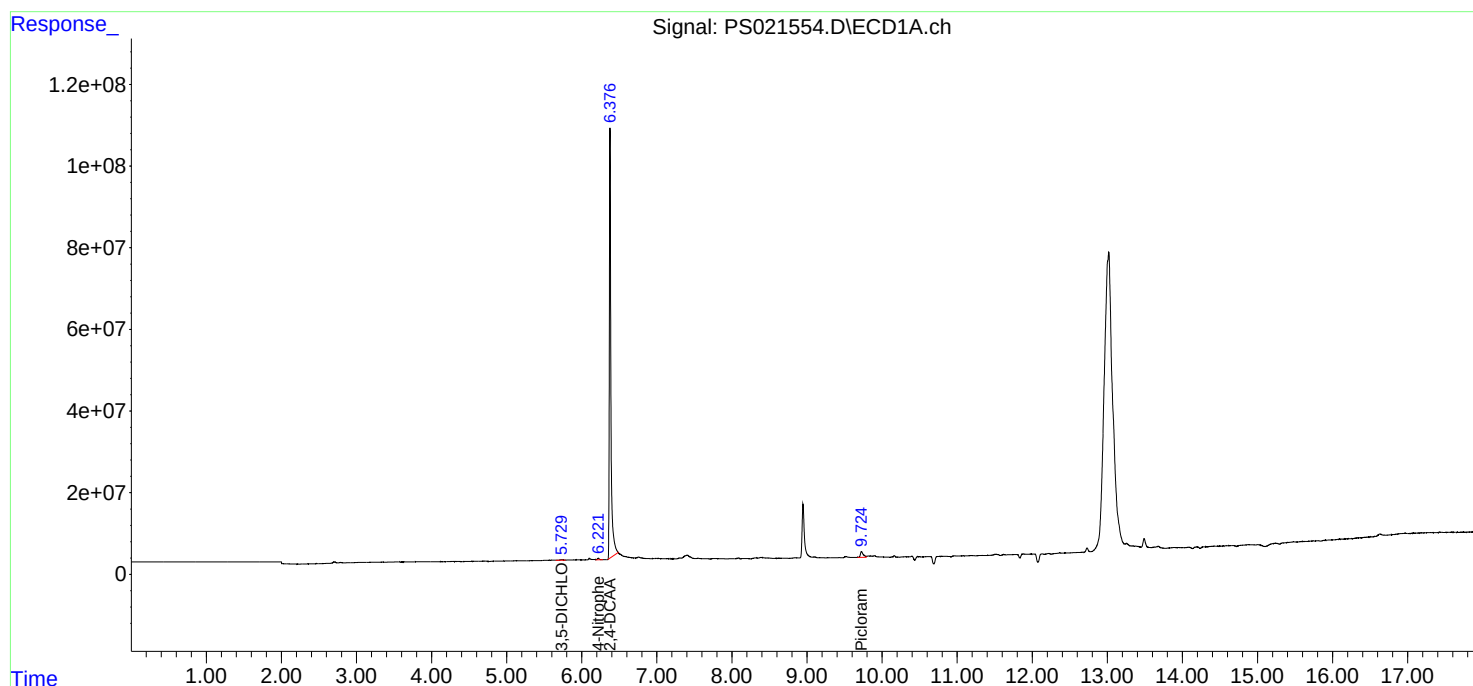


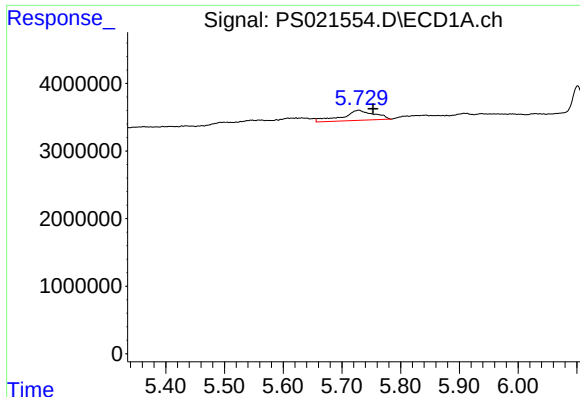

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.728 min
Delta R.T.: -0.024 min
Response: 5687800
Conc: 1.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

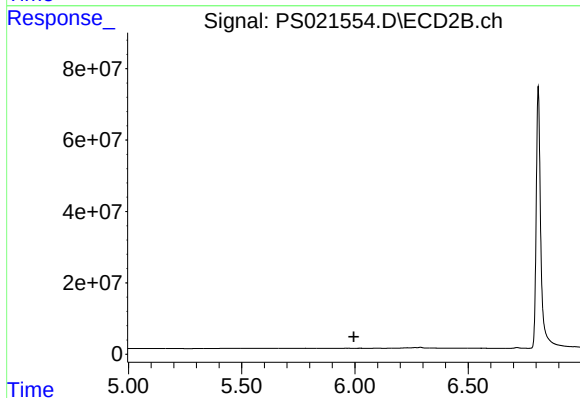


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

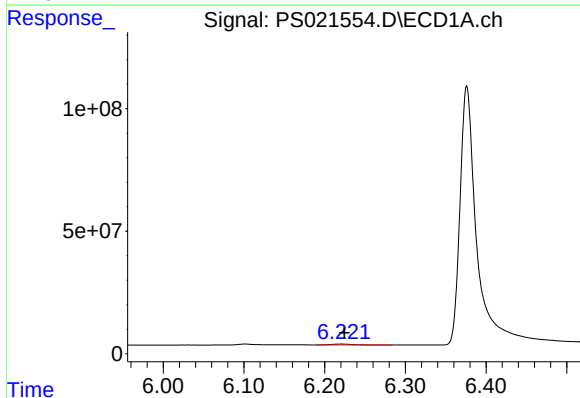


#3 4-Nitrophenol

R.T.: 6.221 min
Delta R.T.: -0.004 min
Response: 7239324
Conc: 4.03 ng/ml

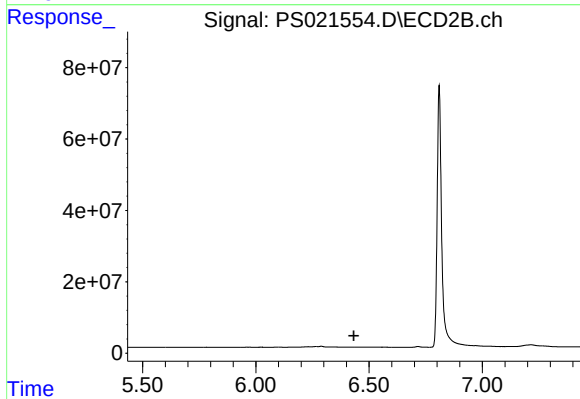

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

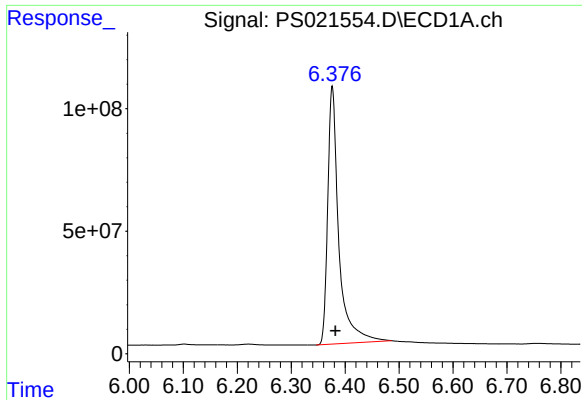

#4 2,4-DCAA


R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 1503498701
Conc: 517.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

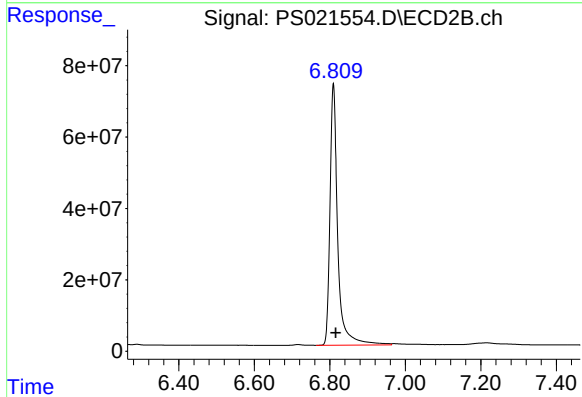


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.006 min
Response: 1045037622
Conc: 606.17 ng/ml

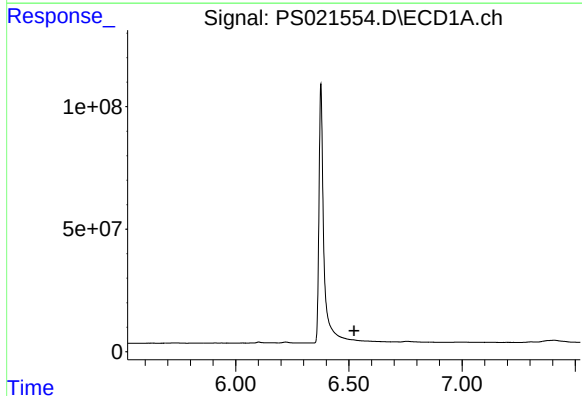


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

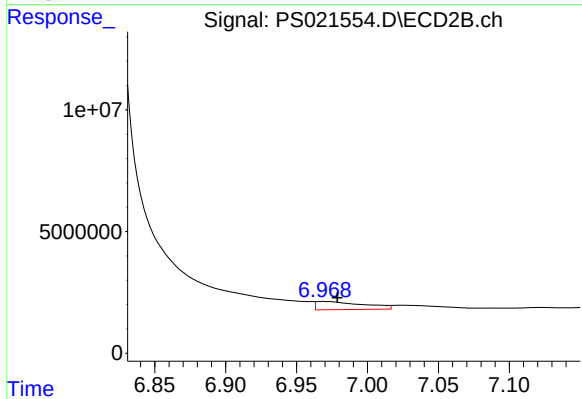

#5 DICAMBA


R.T.: 6.969 min
Delta R.T.: -0.010 min
Response: 7678154
Conc: 1.01 ng/ml

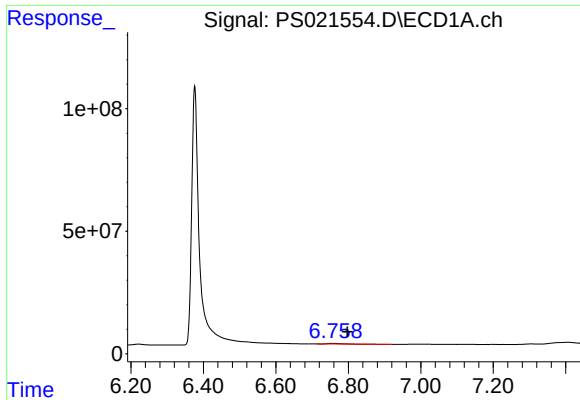

#7 MCPA


R.T.: 6.756 min
Delta R.T.: -0.041 min
Response: 6636029
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

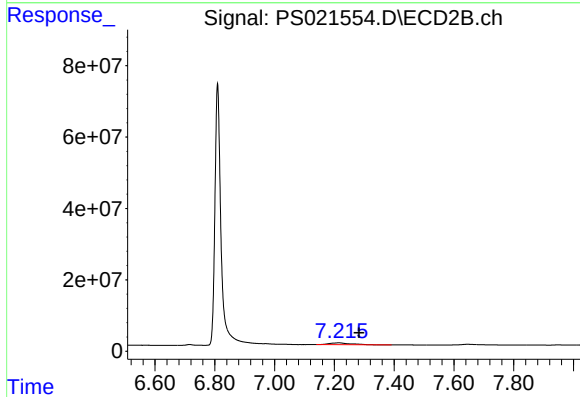


#7 MCPA

R.T.: 7.215 min
Delta R.T.: -0.068 min
Response: 25688496
Conc: 2.91 ug/ml

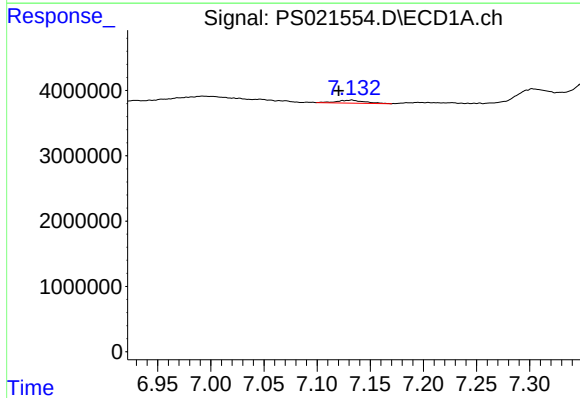


#8 DICHLORPROP

R.T.: 7.132 min
Delta R.T.: 0.012 min
Response: 825054
Conc: N.D.

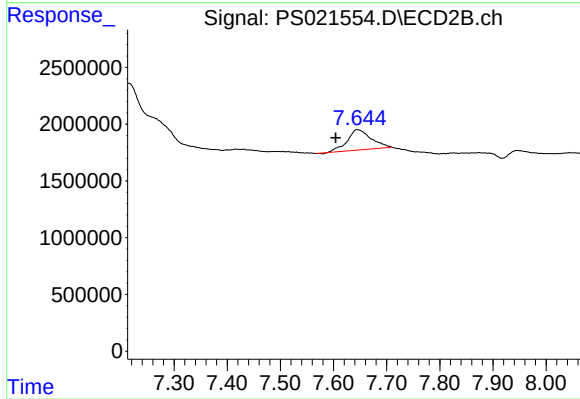

#8 DICHLORPROP


R.T.: 7.644 min
Delta R.T.: 0.041 min
Response: 5559670
Conc: 2.82 ng/ml

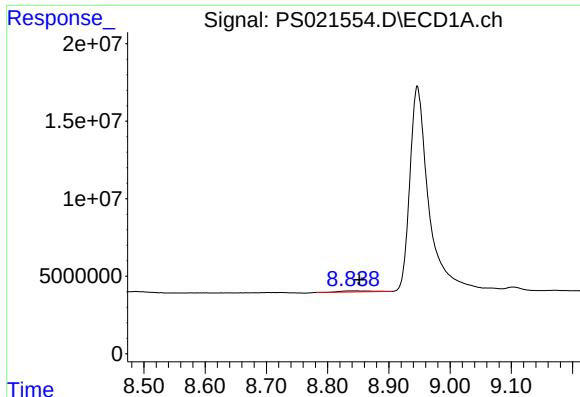

#13 2,4-DB


R.T.: 8.842 min
Delta R.T.: -0.010 min
Response: 2455255
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

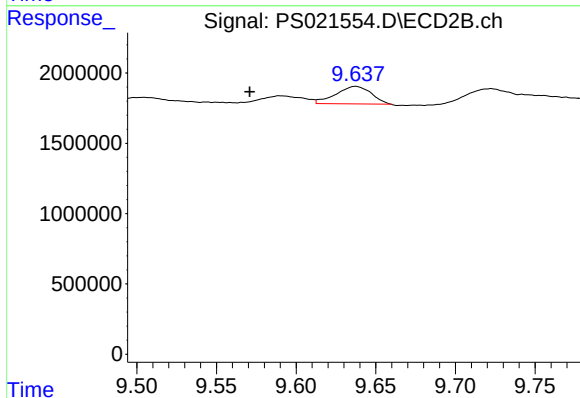


#13 2,4-DB

R.T.: 9.637 min
Delta R.T.: 0.066 min
Response: 1923242
Conc: 1.34 ng/ml

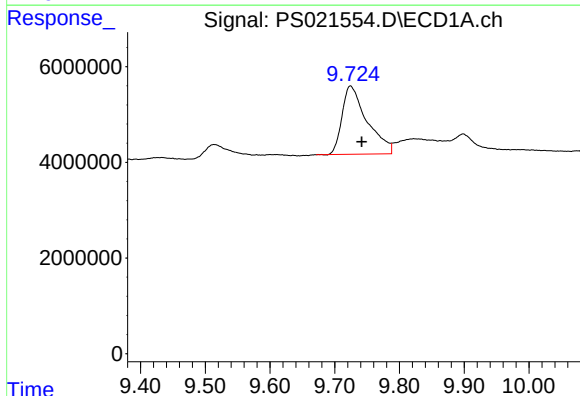

#15 Picloram

R.T.: 9.725 min
Delta R.T.: -0.017 min
Response: 38273338
Conc: 1.34 ng/ml

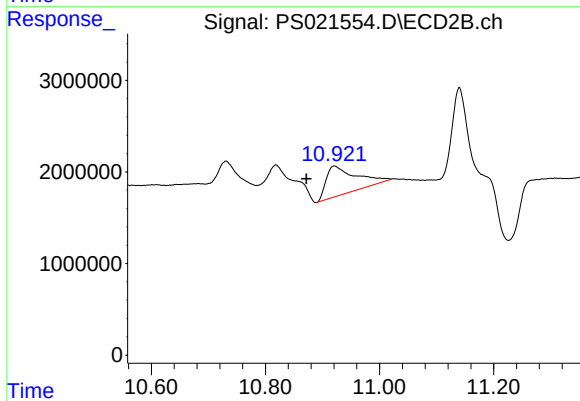

#15 Picloram

R.T.: 10.921 min
Delta R.T.: 0.049 min
Response: 11645505
Conc: N.D.