

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122324\
 Data File : PS028786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 11:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 13:45:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	7.700	1061.6E6	542.0E6	469.322	481.551
Target Compounds							
1) T	Dalapon	0.000	2.719f	0	13967837	N.D.	7.095
2) T	3,5-DICHL...	6.378	0.000	188955	0	<MDL	N.D. #
3) T	4-Nitroph...	7.008	0.000	2957798	0	1.969	N.D. #
5) T	DICAMBA	7.392	0.000	120392	0	<MDL	N.D. #
6) T	MCPD	7.533f	0.000	1231674	0	<MDL	N.D. #
7) T	MCPA	7.744	0.000	1495740	0	<MDL	N.D. #
8) T	DICHLORPROP	8.072f	0.000	1068504	0	<MDL	N.D. #
10) T	Pentachlo...	8.628	0.000	7144741	0	<MDL	N.D. #
12) T	2,4,5-T	9.512	10.264	885531	5491800	<MDL	<MDL #
13) T	2,4-DB	10.087	0.000	1569016	0	<MDL	N.D. #
14) T	DINOSEB	11.283	0.000	3243168	0	<MDL	N.D. #
15) T	Picloram	11.105	12.302	16032610	7803861	<MDL	<MDL #
16) T	DCPA	11.570	0.000	5173790	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122324\
Data File : PS028786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 11:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 13:45:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

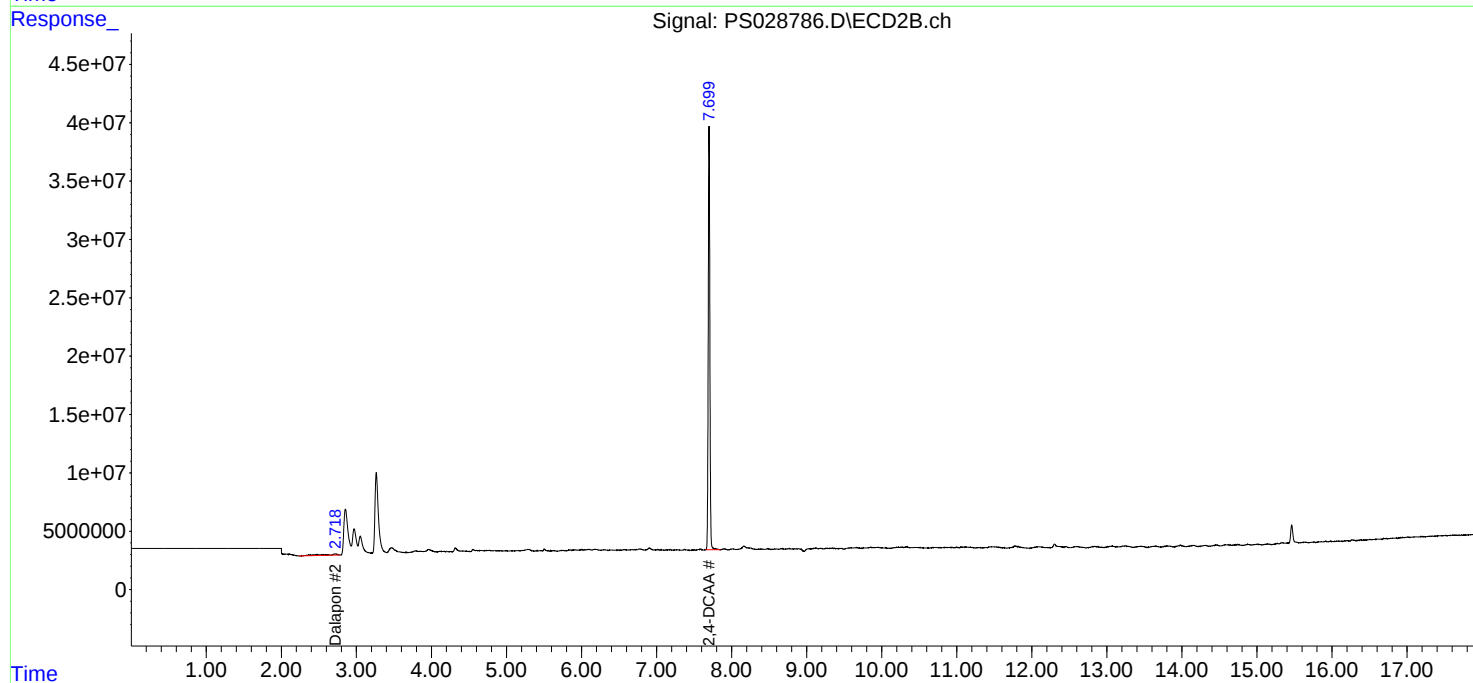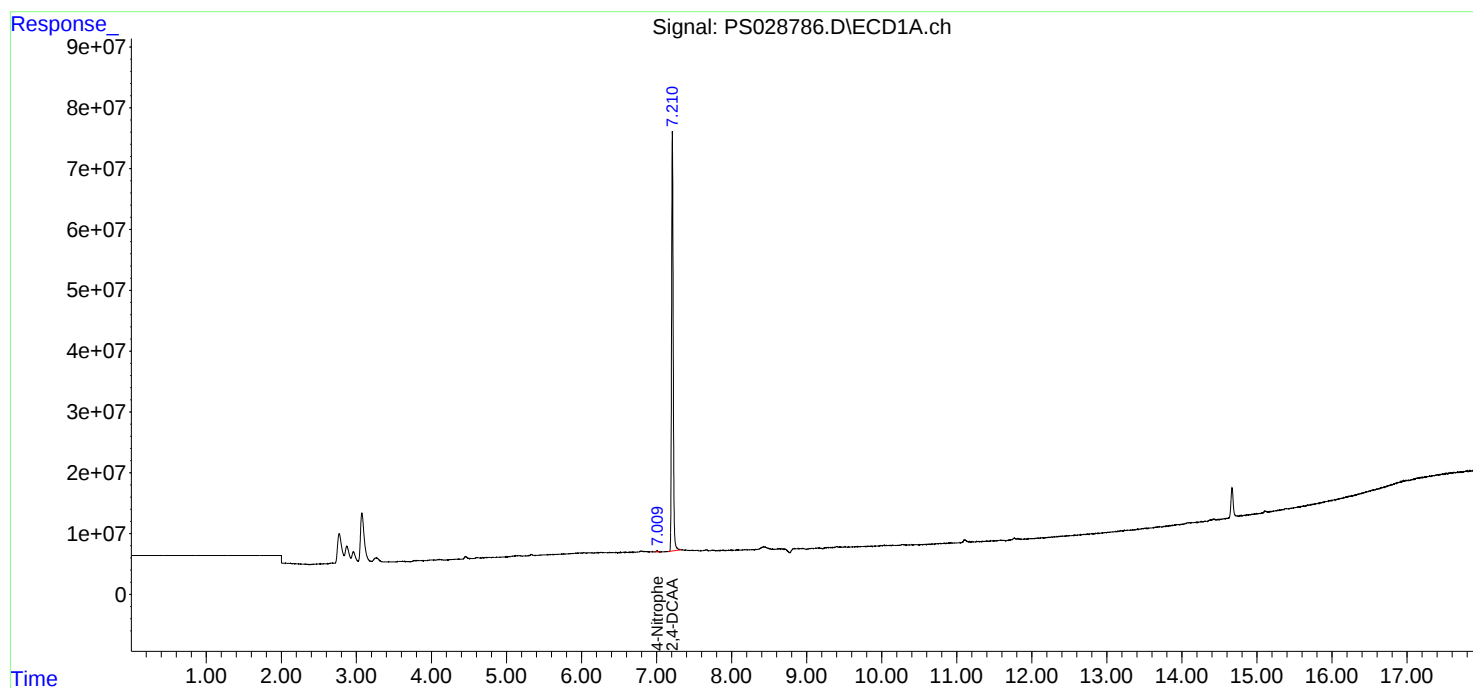


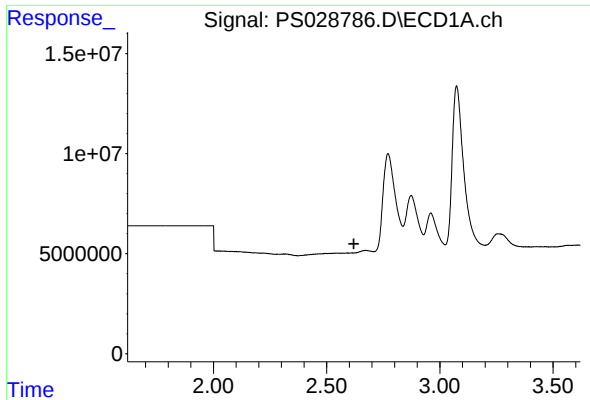

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

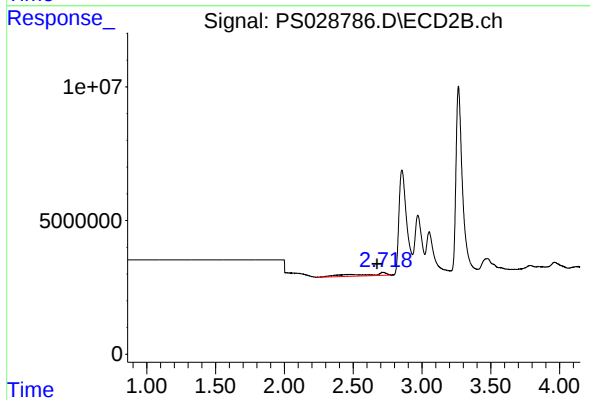


#1 Dalapon

R.T.: 2.719 min
Delta R.T.: 0.047 min
Response: 13967837
Conc: 7.10 ng/ml

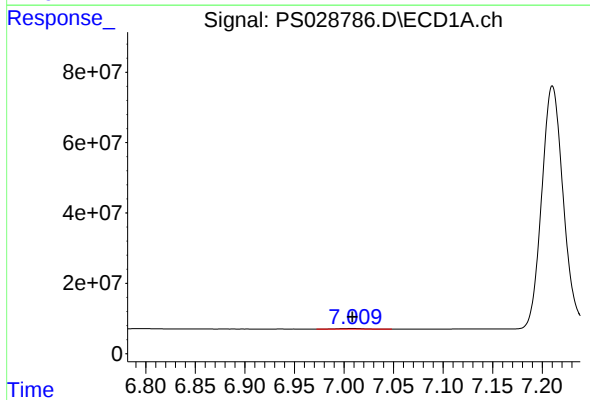


#3 4-Nitrophenol

R.T.: 7.008 min
Delta R.T.: 0.000 min
Response: 2957798
Conc: 1.97 ng/ml

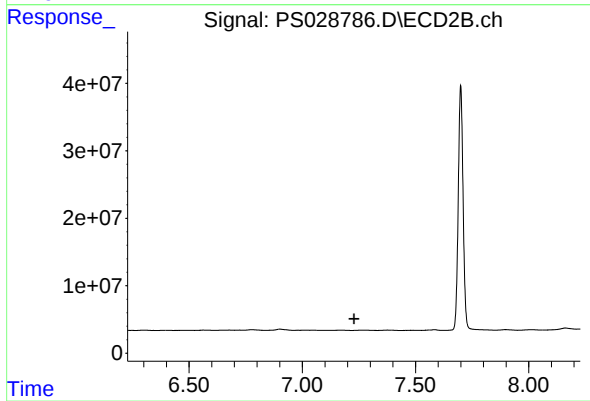

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.228 min
Response: 0
Conc: N.D.

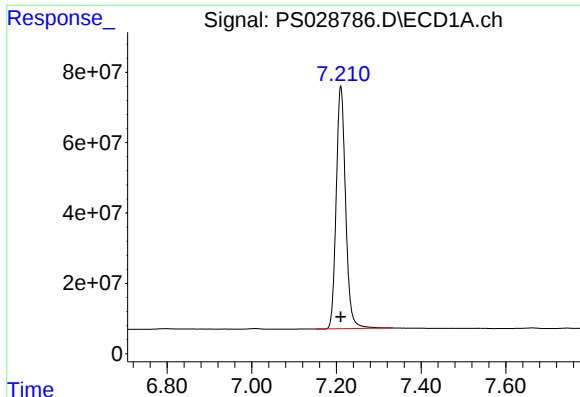

#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: 0.000 min
Response: 1061618688
Conc: 469.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

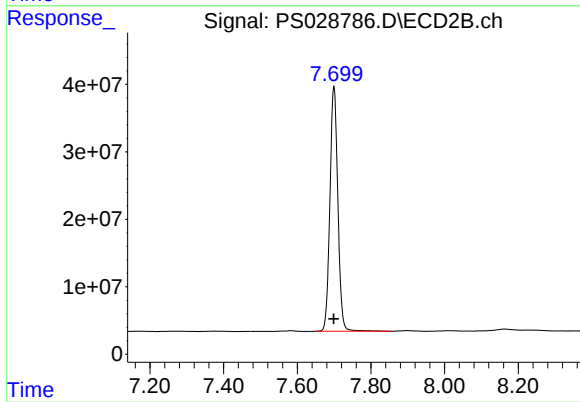

#4 2,4-DCAA

R.T.: 7.700 min
Delta R.T.: 0.000 min
Response: 542003820
Conc: 481.55 ng/ml