

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122324\
 Data File : PS028793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 13:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 14:44:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	7.700	1153.9E6	549.1E6	510.113	487.862
Target Compounds							
1) T	Dalapon	2.667f	0.000	5473380	0	1.943	N.D. #
2) T	3,5-DICHL...	6.383	0.000	1241970	0	<MDL	N.D. #
3) T	4-Nitroph...	7.007	0.000	2948193	0	1.963	N.D. #
5) T	DICAMBA	7.396	7.899	818697	3425289	<MDL	<MDL #
6) T	MCPD	7.536f	0.000	1605428	0	<MDL	N.D. #
7) T	MCPA	7.742	0.000	2218449	0	<MDL	N.D. #
8) T	DICHLORPROP	8.073f	0.000	2676122	0	1.009	N.D. #
10) T	Pentachlo...	8.630	0.000	11549114	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.166f	9.841	686115	1833594	<MDL	<MDL #
12) T	2,4,5-T	9.495	10.262	5562604	5954116	<MDL	<MDL #
13) T	2,4-DB	10.074	0.000	3157573	0	1.012	N.D. #
14) T	DINOSEB	11.250f	0.000	12411859	0	<MDL	N.D. #
15) T	Picloram	11.099	12.299	66383769	20087961	2.476	1.565 #
16) T	DCPA	11.554	0.000	11154050	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122324\
Data File : PS028793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 13:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 14:44:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

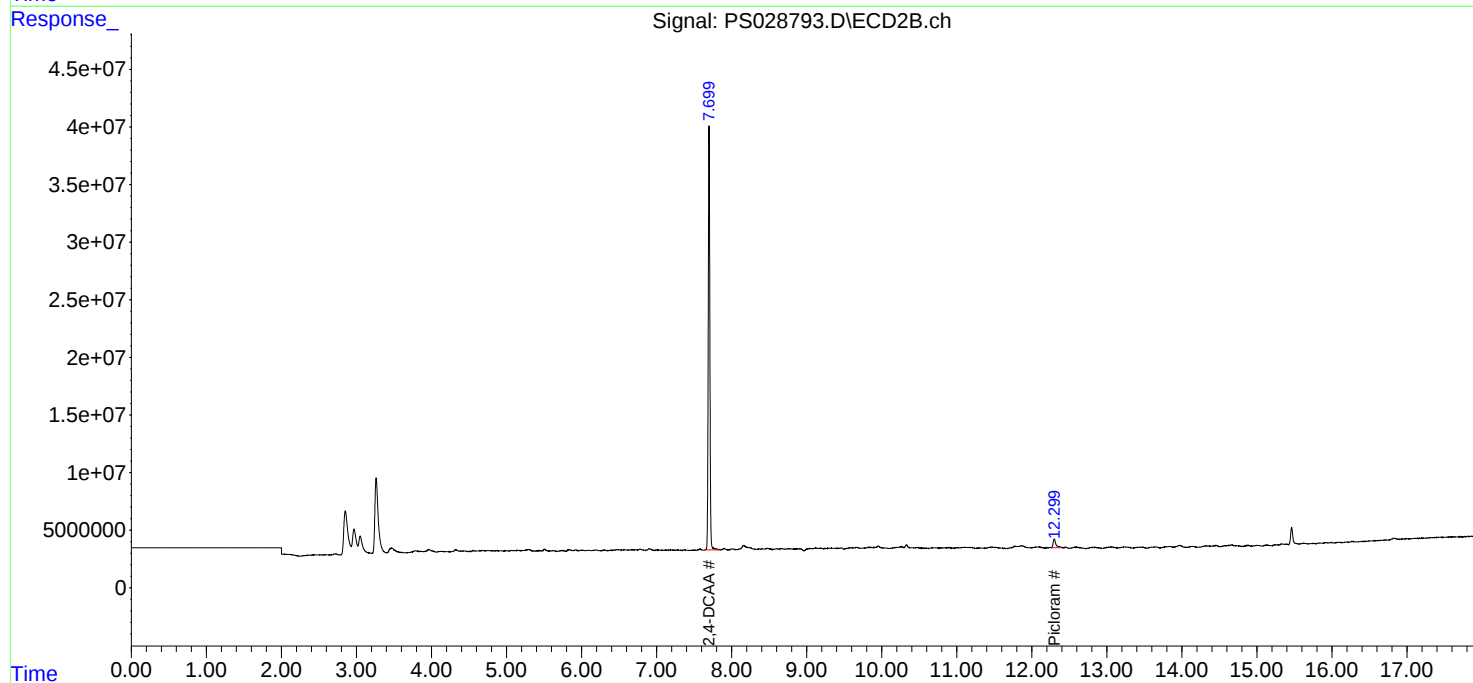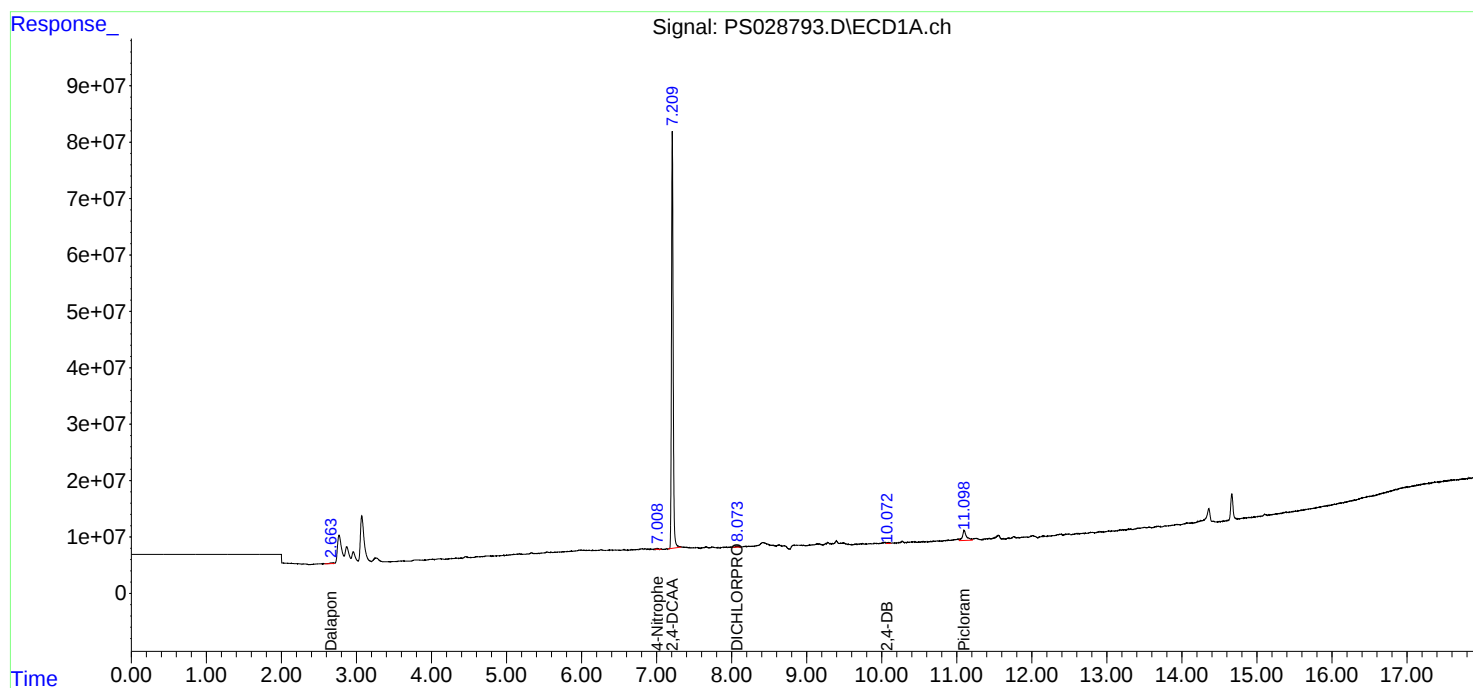


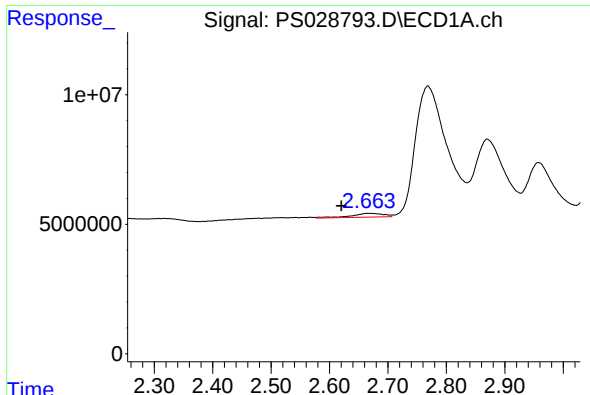

#1 Dalapon


R.T.: 2.667 min
Delta R.T.: 0.047 min
Response: 5473380
Conc: 1.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

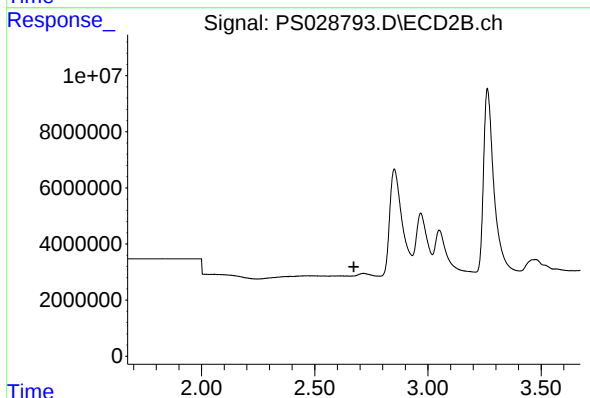


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.673 min
Response: 0
Conc: N.D.

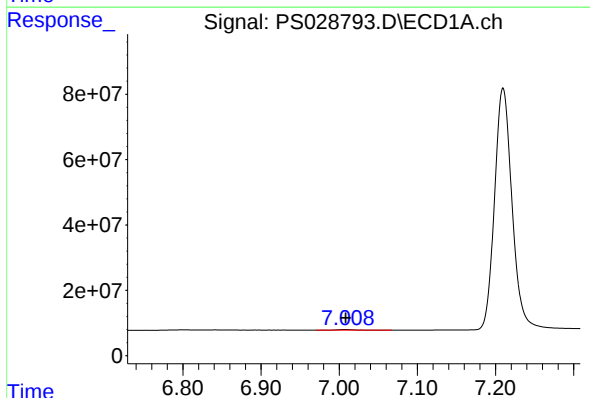


#3 4-Nitrophenol

R.T.: 7.007 min
Delta R.T.: -0.001 min
Response: 2948193
Conc: 1.96 ng/ml

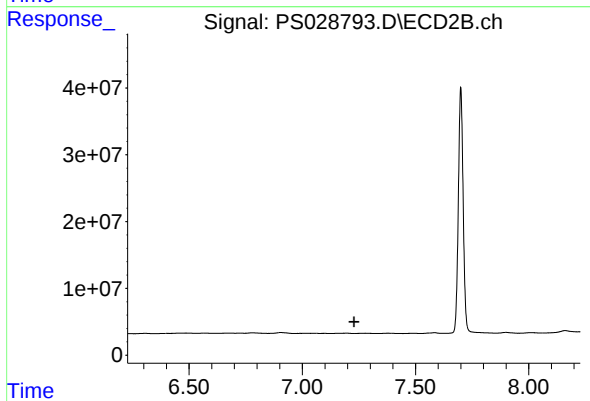

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

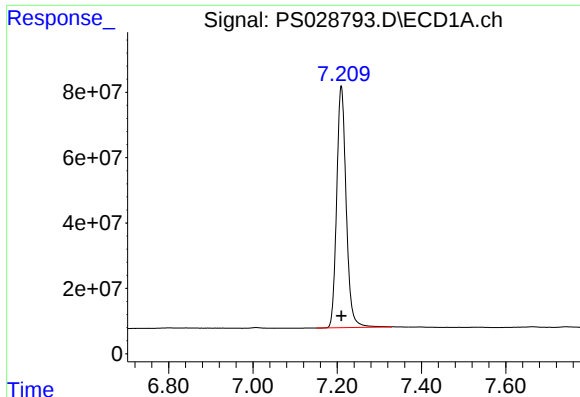

#4 2,4-DCAA


R.T.: 7.210 min
Delta R.T.: 0.000 min
Response: 1153889362
Conc: 510.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

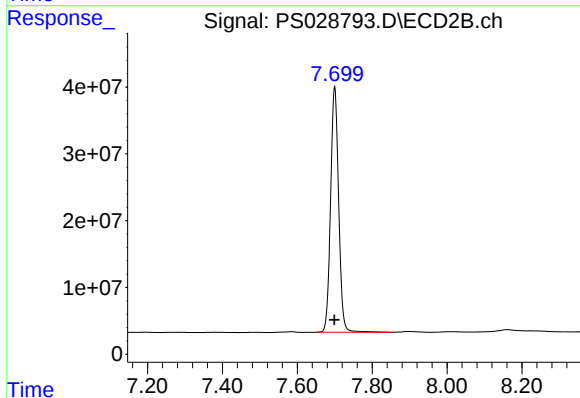


#4 2,4-DCAA

R.T.: 7.700 min
Delta R.T.: 0.000 min
Response: 549106840
Conc: 487.86 ng/ml

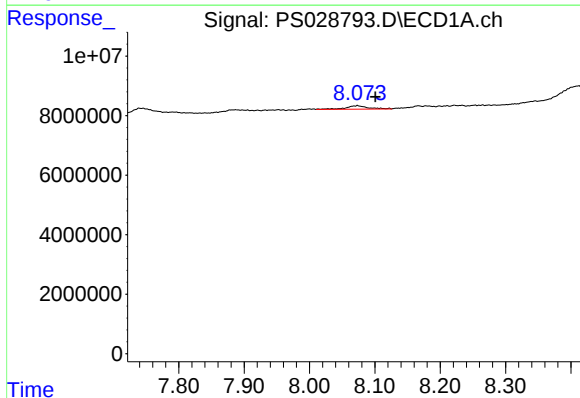


#8 DICHLORPROP

R.T.: 8.073 min
Delta R.T.: -0.028 min
Response: 2676122
Conc: 1.01 ng/ml

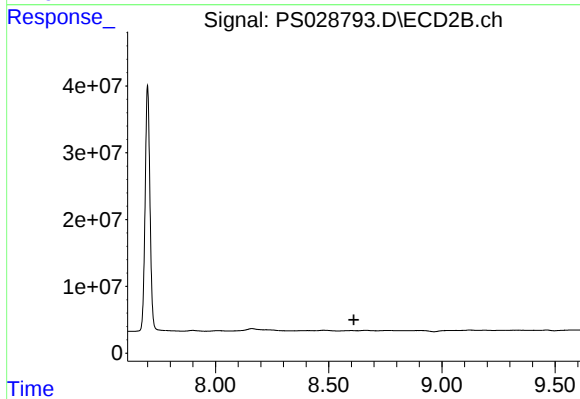

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.611 min
Response: 0
Conc: N.D.

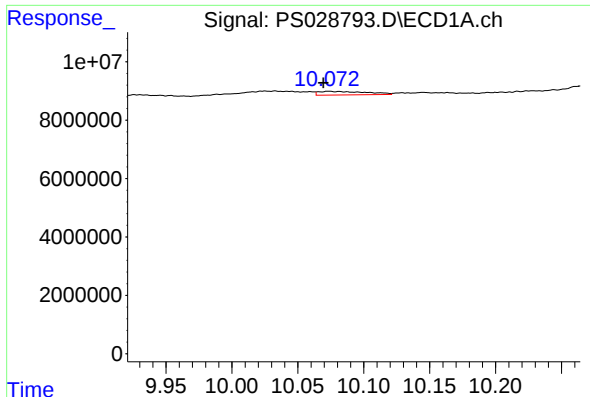

#13 2,4-DB


R.T.: 10.074 min
Delta R.T.: 0.005 min
Response: 3157573
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

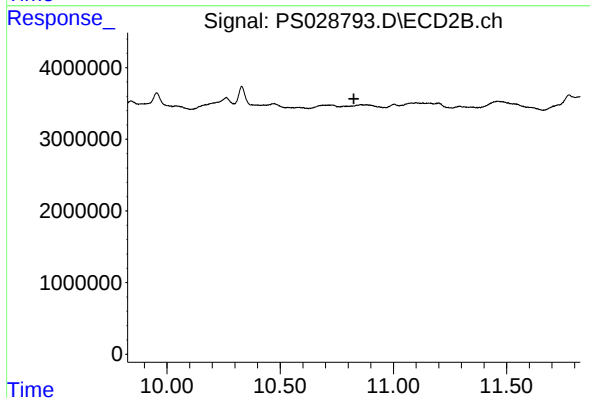


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.826 min
Response: 0
Conc: N.D.

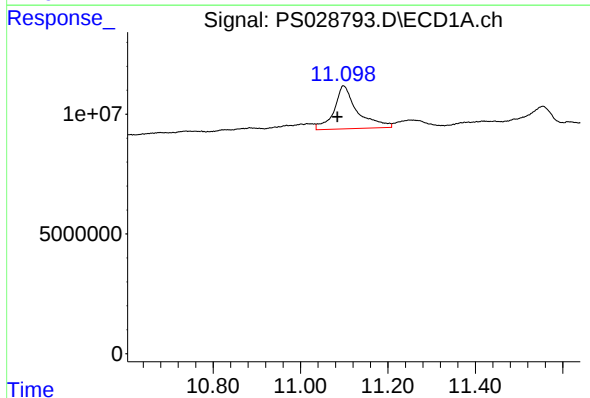

#15 Picloram

R.T.: 11.099 min
Delta R.T.: 0.014 min
Response: 66383769
Conc: 2.48 ng/ml

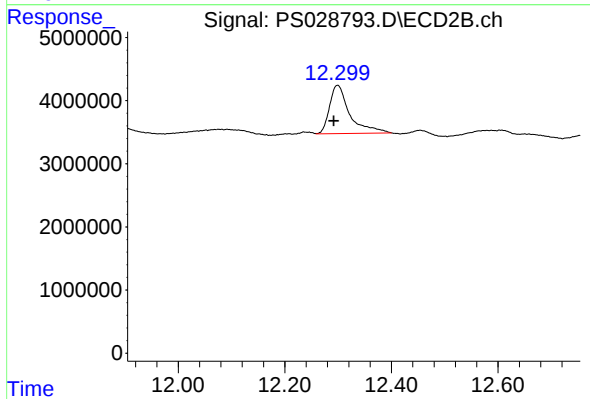

#15 Picloram

R.T.: 12.299 min
Delta R.T.: 0.007 min
Response: 20087961
Conc: 1.56 ng/ml