

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122324\
 Data File : PS028799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 16:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 01:25:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	7.699	1188.4E6	556.2E6	525.365	494.202
Target Compounds							
1) T	Dalapon	0.000	2.718f	0	3929223	N.D.	1.996
2) T	3,5-DICHL...	6.383	0.000	1295489	0	<MDL	N.D. #
3) T	4-Nitroph...	7.005	0.000	4255058	0	2.833	N.D. #
5) T	DICAMBA	7.394	7.895	719812	4222396	<MDL	<MDL #
6) T	MCPD	7.527f	8.004	2052647	3032952	<MDL	<MDL #
7) T	MCPA	7.746	0.000	630114	0	<MDL	N.D. #
8) T	DICHLORPROP	8.069f	8.658f	5074572	5160071	1.913	3.740 #
10) T	Pentachlo...	8.628	0.000	12678222	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.840	0	2164611	N.D.	<MDL
12) T	2,4,5-T	9.498	10.260	5868112	6035006	<MDL	<MDL #
13) T	2,4-DB	10.068	0.000	6415344	0	2.055	N.D. #
14) T	DINOSEB	11.272	0.000	8579553	0	<MDL	N.D. #
15) T	Picloram	11.090	12.296	144.0E6	45407993	5.369	3.537 #
16) T	DCPA	11.559	0.000	6479621	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122324\
Data File : PS028799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 16:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 01:25:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

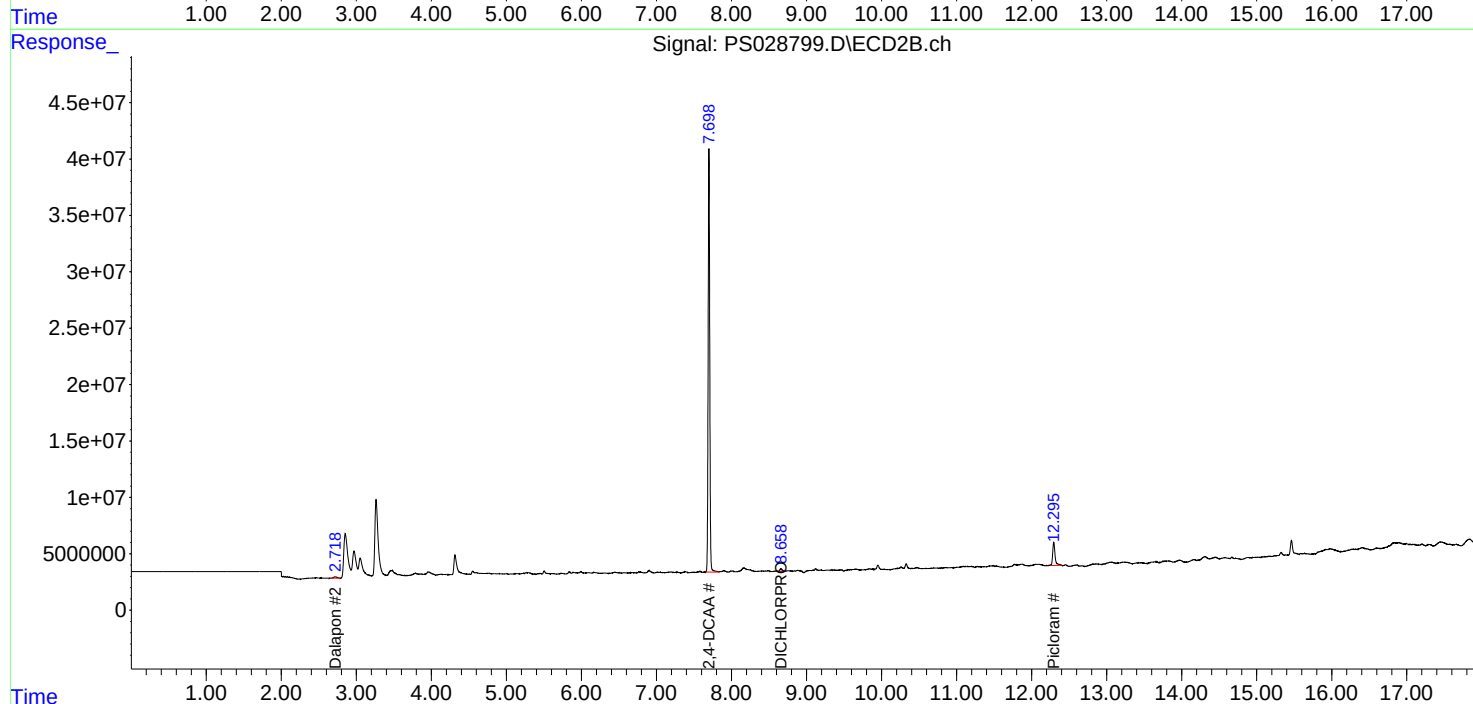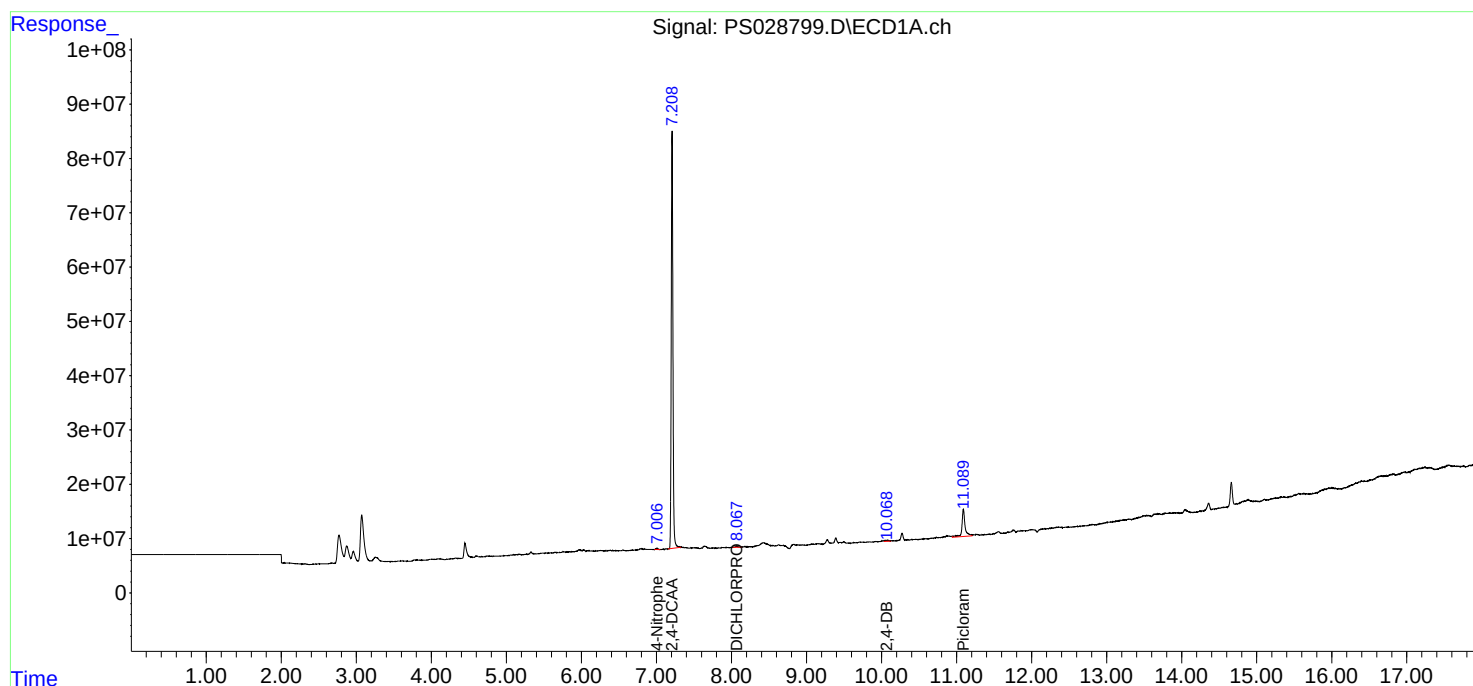


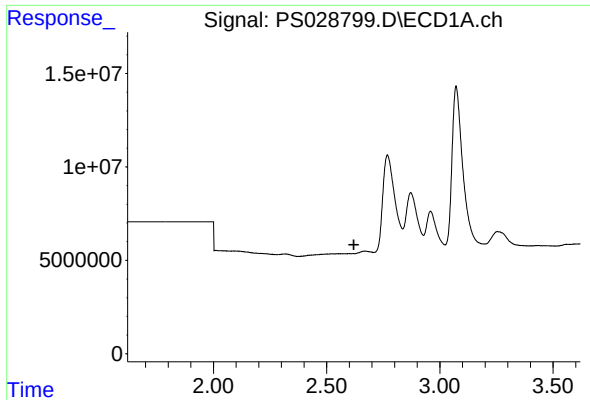

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

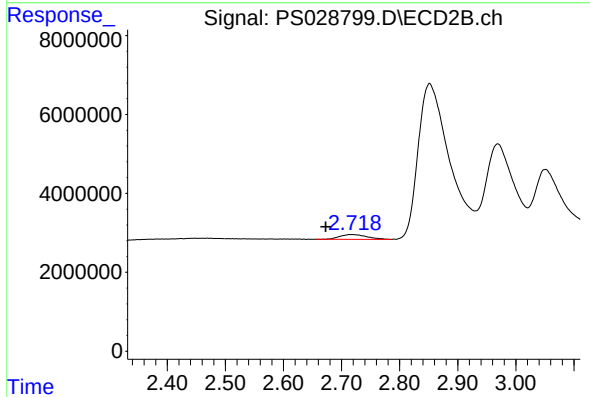


#1 Dalapon

R.T.: 2.718 min
Delta R.T.: 0.045 min
Response: 3929223
Conc: 2.00 ng/ml

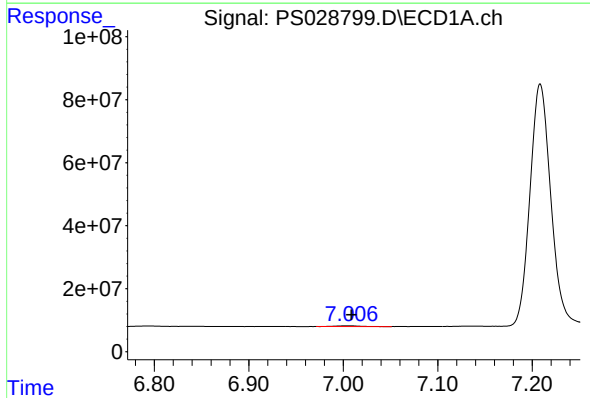


#3 4-Nitrophenol

R.T.: 7.005 min
Delta R.T.: -0.004 min
Response: 4255058
Conc: 2.83 ng/ml

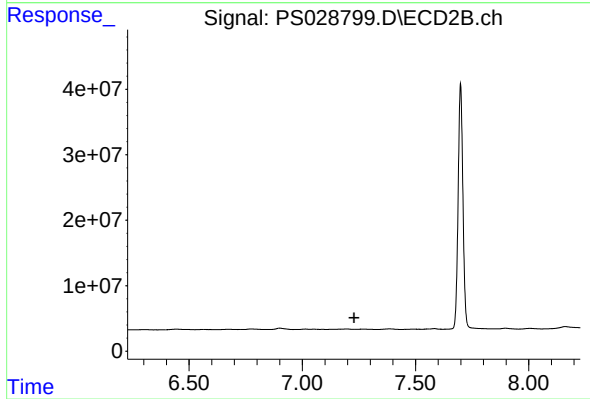

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.228 min
Response: 0
Conc: N.D.

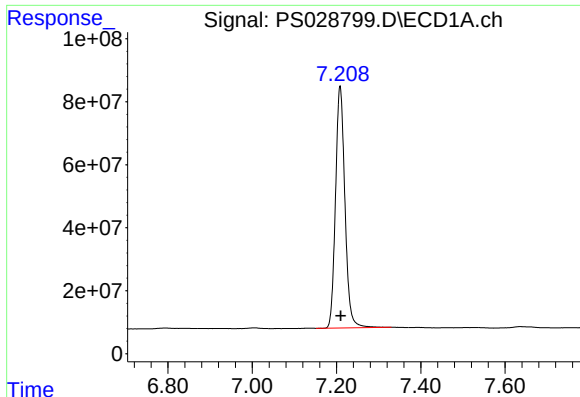

#4 2,4-DCAA


R.T.: 7.209 min
Delta R.T.: -0.001 min
Response: 1188387984
Conc: 525.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

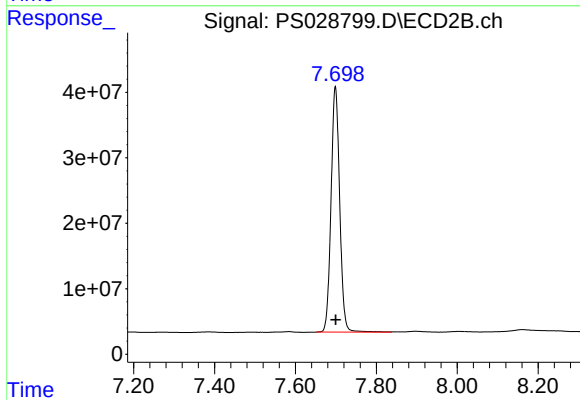


#4 2,4-DCAA

R.T.: 7.699 min
Delta R.T.: 0.000 min
Response: 556242707
Conc: 494.20 ng/ml

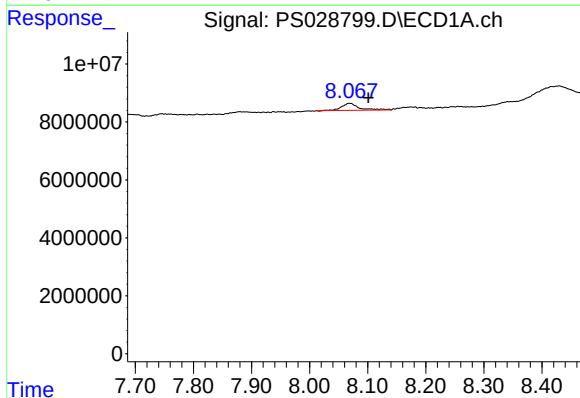


#8 DICHLORPROP

R.T.: 8.069 min
Delta R.T.: -0.032 min
Response: 5074572
Conc: 1.91 ng/ml

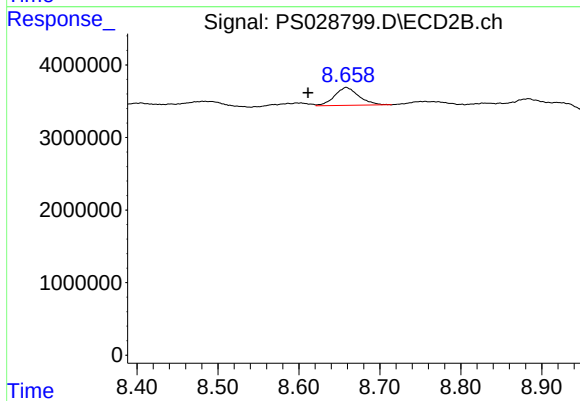

#8 DICHLORPROP


R.T.: 8.658 min
Delta R.T.: 0.047 min
Response: 5160071
Conc: 3.74 ng/ml

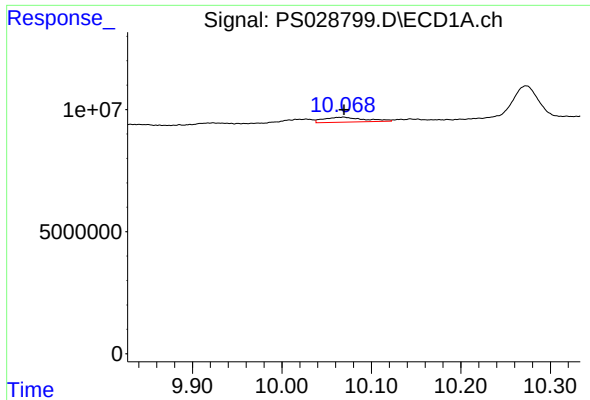

#13 2,4-DB


R.T.: 10.068 min
Delta R.T.: -0.001 min
Response: 6415344
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

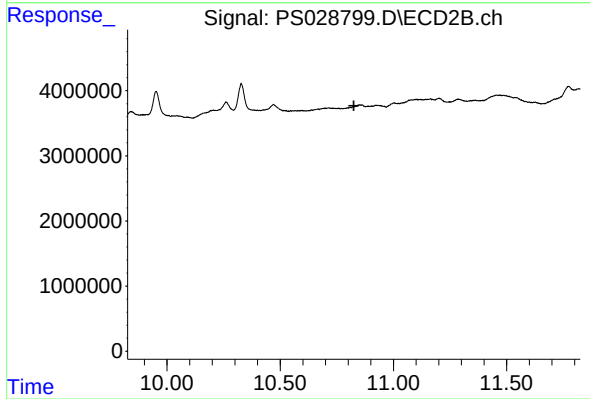


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.826 min
Response: 0
Conc: N.D.

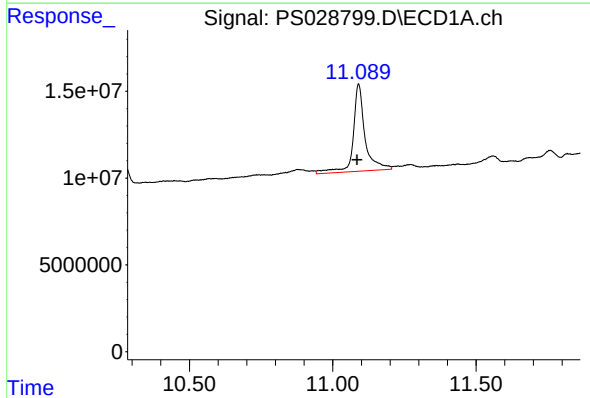

#15 Picloram

R.T.: 11.090 min
Delta R.T.: 0.006 min
Response: 143959582
Conc: 5.37 ng/ml

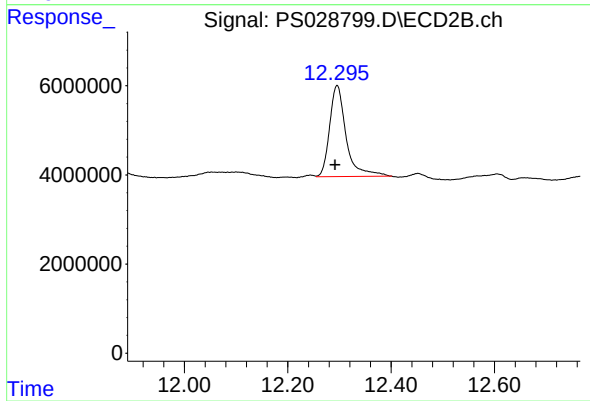

#15 Picloram

R.T.: 12.296 min
Delta R.T.: 0.004 min
Response: 45407993
Conc: 3.54 ng/ml