

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122324\
 Data File : PS028801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 16:58
 Operator : AR\AJ
 Sample : P5306-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OU4-VSL-07-121224

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/26/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 01:54:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.208	7.699	516.9E6	220.7E6	228.510	196.078m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122324\
Data File : PS028801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 16:58
Operator : AR\AJ
Sample : P5306-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
OU4-VSL-07-121224


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/26/2024
Supervised By : Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 01:54:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

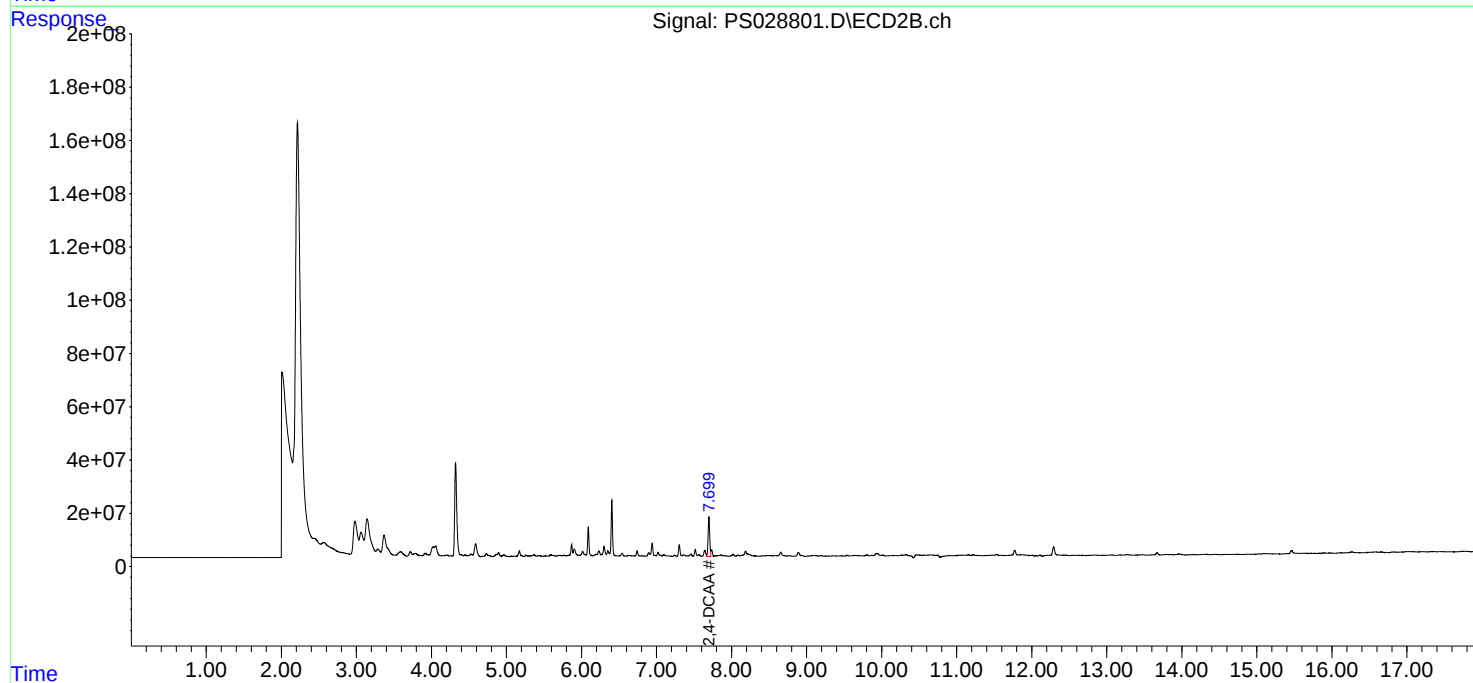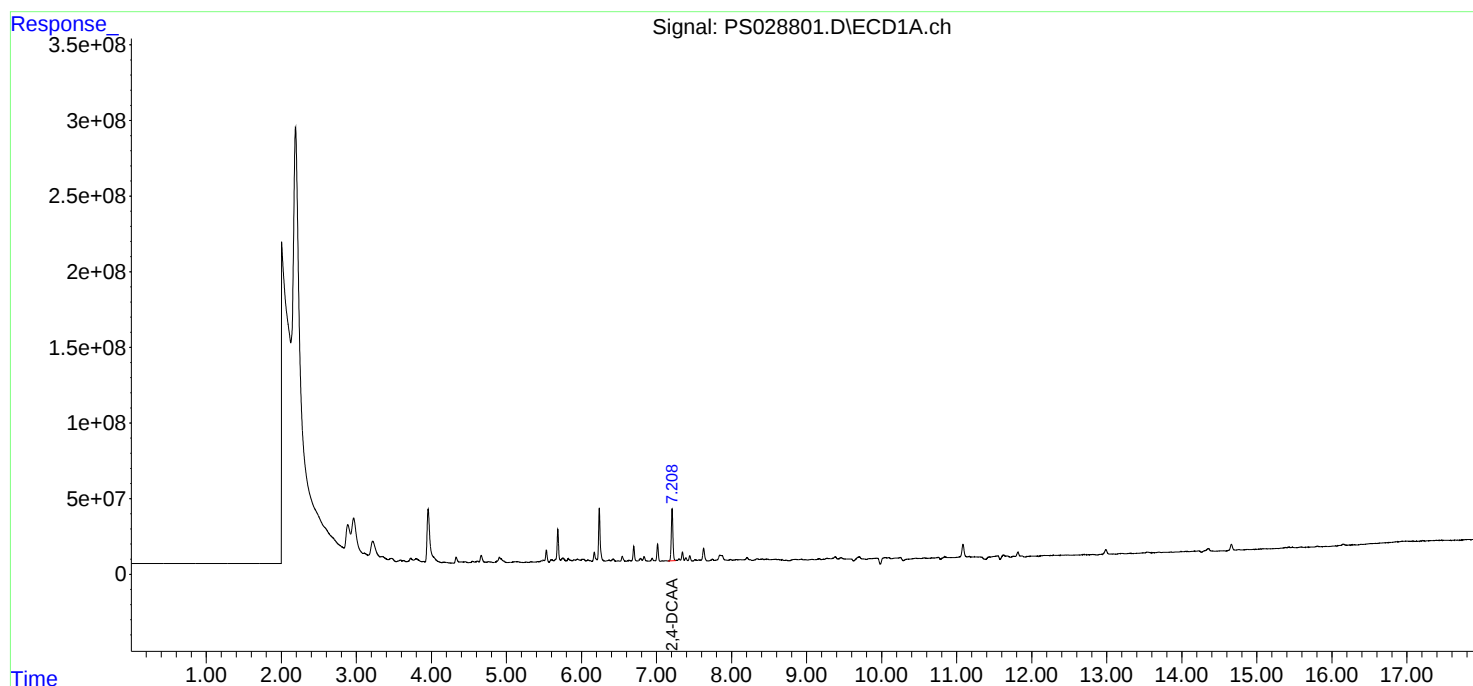

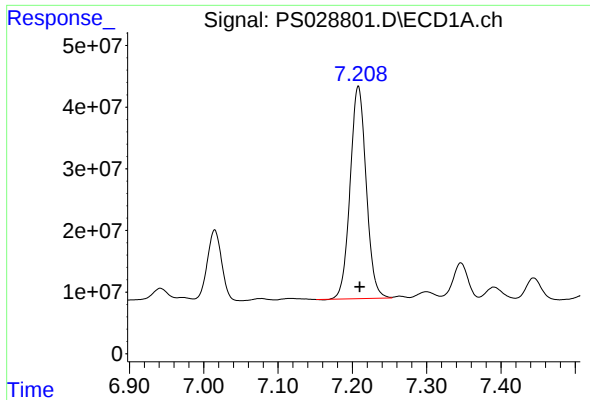


#4 2,4-DCAA

R.T.: 7.208 min
Delta R.T.: -0.002 min
Response: 516895298
Conc: 228.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
OU4-VSL-07-121224

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/26/2024
Supervised By :Ankita Jodhani 12/27/2024

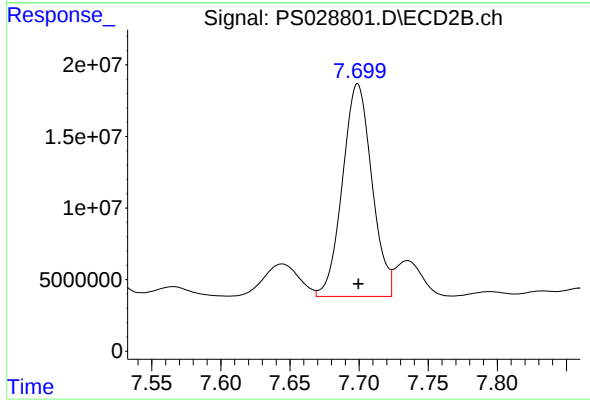

#4 2,4-DCAA

R.T.: 7.699 min
Delta R.T.: 0.000 min
Response: 220693494
Conc: 196.08 ng/ml m