

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122523\
 Data File : PS025182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 13:48
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:28:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	2.507	2.551	3963824	3365426	1.375	2.934 #
2) T	3,5-DICHL...	0.000	5.897f	0	242711	N.D.	<MDL
3) T	4-Nitroph...	6.192	0.000	8399449	0	5.704	N.D. #
5) T	DICAMBA	0.000	6.967	0	459548	N.D.	<MDL
6) T	MCPD	6.678	6.991	3662771	32611	<MDL	<MDL #
7) T	MCPA	0.000	7.177f	0	887191	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.546	0	1483850	N.D.	1.886
9) T	2,4-D	0.000	7.872f	0	448843	N.D.	<MDL
10) T	Pentachlo...	0.000	8.252	0	237300	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.611	0	314826	N.D.	<MDL
12) T	2,4,5-T	8.234f	8.971	5702217	813965	<MDL	<MDL #
13) T	2,4-DB	0.000	9.482	0	379906	N.D.	<MDL
14) T	DINOSEB	0.000	9.785	0	134068	N.D.	<MDL
15) T	Picloram	9.675	10.751	32574505	13860177	1.672	2.118 #
16) T	DCPA	0.000	10.751	0	13860177	N.D.	2.557



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122523\
Data File : PS025182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 13:48
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:28:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

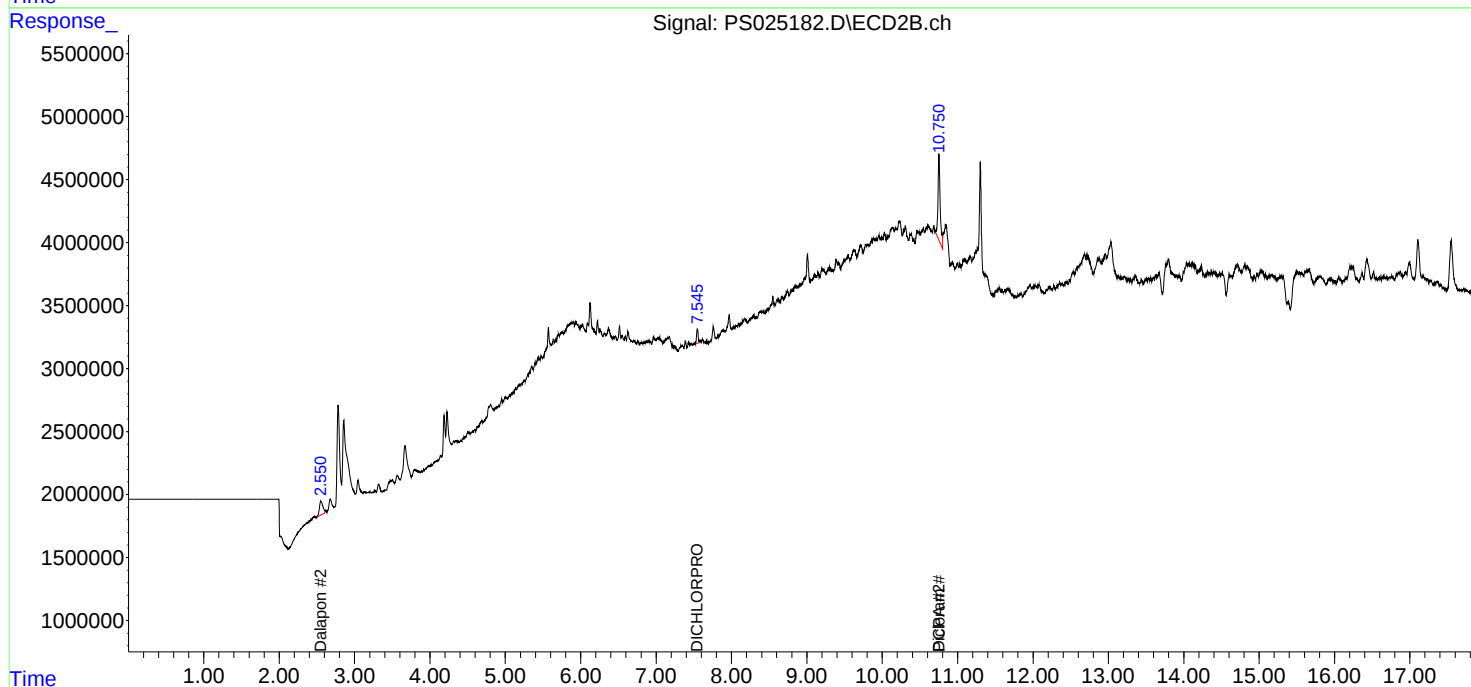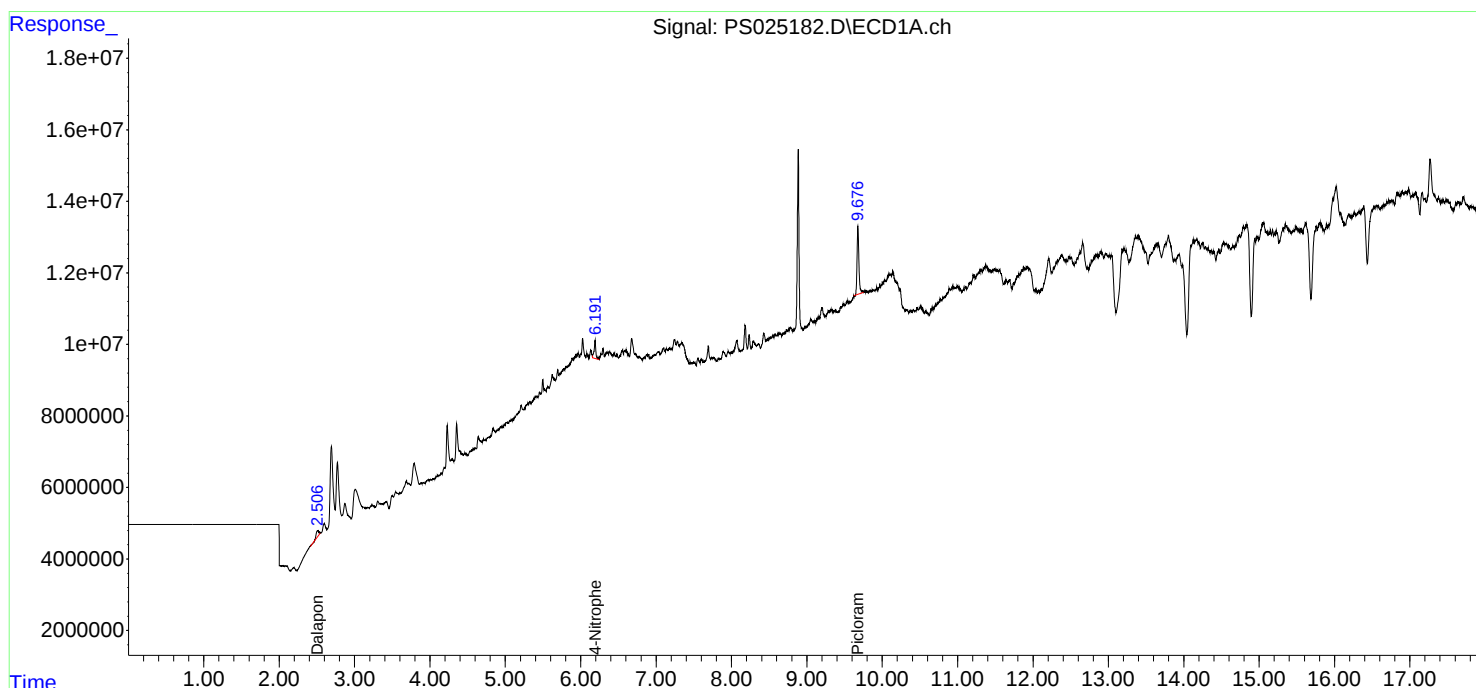


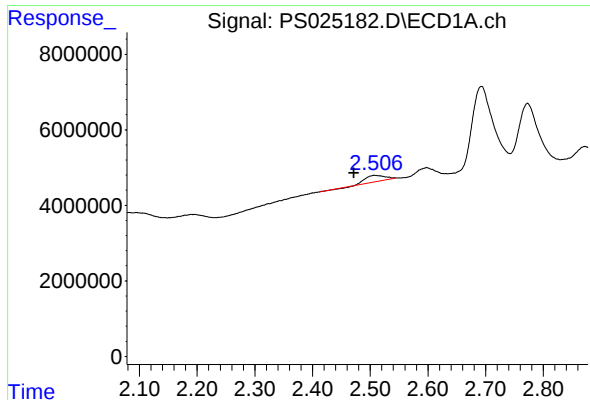

#1 Dalapon


R.T.: 2.507 min
Delta R.T.: 0.035 min
Response: 3963824
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

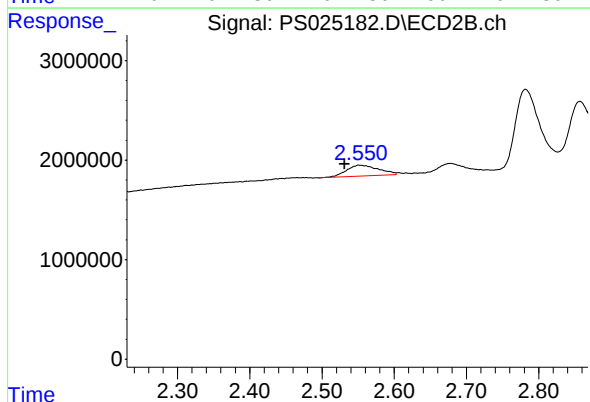


#1 Dalapon

R.T.: 2.551 min
Delta R.T.: 0.019 min
Response: 3365426
Conc: 2.93 ng/ml

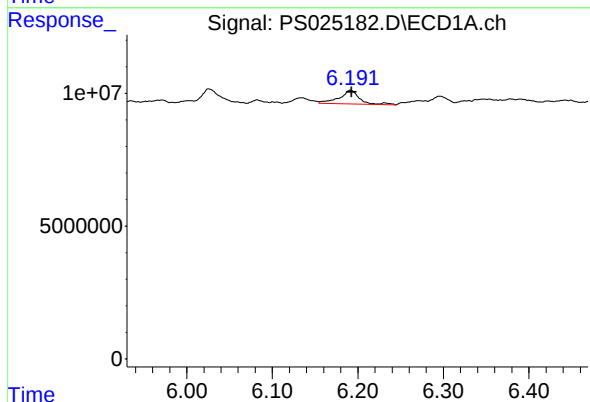


#3 4-Nitrophenol

R.T.: 6.192 min
Delta R.T.: -0.001 min
Response: 8399449
Conc: 5.70 ng/ml

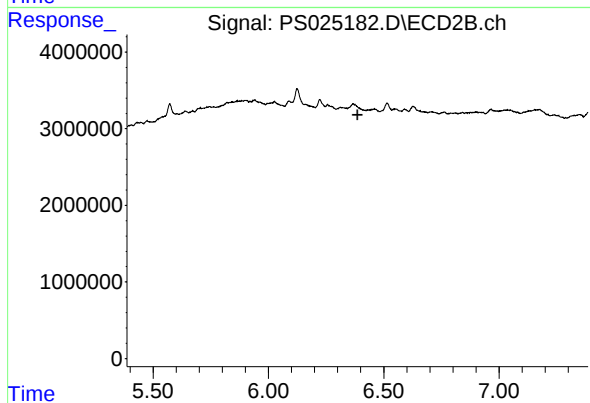

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

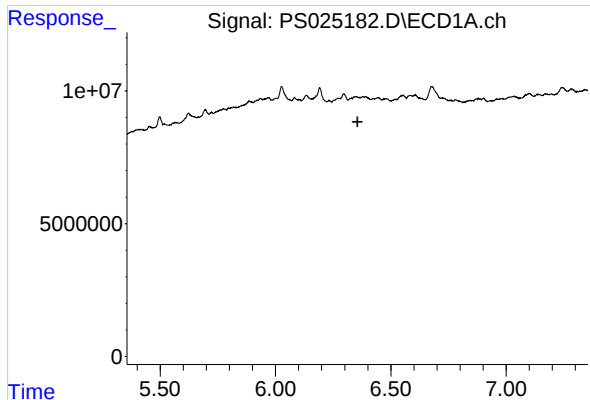

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.355 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

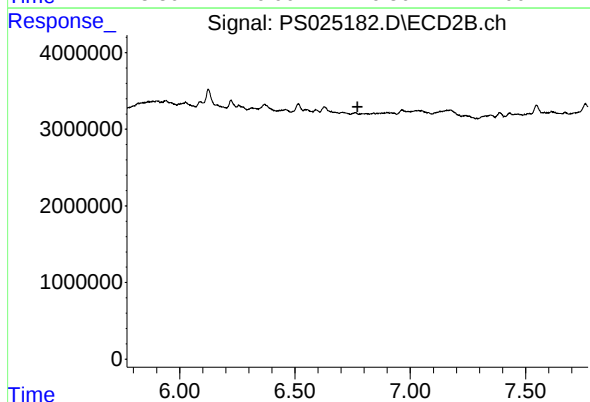


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

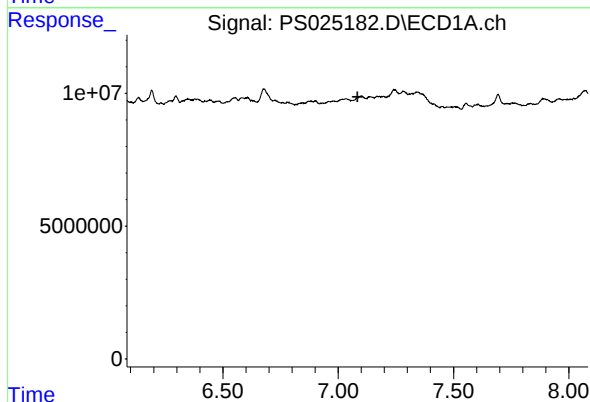


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

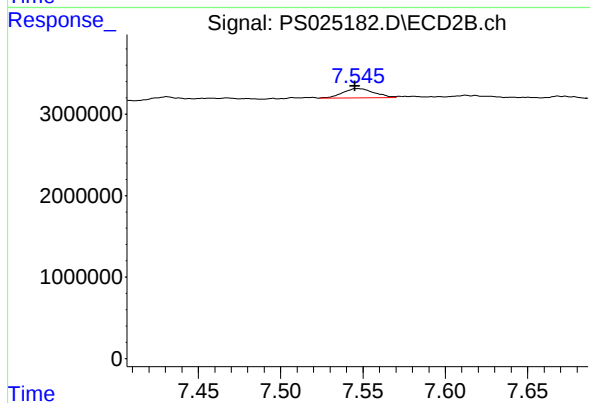

#8 DICHLORPROP


R.T.: 7.546 min
Delta R.T.: 0.000 min
Response: 1483850
Conc: 1.89 ng/ml

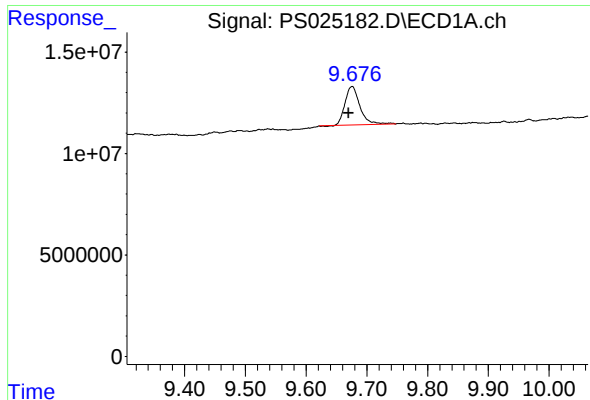

#15 Picloram


R.T.: 9.675 min
Delta R.T.: 0.006 min
Response: 32574505
Conc: 1.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

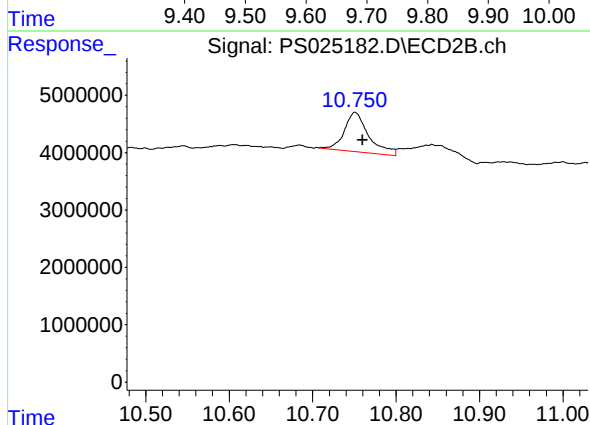


#15 Picloram

R.T.: 10.751 min
Delta R.T.: -0.009 min
Response: 13860177
Conc: 2.12 ng/ml

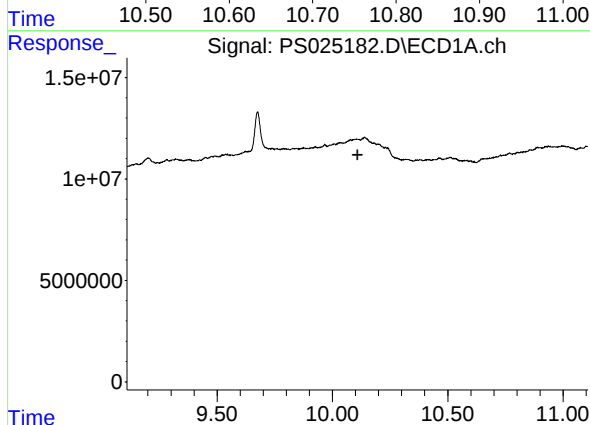

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

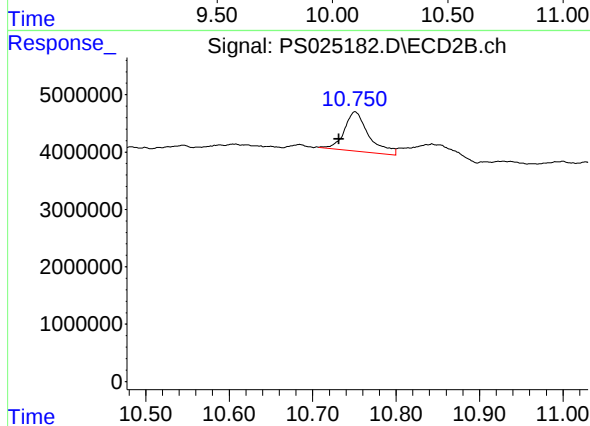

#16 DCPA

R.T.: 10.751 min
Delta R.T.: 0.019 min
Response: 13860177
Conc: 2.56 ng/ml