

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122523\
 Data File : PS025183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 14:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:29:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.353	6.766	1151.7E6	362.4E6	514.626	500.238
Target Compounds							
1) T	Dalapon	2.507	2.562	8580135	3911686	2.975	3.410
3) T	4-Nitroph...	6.195	0.000	10919768	0	7.415	N.D. #
7) T	MCPA	0.000	7.232	0	2623169	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.554	0	1301491	N.D.	1.654
9) T	2,4-D	7.350f	7.764f	74992852	728566	24.690	<MDL #
11) T	2,4,5-TP ...	0.000	8.600	0	389399	N.D.	<MDL
12) T	2,4,5-T	0.000	9.015	0	2451100	N.D.	<MDL
15) T	Picloram	9.681	10.756	27929451	8506648	1.433	1.300
16) T	DCPA	0.000	10.756	0	8506648	N.D.	1.570



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122523\
Data File : PS025183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 14:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:29:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

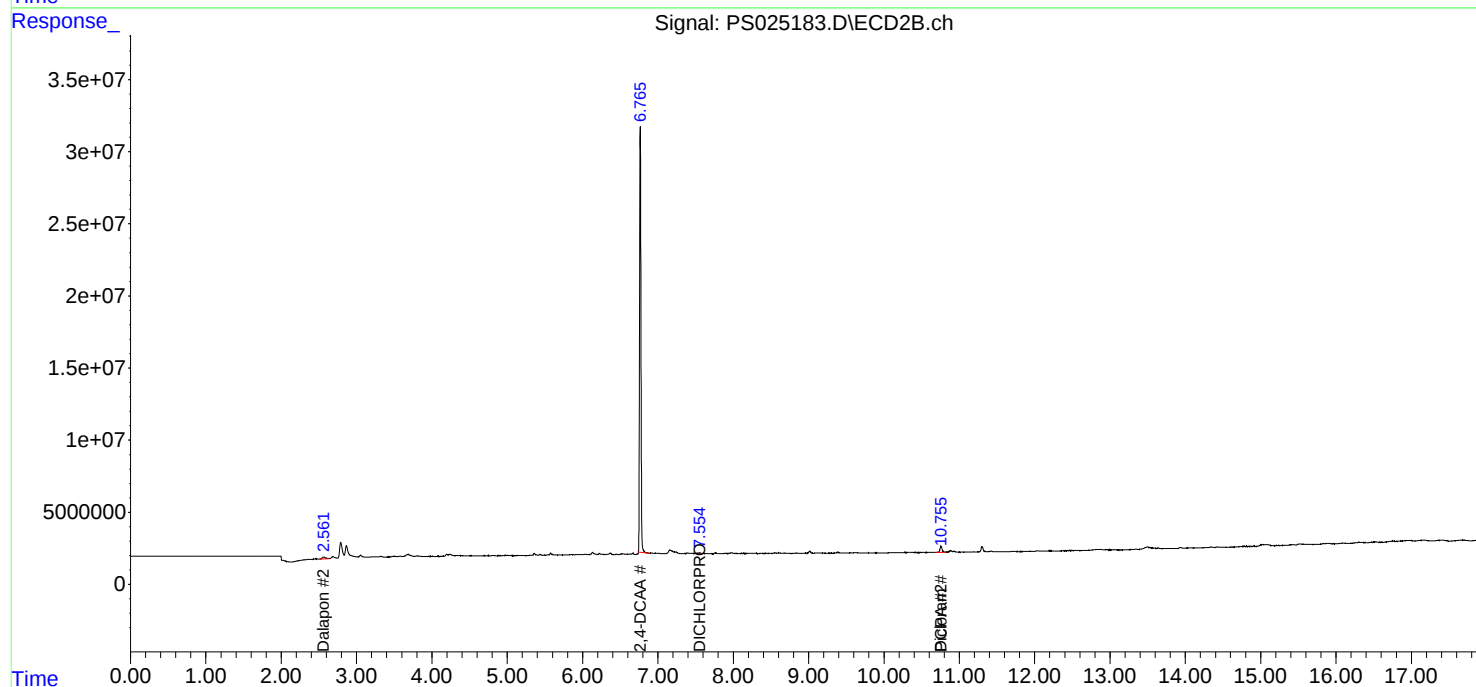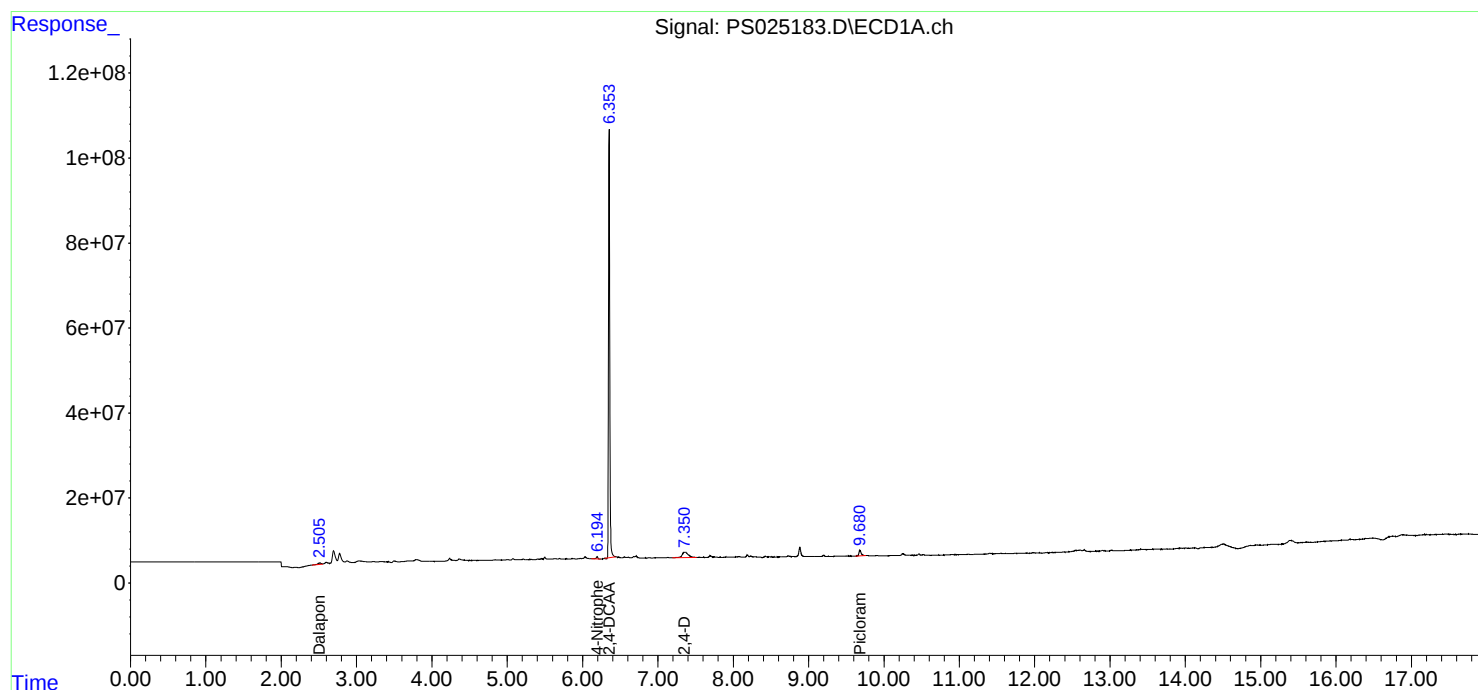


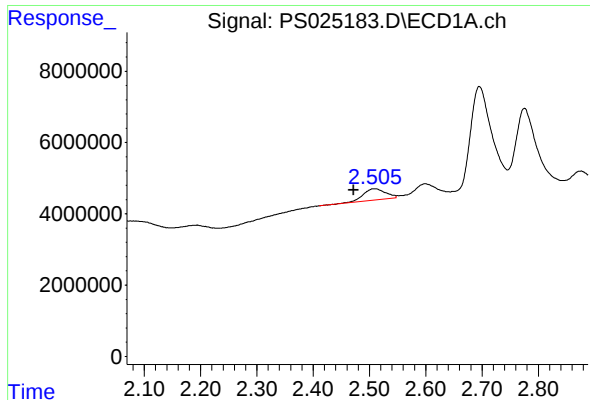

#1 Dalapon


R.T.: 2.507 min
Delta R.T.: 0.035 min
Response: 8580135
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

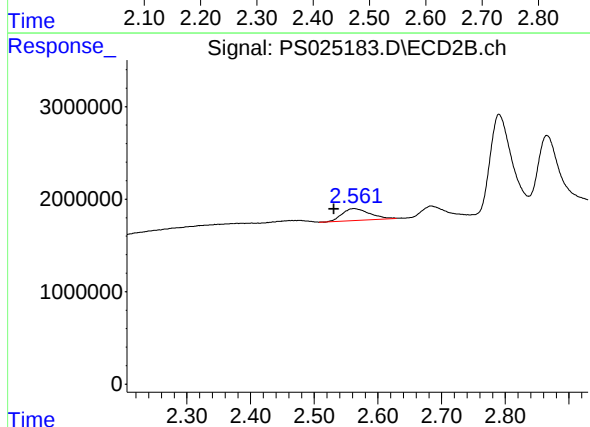


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.031 min
Response: 3911686
Conc: 3.41 ng/ml

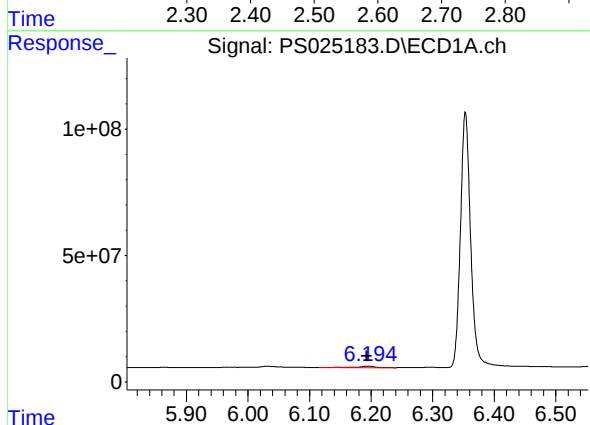


#3 4-Nitrophenol

R.T.: 6.195 min
Delta R.T.: 0.002 min
Response: 10919768
Conc: 7.42 ng/ml

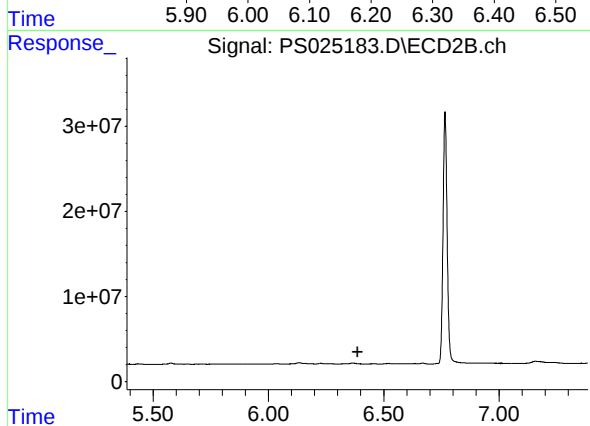

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

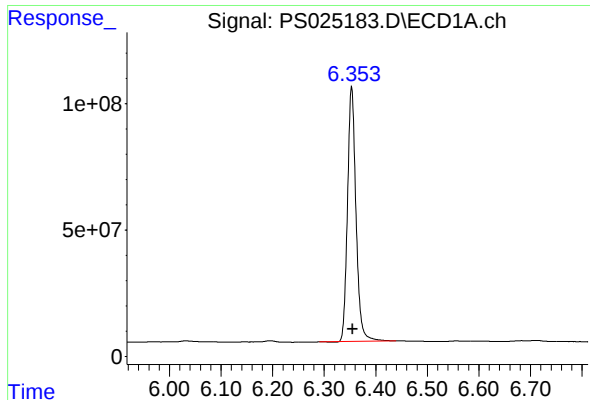

#4 2,4-DCAA


R.T.: 6.353 min
Delta R.T.: -0.002 min
Response: 1151653885
Conc: 514.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

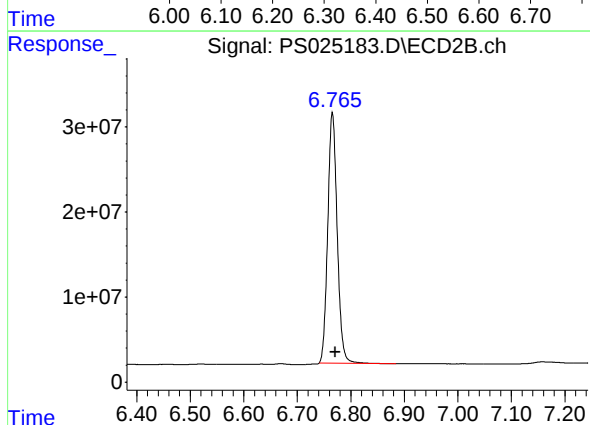


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: -0.006 min
Response: 362449401
Conc: 500.24 ng/ml

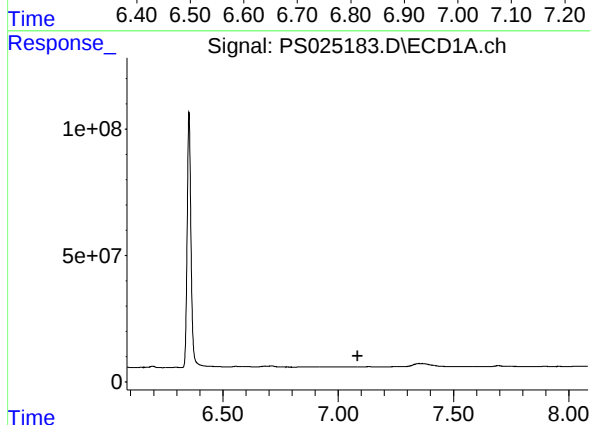


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

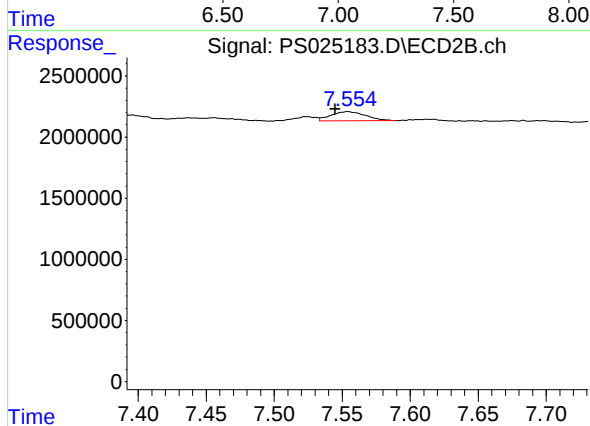

#8 DICHLORPROP


R.T.: 7.554 min
Delta R.T.: 0.009 min
Response: 1301491
Conc: 1.65 ng/ml

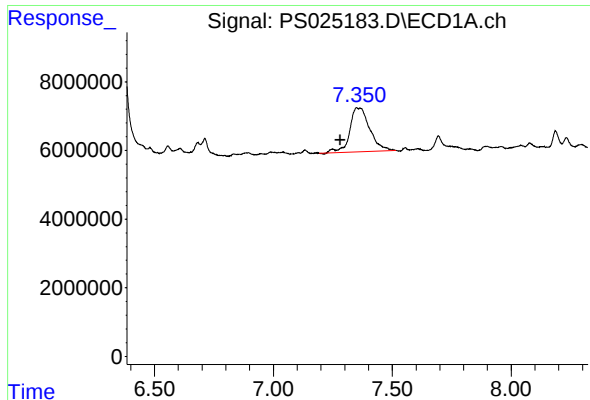

#9 2,4-D


R.T.: 7.350 min
Delta R.T.: 0.069 min
Response: 74992852
Conc: 24.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

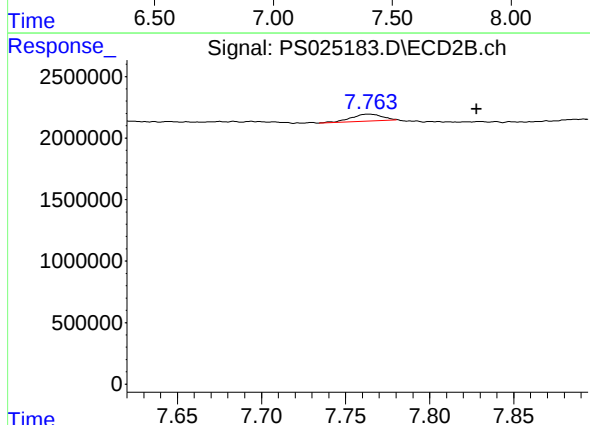


#9 2,4-D

R.T.: 7.764 min
Delta R.T.: -0.064 min
Response: 728566
Conc: N.D.

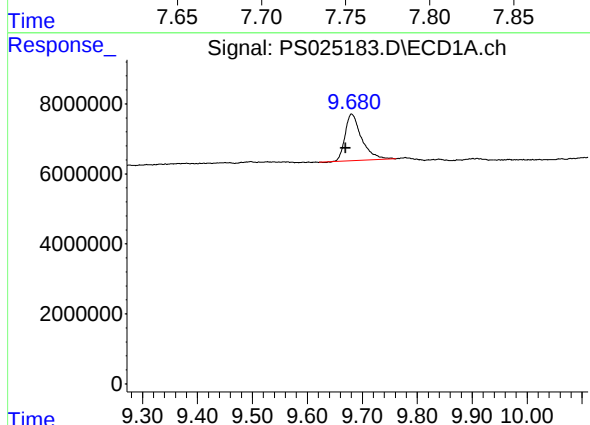


#15 Picloram

R.T.: 9.681 min
Delta R.T.: 0.011 min
Response: 27929451
Conc: 1.43 ng/ml

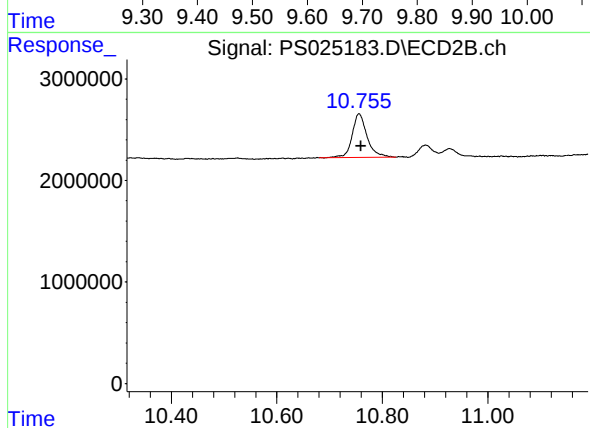

#15 Picloram


R.T.: 10.756 min
Delta R.T.: -0.004 min
Response: 8506648
Conc: 1.30 ng/ml

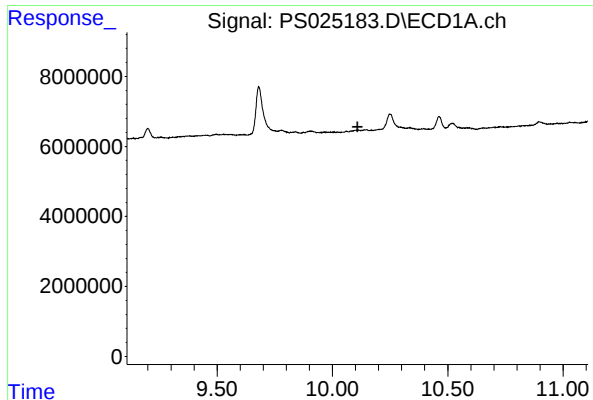

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

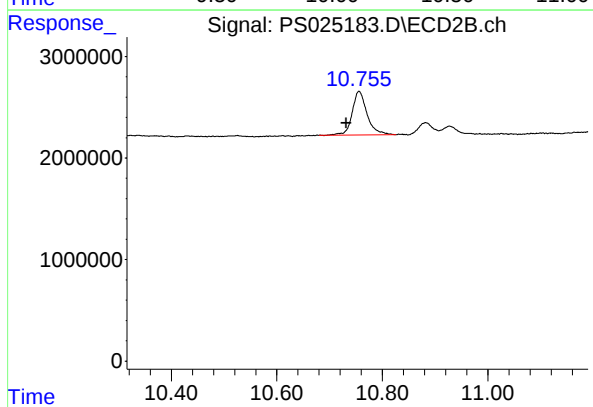

#16 DCPA

R.T.: 10.756 min
Delta R.T.: 0.024 min
Response: 8506648
Conc: 1.57 ng/ml