

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122619\
 Data File : PS008187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2019 05:41
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 06:38:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.383	5.127	772.7E6	367.1E6	382.473	410.005
Target Compounds							
7) T	MCPA	0.000	5.428	0	25110486	N.D.	6.600



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122619\
Data File : PS008187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2019 05:41
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 06:38:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

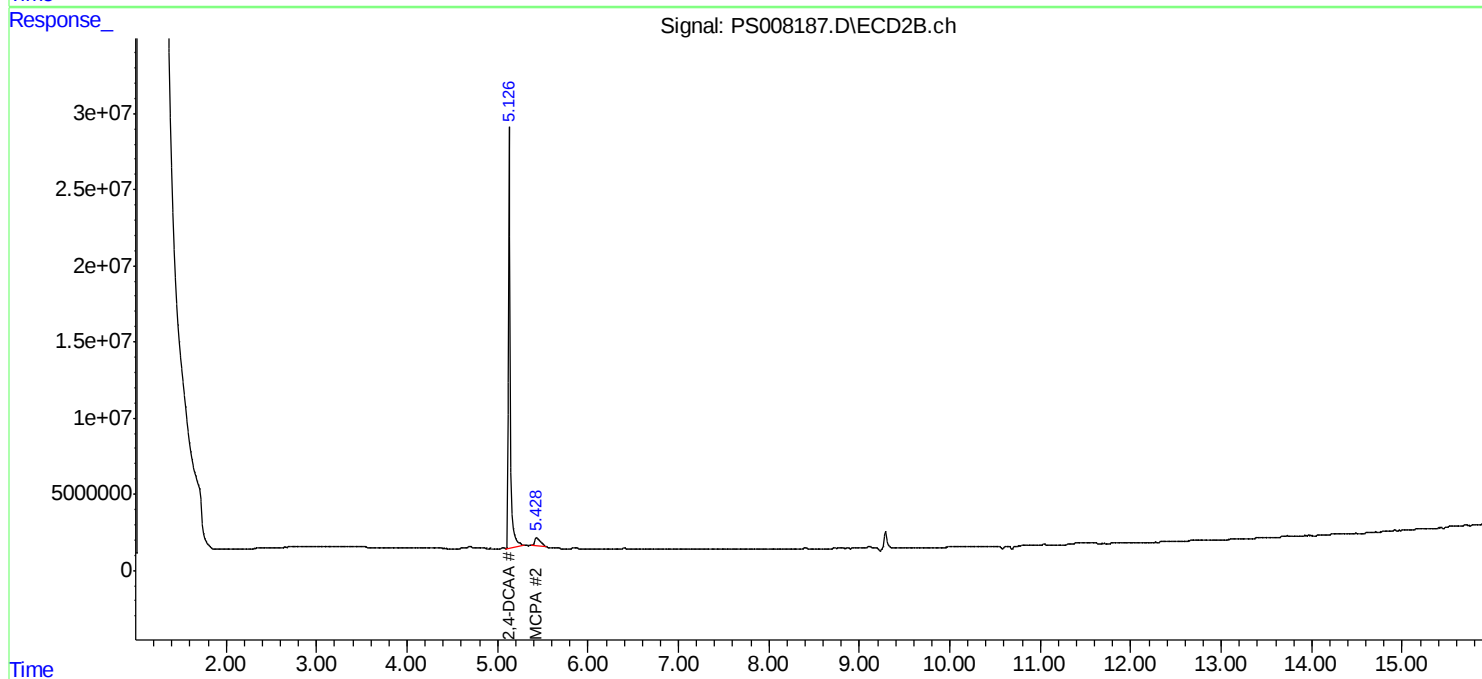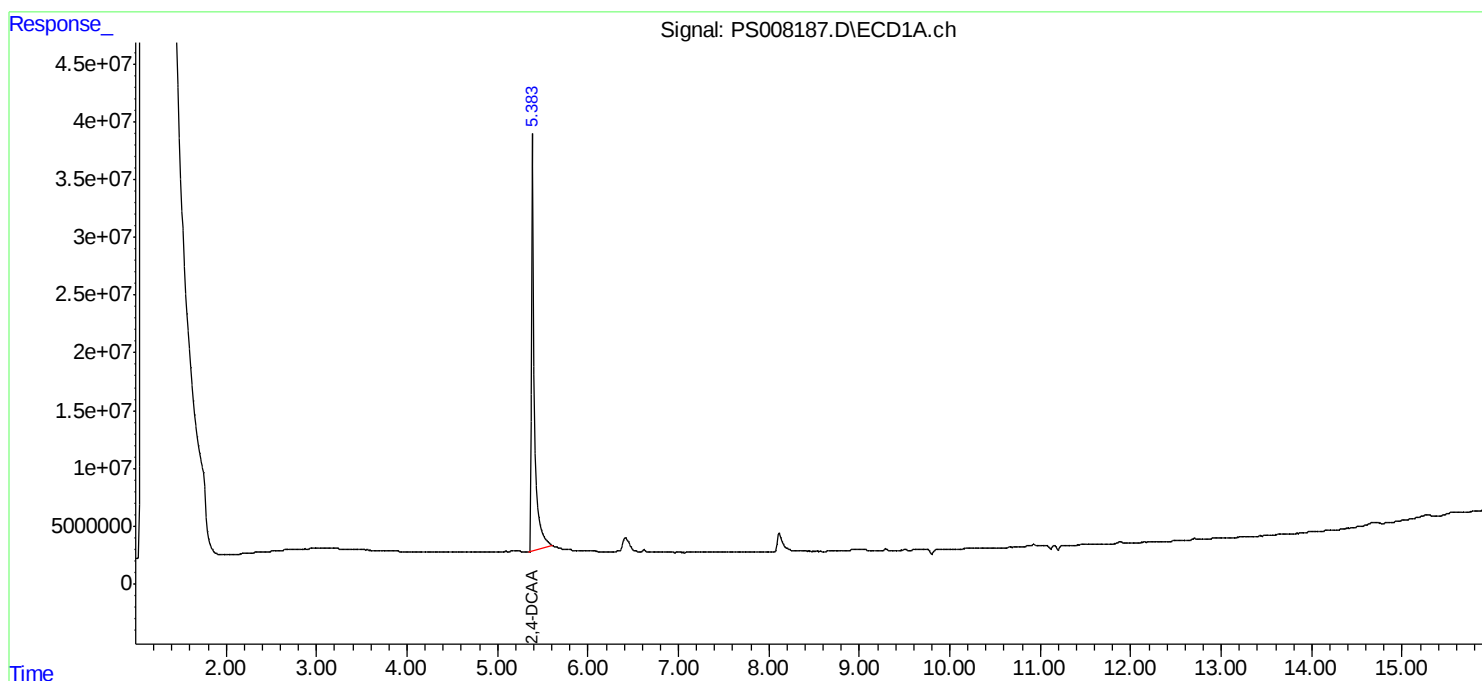


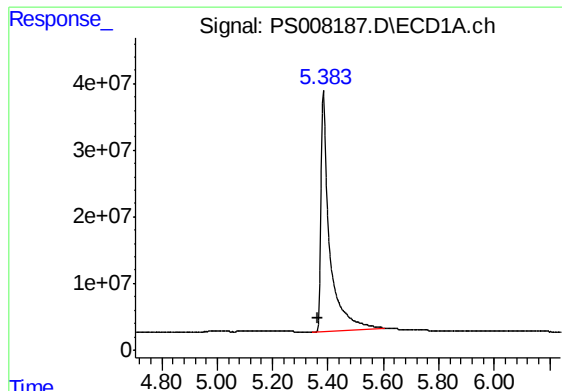

#4 2,4-DCAA


R.T.: 5.383 min
Delta R.T.: 0.022 min
Response: 772726383
Conc: 382.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

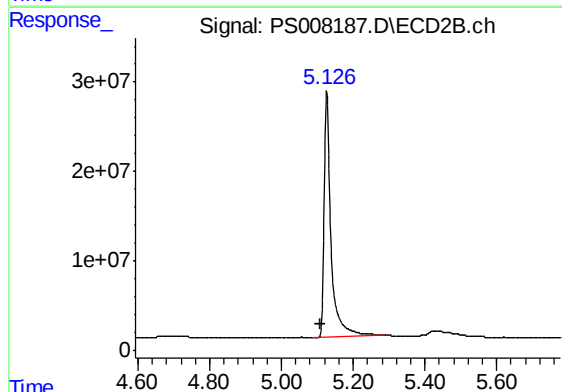


#4 2,4-DCAA

R.T.: 5.127 min
Delta R.T.: 0.018 min
Response: 367110831
Conc: 410.00 ng/ml

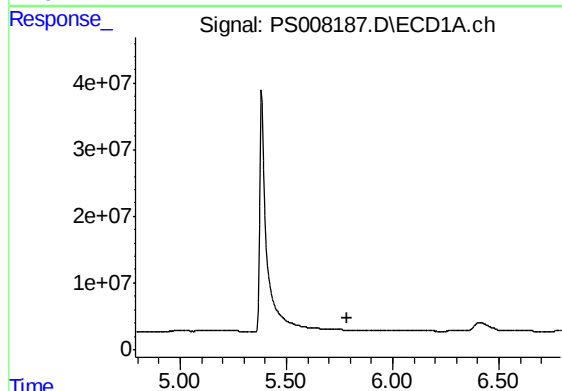

#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.789 min
Response: 0
Conc: N.D.

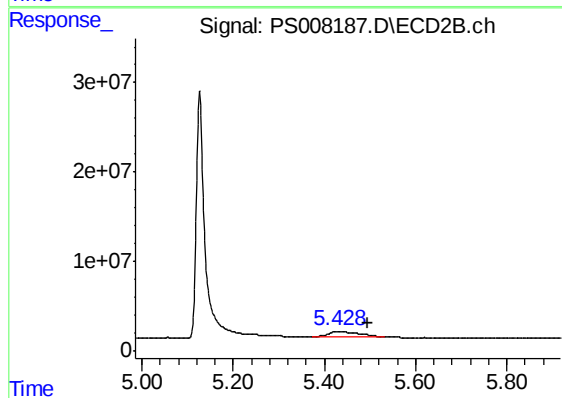

#7 MCPA

R.T.: 5.428 min
Delta R.T.: -0.066 min
Response: 25110486
Conc: 6.60 ug/ml