

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122623\
 Data File : PS025223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2023 14:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 22:23:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.354	6.765	1175.7E6	370.9E6	525.375	511.944
Target Compounds							
1) T	Dalapon	0.000	2.561	0	2843559	N.D.	2.479
2) T	3,5-DICHL...	5.696	0.000	2191826	0	<MDL	N.D. #
3) T	4-Nitroph...	6.195	0.000	11292738	0	7.668	N.D. #
5) T	DICAMBA	0.000	6.964	0	1997164	N.D.	<MDL
6) T	MCP	6.680	6.964f	9012993	1997164	1.316	<MDL #
8) T	DICHLORPROP	0.000	7.551	0	9210117	N.D.	11.708
9) T	2,4-D	7.245	7.764f	16929356	1064602	5.574	1.093 #
11) T	2,4,5-TP ...	0.000	8.600	0	616741	N.D.	<MDL
12) T	2,4,5-T	0.000	9.014	0	5204312	N.D.	1.206
13) T	2,4-DB	0.000	9.463	0	891477	N.D.	1.611
15) T	Picloram	9.683	10.756	66068204	19424308	3.391	2.968
16) T	DCPA	0.000	10.756	0	19424308	N.D.	3.584



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122623\
Data File : PS025223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2023 14:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 22:23:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

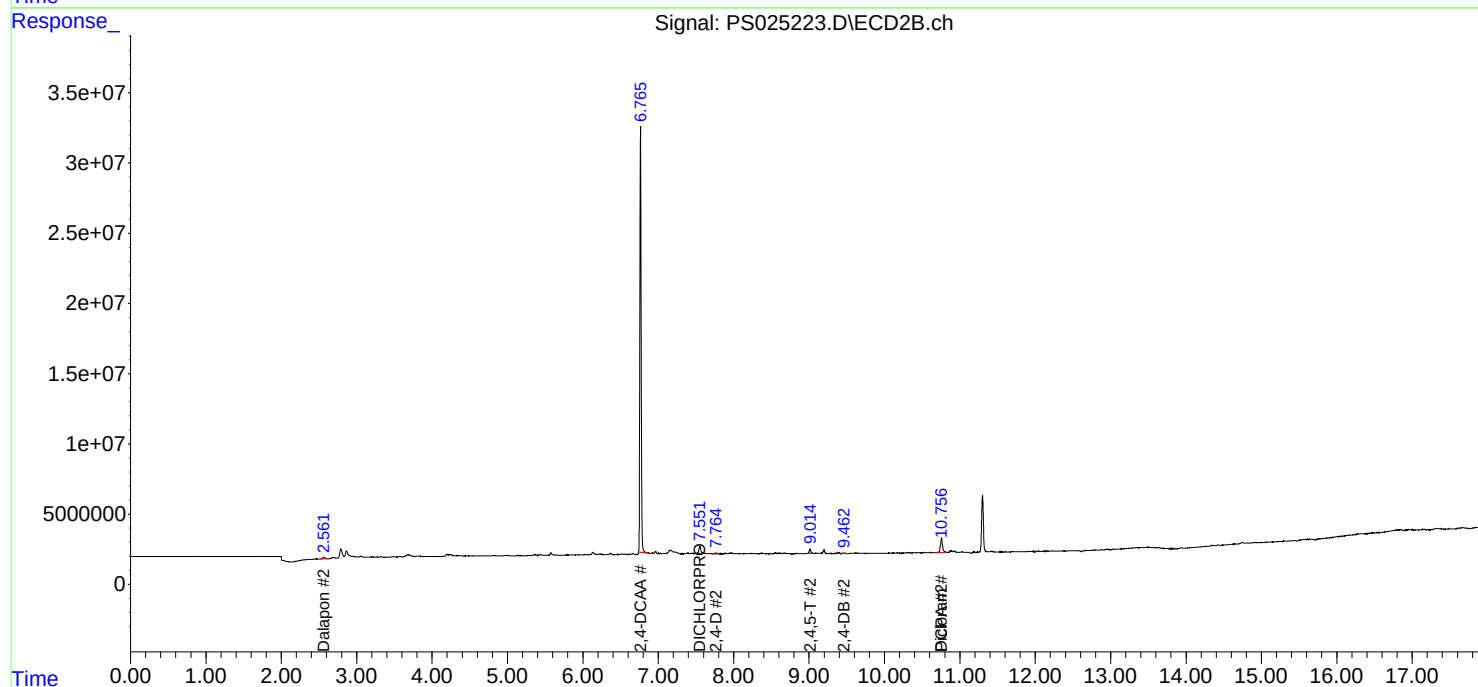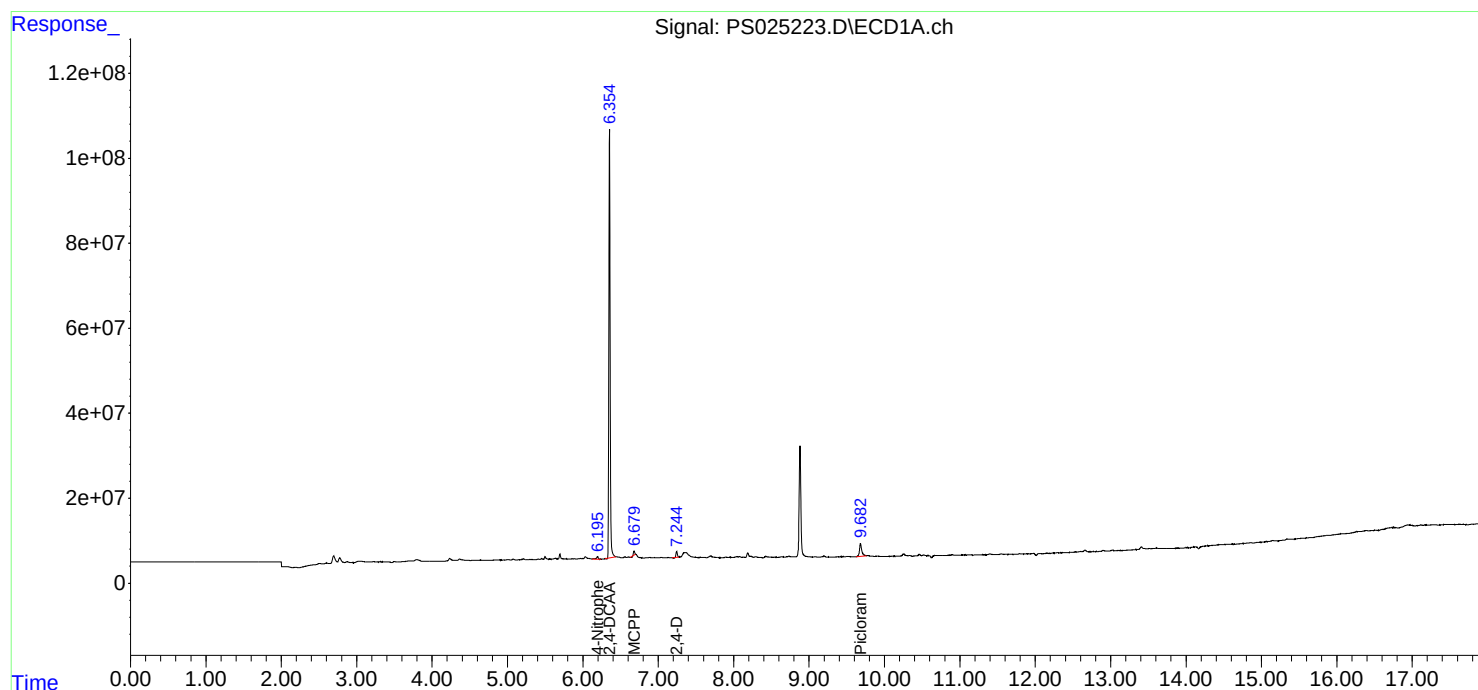


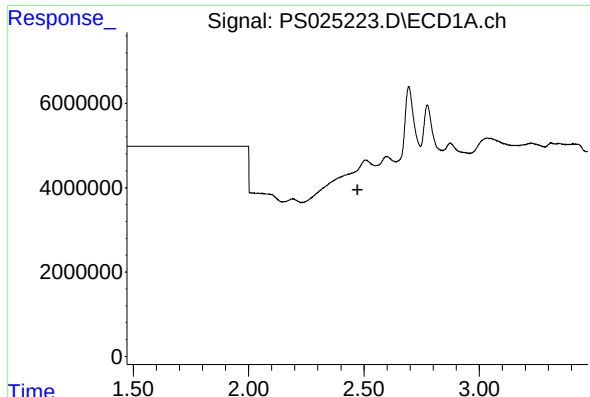

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

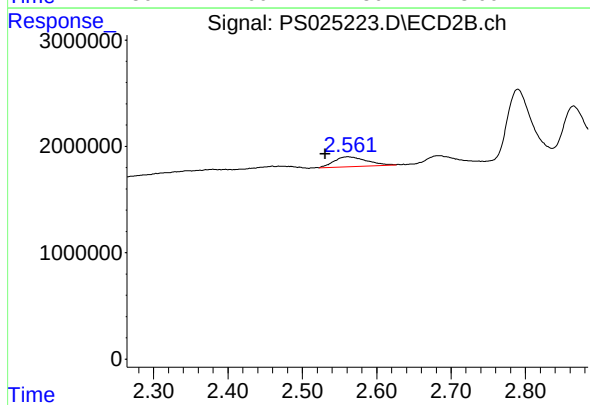


#1 Dalapon

R.T.: 2.561 min
Delta R.T.: 0.030 min
Response: 2843559
Conc: 2.48 ng/ml

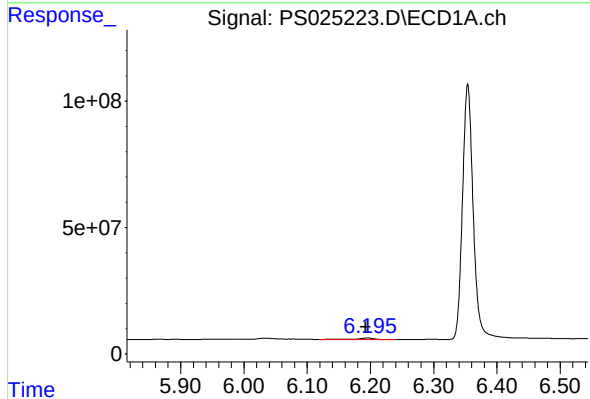


#3 4-Nitrophenol

R.T.: 6.195 min
Delta R.T.: 0.002 min
Response: 11292738
Conc: 7.67 ng/ml

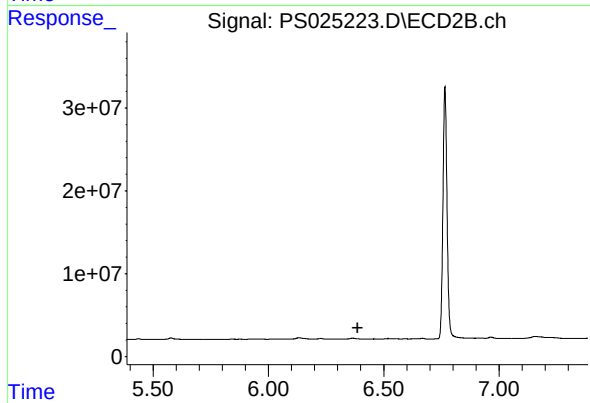

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

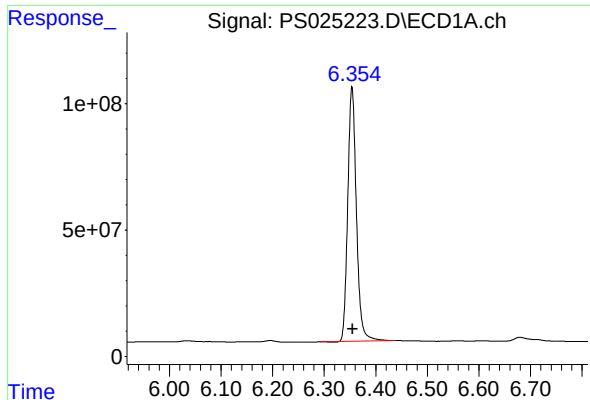

#4 2,4-DCAA


R.T.: 6.354 min
Delta R.T.: -0.001 min
Response: 1175708065
Conc: 525.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

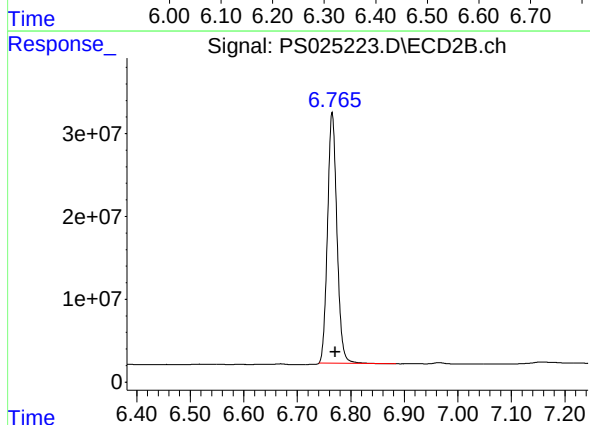


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.006 min
Response: 370931509
Conc: 511.94 ng/ml

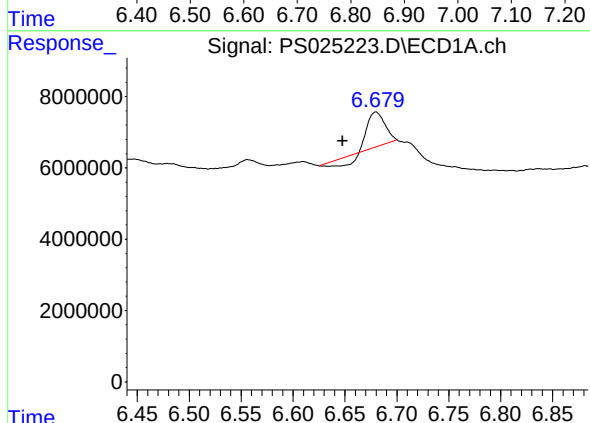


#6 MCPP

R.T.: 6.680 min
Delta R.T.: 0.032 min
Response: 9012993
Conc: 1.32 ug/ml

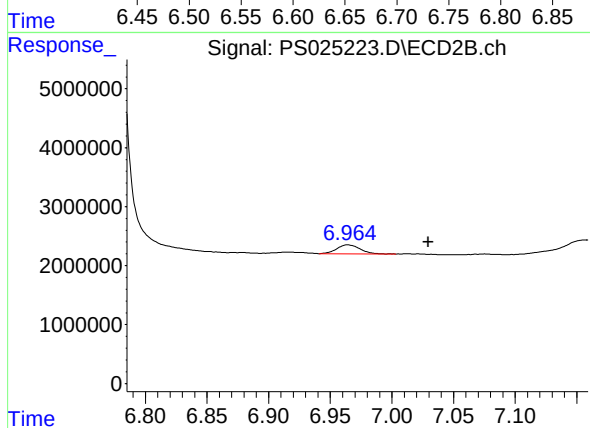

#6 MCPP


R.T.: 6.964 min
Delta R.T.: -0.065 min
Response: 1997164
Conc: N.D.

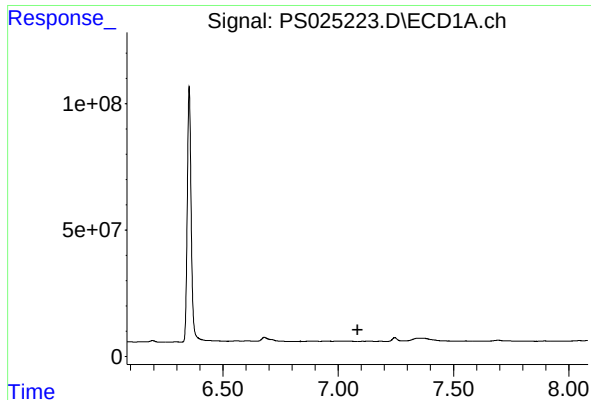

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

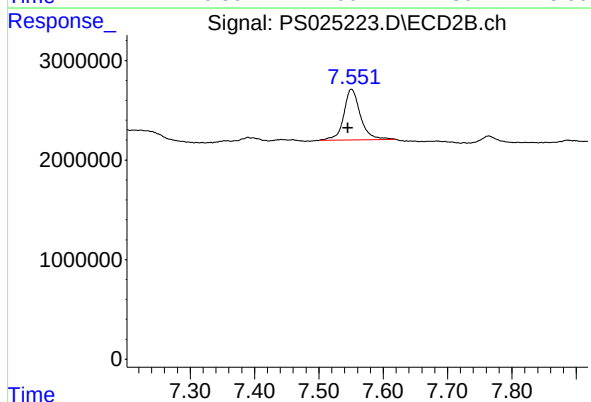


#8 DICHLORPROP

R.T.: 7.551 min
Delta R.T.: 0.006 min
Response: 9210117
Conc: 11.71 ng/ml

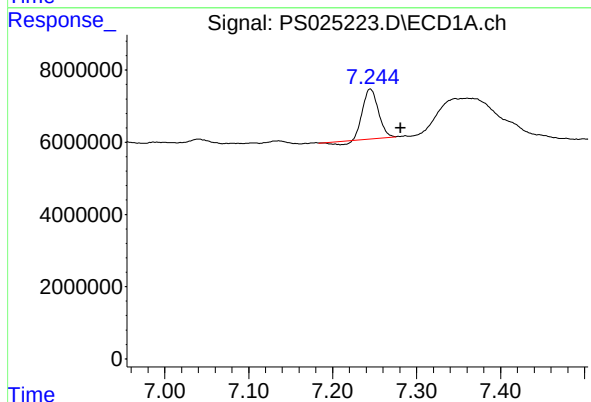


#9 2,4-D

R.T.: 7.245 min
Delta R.T.: -0.036 min
Response: 16929356
Conc: 5.57 ng/ml

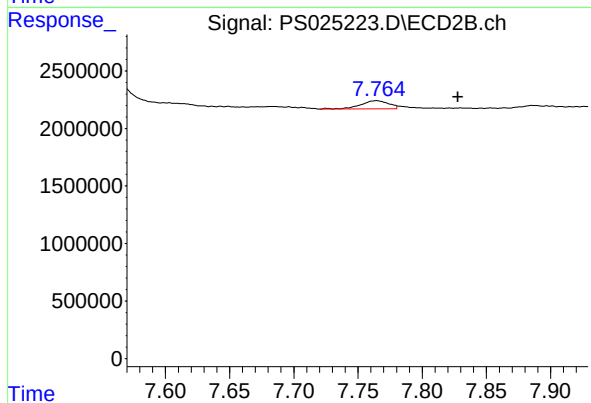

#9 2,4-D


R.T.: 7.764 min
Delta R.T.: -0.063 min
Response: 1064602
Conc: 1.09 ng/ml

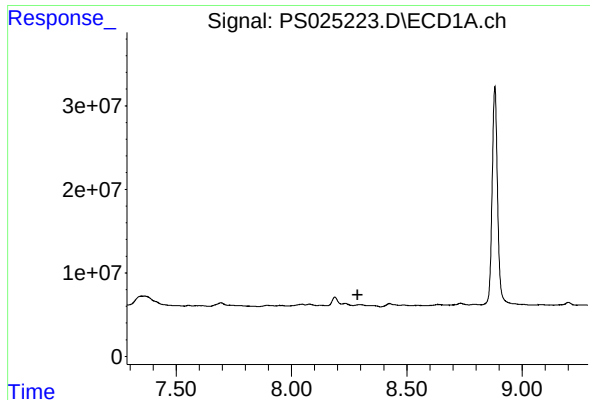

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

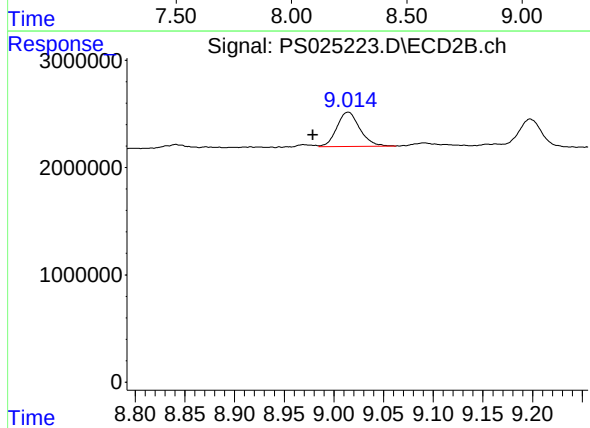


#12 2,4,5-T

R.T.: 9.014 min
Delta R.T.: 0.035 min
Response: 5204312
Conc: 1.21 ng/ml

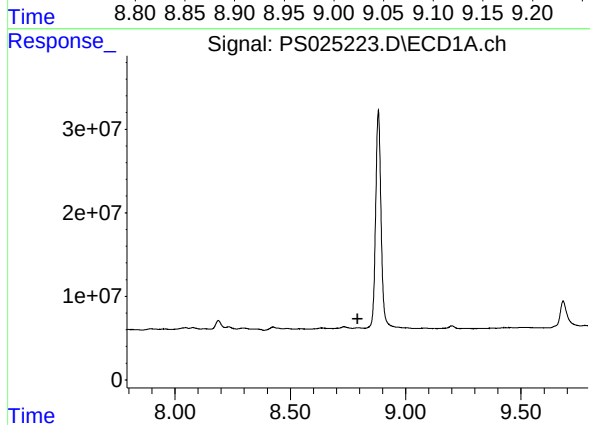


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

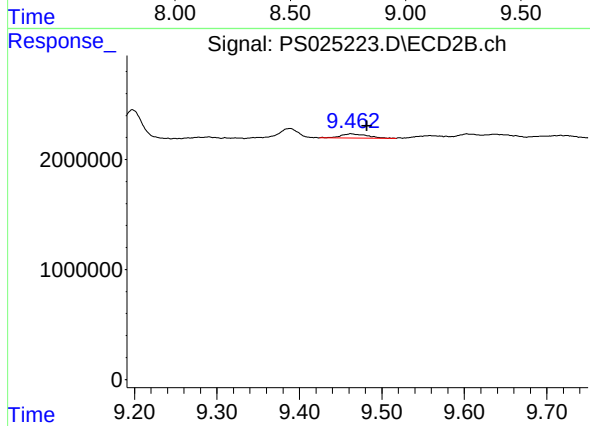

#13 2,4-DB


R.T.: 9.463 min
Delta R.T.: -0.019 min
Response: 891477
Conc: 1.61 ng/ml

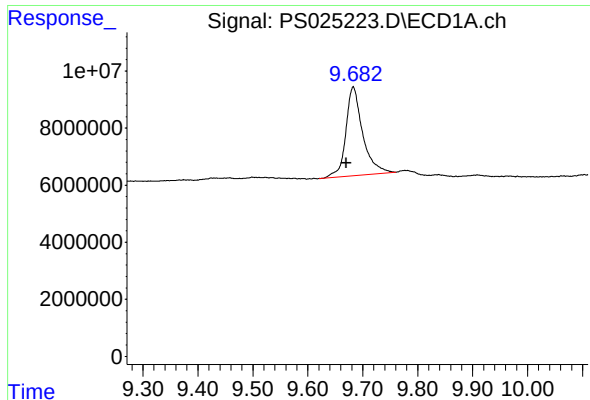

#15 Picloram


R.T.: 9.683 min
Delta R.T.: 0.013 min
Response: 66068204
Conc: 3.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

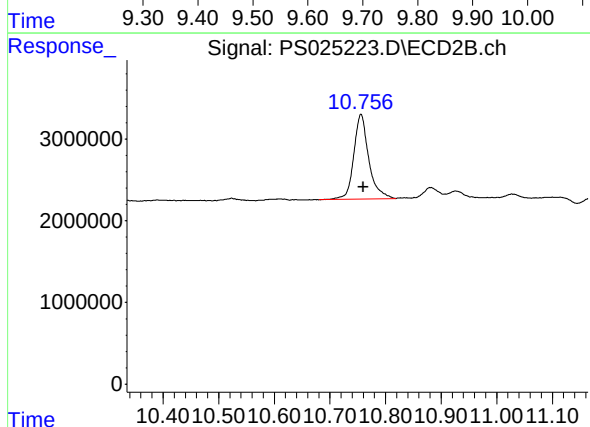


#15 Picloram

R.T.: 10.756 min
Delta R.T.: -0.004 min
Response: 19424308
Conc: 2.97 ng/ml

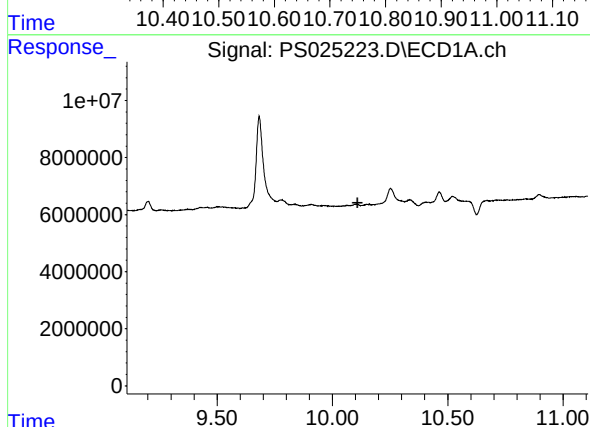

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

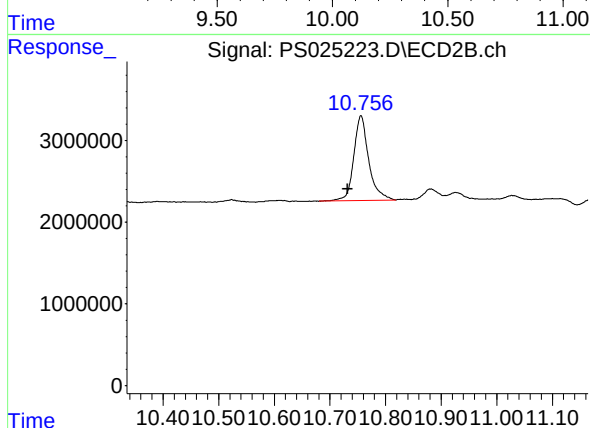

#16 DCPA

R.T.: 10.756 min
Delta R.T.: 0.024 min
Response: 19424308
Conc: 3.58 ng/ml