

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122624\
 Data File : PS028818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 10:19
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 02:40:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.588f	0.000	488457	0	<MDL	N.D.	#
2) T	3,5-DICHL...	6.372	0.000	179572	0	<MDL	N.D.	#
3) T	4-Nitroph...	6.991	0.000	1458320	0	<MDL	N.D.	#
5) T	DICAMBA	7.370f	0.000	351706	0	<MDL	N.D.	#
6) T	MCP	7.528f	0.000	854717	0	<MDL	N.D.	#
7) T	MCPA	7.704	8.226	273978	3943634	<MDL	<MDL	#
8) T	DICHLORPROP	8.102	8.657f	803655	2938581	<MDL	2.130	#
11) T	2,4,5-TP ...	9.167f	0.000	500356	0	<MDL	N.D.	#
12) T	2,4,5-T	9.545f	0.000	380163	0	<MDL	N.D.	#
13) T	2,4-DB	10.074	0.000	2328069	0	<MDL	N.D.	#
14) T	DINOSEB	11.298	0.000	260839	0	<MDL	N.D.	#
15) T	Picloram	11.092	12.292	50253823	23874301	1.874	1.860	
16) T	DCPA	11.545	12.292f	2384043	23874301	<MDL	2.222	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122624\
Data File : PS028818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 10:19
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 02:40:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

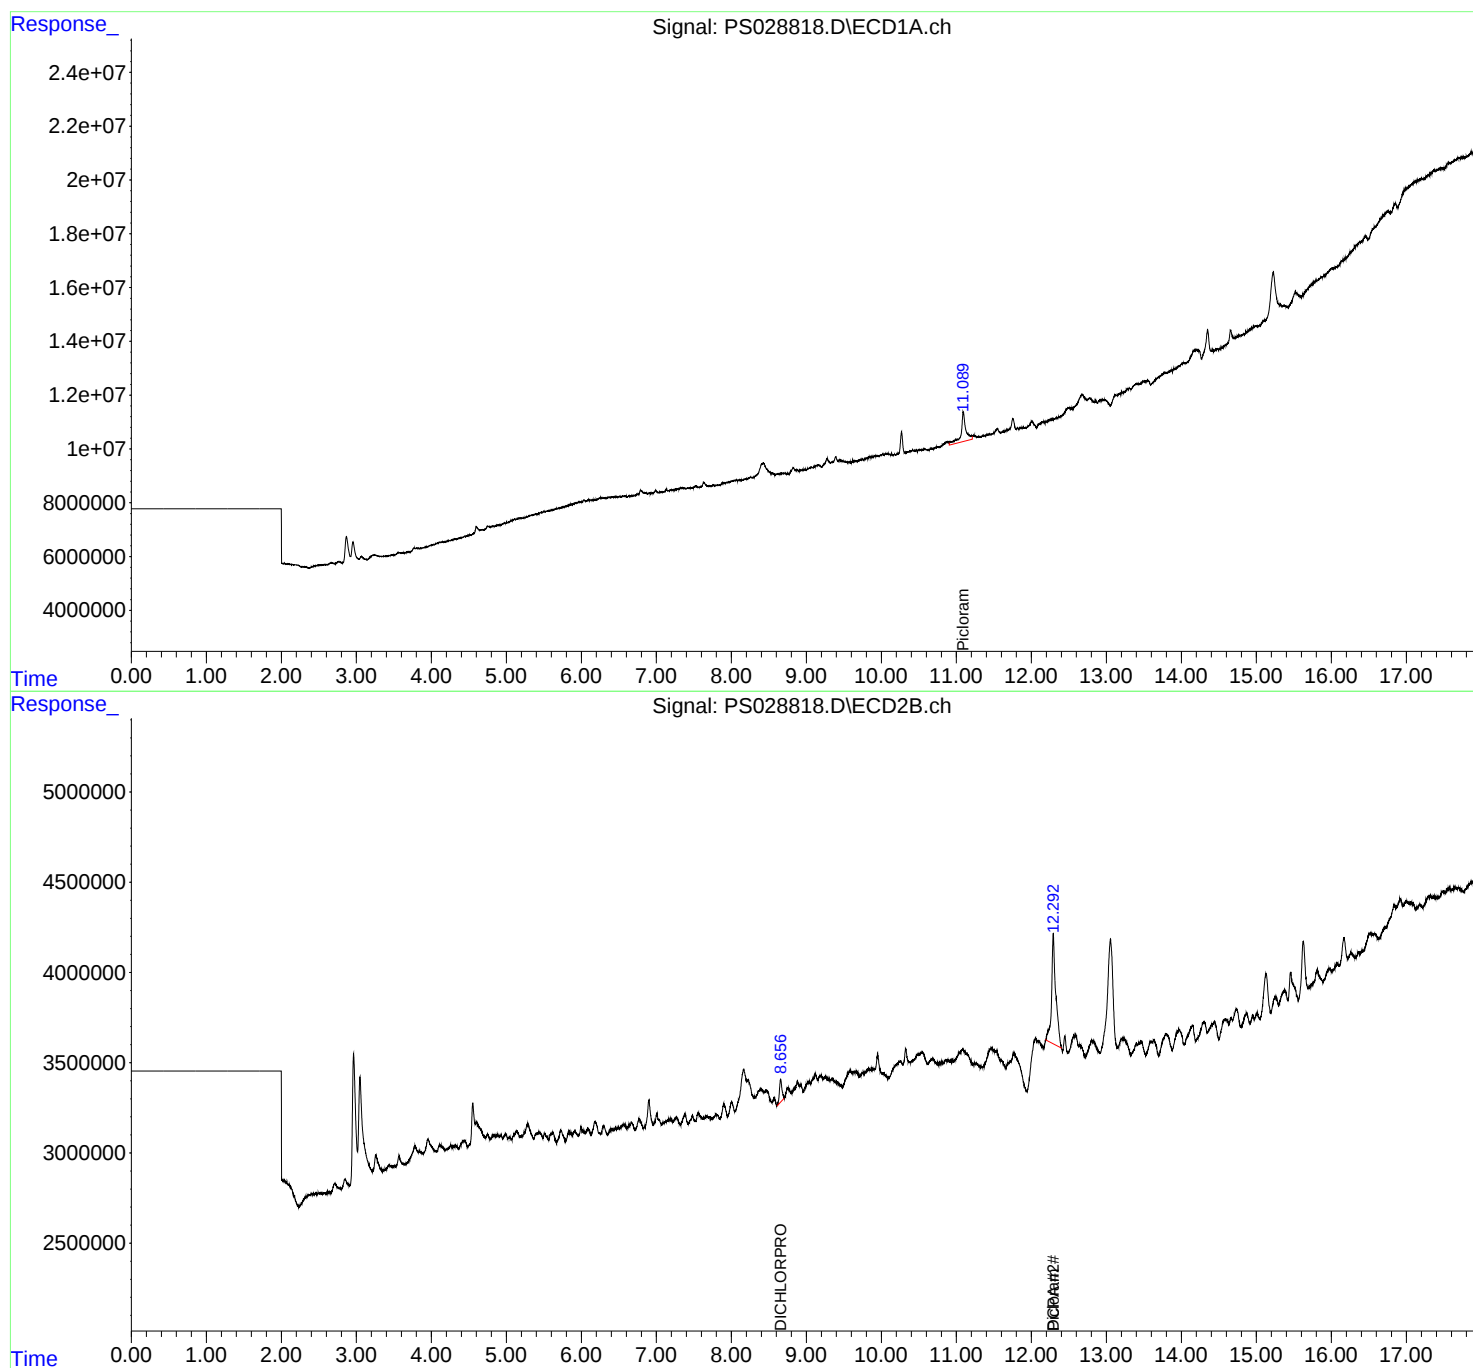


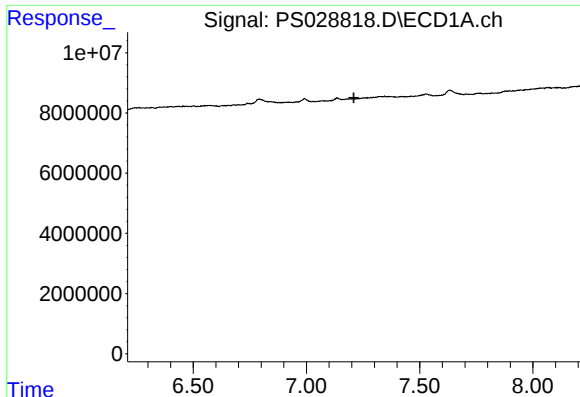

#4 2,4-DCAA


R.T.: 7.258 min
Delta R.T.: 0.048 min
Response: -7430
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

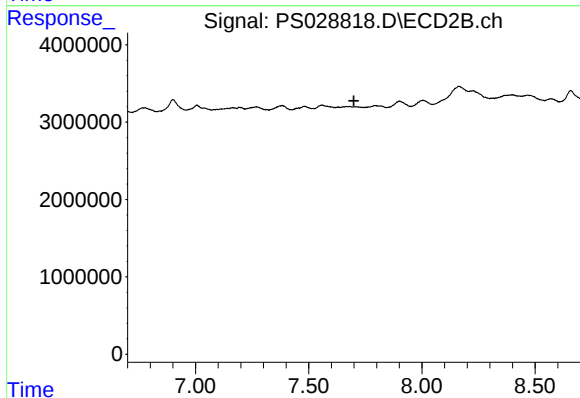


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.699 min
Response: 0
Conc: N.D.

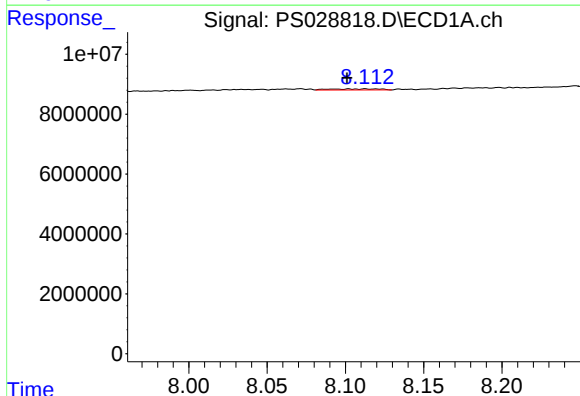


#8 DICHLORPROP

R.T.: 8.102 min
Delta R.T.: 0.001 min
Response: 803655
Conc: N.D.

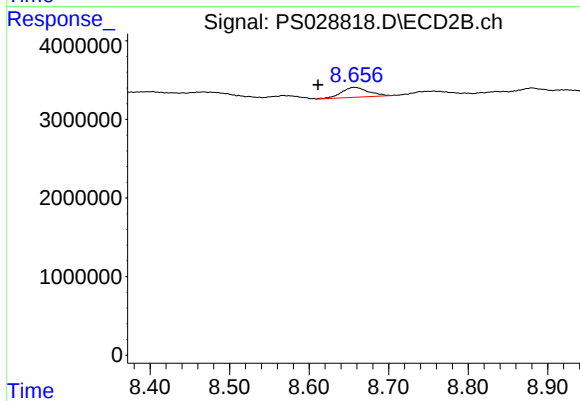

#8 DICHLORPROP


R.T.: 8.657 min
Delta R.T.: 0.046 min
Response: 2938581
Conc: 2.13 ng/ml

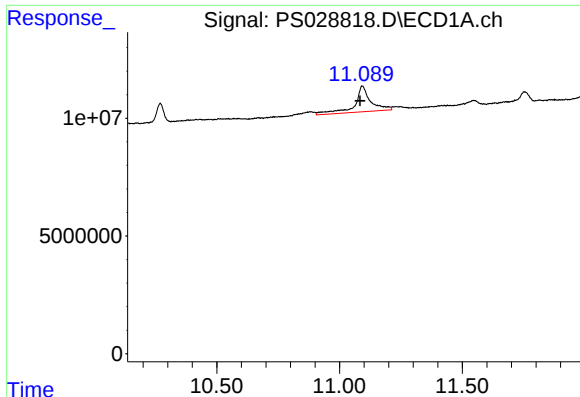

#15 Picloram


R.T.: 11.092 min
Delta R.T.: 0.008 min
Response: 50253823
Conc: 1.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

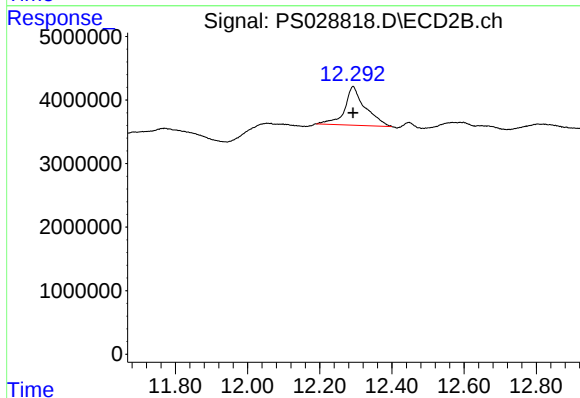


#15 Picloram

R.T.: 12.292 min
Delta R.T.: 0.000 min
Response: 23874301
Conc: 1.86 ng/ml

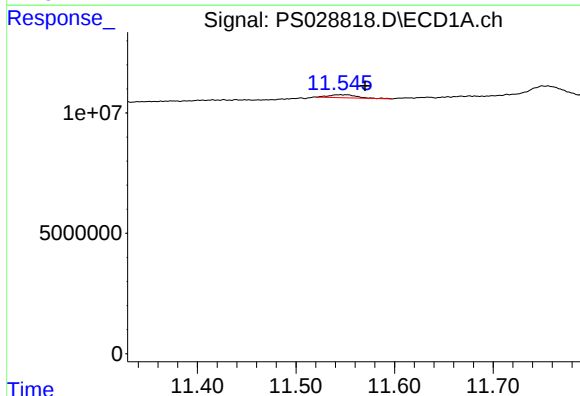

#16 DCPA

R.T.: 11.545 min
Delta R.T.: -0.025 min
Response: 2384043
Conc: N.D.

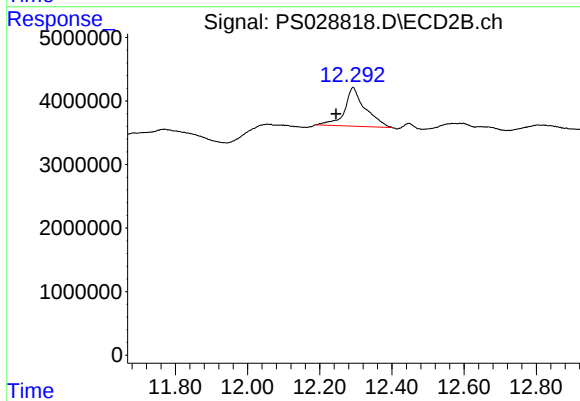

#16 DCPA

R.T.: 12.292 min
Delta R.T.: 0.047 min
Response: 23874301
Conc: 2.22 ng/ml