

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122624\
 Data File : PS028819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 10:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 02:41:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.206	7.695	1280.8E6	567.1E6	566.218	503.857
Target Compounds							
1) T	Dalapon	2.574f	2.718f	8401792	3655707	2.983	1.857 #
2) T	3,5-DICHL...	6.395	0.000	356180	0	<MDL	N.D. #
3) T	4-Nitroph...	7.004	0.000	3760164	0	2.503	N.D. #
5) T	DICAMBA	7.393	7.897	527325	3070845	<MDL	<MDL #
7) T	MCPA	7.746	0.000	318867	0	<MDL	N.D. #
8) T	DICHLORPROP	8.069f	8.658f	3633364	2419723	1.369	1.754 #
10) T	Pentachlo...	8.625	0.000	2463049	0	<MDL	N.D. #
12) T	2,4,5-T	9.503	0.000	1365612	0	<MDL	N.D. #
13) T	2,4-DB	10.081	0.000	1134561	0	<MDL	N.D. #
14) T	DINOSEB	11.265	0.000	2343493	0	<MDL	N.D. #
15) T	Picloram	11.097	12.296	34815003	13428314	1.298	1.046
16) T	DCPA	11.554	0.000	1972294	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122624\
Data File : PS028819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 10:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 02:41:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

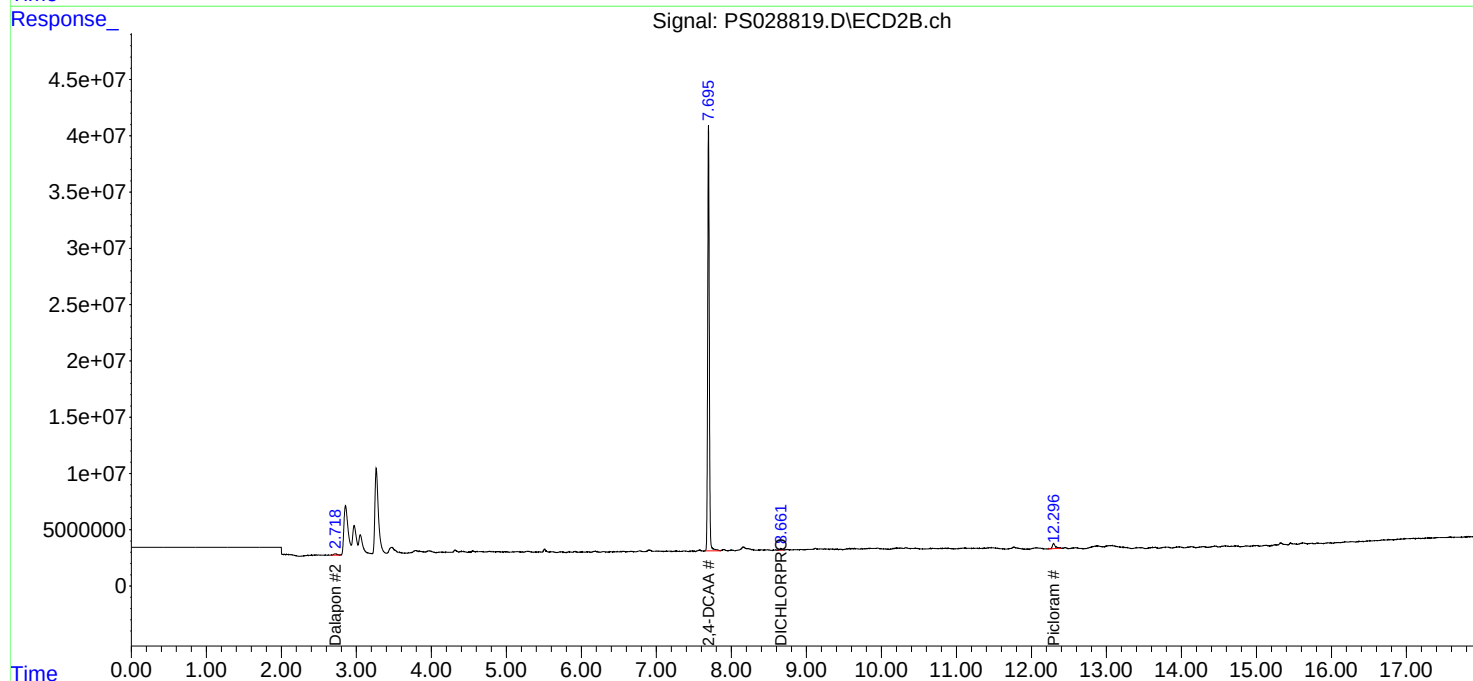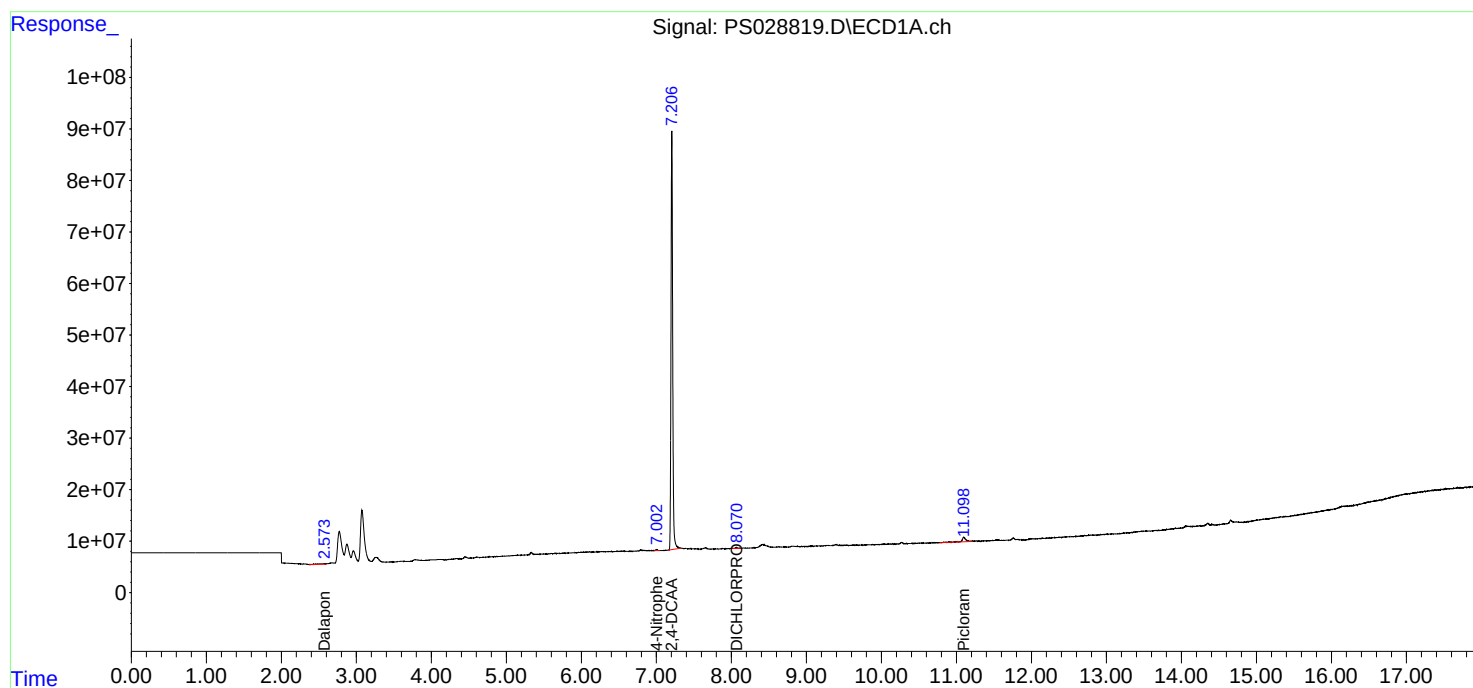


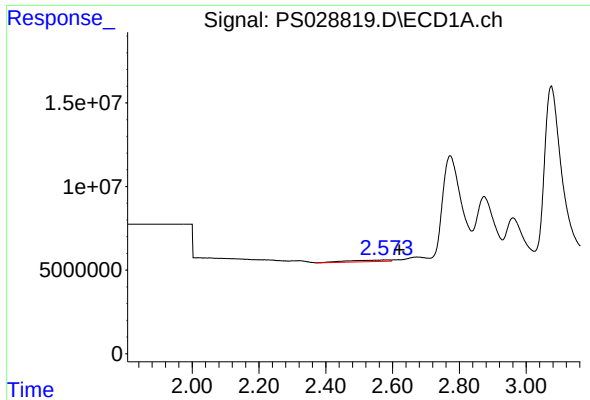

#1 Dalapon


R.T.: 2.574 min
Delta R.T.: -0.046 min
Response: 8401792
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

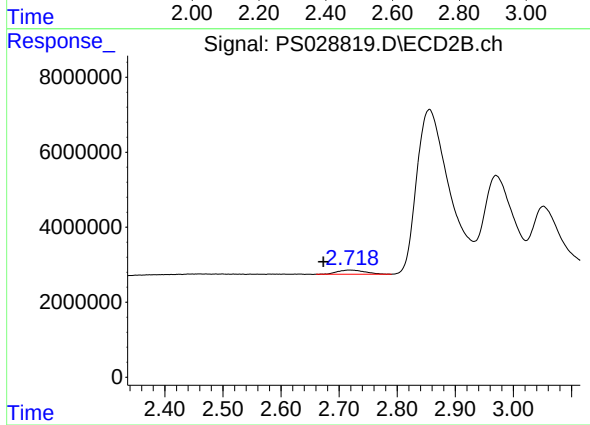


#1 Dalapon

R.T.: 2.718 min
Delta R.T.: 0.045 min
Response: 3655707
Conc: 1.86 ng/ml

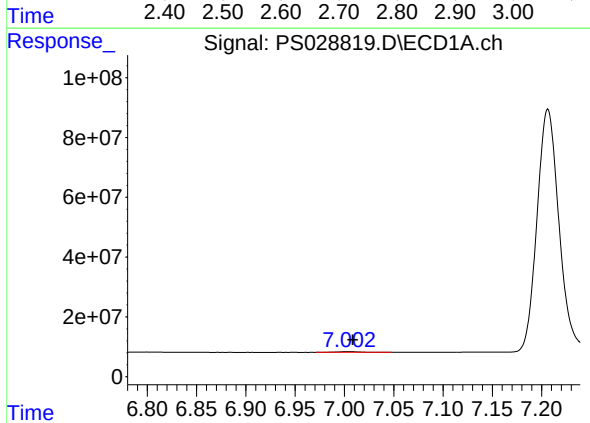


#3 4-Nitrophenol

R.T.: 7.004 min
Delta R.T.: -0.005 min
Response: 3760164
Conc: 2.50 ng/ml

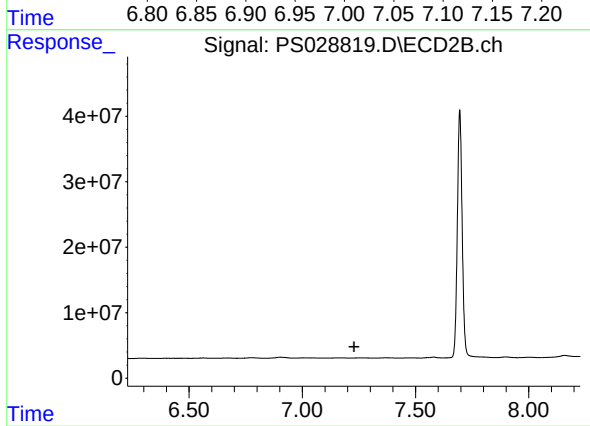

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

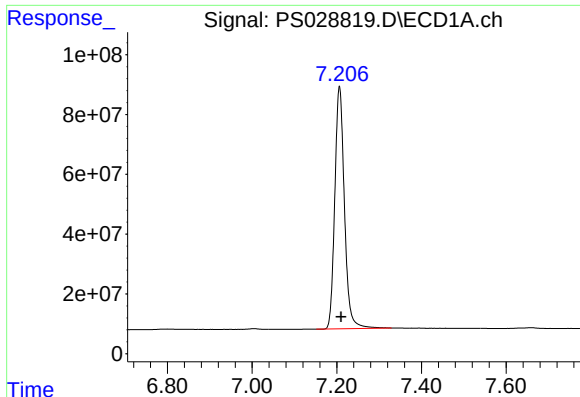

#4 2,4-DCAA


R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 1280799268
Conc: 566.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

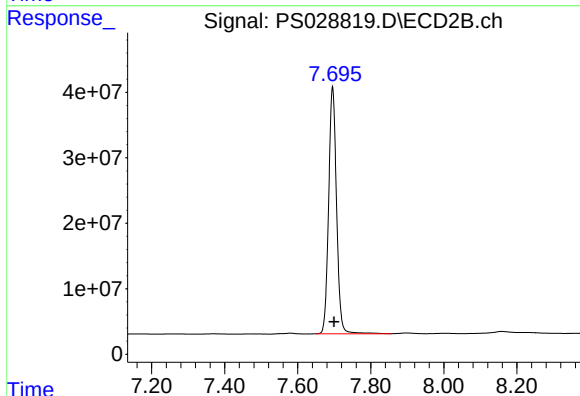


#4 2,4-DCAA

R.T.: 7.695 min
Delta R.T.: -0.004 min
Response: 567110426
Conc: 503.86 ng/ml

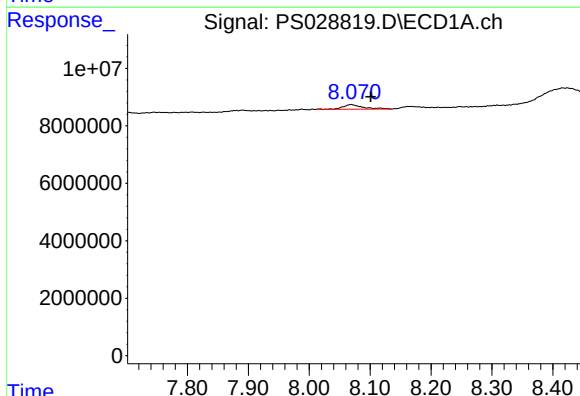


#8 DICHLORPROP

R.T.: 8.069 min
Delta R.T.: -0.032 min
Response: 3633364
Conc: 1.37 ng/ml

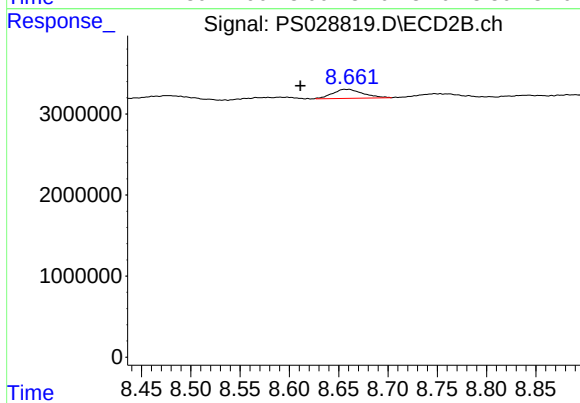

#8 DICHLORPROP


R.T.: 8.658 min
Delta R.T.: 0.047 min
Response: 2419723
Conc: 1.75 ng/ml

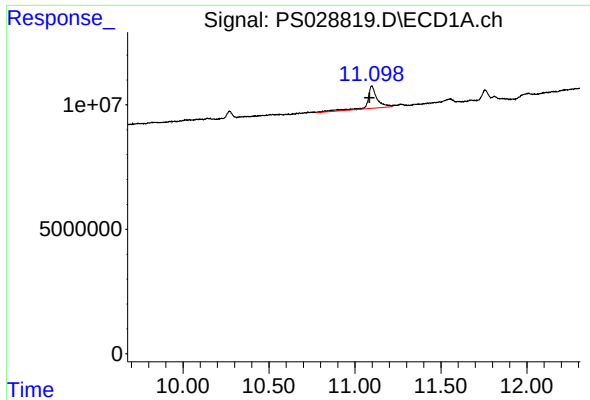

#15 Picloram

R.T.: 11.097 min
Delta R.T.: 0.013 min
Response: 34815003
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

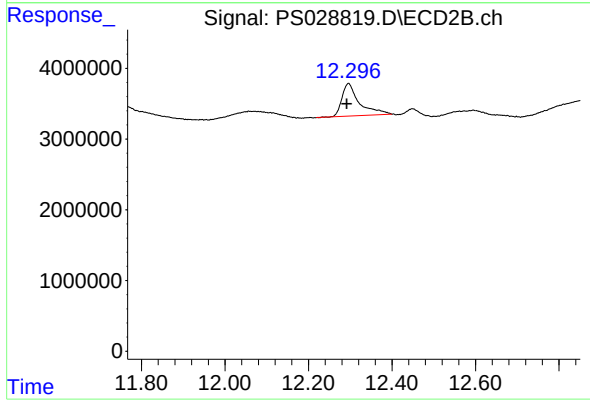

#15 Picloram

R.T.: 12.296 min
Delta R.T.: 0.004 min
Response: 13428314
Conc: 1.05 ng/ml