

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122719\
 Data File : PS008214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2019 18:19
 Operator : SM\AJ
 Sample : PB125754BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125754BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 04:27:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.365	5.110	704.2E6	360.7E6	348.532	402.799
Target Compounds							
1) T	Dalapon	1.939	1.656	113.6E6	100.1E6	47.335	98.158 #
2) T	3,5-DICHL...	0.000	4.448	0	56755632	N.D.	48.742
5) T	DICAMBA	5.448	5.209	93028749	11512405	12.794	3.379 #
7) T	MCPA	5.815	5.472	56402734	28979335	7.375	7.617
8) T	DICHLORPROP	0.000	5.774	0	22449950	N.D.	26.226
9) T	2,4-D	6.393	5.998	83418302	7377065	50.834	7.266 #
10) T	Pentachlo...	0.000	6.384	0	7039694	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.694	0	112.8E6	N.D.	22.567
14) T	DINOSEB	0.000	7.872	0	5849734	N.D.	1.562



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122719\
Data File : PS008214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2019 18:19
Operator : SM\AJ
Sample : PB125754BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB125754BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 04:27:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

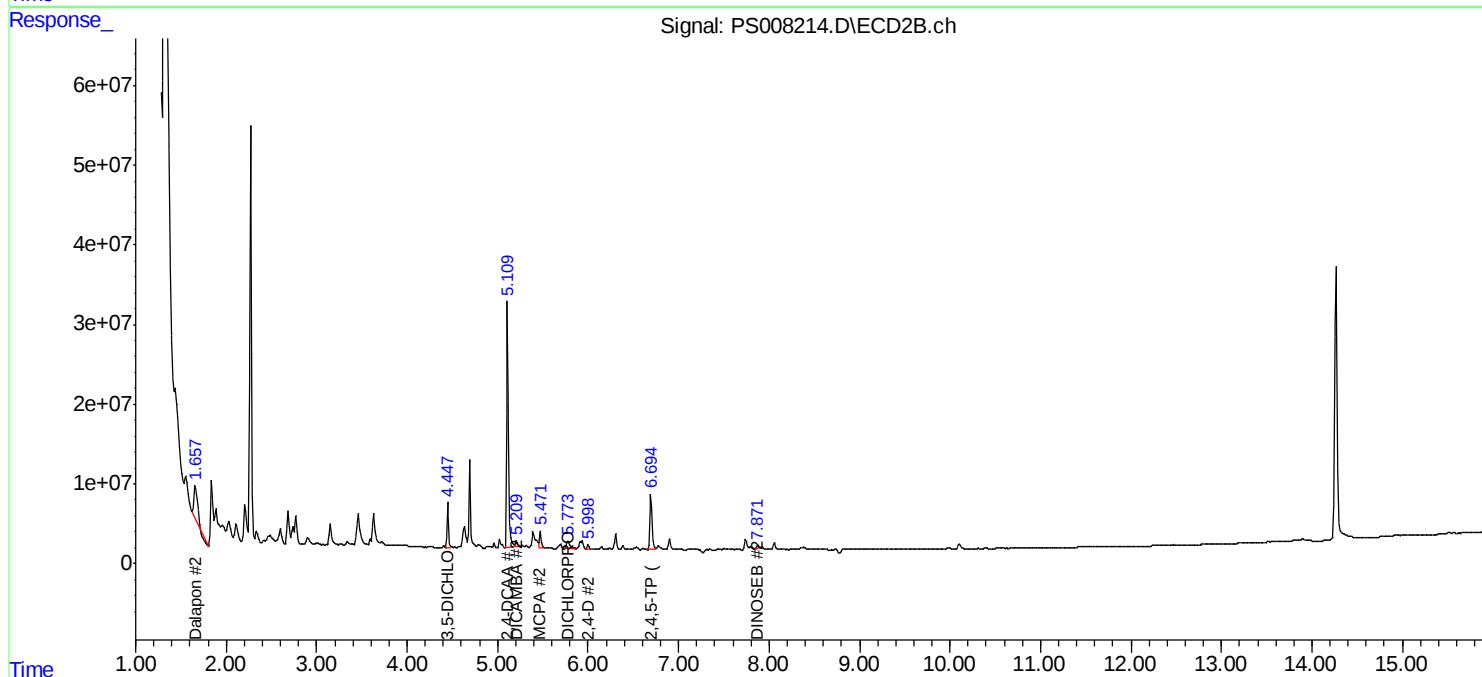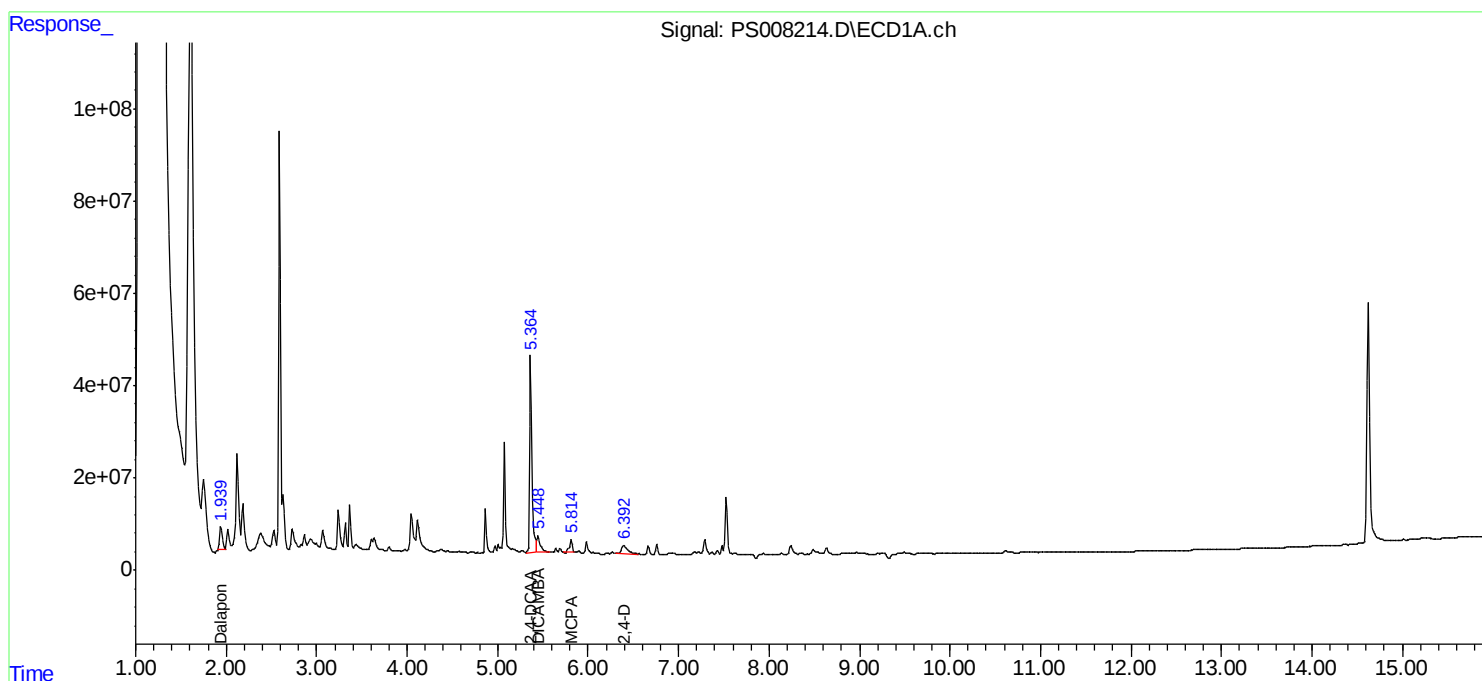


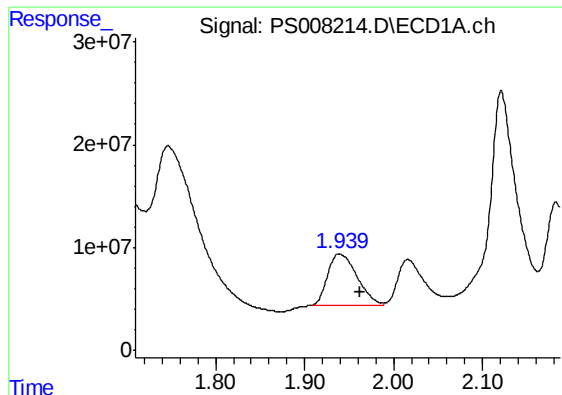

#1 Dalapon


R.T.: 1.939 min
Delta R.T.: -0.024 min
Response: 113634418
Conc: 47.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125754BL

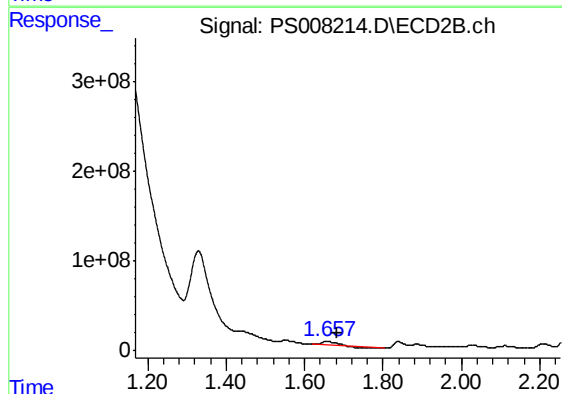


#1 Dalapon

R.T.: 1.656 min
Delta R.T.: -0.026 min
Response: 100134045
Conc: 98.16 ng/ml

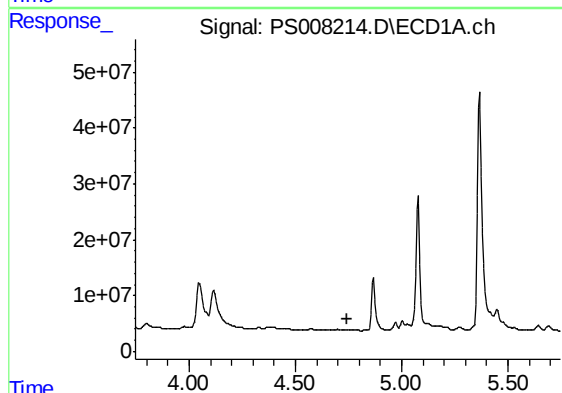


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

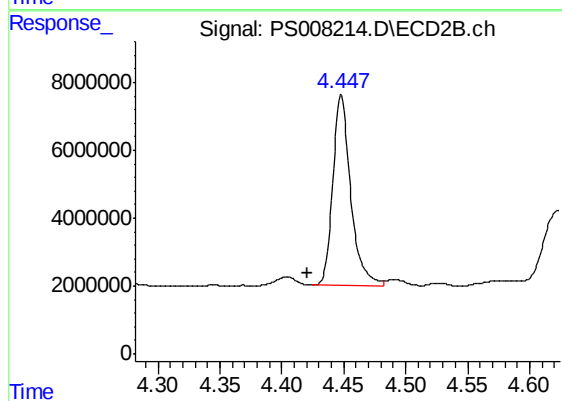

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.448 min
Delta R.T.: 0.028 min
Response: 56755632
Conc: 48.74 ng/ml

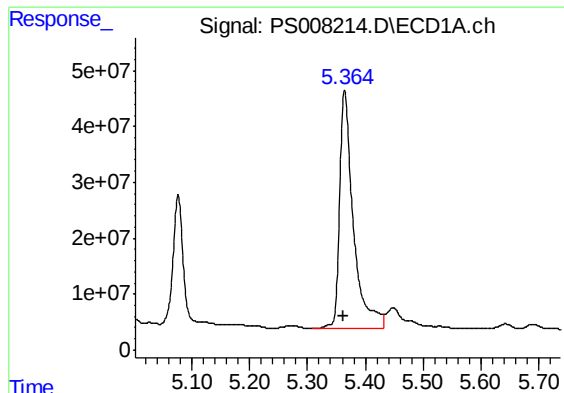

#4 2,4-DCAA


R.T.: 5.365 min
Delta R.T.: 0.003 min
Response: 704153978
Conc: 348.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125754BL

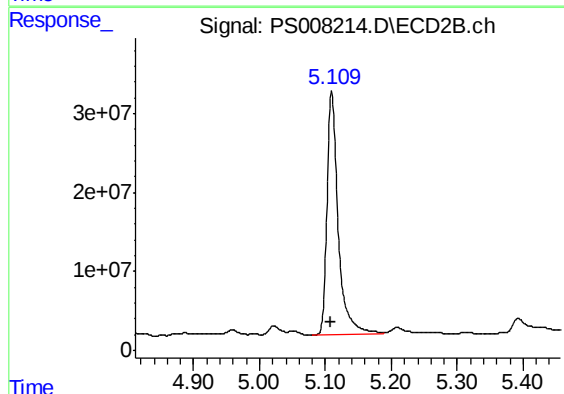


#4 2,4-DCAA

R.T.: 5.110 min
Delta R.T.: 0.002 min
Response: 360659062
Conc: 402.80 ng/ml

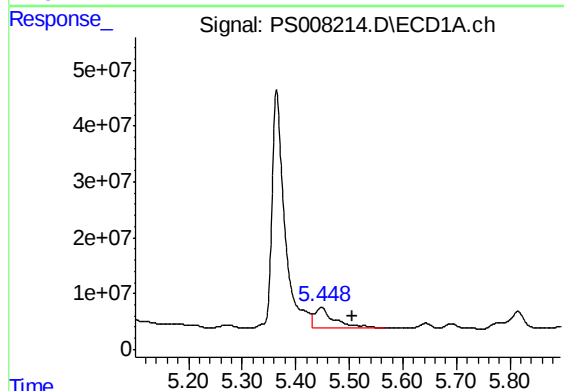


#5 DICAMBA

R.T.: 5.448 min
Delta R.T.: -0.057 min
Response: 93028749
Conc: 12.79 ng/ml

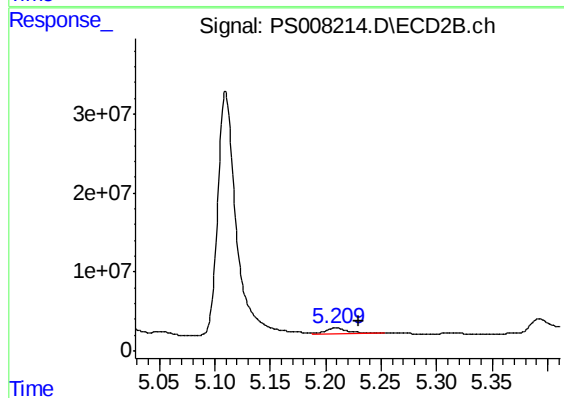

#5 DICAMBA


R.T.: 5.209 min
Delta R.T.: -0.021 min
Response: 11512405
Conc: 3.38 ng/ml

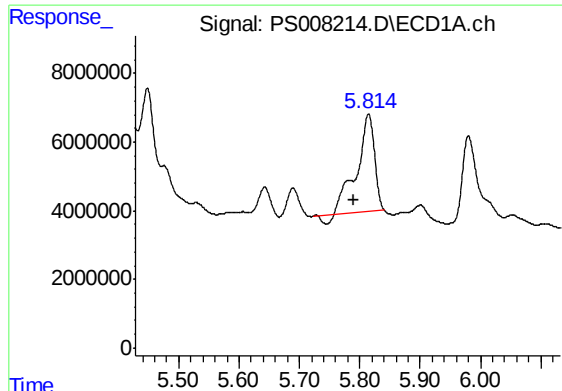

#7 MCPA


R.T.: 5.815 min
Delta R.T.: 0.025 min
Response: 56402734
Conc: 7.37 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125754BL

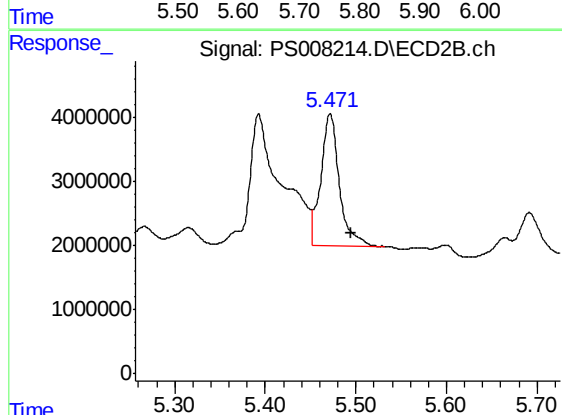


#7 MCPA

R.T.: 5.472 min
Delta R.T.: -0.023 min
Response: 28979335
Conc: 7.62 ug/ml

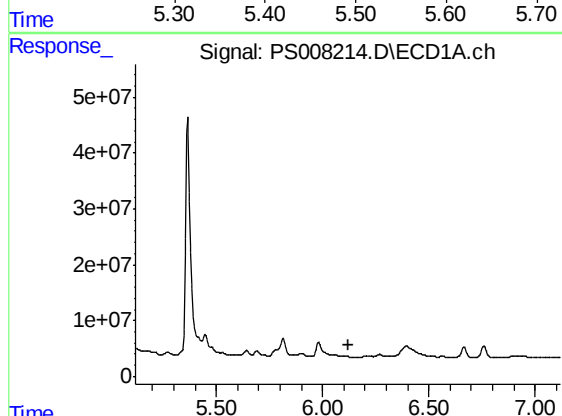


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

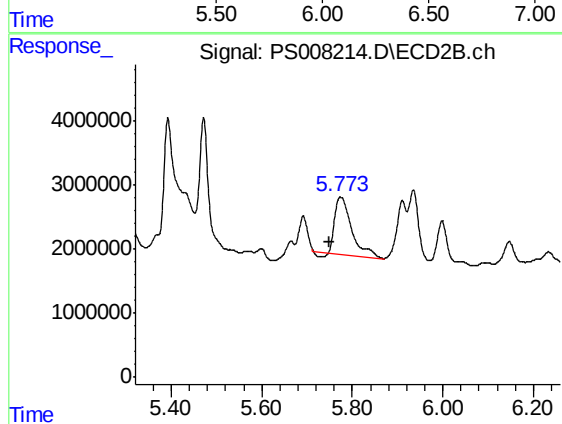

#8 DICHLORPROP


R.T.: 5.774 min
Delta R.T.: 0.024 min
Response: 22449950
Conc: 26.23 ng/ml

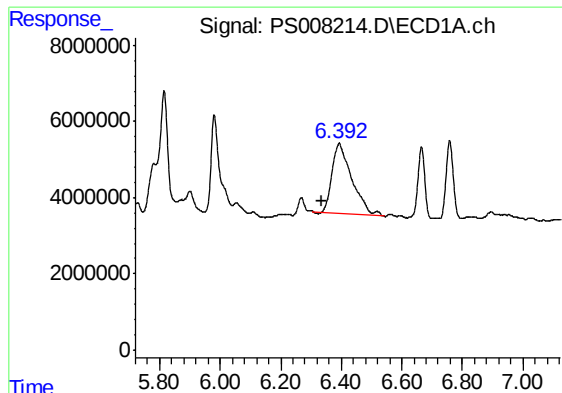

#9 2,4-D


R.T.: 6.393 min
Delta R.T.: 0.059 min
Response: 83418302
Conc: 50.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125754BL

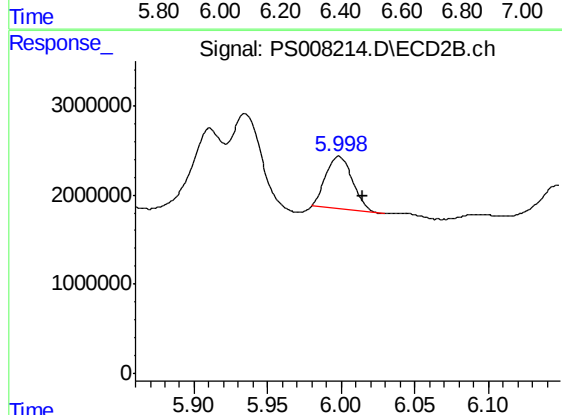


#9 2,4-D

R.T.: 5.998 min
Delta R.T.: -0.016 min
Response: 7377065
Conc: 7.27 ng/ml

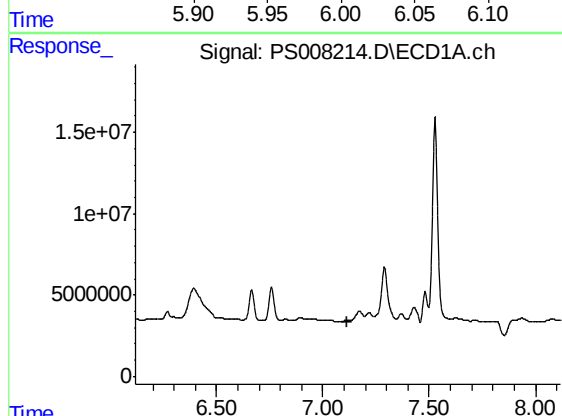


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

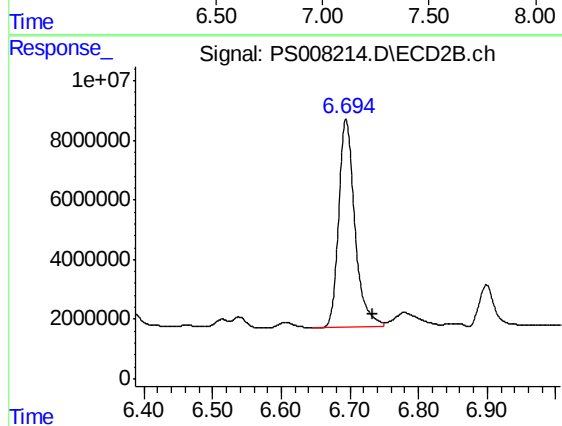

#11 2,4,5-TP (SILVEX)


R.T.: 6.694 min
Delta R.T.: -0.040 min
Response: 112769081
Conc: 22.57 ng/ml

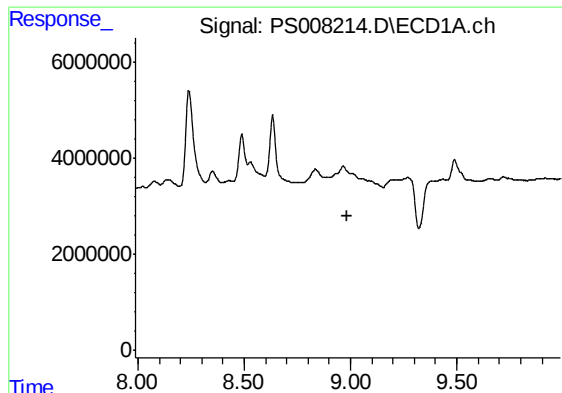

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125754BL

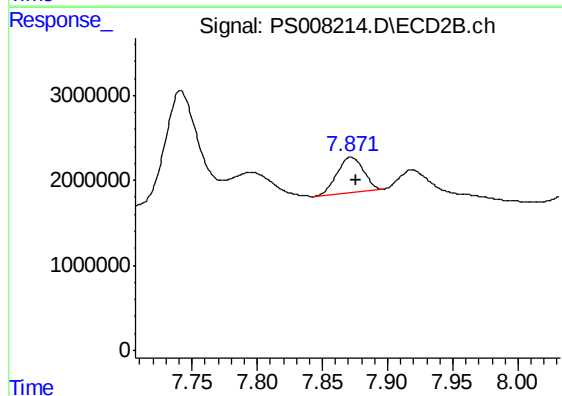

#14 DINOSEB

R.T.: 7.872 min
Delta R.T.: -0.004 min
Response: 5849734
Conc: 1.56 ng/ml