

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122719\
 Data File : PS008240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2019 05:18
 Operator : SM\AJ
 Sample : K6443-03
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 01:24:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	5.058	0	7879744	N.D.	8.800
Target Compounds							
1) T	Dalapon	1.975	1.688	64784036	38561769	26.986	37.801 #
2) T	3,5-DICHL...	0.000	4.483	0	27449142	N.D.	23.573
5) T	DICAMBA	5.483	5.254	44301981	10064149	6.093	2.954 #
6) T	MCP	0.000	5.254	0	10064149	N.D.	3.889
7) T	MCPA	0.000	5.508	0	17697254	N.D.	4.652
8) T	DICHLORPROP	0.000	5.796	0	18687459	N.D.	21.830
9) T	2,4-D	0.000	5.971	0	4993386	N.D.	4.918
10) T	Pentachlo...	0.000	6.339	0	40021904	N.D.	3.145
11) T	2,4,5-TP ...	0.000	6.726	0	18962286	N.D.	3.795
12) T	2,4,5-T	7.323	0.000	83175730	0	6.922	N.D. #
15) T	Picloram	0.000	8.758	0	22219542	N.D.	3.404
16) T	DCPA	0.000	8.758	0	22219542	N.D.	3.331



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122719\
Data File : PS008240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2019 05:18
Operator : SM\AJ
Sample : K6443-03
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 01:24:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

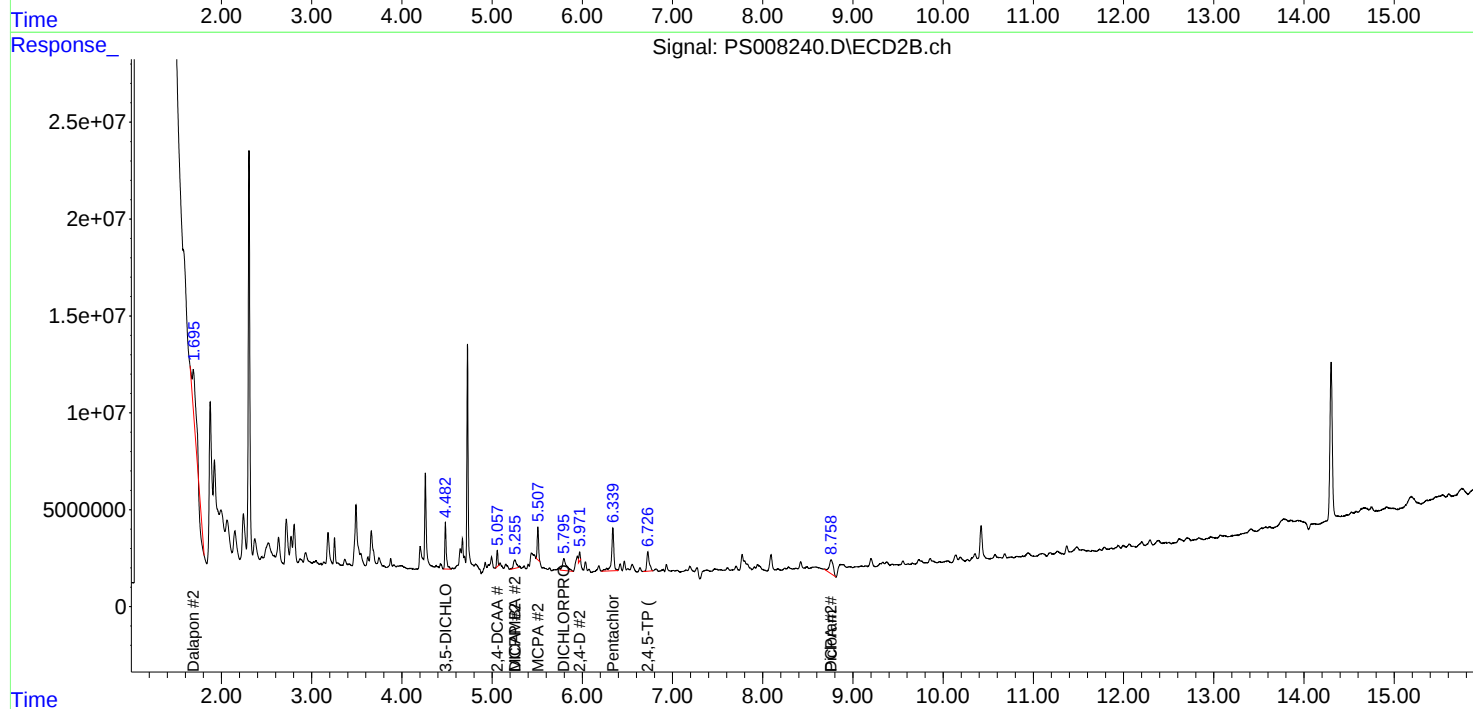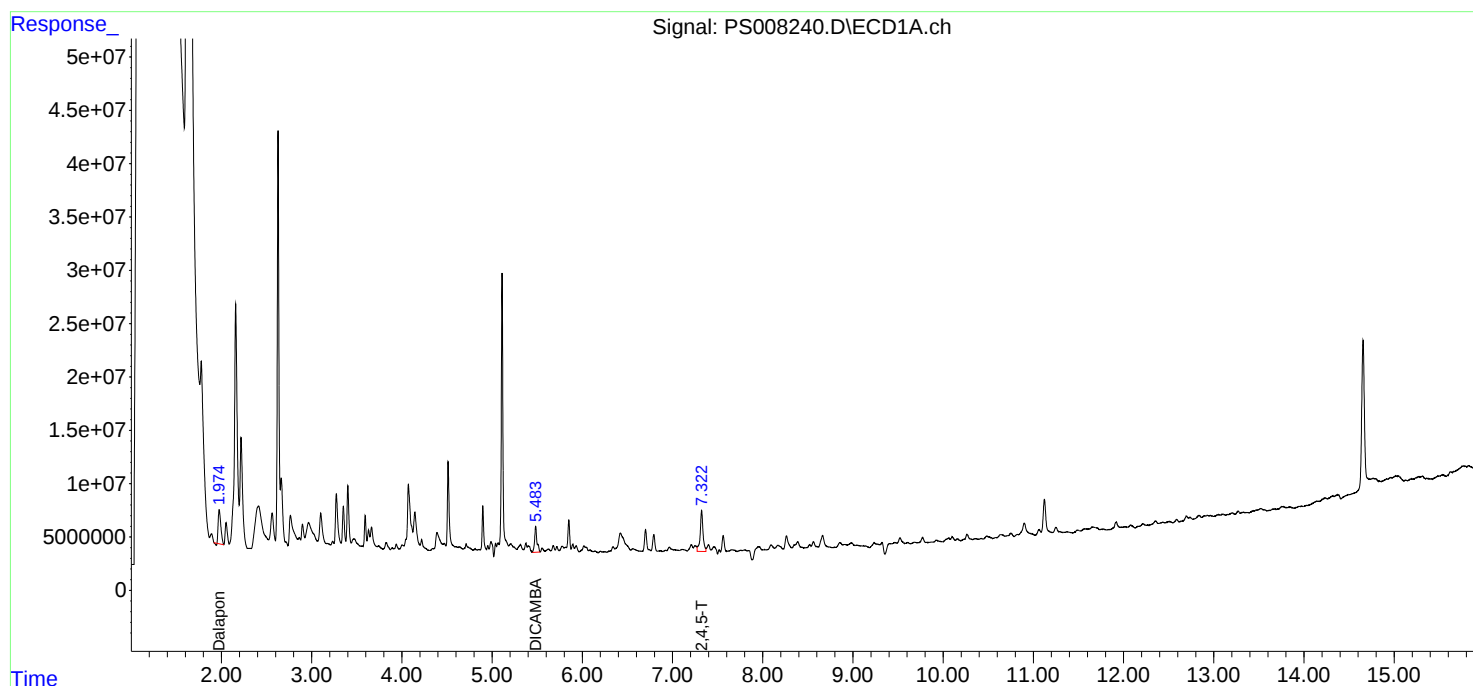


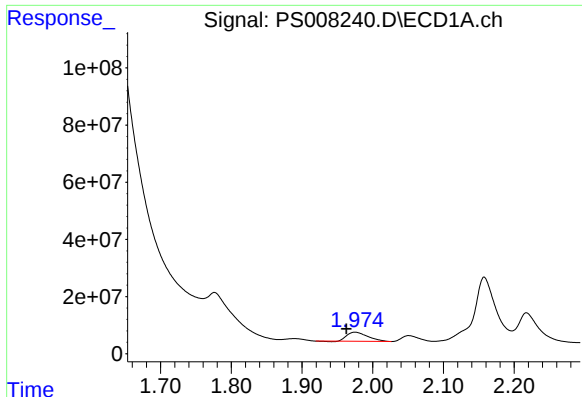

#1 Dalapon


R.T.: 1.975 min
Delta R.T.: 0.012 min
Response: 64784036
Conc: 26.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

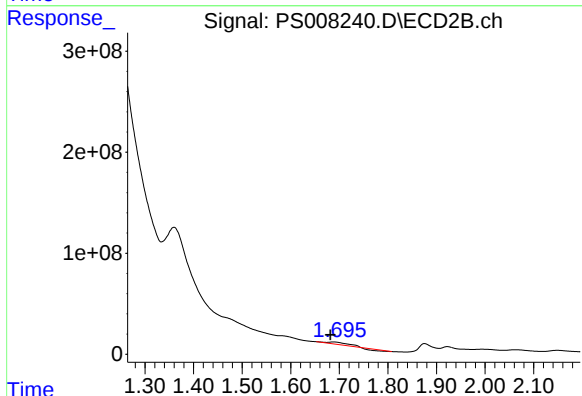


#1 Dalapon

R.T.: 1.688 min
Delta R.T.: 0.005 min
Response: 38561769
Conc: 37.80 ng/ml

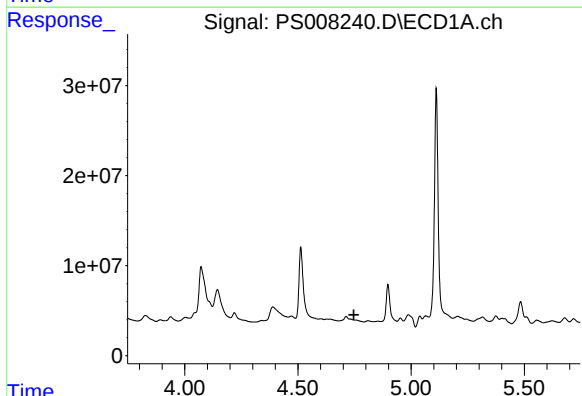


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

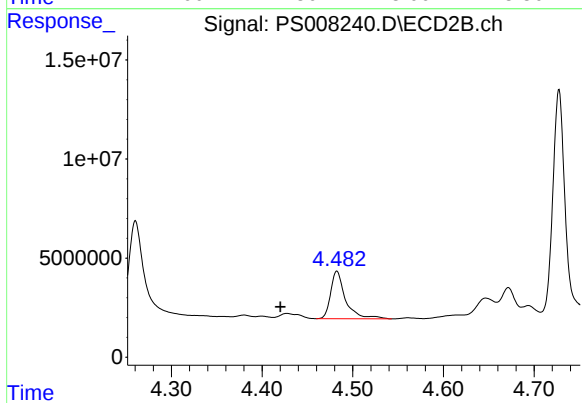

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.483 min
Delta R.T.: 0.062 min
Response: 27449142
Conc: 23.57 ng/ml

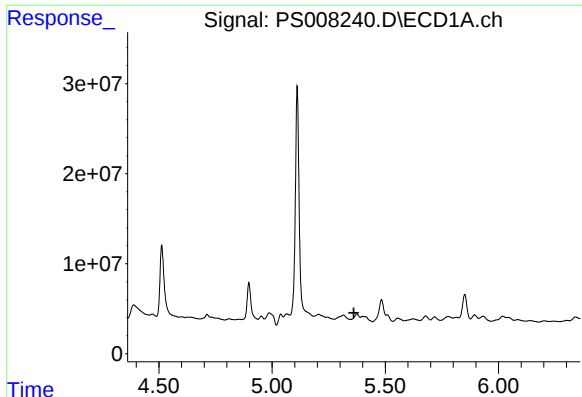

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

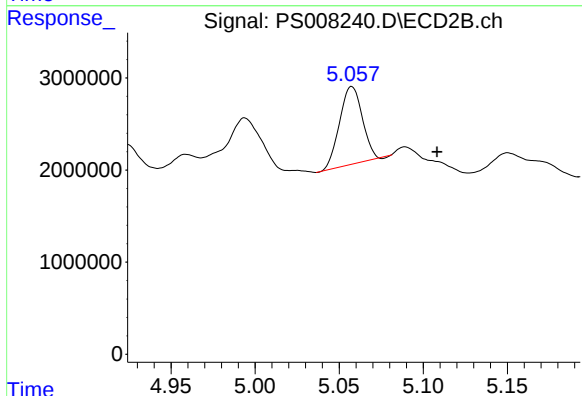


#4 2,4-DCAA

R.T.: 5.058 min
Delta R.T.: -0.051 min
Response: 7879744
Conc: 8.80 ng/ml

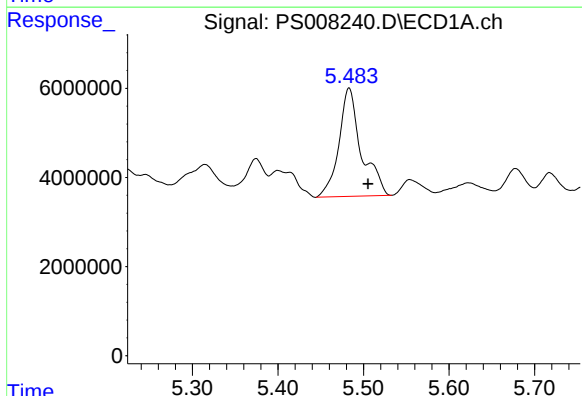


#5 DICAMBA

R.T.: 5.483 min
Delta R.T.: -0.022 min
Response: 44301981
Conc: 6.09 ng/ml

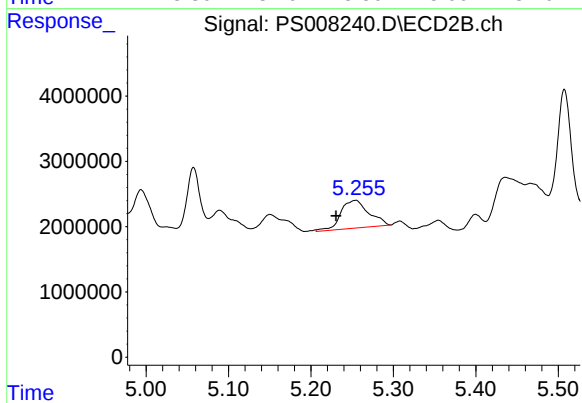

#5 DICAMBA


R.T.: 5.254 min
Delta R.T.: 0.023 min
Response: 10064149
Conc: 2.95 ng/ml

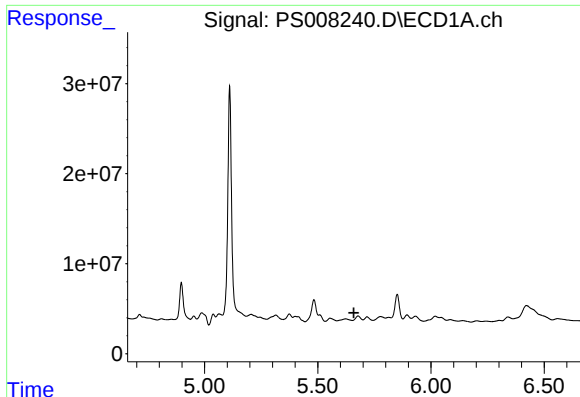

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.659 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

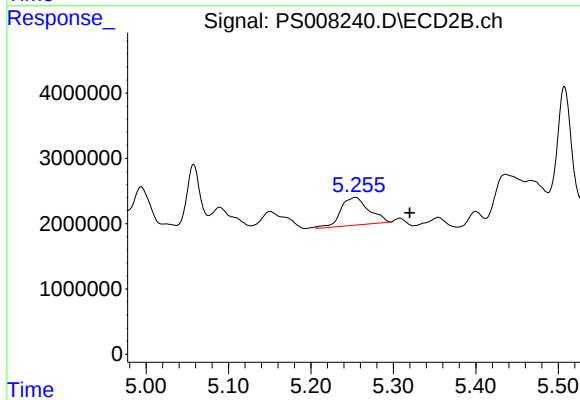


#6 MCPP

R.T.: 5.254 min
Delta R.T.: -0.066 min
Response: 10064149
Conc: 3.89 ug/ml

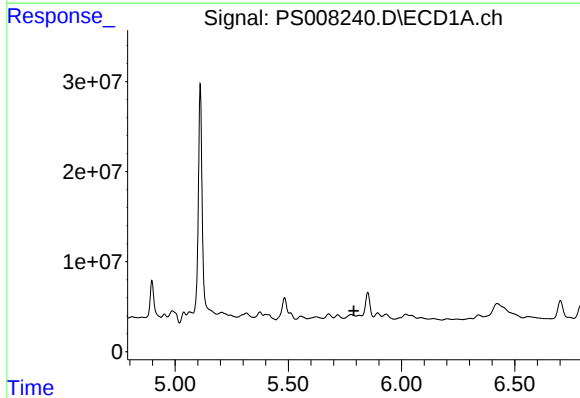


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 5.789 min
Response: 0
Conc: N.D.

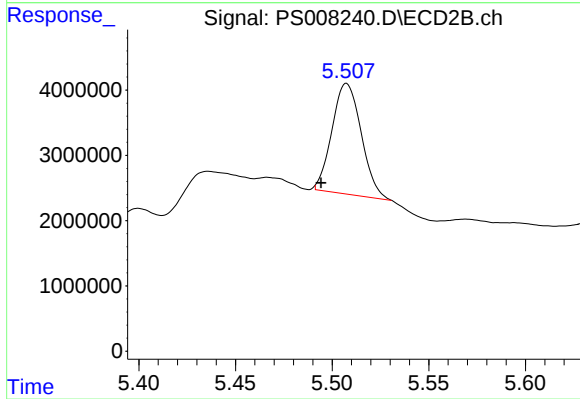

#7 MCPA


R.T.: 5.508 min
Delta R.T.: 0.013 min
Response: 17697254
Conc: 4.65 ug/ml

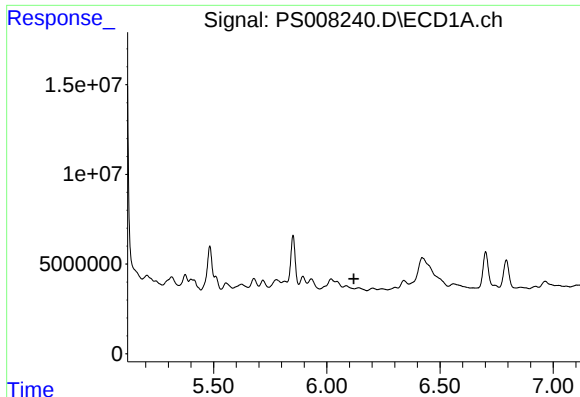

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.120 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

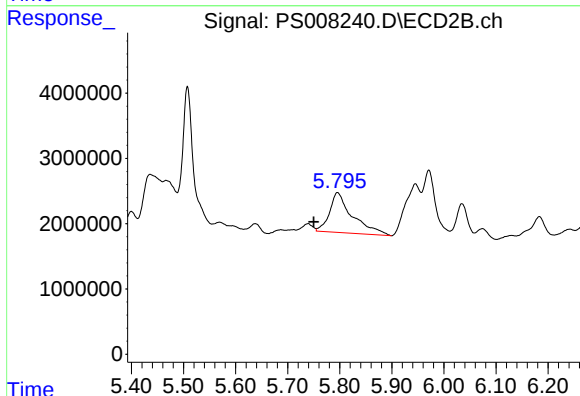


#8 DICHLORPROP

R.T.: 5.796 min
Delta R.T.: 0.046 min
Response: 18687459
Conc: 21.83 ng/ml

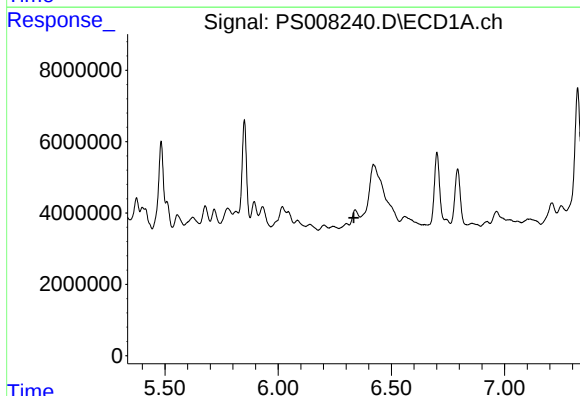


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.334 min
Response: 0
Conc: N.D.

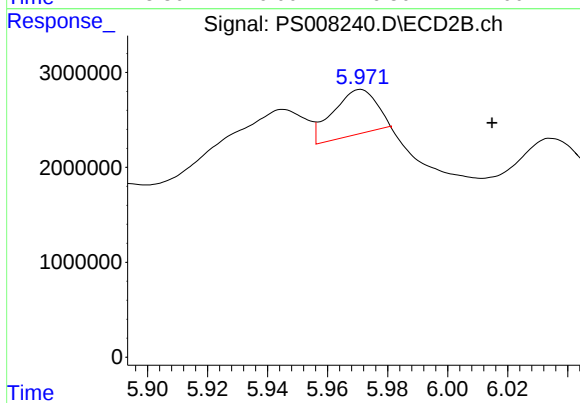

#9 2,4-D


R.T.: 5.971 min
Delta R.T.: -0.044 min
Response: 4993386
Conc: 4.92 ng/ml

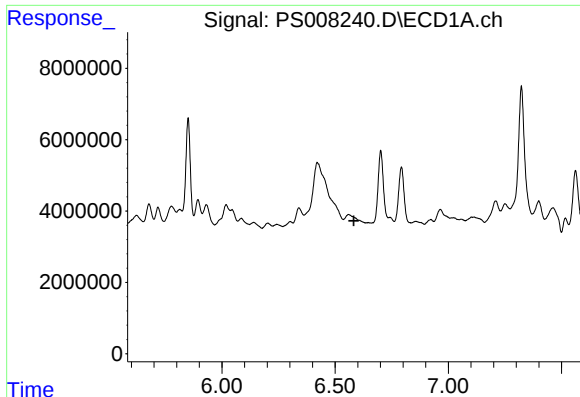

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

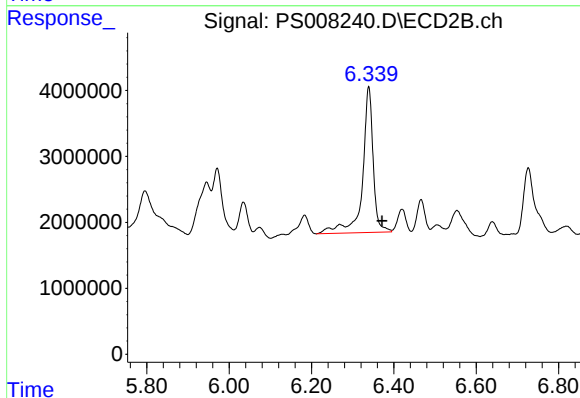


#10 Pentachlorophenol

R.T.: 6.339 min
Delta R.T.: -0.033 min
Response: 40021904
Conc: 3.14 ng/ml

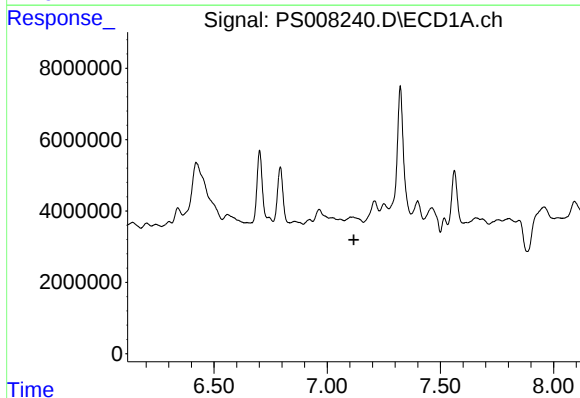


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

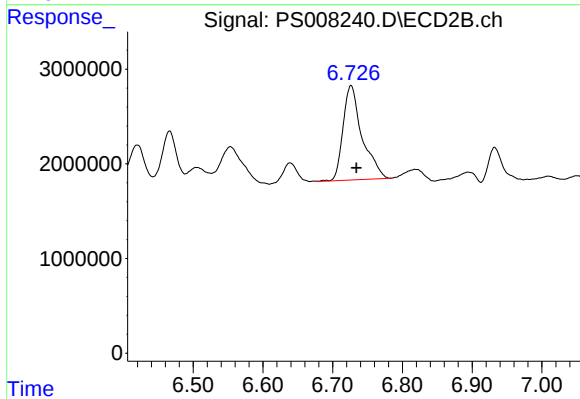

#11 2,4,5-TP (SILVEX)


R.T.: 6.726 min
Delta R.T.: -0.008 min
Response: 18962286
Conc: 3.79 ng/ml

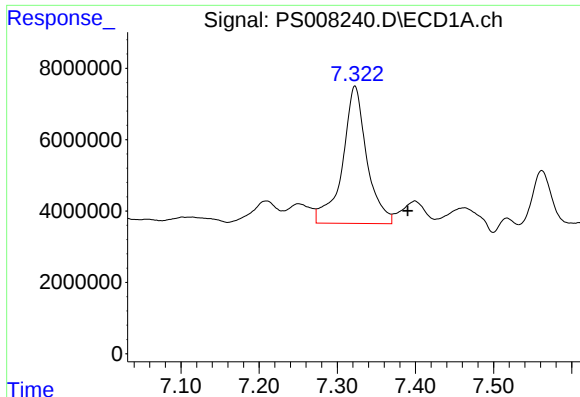

#12 2,4,5-T


R.T.: 7.323 min
Delta R.T.: -0.067 min
Response: 83175730
Conc: 6.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

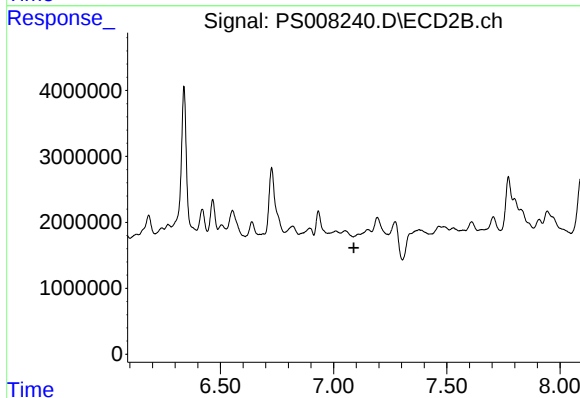


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

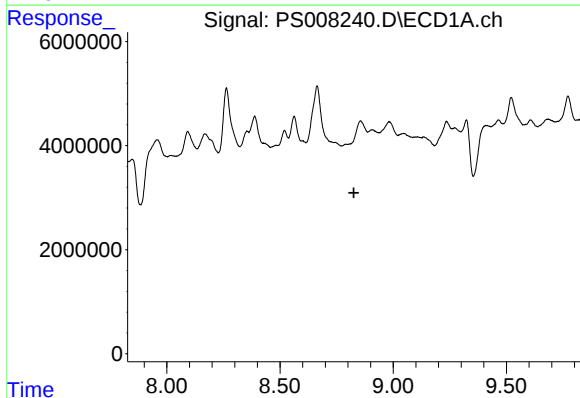


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.826 min
Response: 0
Conc: N.D.

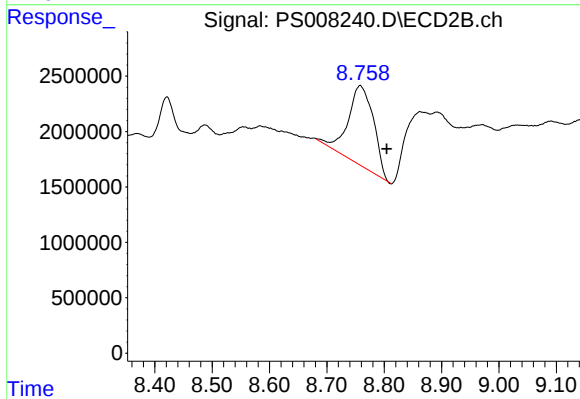

#15 Picloram


R.T.: 8.758 min
Delta R.T.: -0.047 min
Response: 22219542
Conc: 3.40 ng/ml

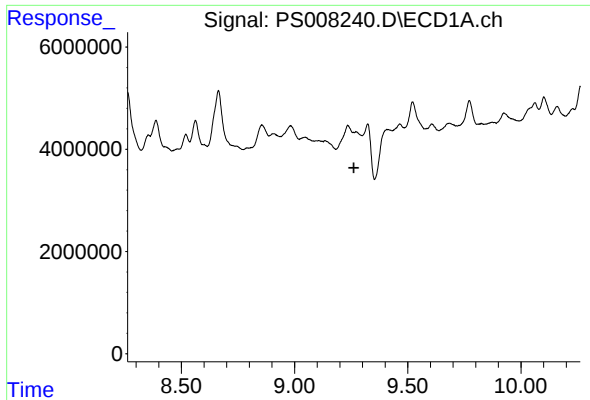

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.262 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

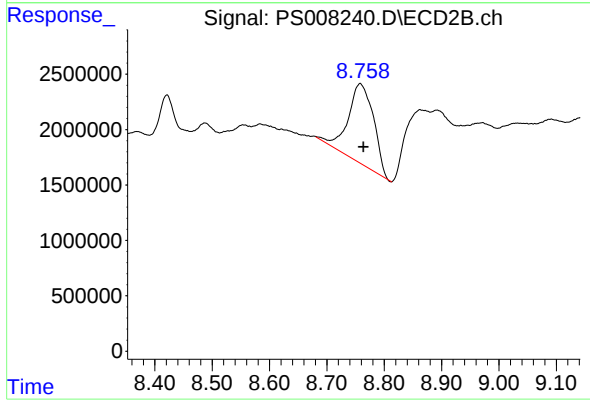

#16 DCPA

R.T.: 8.758 min
Delta R.T.: -0.006 min
Response: 22219542
Conc: 3.33 ng/ml