

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122722\
 Data File : PS021555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2022 09:13
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 21:03:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.406	0.000	78333	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	5.759	0.000	1980251	0	<MDL	N.D. #
3) T	4-Nitroph...	6.216	0.000	2533718	0	1.409	N.D. #
5) T	DICAMBA	6.528	0.000	233444	0	<MDL	N.D. #
7) T	MCPA	0.000	7.226f	0	16410305	N.D.	1.856
8) T	DICHLORPROP	7.142	0.000	135357	0	<MDL	N.D. #
10) T	Pentachlo...	7.553	8.319	936623	902456	<MDL	<MDL #
11) T	2,4,5-TP ...	8.095	0.000	907225	0	<MDL	N.D. #
12) T	2,4,5-T	8.354	0.000	7210365	0	<MDL	N.D. #
13) T	2,4-DB	8.839	9.638f	365488	1175154	<MDL	<MDL #
14) T	DINOSEB	9.859f	0.000	34637412	0	2.174	N.D. #
15) T	Picloram	9.761	10.921f	970030	21306039	<MDL	1.310 #
16) T	DCPA	10.168	10.821	1048045	1030943	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122722\
Data File : PS021555.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2022 09:13
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 21:03:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

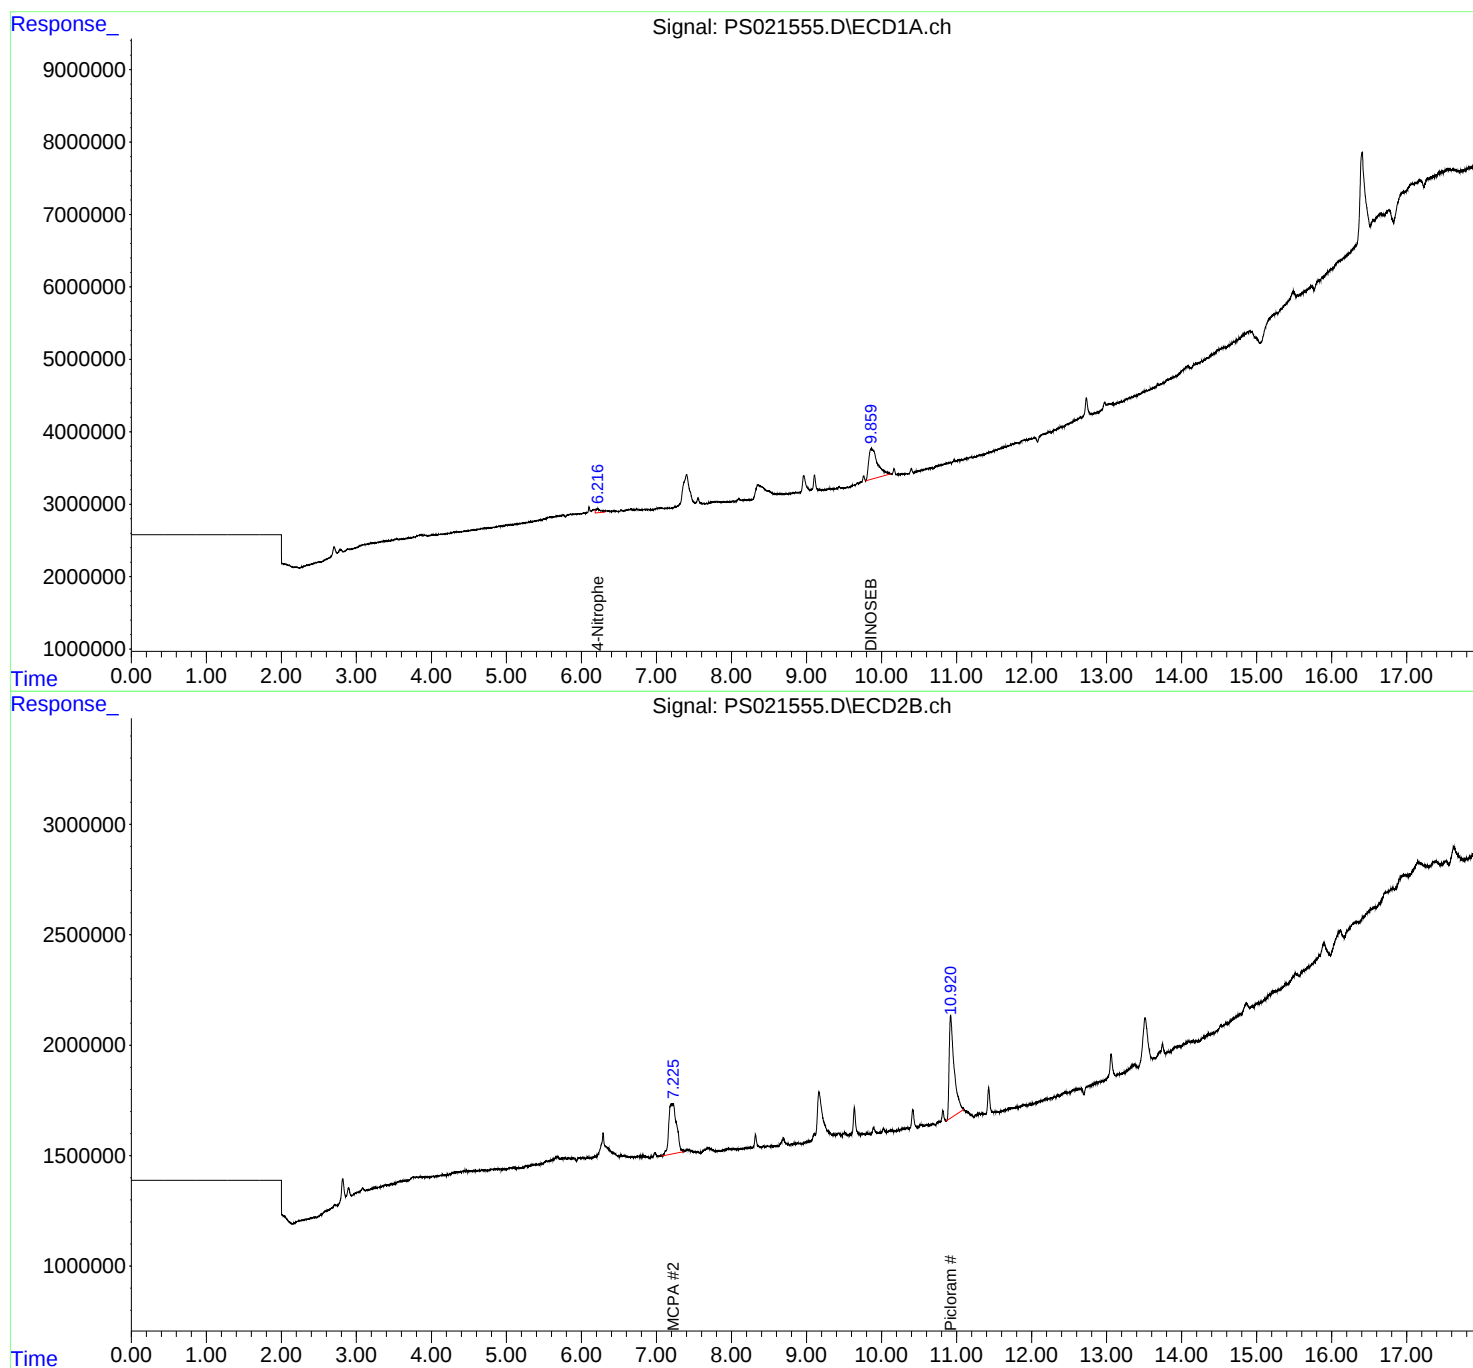


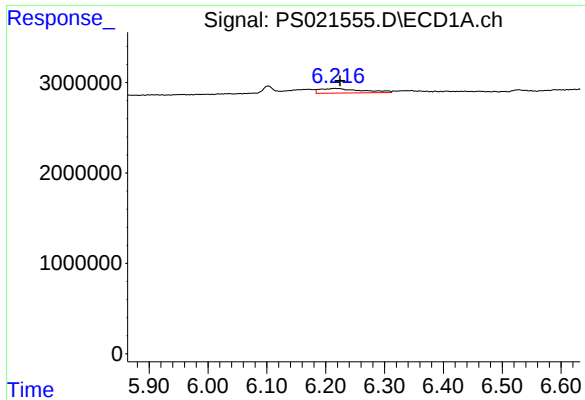

#3 4-Nitrophenol


R.T.: 6.216 min
Delta R.T.: -0.009 min
Response: 2533718
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

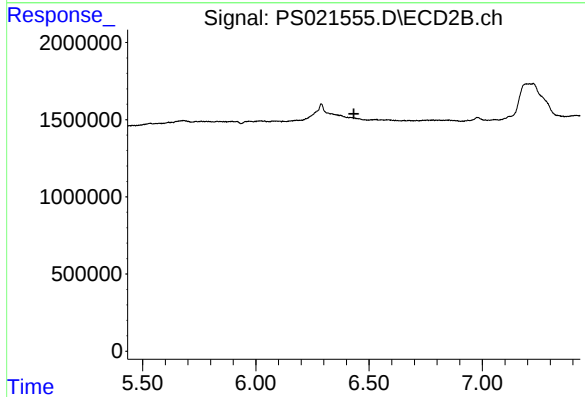


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

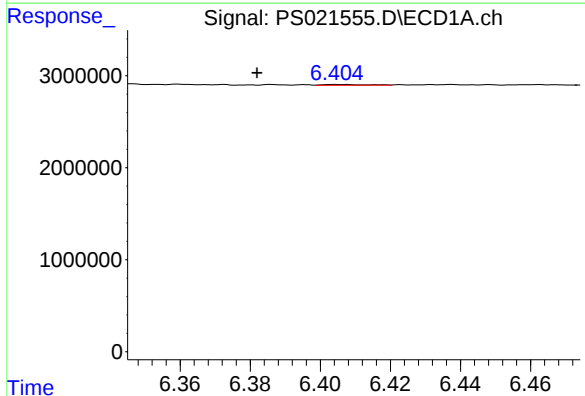


#4 2,4-DCAA

R.T.: 6.406 min
Delta R.T.: 0.024 min
Response: 78333
Conc: N.D.

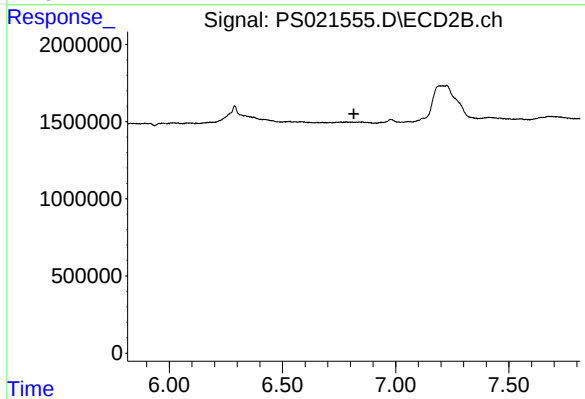

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.816 min
Response: 0
Conc: N.D.

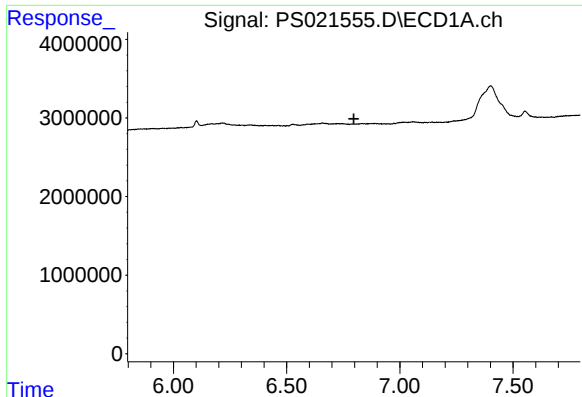

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.797 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

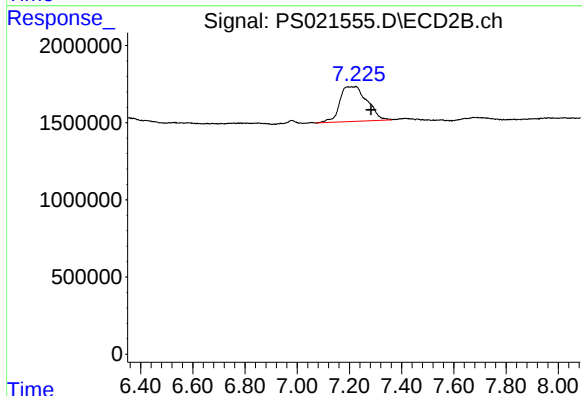


#7 MCPA

R.T.: 7.226 min
Delta R.T.: -0.057 min
Response: 16410305
Conc: 1.86 ug/ml

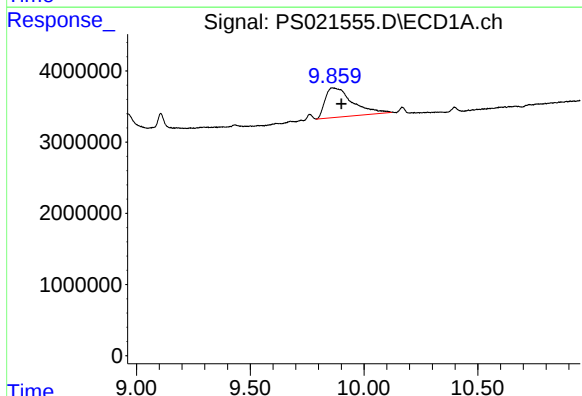


#14 DINOSEB

R.T.: 9.859 min
Delta R.T.: -0.042 min
Response: 34637412
Conc: 2.17 ng/ml

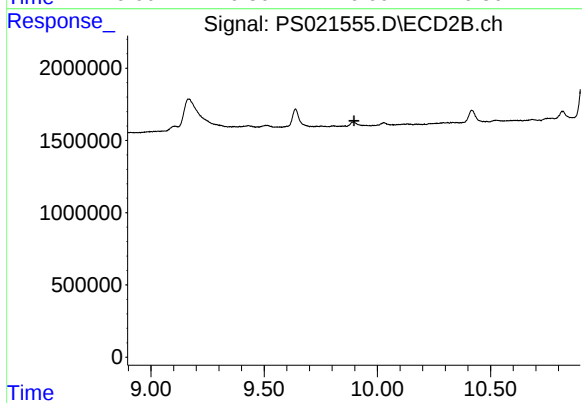

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.897 min
Response: 0
Conc: N.D.

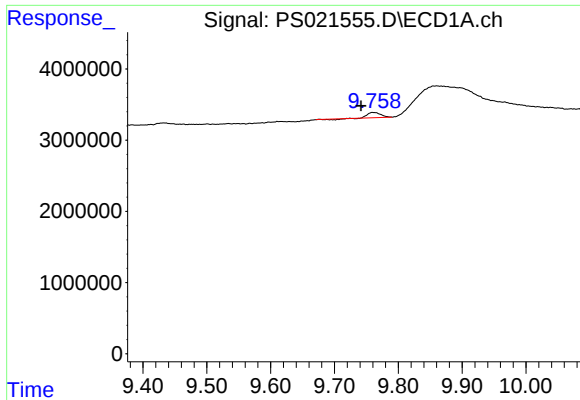

#15 Picloram

R.T.: 9.761 min
Delta R.T.: 0.019 min
Response: 970030
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

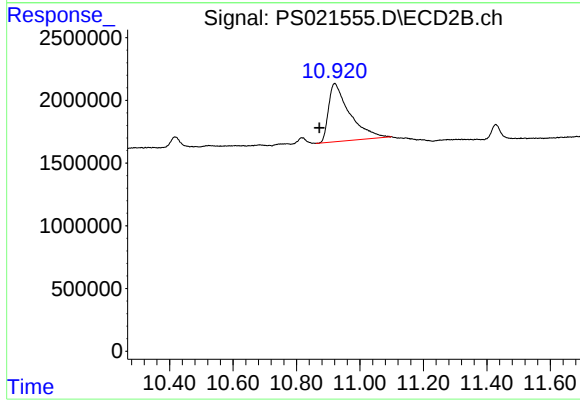

#15 Picloram

R.T.: 10.921 min
Delta R.T.: 0.049 min
Response: 21306039
Conc: 1.31 ng/ml