

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122722\
 Data File : PS021556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2022 09:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 21:03:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.380	6.809	1122.3E6	882.4E6	386.284	511.851 #
Target Compounds							
1) T	Dalapon	2.528f	0.000	252159	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.743	0.000	2048841	0	<MDL	N.D. #
3) T	4-Nitroph...	6.229	0.000	4202501	0	2.337	N.D. #
7) T	MCPA	6.763	7.217f	1143325	27413210	<MDL	3.100 #
9) T	2,4-D	7.331	0.000	24738919	0	6.474	N.D. #
10) T	Pentachlo...	7.554	0.000	436653	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.087	0.000	7050872	0	<MDL	N.D. #
12) T	2,4,5-T	8.348	0.000	13010429	0	<MDL	N.D. #
13) T	2,4-DB	8.881	9.637f	614651	1994927	<MDL	1.388 #
14) T	DINOSEB	9.870	0.000	36411372	0	2.285	N.D. #
15) T	Picloram	9.764	10.917f	1468366	22824909	<MDL	1.404 #
16) T	DCPA	10.168	0.000	1181973	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122722\
Data File : PS021556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2022 09:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 21:03:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

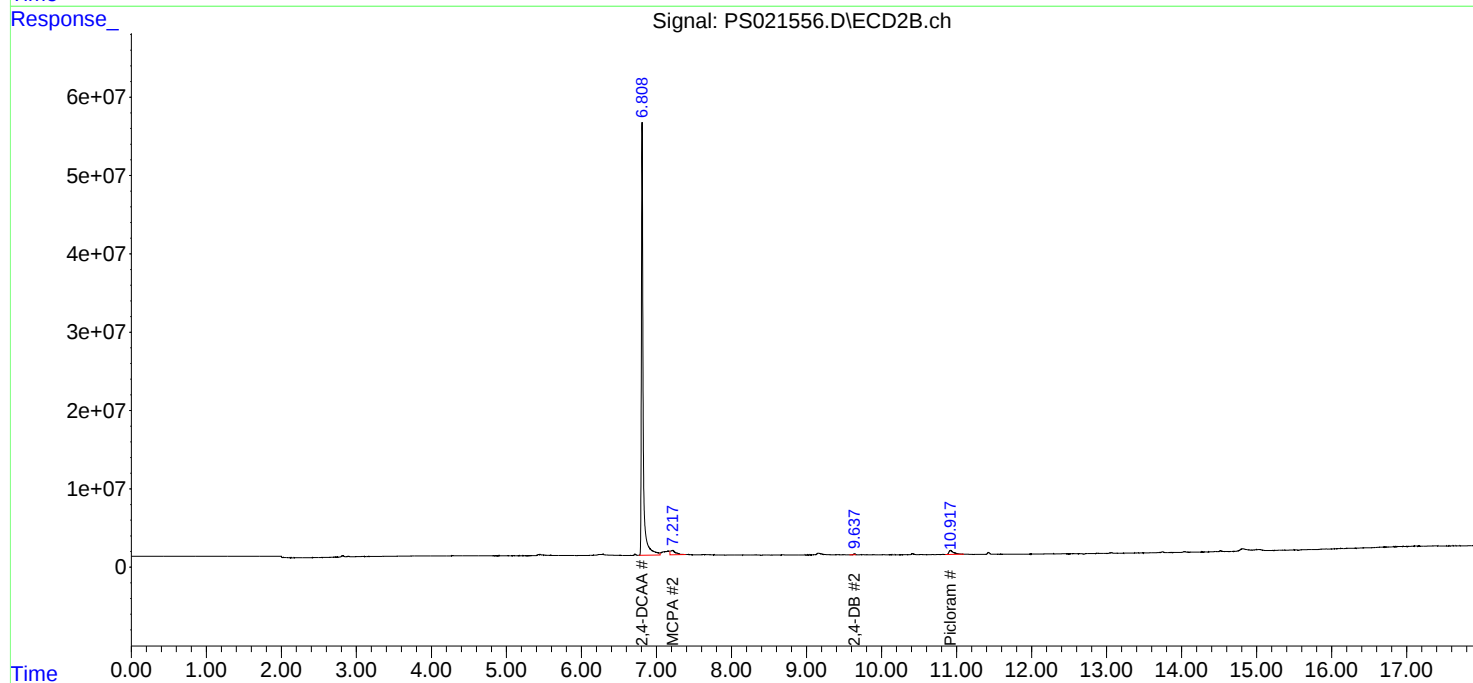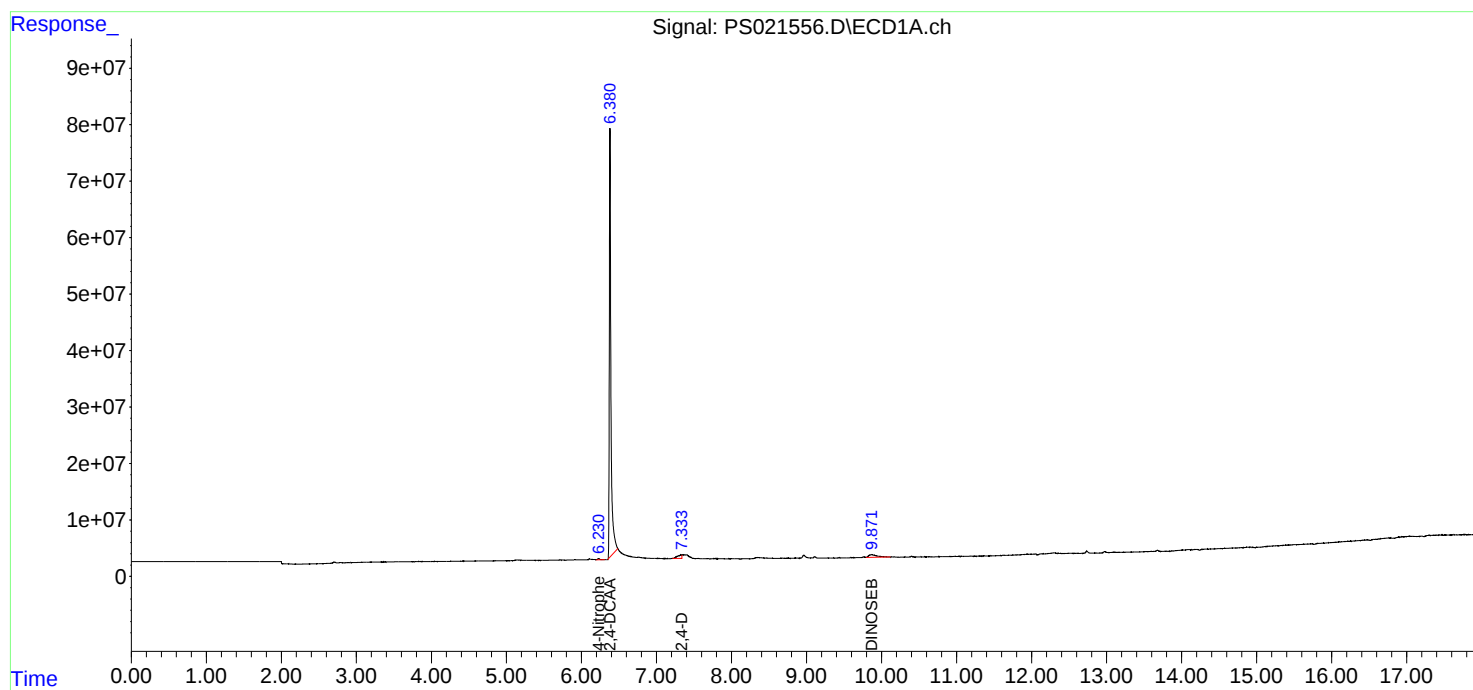


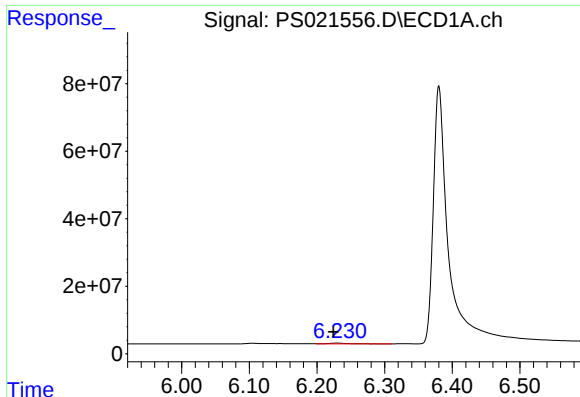

#3 4-Nitrophenol


R.T.: 6.229 min
Delta R.T.: 0.005 min
Response: 4202501
Conc: 2.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

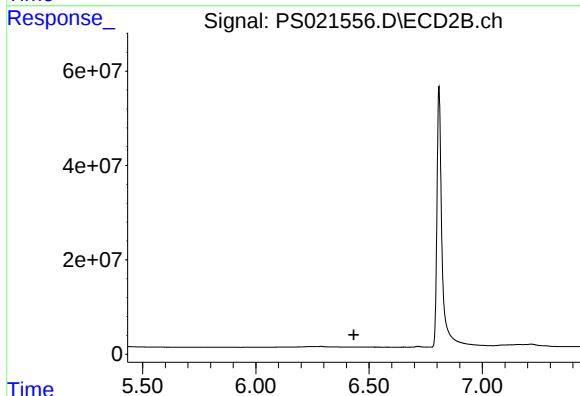


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

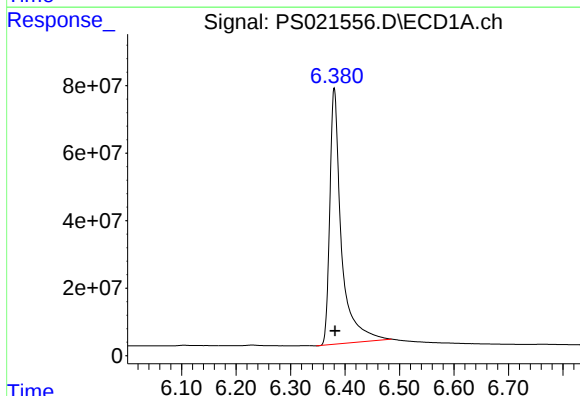


#4 2,4-DCAA

R.T.: 6.380 min
Delta R.T.: -0.001 min
Response: 1122344470
Conc: 386.28 ng/ml

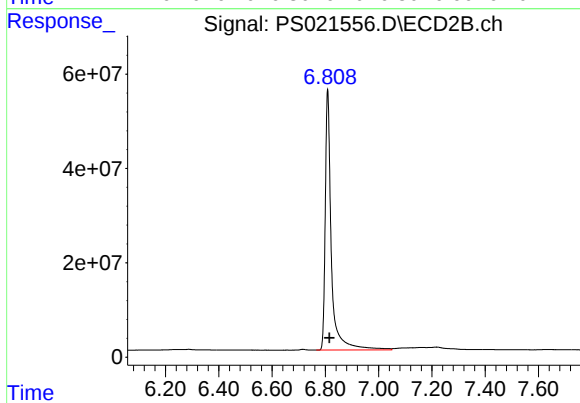

#4 2,4-DCAA


R.T.: 6.809 min
Delta R.T.: -0.007 min
Response: 882427897
Conc: 511.85 ng/ml

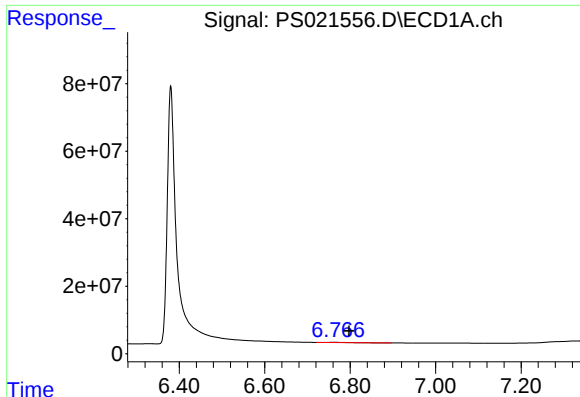

#7 MCPA


R.T.: 6.763 min
Delta R.T.: -0.034 min
Response: 1143325
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

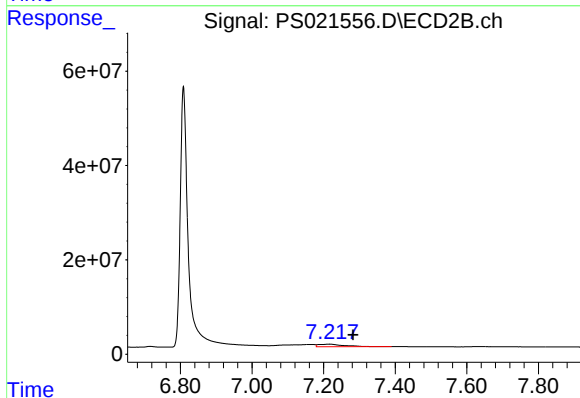


#7 MCPA

R.T.: 7.217 min
Delta R.T.: -0.066 min
Response: 27413210
Conc: 3.10 ug/ml

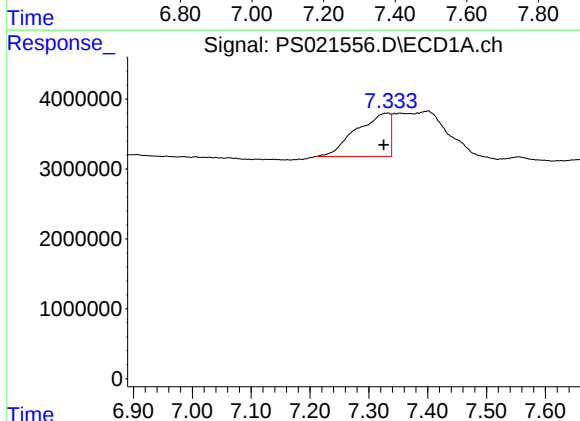


#9 2,4-D

R.T.: 7.331 min
Delta R.T.: 0.006 min
Response: 24738919
Conc: 6.47 ng/ml

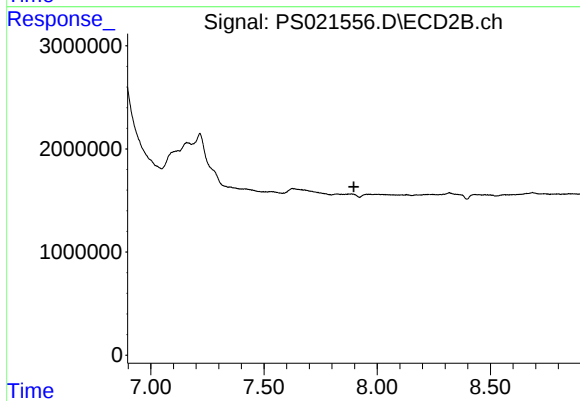

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.897 min
Response: 0
Conc: N.D.

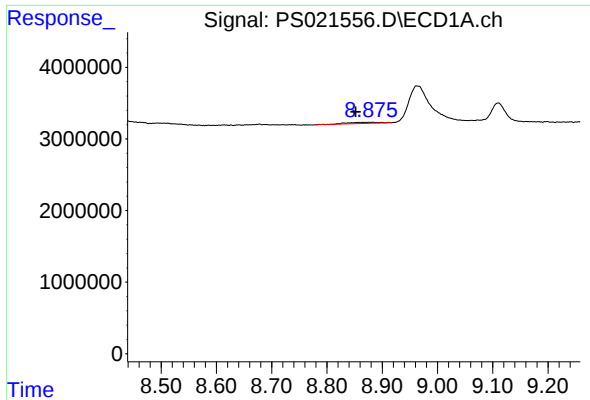

#13 2,4-DB


R.T.: 8.881 min
Delta R.T.: 0.028 min
Response: 614651
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

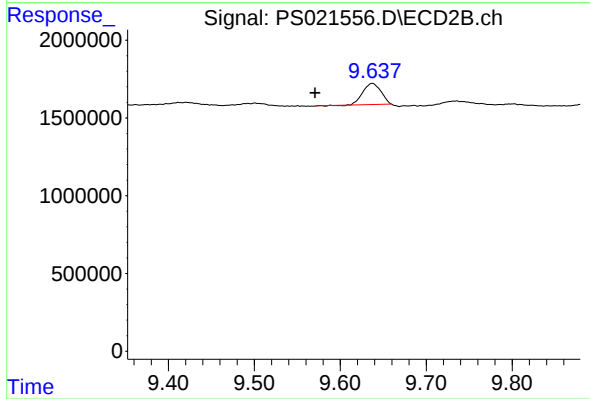


#13 2,4-DB

R.T.: 9.637 min
Delta R.T.: 0.066 min
Response: 1994927
Conc: 1.39 ng/ml

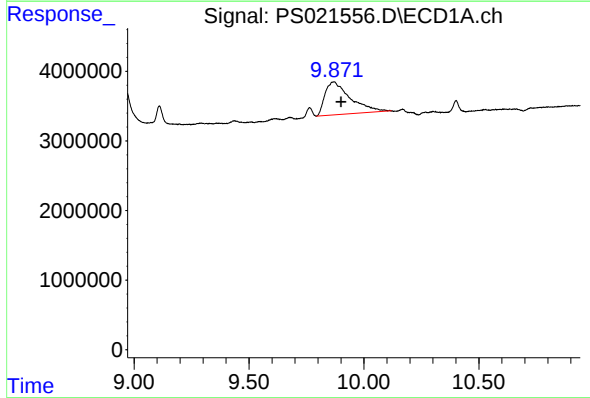


#14 DINOSEB

R.T.: 9.870 min
Delta R.T.: -0.031 min
Response: 36411372
Conc: 2.29 ng/ml

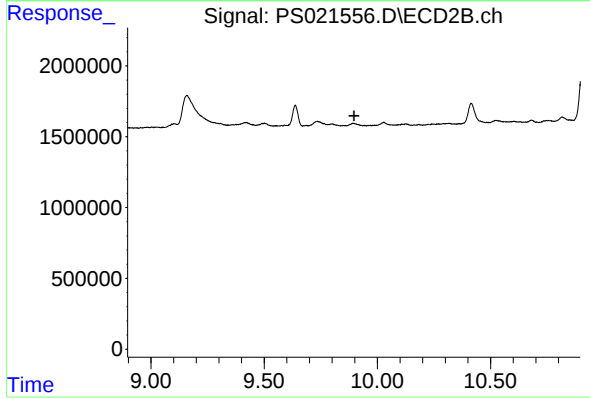

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.897 min
Response: 0
Conc: N.D.

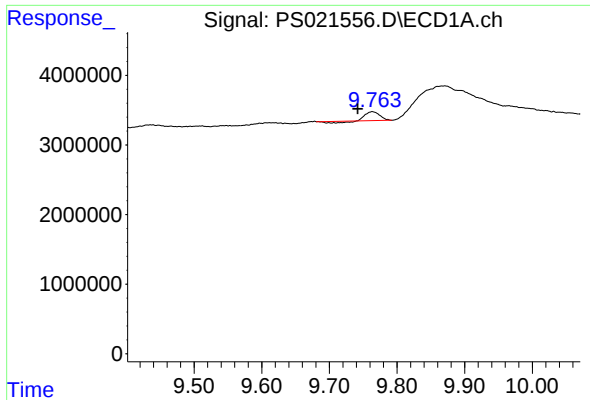

#15 Picloram

R.T.: 9.764 min
Delta R.T.: 0.022 min
Response: 1468366
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

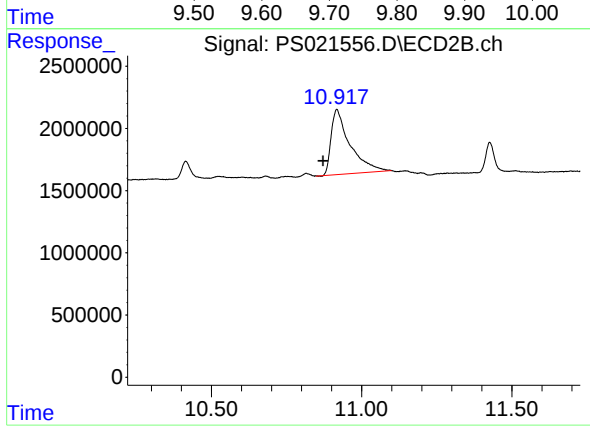

#15 Picloram

R.T.: 10.917 min
Delta R.T.: 0.045 min
Response: 22824909
Conc: 1.40 ng/ml