

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122724\
 Data File : PS028827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2024 10:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:05:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.206	7.694	1272.9E6	571.8E6	562.744	508.041
Target Compounds							
1) T	Dalapon	2.667f	0.000	19207538	0	6.819	N.D. #
2) T	3,5-DICHL...	6.386	0.000	479486	0	<MDL	N.D. #
3) T	4-Nitroph...	7.002	0.000	4331109	0	2.883	N.D. #
5) T	DICAMBA	7.393	7.893	239075	3285080	<MDL	<MDL #
6) T	MCP	7.528f	0.000	946480	0	<MDL	N.D. #
8) T	DICHLORPROP	8.069f	8.654f	4552376	3016178	1.716	2.186 #
10) T	Pentachlo...	8.624	0.000	1831633	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.185	0.000	495599	0	<MDL	N.D. #
12) T	2,4,5-T	9.502	0.000	1548295	0	<MDL	N.D. #
13) T	2,4-DB	10.029f	0.000	1828096	0	<MDL	N.D. #
14) T	DINOSEB	11.271	0.000	1856878	0	<MDL	N.D. #
15) T	Picloram	11.101	12.292	28228484	15143502	1.053	1.179
16) T	DCPA	11.560	12.292f	1283862	15143502	<MDL	1.409 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122724\
Data File : PS028827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2024 10:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:05:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

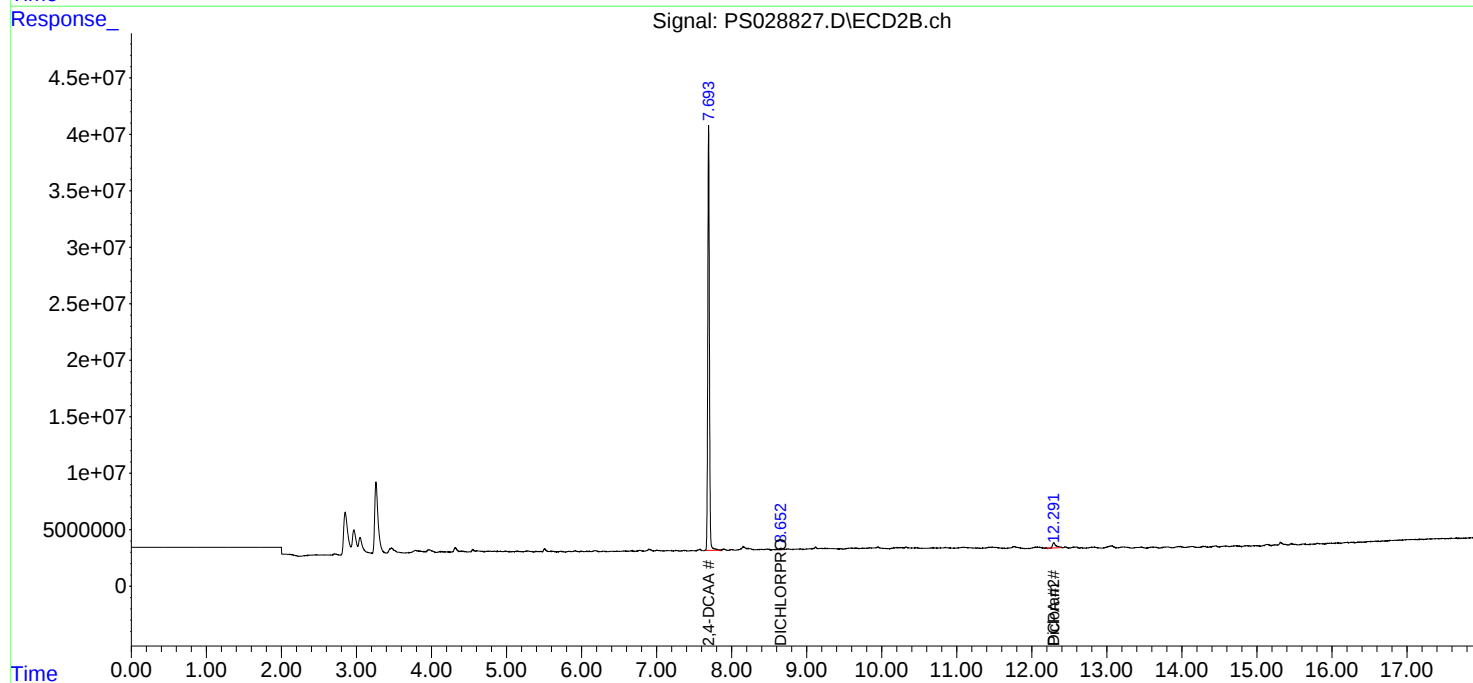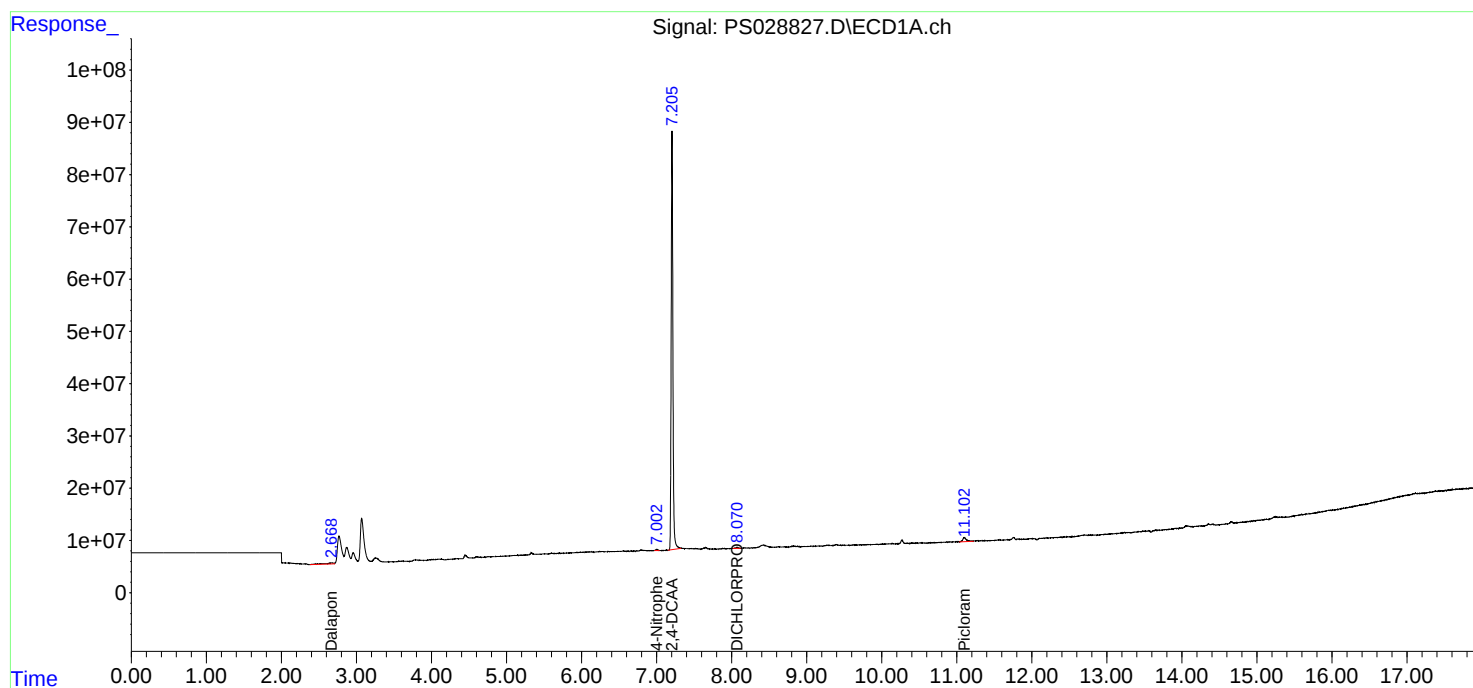


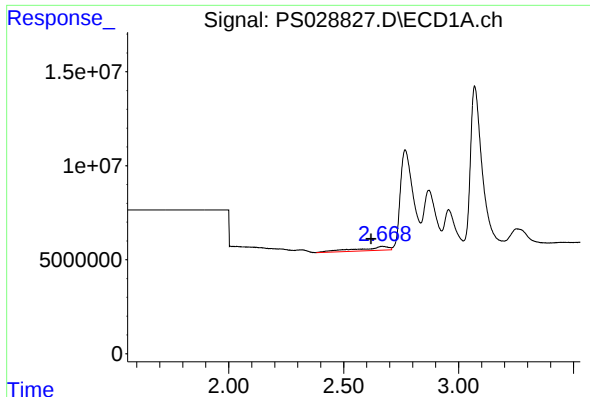

#1 Dalapon


R.T.: 2.667 min
Delta R.T.: 0.047 min
Response: 19207538
Conc: 6.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

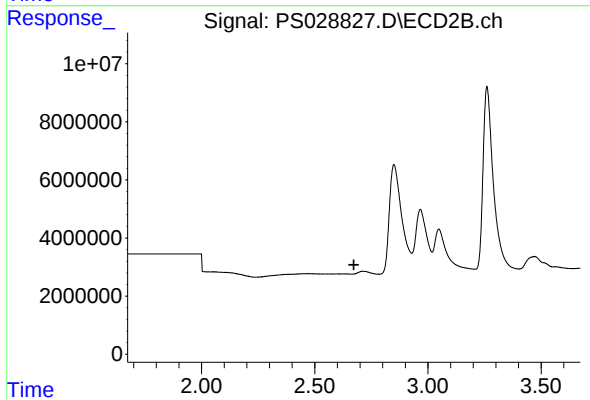


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.673 min
Response: 0
Conc: N.D.

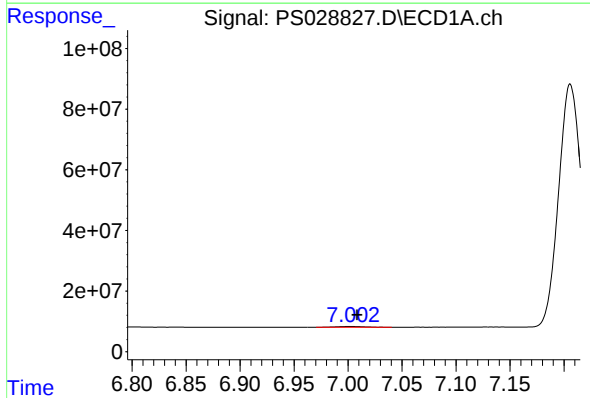


#3 4-Nitrophenol

R.T.: 7.002 min
Delta R.T.: -0.006 min
Response: 4331109
Conc: 2.88 ng/ml

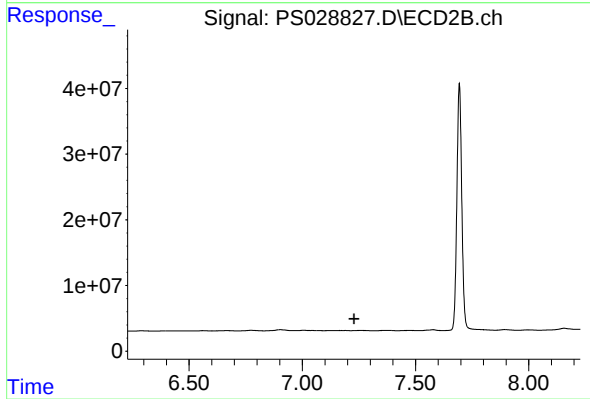

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

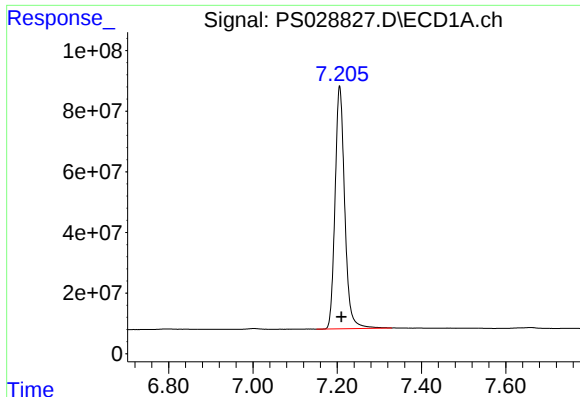

#4 2,4-DCAA


R.T.: 7.206 min
Delta R.T.: -0.004 min
Response: 1272941847
Conc: 562.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

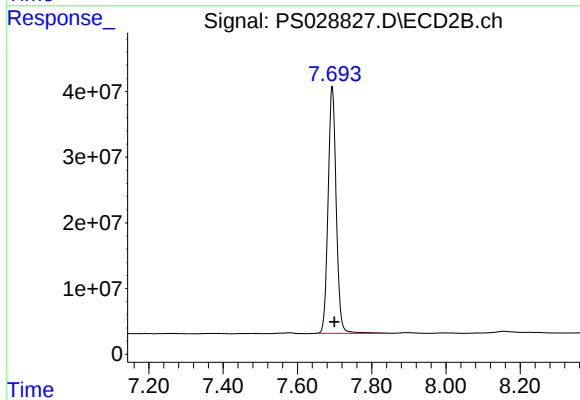


#4 2,4-DCAA

R.T.: 7.694 min
Delta R.T.: -0.006 min
Response: 571819063
Conc: 508.04 ng/ml

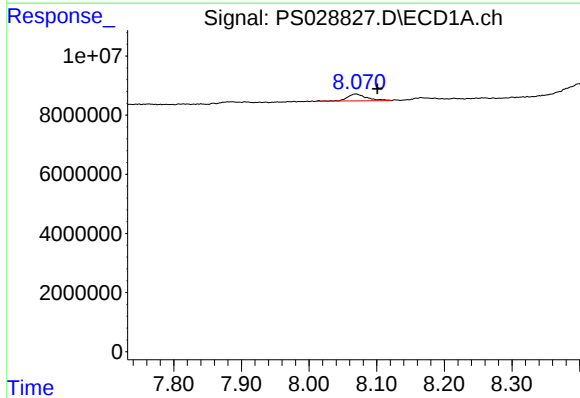


#8 DICHLORPROP

R.T.: 8.069 min
Delta R.T.: -0.032 min
Response: 4552376
Conc: 1.72 ng/ml

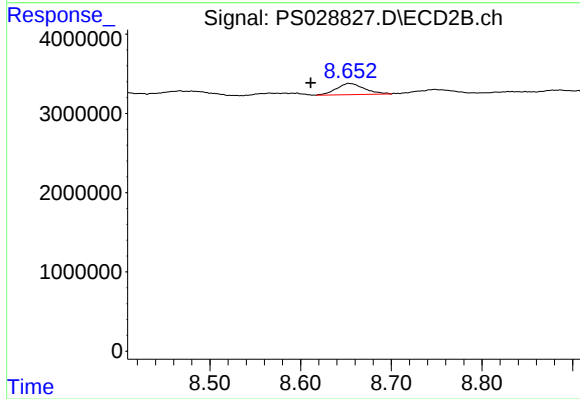

#8 DICHLORPROP


R.T.: 8.654 min
Delta R.T.: 0.043 min
Response: 3016178
Conc: 2.19 ng/ml

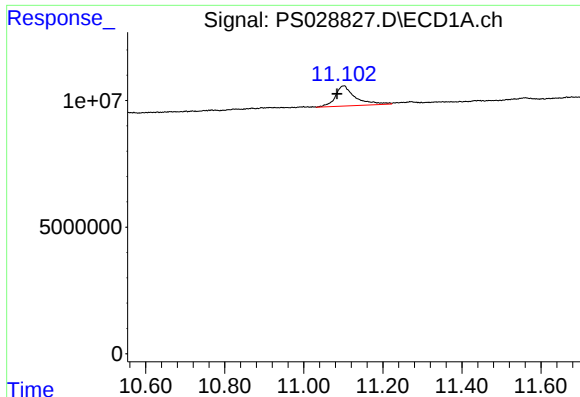

#15 Picloram


R.T.: 11.101 min
Delta R.T.: 0.017 min
Response: 28228484
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

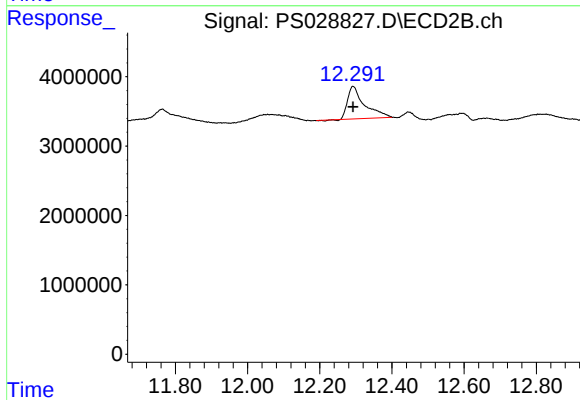


#15 Picloram

R.T.: 12.292 min
Delta R.T.: 0.000 min
Response: 15143502
Conc: 1.18 ng/ml

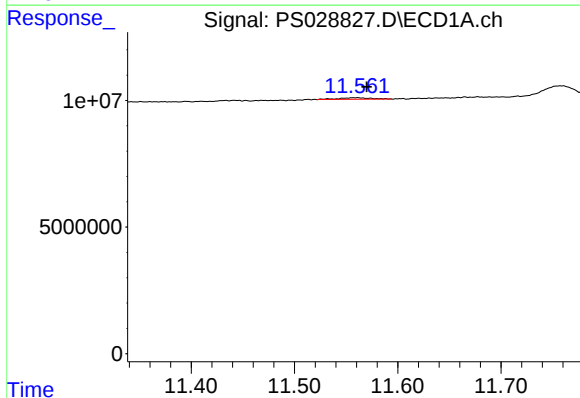

#16 DCPA

R.T.: 11.560 min
Delta R.T.: -0.010 min
Response: 1283862
Conc: N.D.

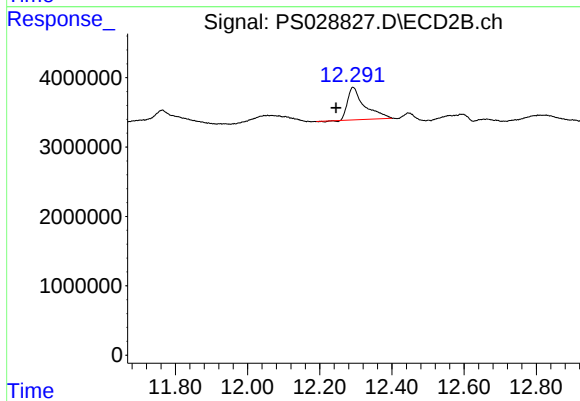

#16 DCPA

R.T.: 12.292 min
Delta R.T.: 0.047 min
Response: 15143502
Conc: 1.41 ng/ml