

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122724\
 Data File : PS028838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2024 21:08
 Operator : AR\AJ
 Sample : PB165896BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:07:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.205	7.694	1311.5E6	567.1E6	579.798	503.831
Target Compounds							
1) T	Dalapon	0.000	2.638f	0	945.1E6	N.D.	480.104
2) T	3,5-DICHL...	6.397	6.681	6803538	21300912	2.065	12.851 #
5) T	DICAMBA	7.398	7.886	625615	8343745	<MDL	1.520 #
6) T	MCP	7.550	7.991	4522264	5377028	<MDL	1.645 #
7) T	MCPA	7.718	8.232	4999431	14585640	<MDL	3.148 #
8) T	DICHLORPROP	8.109	8.648f	8776895	84941780	3.308	61.567 #
9) T	2,4-D	8.341	8.985f	10172226	2480238	3.570	1.719 #
10) T	Pentachlo...	8.625	9.457	15284246	6813589	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.869f	0	35262438	N.D.	3.925
12) T	2,4,5-T	9.493	10.229f	38207864	68042065	2.348	7.813 #
13) T	2,4-DB	10.051	10.844	502.1E6	2063065	160.853	2.124 #
14) T	DINOSEB	0.000	11.198	0	18283523	N.D.	2.969
15) T	Picloram	11.080	12.283	316.4E6	80269316	11.799	6.252 #
16) T	DCPA	0.000	12.236	0	3172141	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122724\
Data File : PS028838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2024 21:08
Operator : AR\AJ
Sample : PB165896BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:07:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

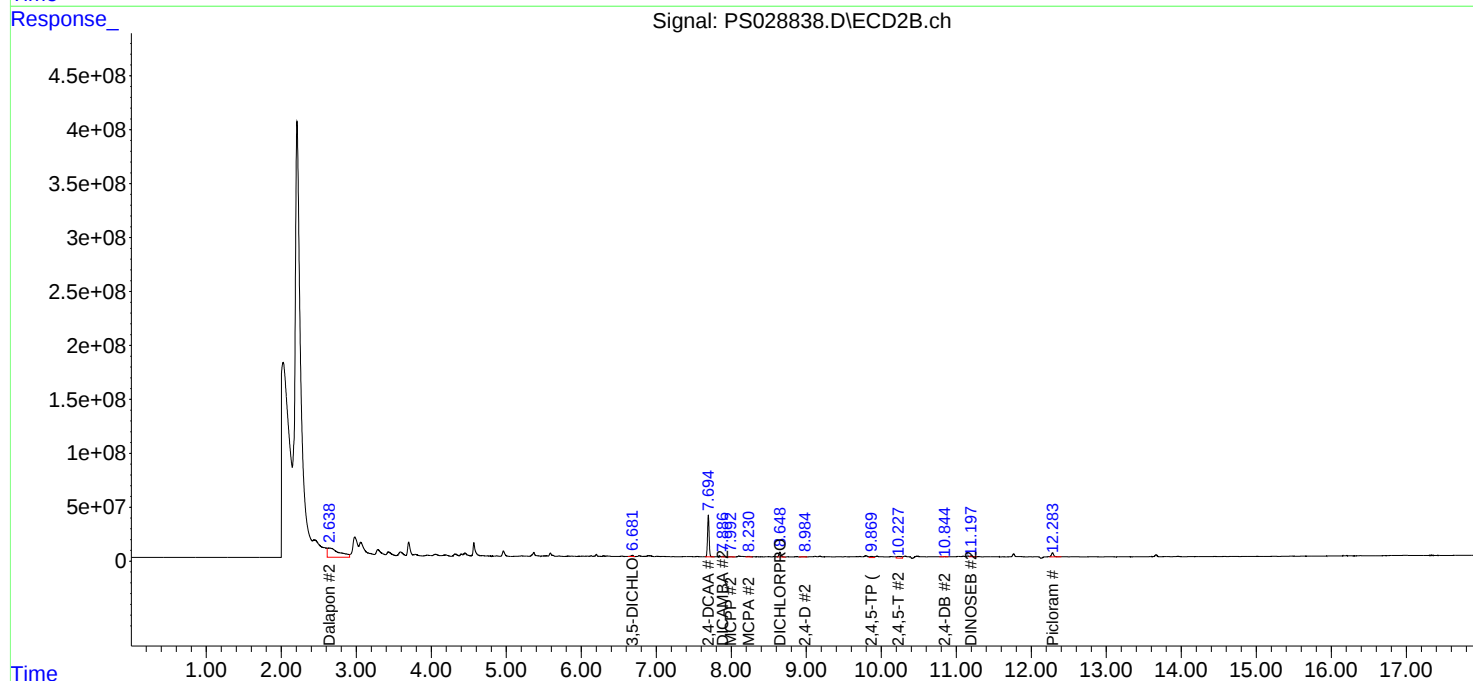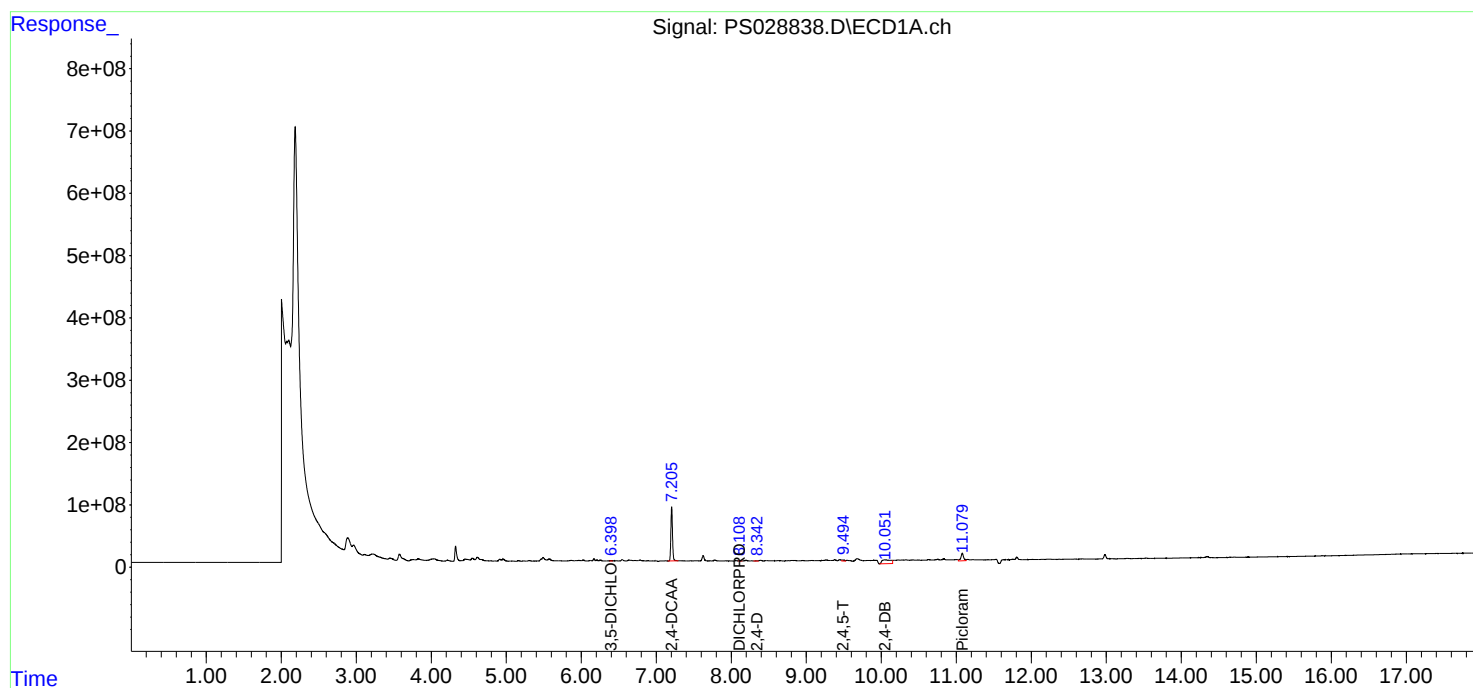


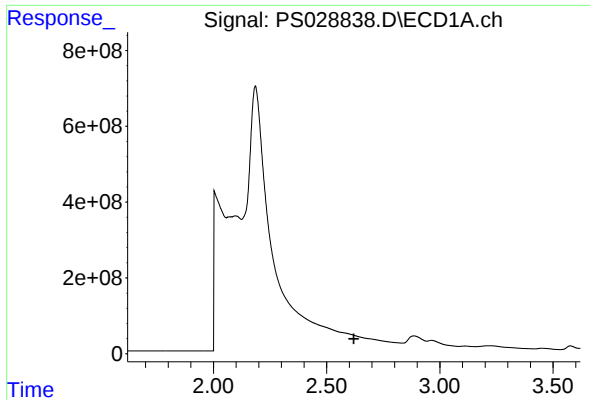

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

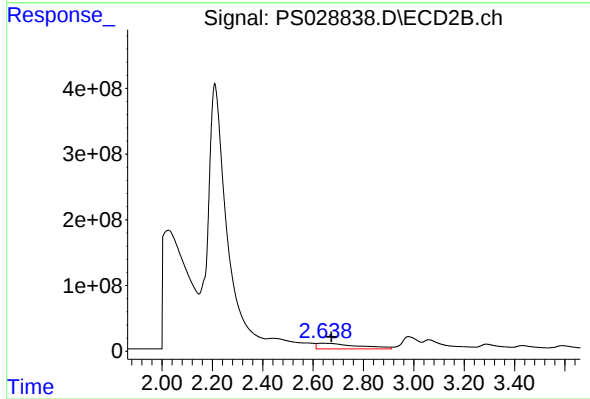


#1 Dalapon

R.T.: 2.638 min
Delta R.T.: -0.035 min
Response: 945133686
Conc: 480.10 ng/ml

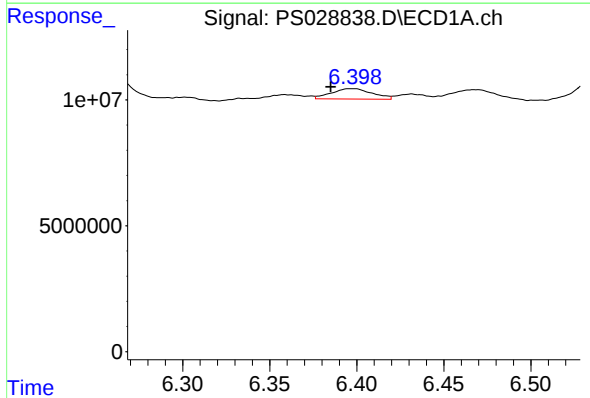


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.397 min
Delta R.T.: 0.012 min
Response: 6803538
Conc: 2.06 ng/ml

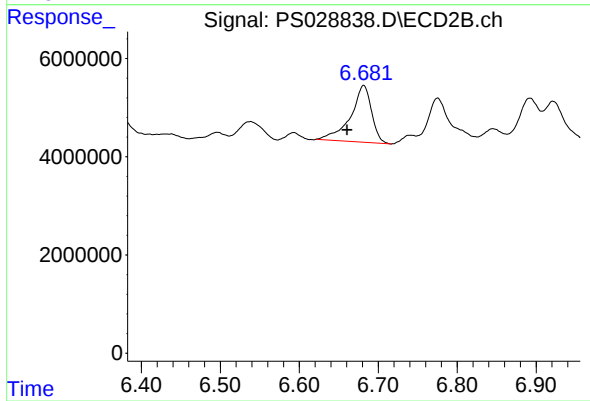

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.681 min
Delta R.T.: 0.021 min
Response: 21300912
Conc: 12.85 ng/ml

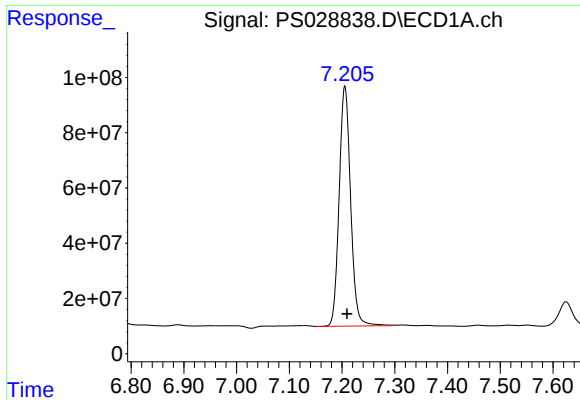

#4 2,4-DCAA


R.T.: 7.205 min
Delta R.T.: -0.004 min
Response: 1311518270
Conc: 579.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

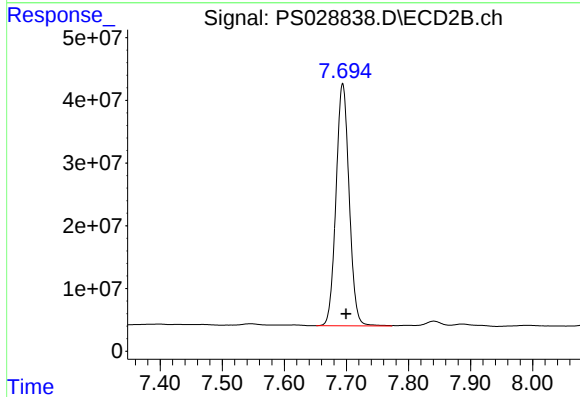


#4 2,4-DCAA

R.T.: 7.694 min
Delta R.T.: -0.005 min
Response: 567080708
Conc: 503.83 ng/ml

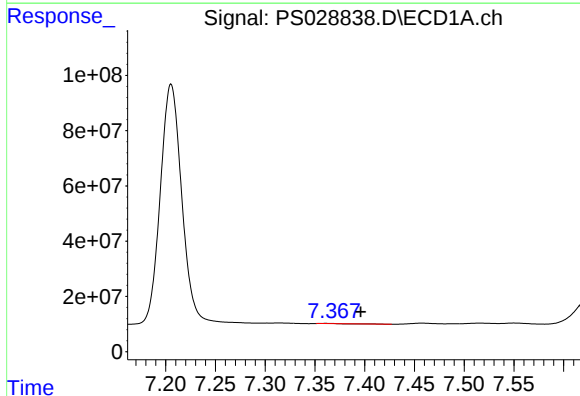


#5 DICAMBA

R.T.: 7.398 min
Delta R.T.: 0.002 min
Response: 625615
Conc: N.D.

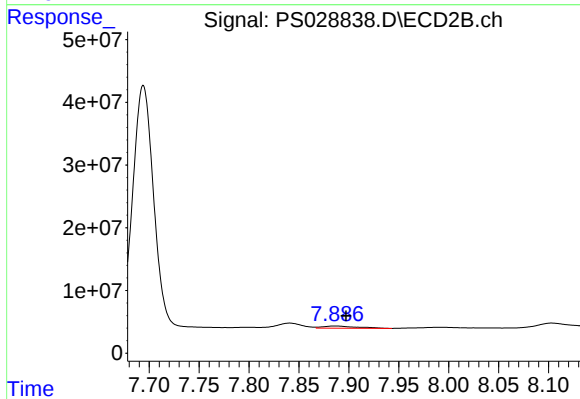

#5 DICAMBA


R.T.: 7.886 min
Delta R.T.: -0.011 min
Response: 8343745
Conc: 1.52 ng/ml

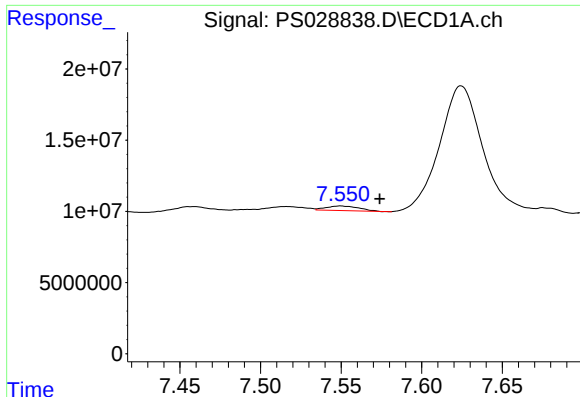

#6 MCP


R.T.: 7.550 min
Delta R.T.: -0.024 min
Response: 4522264
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

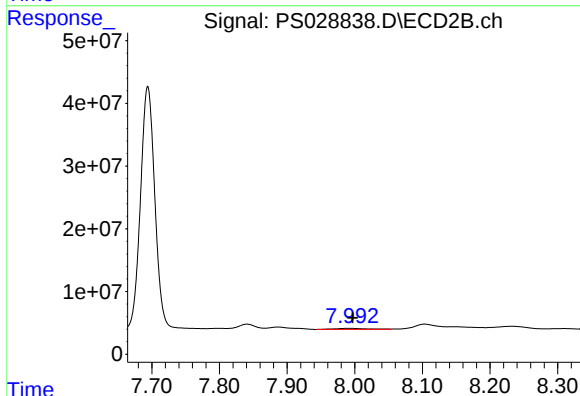


#6 MCP

R.T.: 7.991 min
Delta R.T.: -0.007 min
Response: 5377028
Conc: 1.65 ug/ml

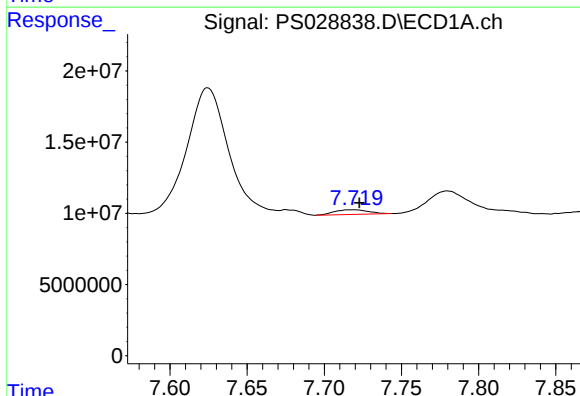


#7 MCPA

R.T.: 7.718 min
Delta R.T.: -0.005 min
Response: 4999431
Conc: N.D.

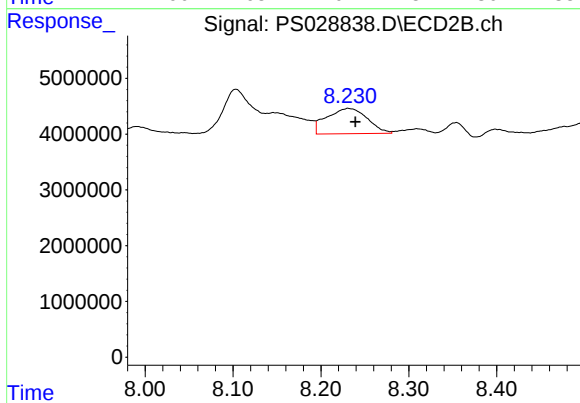

#7 MCPA


R.T.: 8.232 min
Delta R.T.: -0.008 min
Response: 14585640
Conc: 3.15 ug/ml

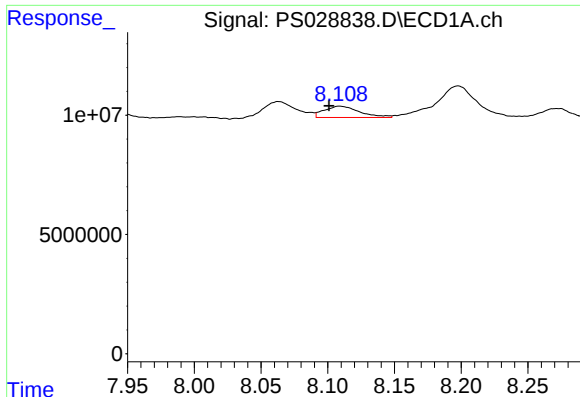

#8 DICHLORPROP


R.T.: 8.109 min
Delta R.T.: 0.008 min
Response: 8776895
Conc: 3.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

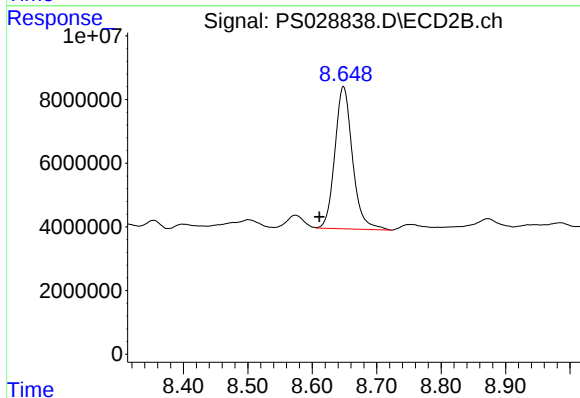


#8 DICHLORPROP

R.T.: 8.648 min
Delta R.T.: 0.037 min
Response: 84941780
Conc: 61.57 ng/ml

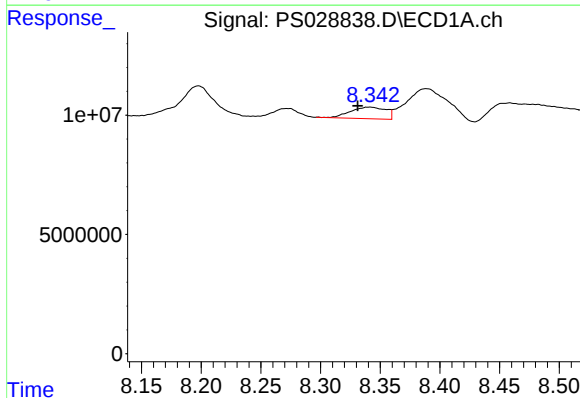


#9 2,4-D

R.T.: 8.341 min
Delta R.T.: 0.010 min
Response: 10172226
Conc: 3.57 ng/ml

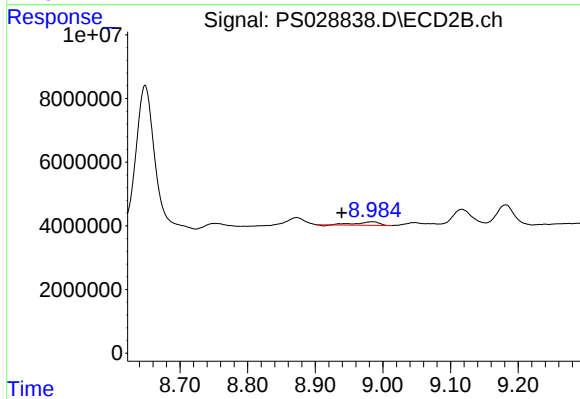

#9 2,4-D


R.T.: 8.985 min
Delta R.T.: 0.045 min
Response: 2480238
Conc: 1.72 ng/ml

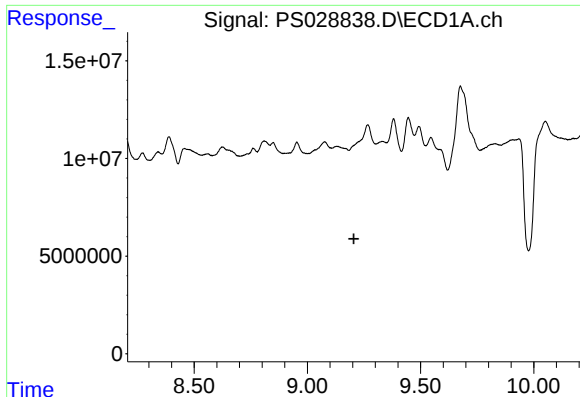

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

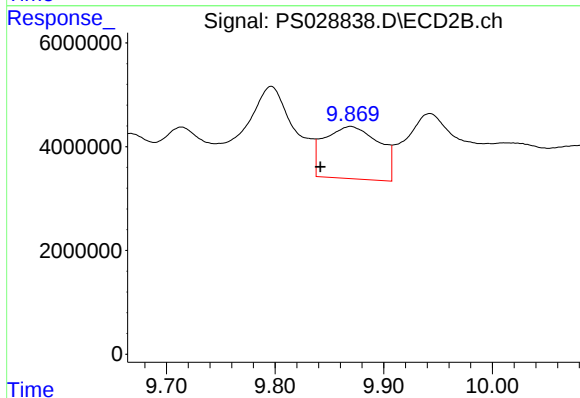


#11 2,4,5-TP (SILVEX)

R.T.: 9.869 min
Delta R.T.: 0.028 min
Response: 35262438
Conc: 3.93 ng/ml

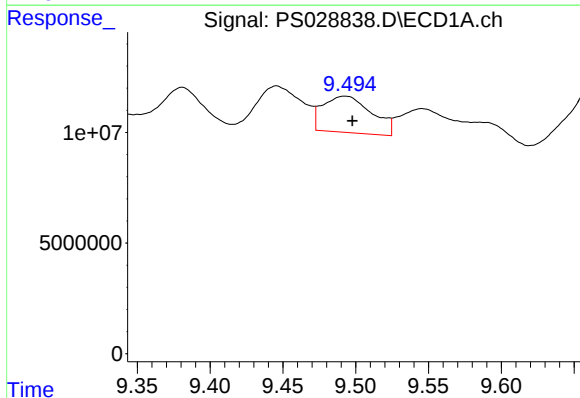


#12 2,4,5-T

R.T.: 9.493 min
Delta R.T.: -0.005 min
Response: 38207864
Conc: 2.35 ng/ml

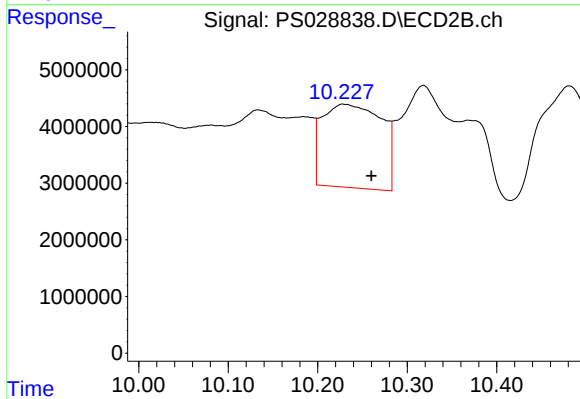

#12 2,4,5-T


R.T.: 10.229 min
Delta R.T.: -0.031 min
Response: 68042065
Conc: 7.81 ng/ml

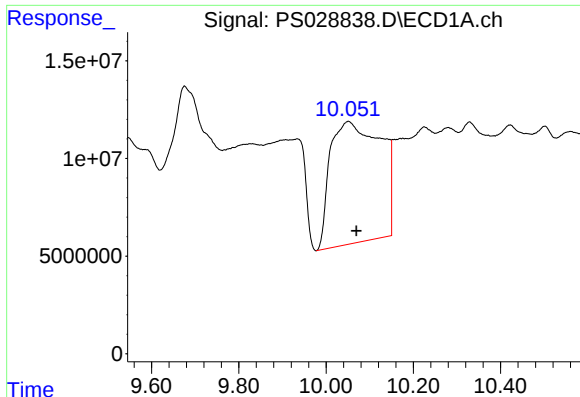

#13 2,4-DB


R.T.: 10.051 min
Delta R.T.: -0.018 min
Response: 502119623
Conc: 160.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

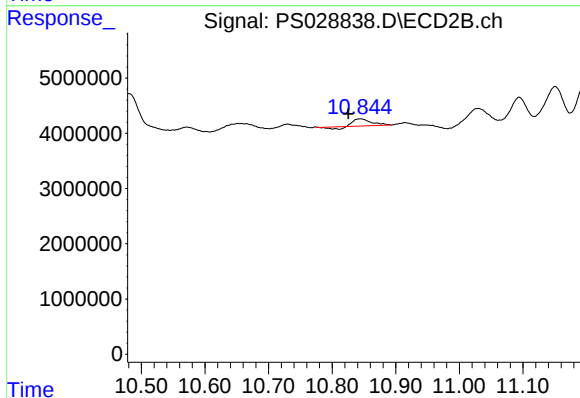


#13 2,4-DB

R.T.: 10.844 min
Delta R.T.: 0.018 min
Response: 2063065
Conc: 2.12 ng/ml

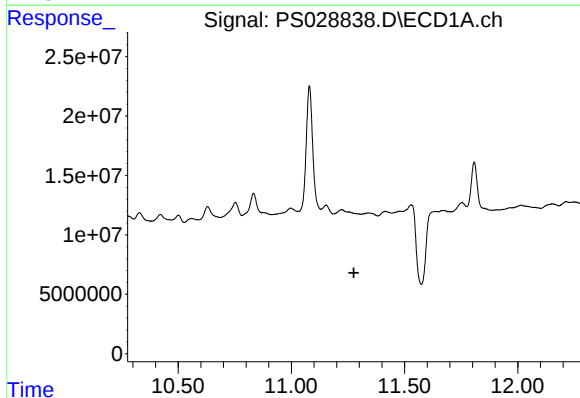


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.276 min
Response: 0
Conc: N.D.

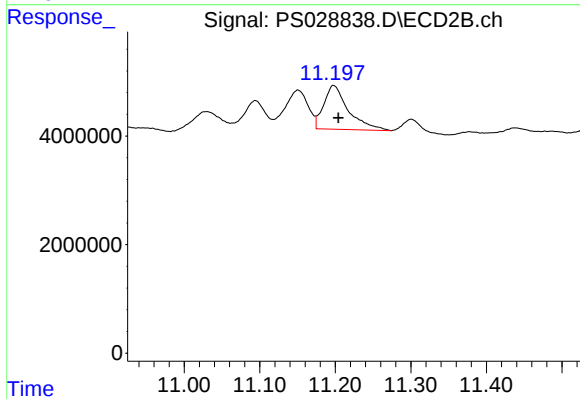

#14 DINOSEB


R.T.: 11.198 min
Delta R.T.: -0.006 min
Response: 18283523
Conc: 2.97 ng/ml

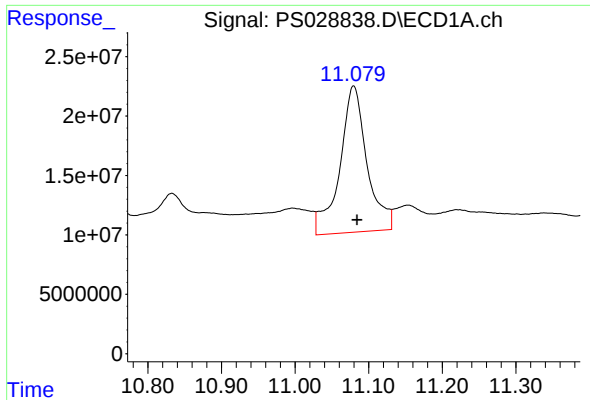

#15 Picloram

R.T.: 11.080 min
Delta R.T.: -0.004 min
Response: 316354922
Conc: 11.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

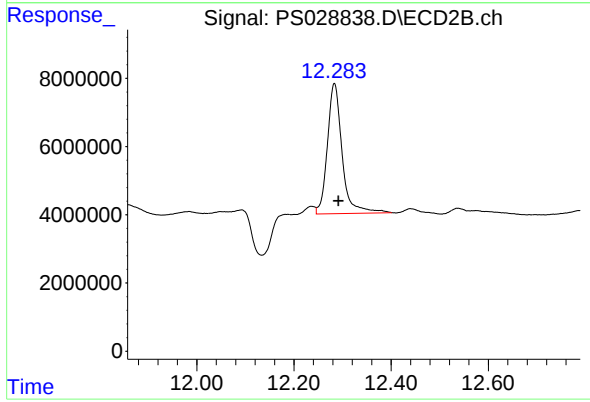

#15 Picloram

R.T.: 12.283 min
Delta R.T.: -0.009 min
Response: 80269316
Conc: 6.25 ng/ml