

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122818\
 Data File : PS002702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2018 12:07
 Operator : EI\SJ
 Sample : J6547-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 15:15:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.412	10.909	38232613	36769657	120.448	95.069
Target Compounds							
1) T	Dalapon	2.888	0.000	6075227	0	13.198	N.D. #
2) T	3,5-DICHL...	0.000	9.005	0	3770247	N.D.	7.846 #
5) T	DICAMBA	0.000	11.148	0	76678710	N.D.	53.787 #
6) T	MCP	12.089	0.000	60170616	0	60.306	N.D. #
7) T	MCPA	0.000	11.813	0	379785	N.D.	0.264 #
8) T	DICHLORPROP	0.000	12.263	0	120863	N.D.	0.338 #
10) T	Pentachlo...	13.641	13.328	7321171	6331232	1.460	1.203
14) T	DINOSEB	0.000	15.643	0	1604043	N.D.	1.051 #
16) T	DCPA	0.000	16.879	0	4561748	N.D.	1.570 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122818\
Data File : PS002702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2018 12:07
Operator : EI\SJ
Sample : J6547-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 15:15:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

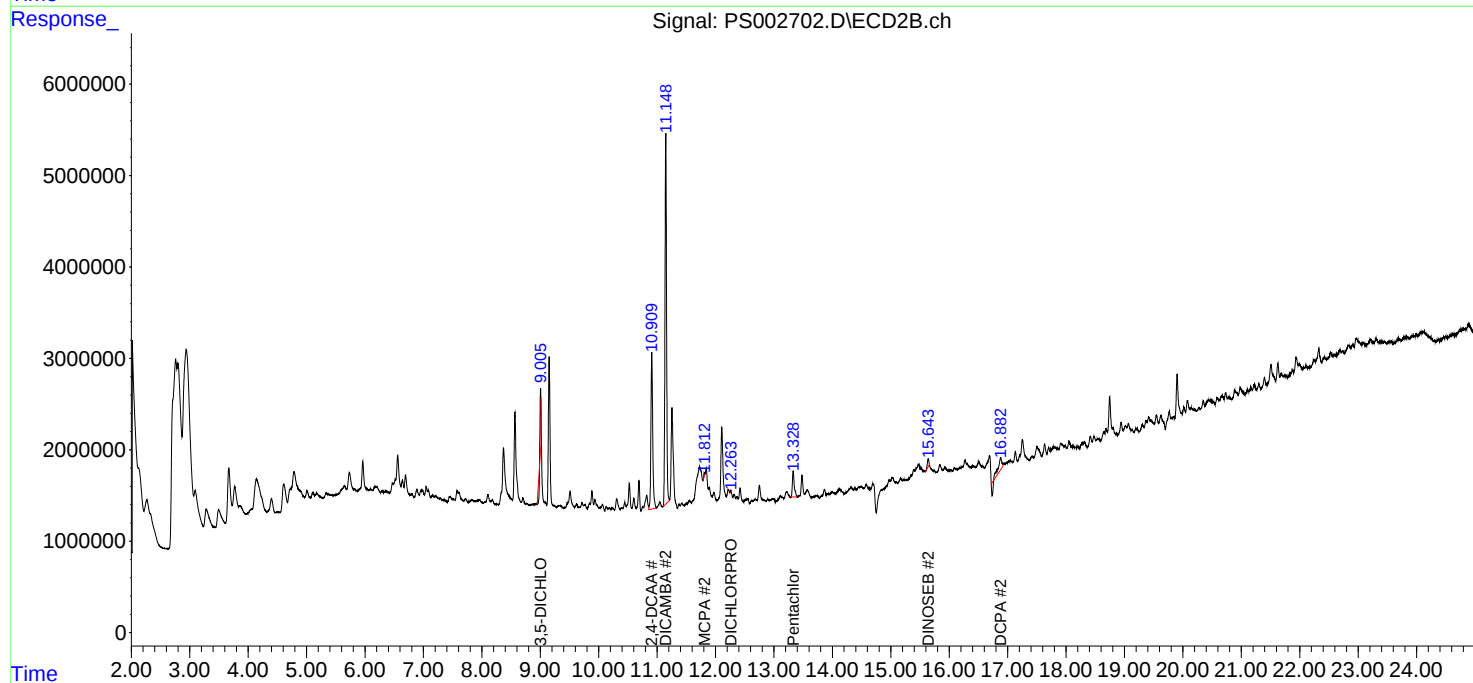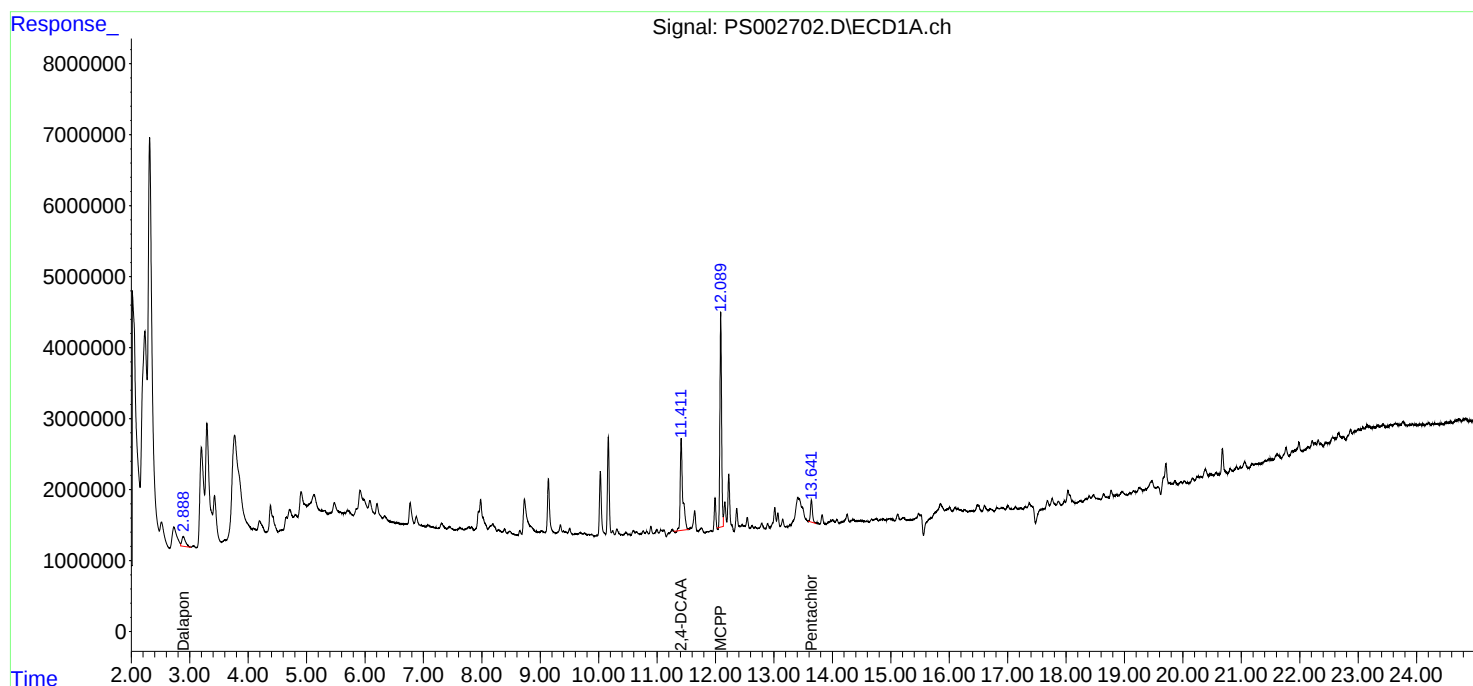


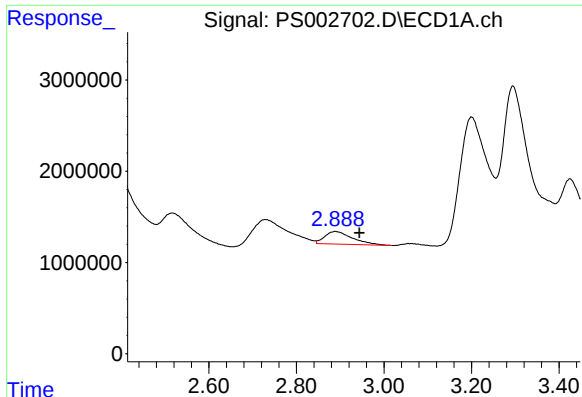

#1 Dalapon


R.T.: 2.888 min
Delta R.T.: -0.056 min
Response: 6075227
Conc: 13.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

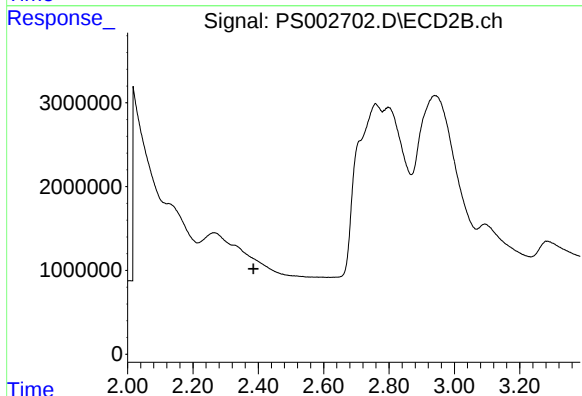


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.385 min
Response: 0
Conc: N.D.

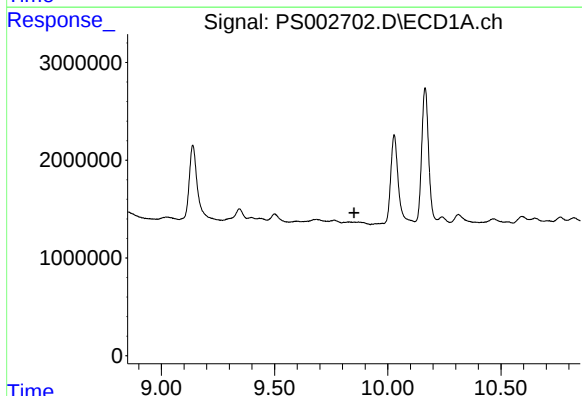


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.851 min
Response: 0
Conc: N.D.

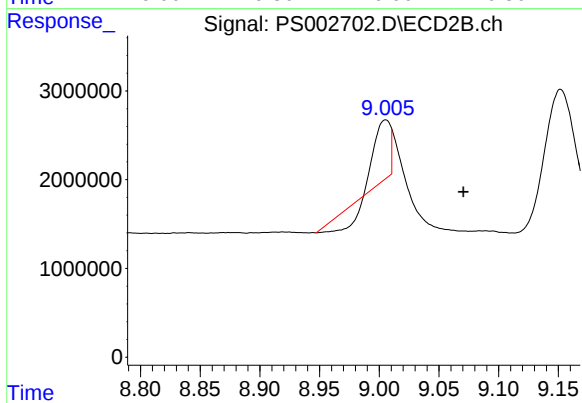

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.005 min
Delta R.T.: -0.065 min
Response: 3770247
Conc: 7.85 ng/ml

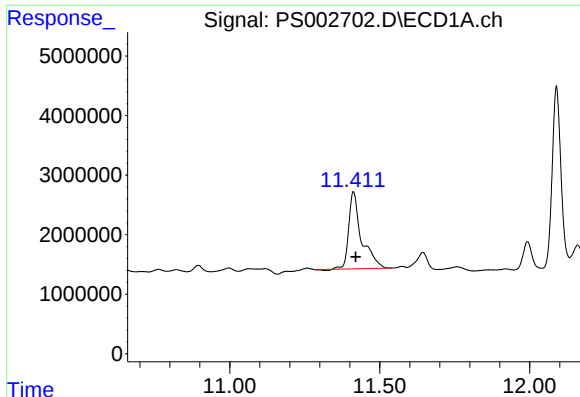

#4 2,4-DCAA


R.T.: 11.412 min
Delta R.T.: -0.008 min
Response: 38232613
Conc: 120.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

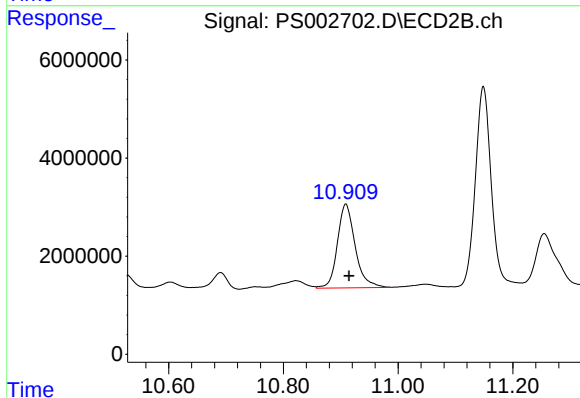


#4 2,4-DCAA

R.T.: 10.909 min
Delta R.T.: -0.006 min
Response: 36769657
Conc: 95.07 ng/ml

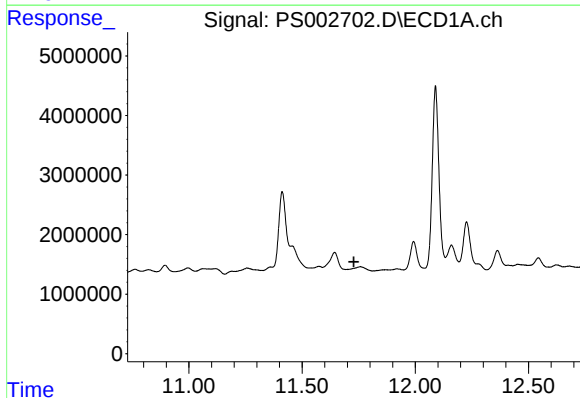


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.729 min
Response: 0
Conc: N.D.

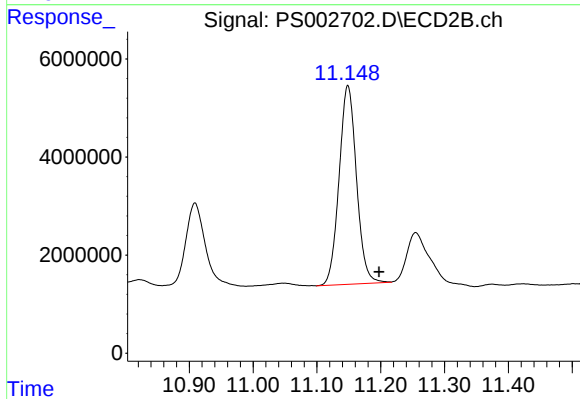

#5 DICAMBA


R.T.: 11.148 min
Delta R.T.: -0.049 min
Response: 76678710
Conc: 53.79 ng/ml

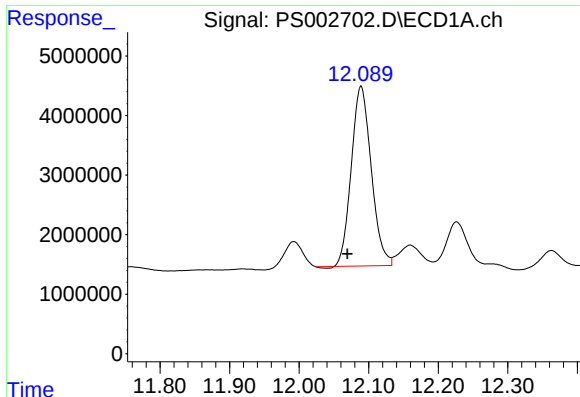

#6 MCPP


R.T.: 12.089 min
Delta R.T.: 0.020 min
Response: 60170616
Conc: 60.31 ug/ml

Instrument :
ECD_S
ClientSampleId :

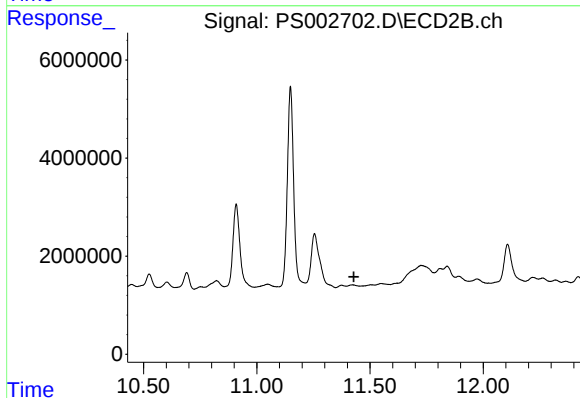


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.429 min
Response: 0
Conc: N.D.

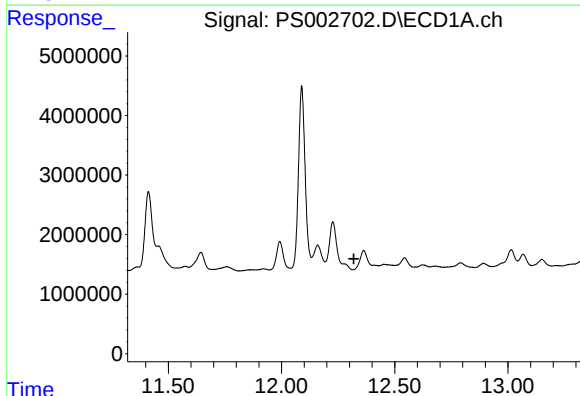


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.319 min
Response: 0
Conc: N.D.

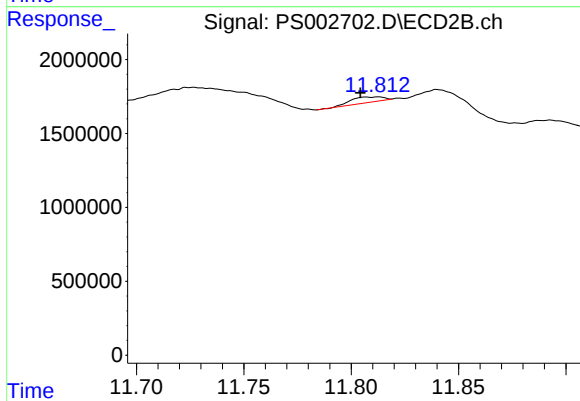

#7 MCPA


R.T.: 11.813 min
Delta R.T.: 0.008 min
Response: 379785
Conc: 0.26 ug/ml

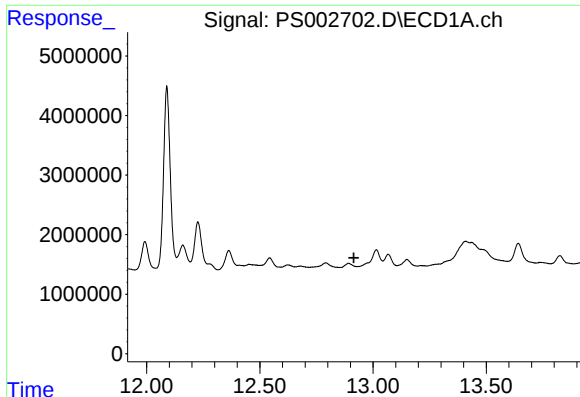

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

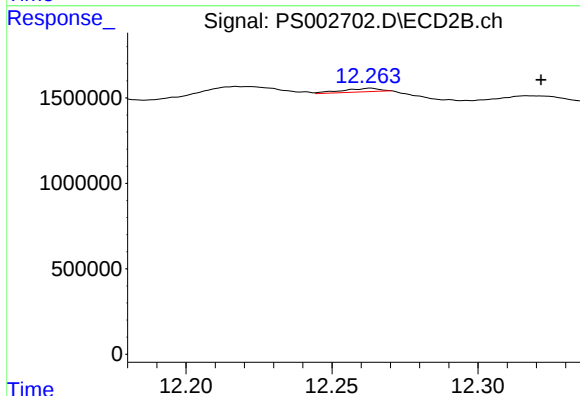


#8 DICHLORPROP

R.T.: 12.263 min
Delta R.T.: -0.058 min
Response: 120863
Conc: 0.34 ng/ml

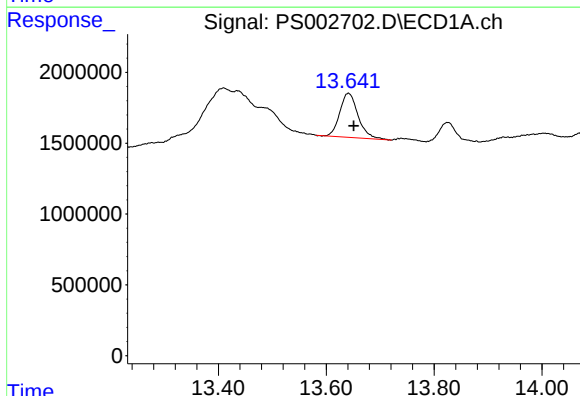


#10 Pentachlorophenol

R.T.: 13.641 min
Delta R.T.: -0.010 min
Response: 7321171
Conc: 1.46 ng/ml

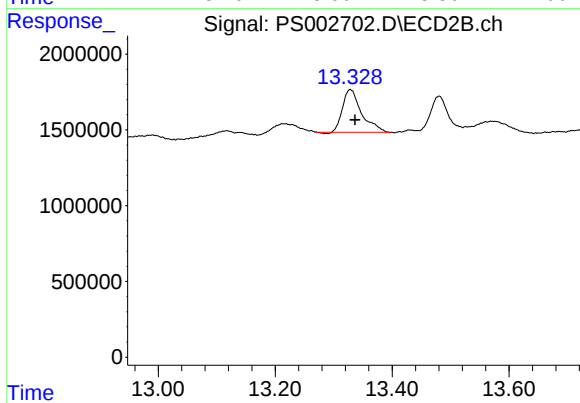

#10 Pentachlorophenol


R.T.: 13.328 min
Delta R.T.: -0.008 min
Response: 6331232
Conc: 1.20 ng/ml

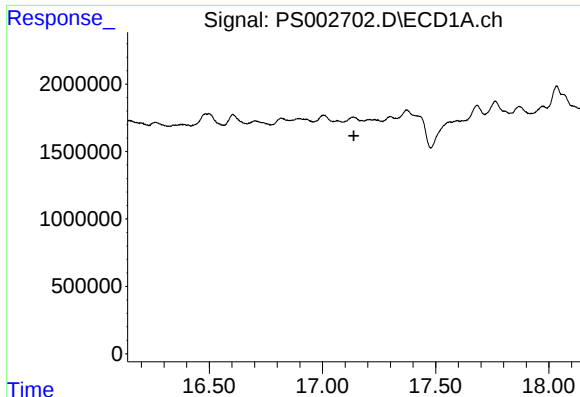

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

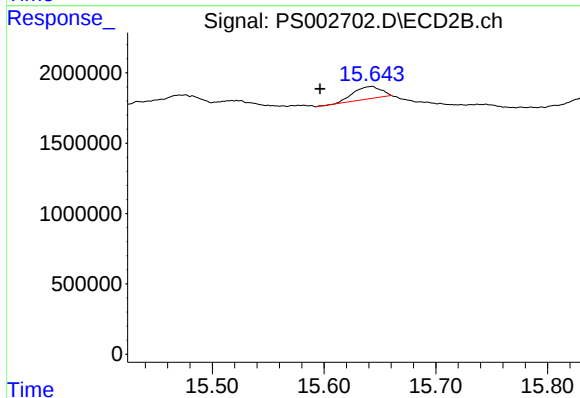


#14 DINOSEB

R.T.: 15.643 min
Delta R.T.: 0.046 min
Response: 1604043
Conc: 1.05 ng/ml

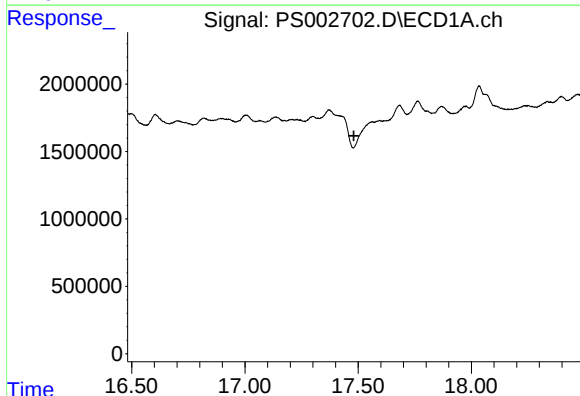

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.481 min
Response: 0
Conc: N.D.

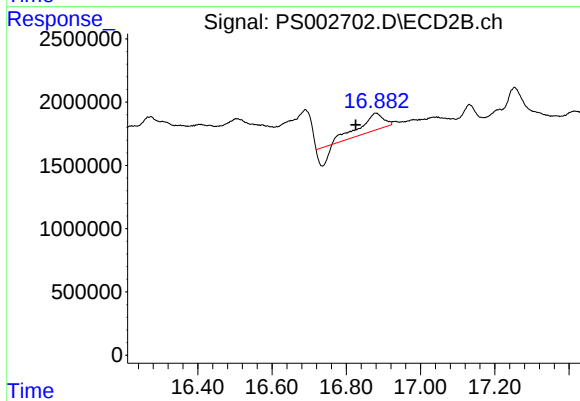

#16 DCPA

R.T.: 16.879 min
Delta R.T.: 0.054 min
Response: 4561748
Conc: 1.57 ng/ml