

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122818\
 Data File : PS002721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2018 19:25
 Operator : EI\SJ
 Sample : J6584-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RECLAIMER-PIT

Manual Integrations
 APPROVED

Sohil
 1/2/2019 12:09:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 07:25:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	11.388	10.888	170.5E6	178.1E6	537.172m	460.579
------	----------	--------	--------	---------	---------	----------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122818\
Data File : PS002721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2018 19:25
Operator : EI\SJ
Sample : J6584-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
RECLAIMER-PIT


Manual Integrations
APPROVED

Sohil
1/2/2019 12:09:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 07:25:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

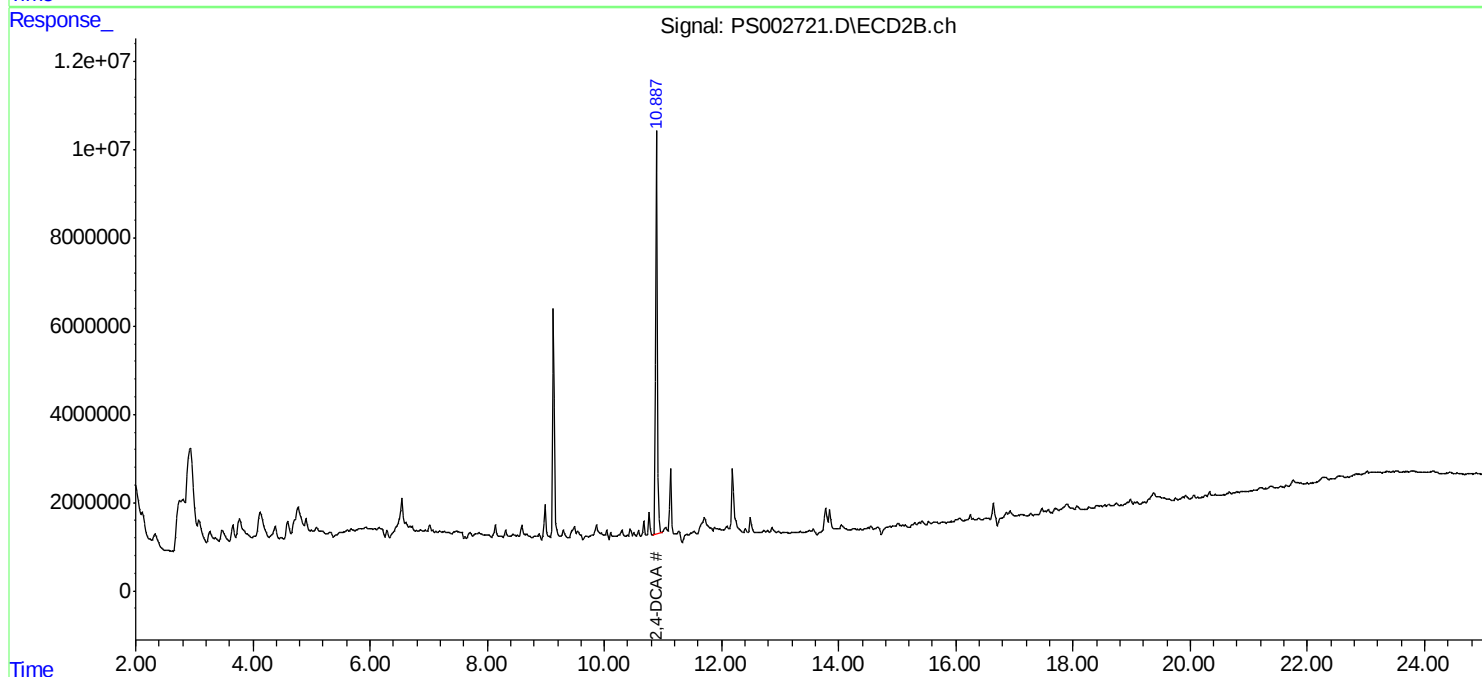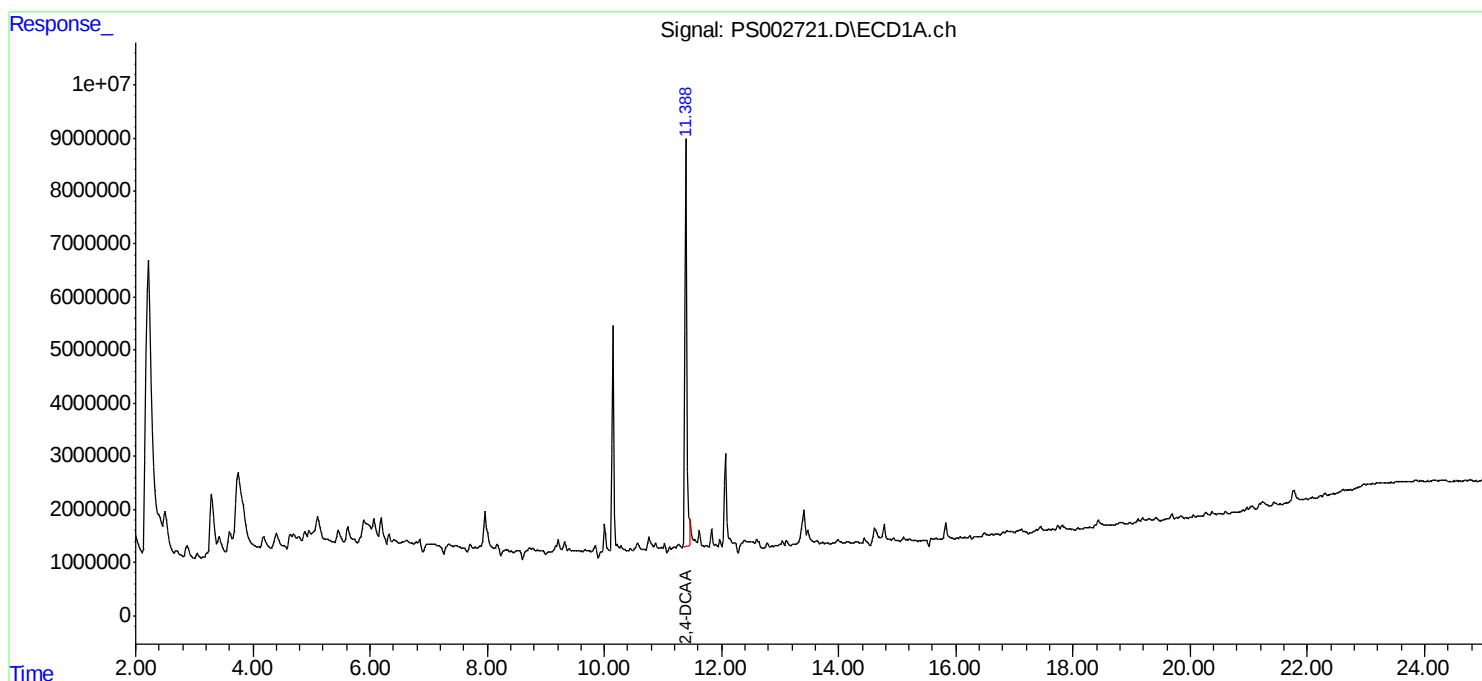

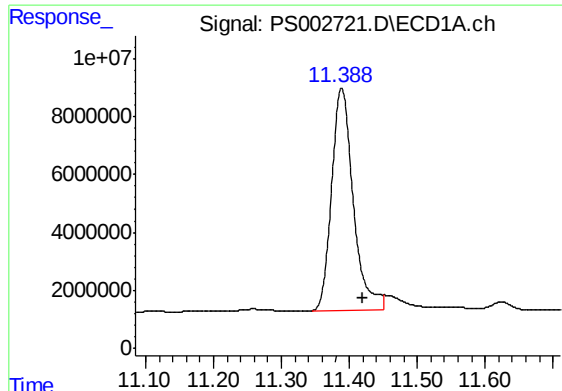


#4 2,4-DCAA

R.T.: 11.388 min
Delta R.T.: -0.032 min
Response: 170508876
Conc: 537.17 ng/ml m

Instrument :
ECD_S
ClientSampleId :
RECLAIMER-PIT

Manual Integrations
APPROVED

Sohil
1/2/2019 12:09:50 PM

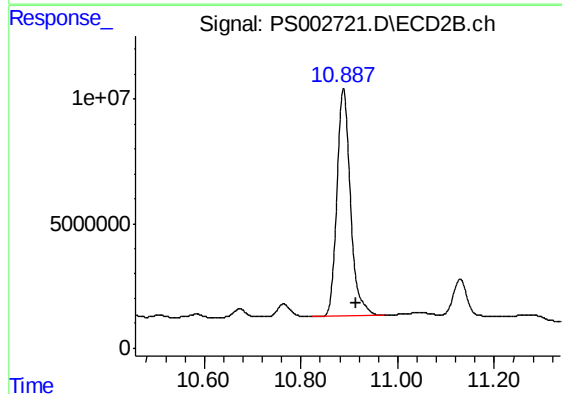

#4 2,4-DCAA

R.T.: 10.888 min
Delta R.T.: -0.027 min
Response: 178137864
Conc: 460.58 ng/ml