

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS122821\  
 Data File : PS017860.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 29 Dec 2021 01:09  
 Operator : AJ\MA  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 29 01:30:13 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS121421.M  
 Quant Title : 8080.M  
 QLast Update : Tue Dec 14 13:29:21 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|-------|---------|---------|---------|---------|
| -----                       |              |        |       |         |         |         |         |
| System Monitoring Compounds |              |        |       |         |         |         |         |
| 4) S                        | 2,4-DCAA     | 7.127  | 6.717 | 692.9E6 | 280.9E6 | 443.321 | 471.189 |
| Target Compounds            |              |        |       |         |         |         |         |
| 2) T                        | 3,5-DICHL... | 6.396  | 0.000 | 6311232 | 0       | 2.825   | N.D. #  |
| 15) T                       | Picloram     | 10.886 | 0.000 | 4112573 | 0       | <MDL    | N.D. #  |
| -----                       |              |        |       |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS122821\  
Data File : PS017860.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 29 Dec 2021 01:09  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 29 01:30:13 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS121421.M  
Quant Title : 8080.M  
QLast Update : Tue Dec 14 13:29:21 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

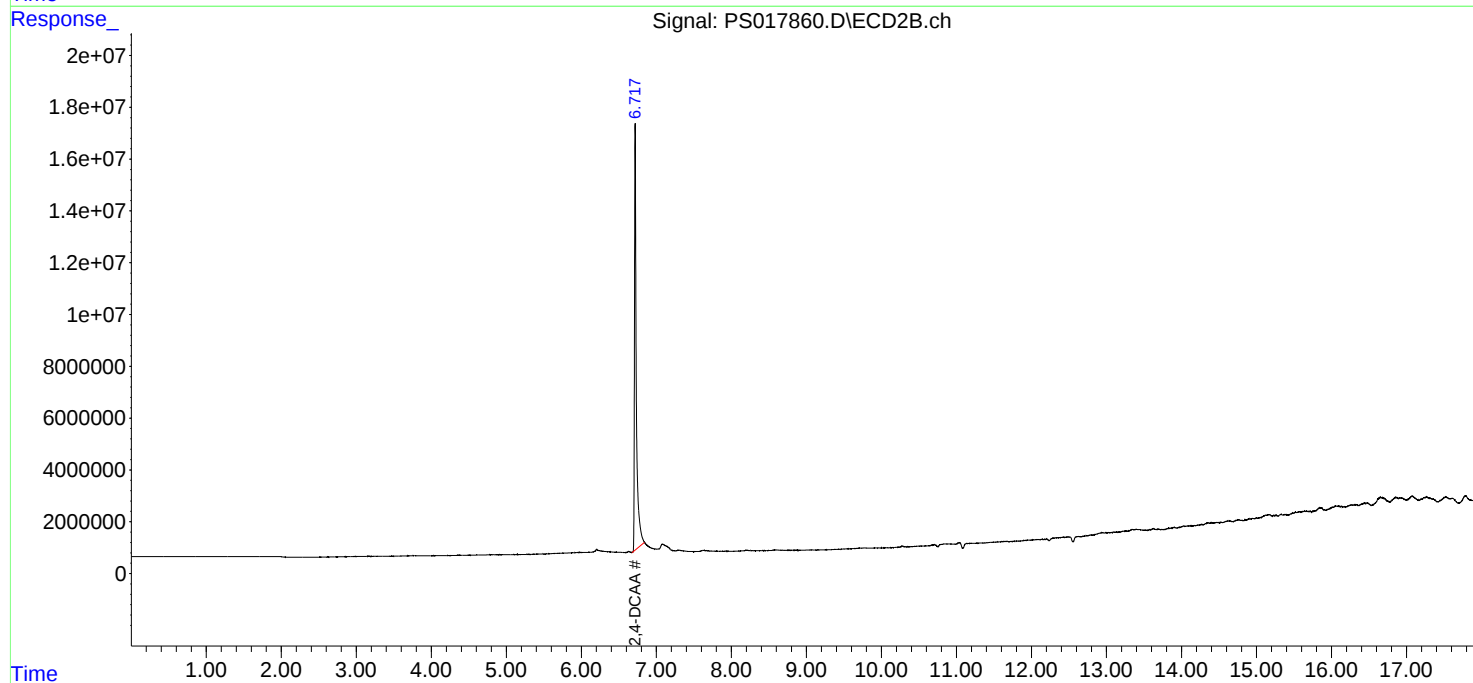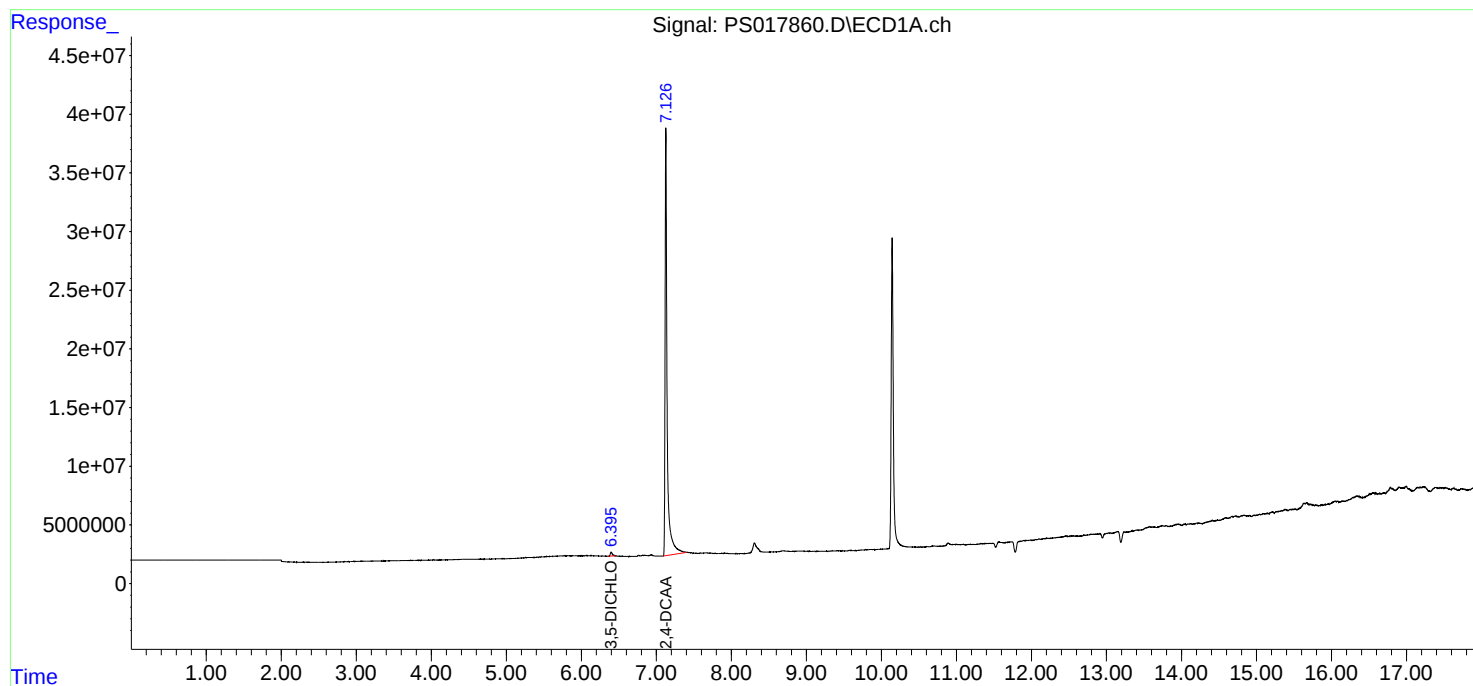


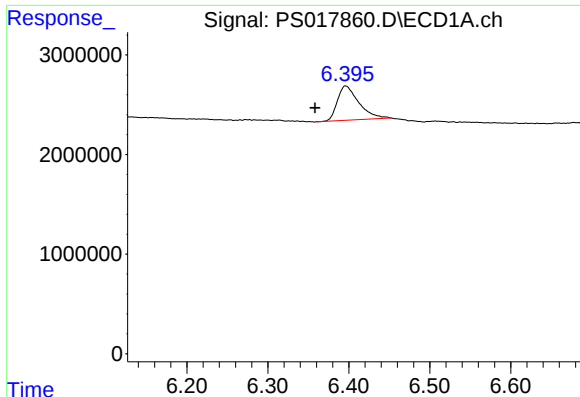

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.396 min  
Delta R.T.: 0.038 min  
Response: 6311232  
Conc: 2.82 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

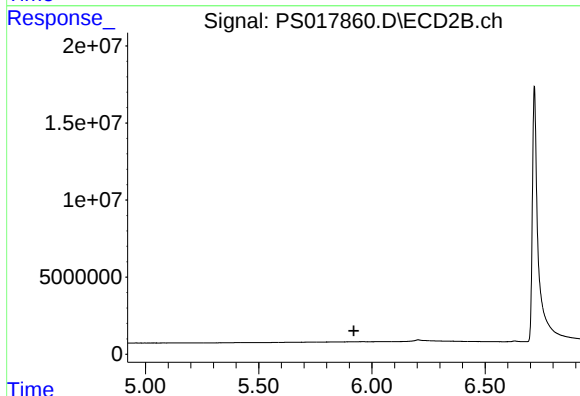


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 5.921 min  
Response: 0  
Conc: N.D.

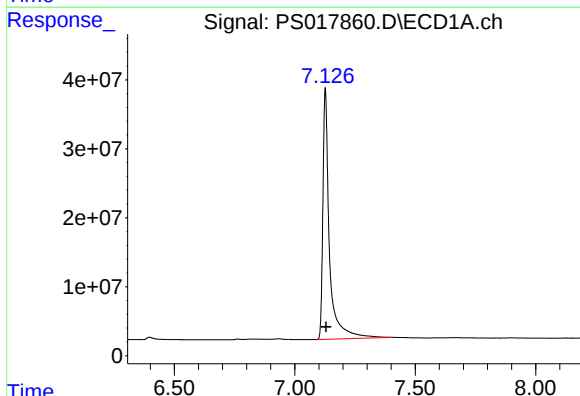

#4 2,4-DCAA

R.T.: 7.127 min  
Delta R.T.: -0.003 min  
Response: 692885889  
Conc: 443.32 ng/ml

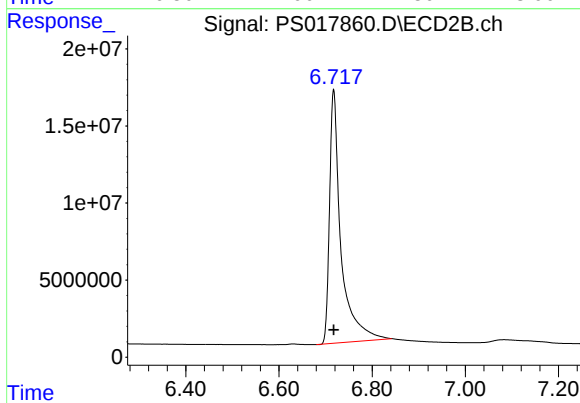

#4 2,4-DCAA

R.T.: 6.717 min  
Delta R.T.: 0.000 min  
Response: 280876752  
Conc: 471.19 ng/ml