

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122822\
 Data File : PS021573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2022 09:13
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 20:58:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.394	0.000	887788	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.502	0.000	617139	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.766	0.000	2600433	0	<MDL	N.D. #
3) T	4-Nitroph...	6.214	6.409	2930953	962963	1.630	<MDL #
5) T	DICAMBA	6.525	6.972	890812	1920644	<MDL	<MDL #
6) T	MCPD	6.698	7.114f	-704348	1138844	N.D.	<MDL
7) T	MCPA	6.839f	0.000	234431	0	<MDL	N.D. #
8) T	DICHLORPROP	7.136	7.628	328275	2430327	<MDL	1.234 #
9) T	2,4-D	7.307	7.909	7222984	787282	1.890	<MDL #
10) T	Pentachlo...	7.553	8.314	2418831	1350872	<MDL	<MDL #
11) T	2,4,5-TP ...	8.087	8.680	3366882	887847	<MDL	<MDL #
12) T	2,4,5-T	8.360	9.068	12958366	2700995	<MDL	<MDL #
13) T	2,4-DB	0.000	9.636f	0	1185665	N.D.	<MDL
15) T	Picloram	9.726	10.879	3986378	109.7E6	<MDL	6.744 #
16) T	DCPA	10.170	10.813	1804049	17387344	<MDL	1.281 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122822\
Data File : PS021573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2022 09:13
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 20:58:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

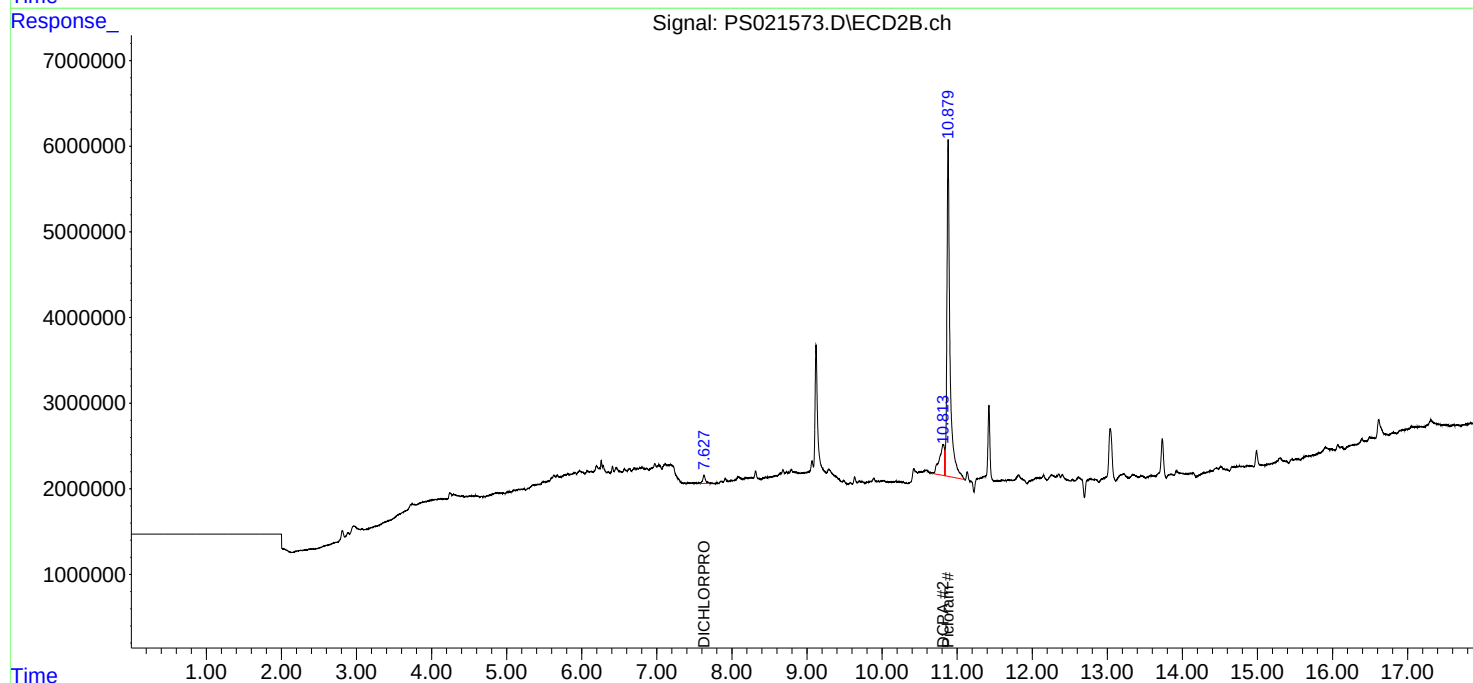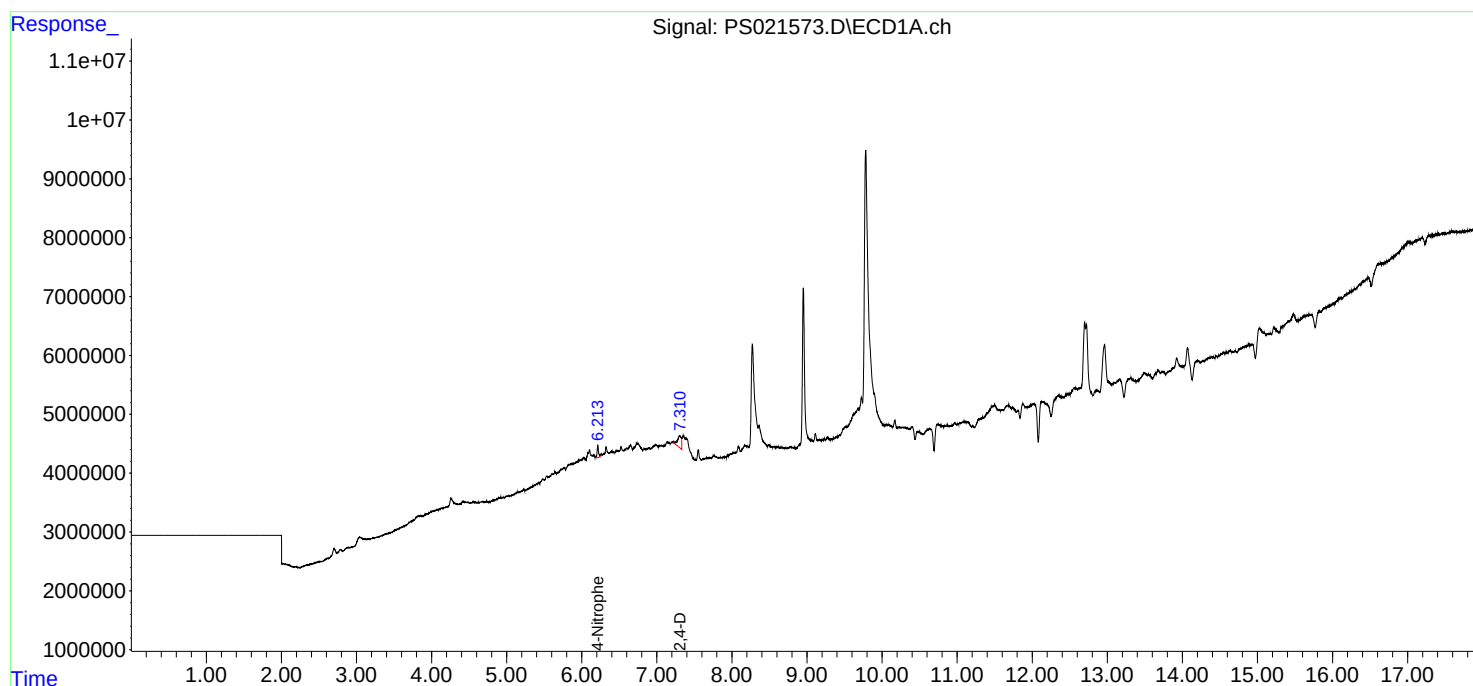


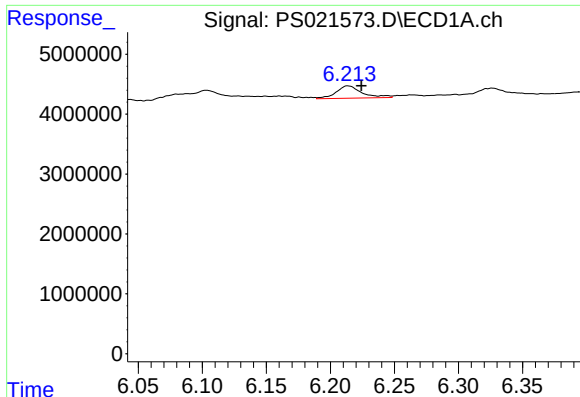

#3 4-Nitrophenol


R.T.: 6.214 min
Delta R.T.: -0.011 min
Response: 2930953
Conc: 1.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

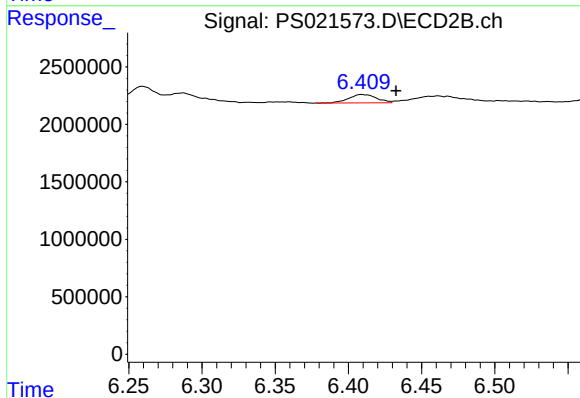


#3 4-Nitrophenol

R.T.: 6.409 min
Delta R.T.: -0.023 min
Response: 962963
Conc: N.D.

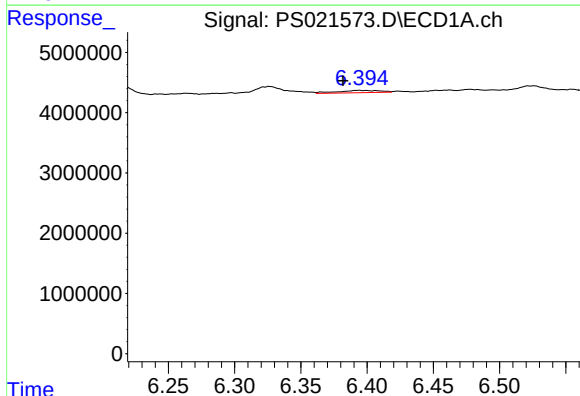


#4 2,4-DCAA

R.T.: 6.394 min
Delta R.T.: 0.012 min
Response: 887788
Conc: N.D.

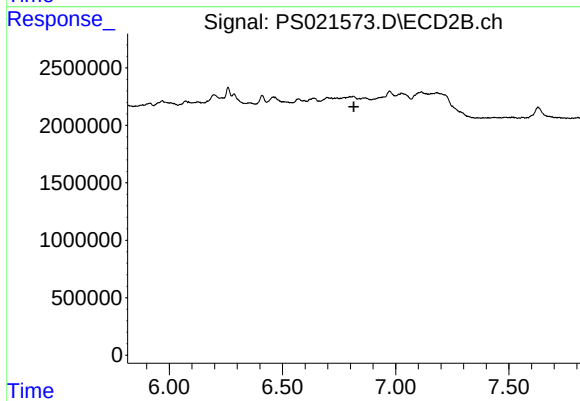

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.816 min
Response: 0
Conc: N.D.

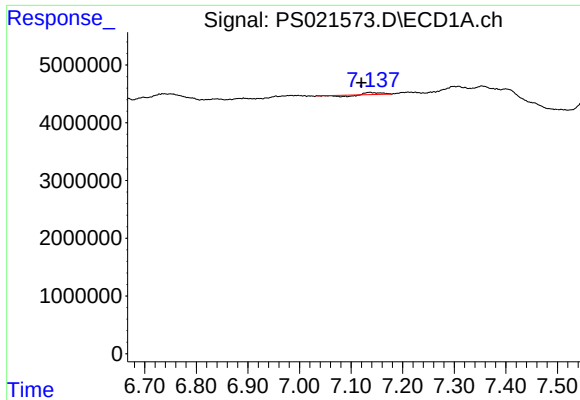

#8 DICHLORPROP


R.T.: 7.136 min
Delta R.T.: 0.015 min
Response: 328275
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

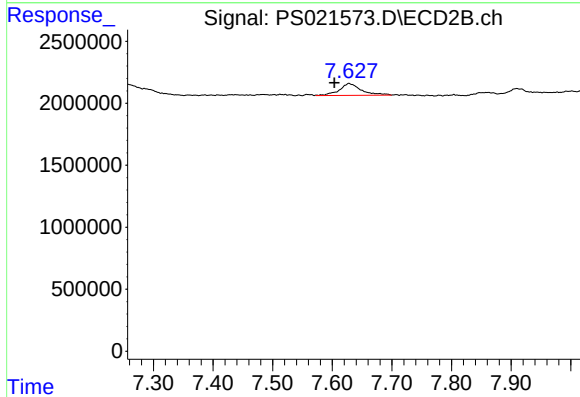


#8 DICHLORPROP

R.T.: 7.628 min
Delta R.T.: 0.024 min
Response: 2430327
Conc: 1.23 ng/ml

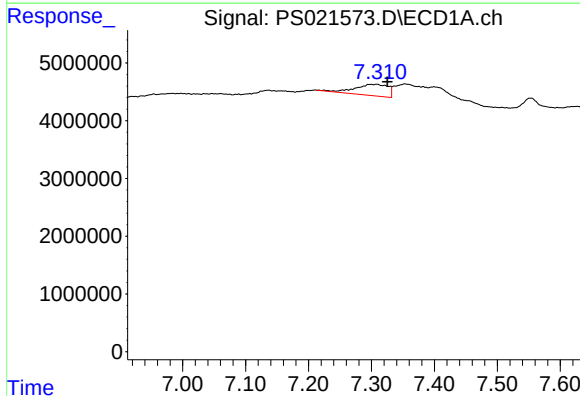


#9 2,4-D

R.T.: 7.307 min
Delta R.T.: -0.018 min
Response: 7222984
Conc: 1.89 ng/ml

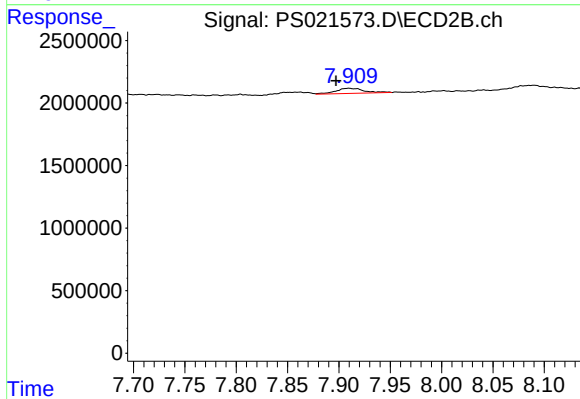

#9 2,4-D


R.T.: 7.909 min
Delta R.T.: 0.012 min
Response: 787282
Conc: N.D.

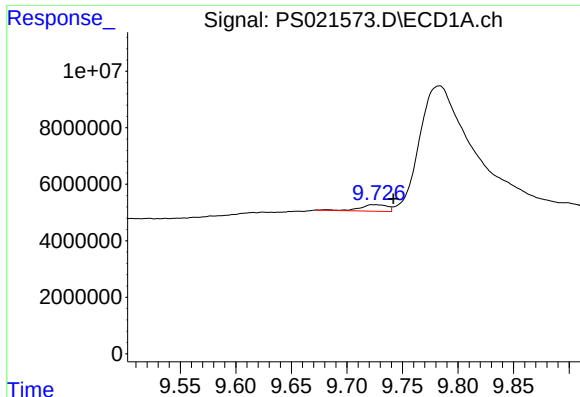

#15 Picloram


R.T.: 9.726 min
Delta R.T.: -0.016 min
Response: 3986378
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

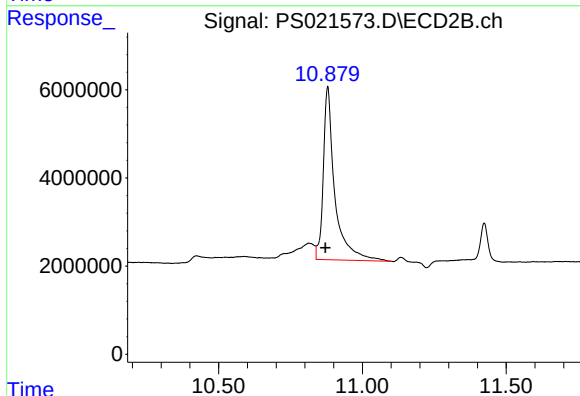


#15 Picloram

R.T.: 10.879 min
Delta R.T.: 0.007 min
Response: 109671930
Conc: 6.74 ng/ml

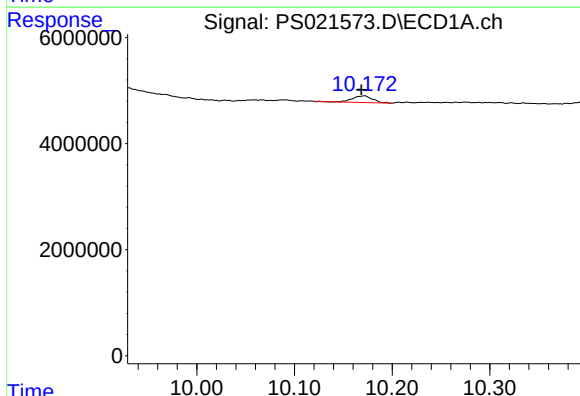

#16 DCPA

R.T.: 10.170 min
Delta R.T.: 0.002 min
Response: 1804049
Conc: N.D.

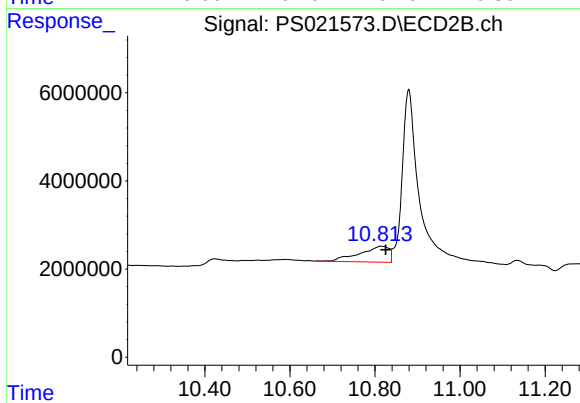

#16 DCPA

R.T.: 10.813 min
Delta R.T.: -0.012 min
Response: 17387344
Conc: 1.28 ng/ml