

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122822\
 Data File : PS021574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2022 09:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 20:58:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.378	6.809	1290.6E6	977.9E6	444.188	567.208 #
Target Compounds							
1) T	Dalapon	2.467	0.000	441653	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.734	0.000	5141761	0	1.294	N.D. #
3) T	4-Nitroph...	6.228	0.000	5002548	0	2.782	N.D. #
6) T	MCP	0.000	7.116f	0	4498782	N.D.	<MDL
7) T	MCPA	6.766	7.220f	3392428	20778683	<MDL	2.350 #
8) T	DICHLORPROP	0.000	7.669f	0	1552349	N.D.	<MDL
9) T	2,4-D	7.318	7.961f	781289	501546	<MDL	<MDL #
10) T	Pentachlo...	7.552	0.000	1141394	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.088	8.688	7527207	1693640	<MDL	<MDL #
12) T	2,4,5-T	8.337	9.092	38073294	1727473	2.018	<MDL #
13) T	2,4-DB	8.872	9.636f	579930	2531640	<MDL	1.761 #
14) T	DINOSEB	9.843f	0.000	129.4E6	0	8.121	N.D. #
15) T	Picloram	9.757	10.909	1772146	76841190	<MDL	4.725 #
16) T	DCPA	10.165	10.817	2393997	1207269	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122822\
Data File : PS021574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2022 09:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 20:58:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

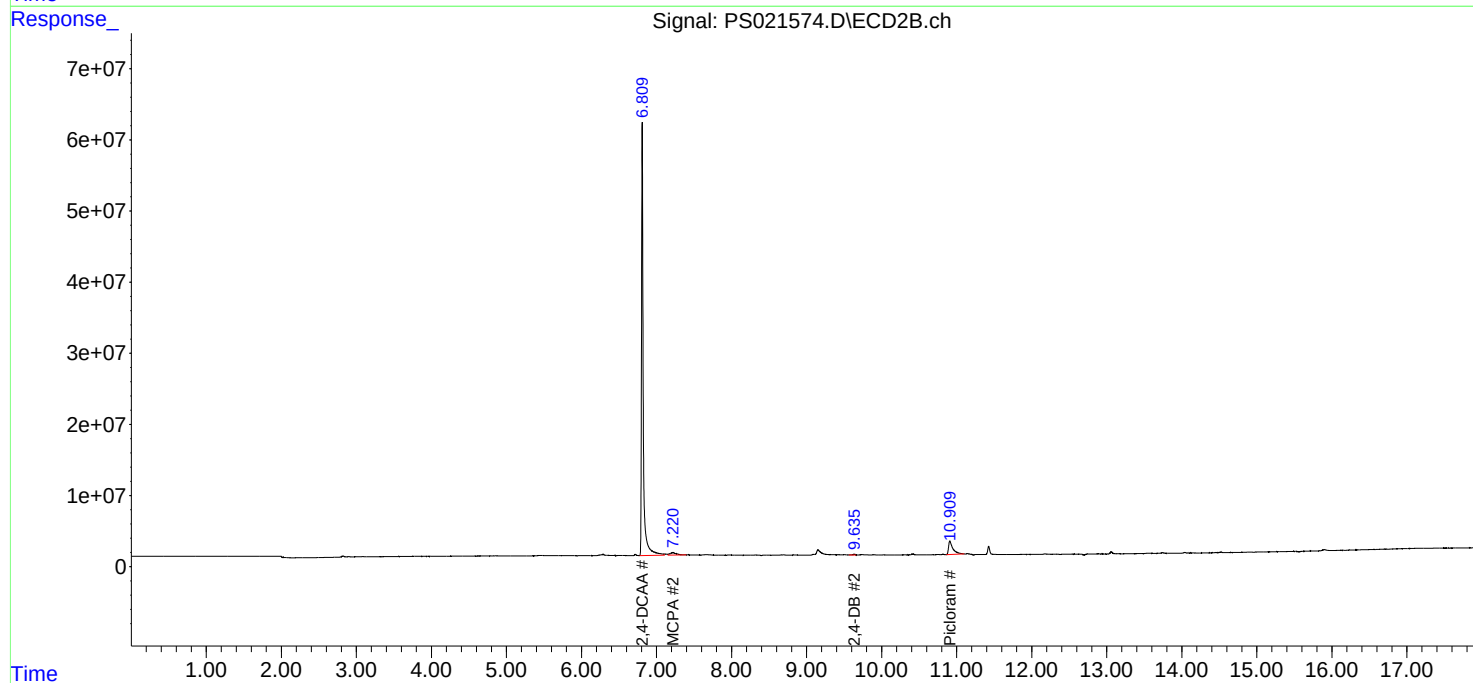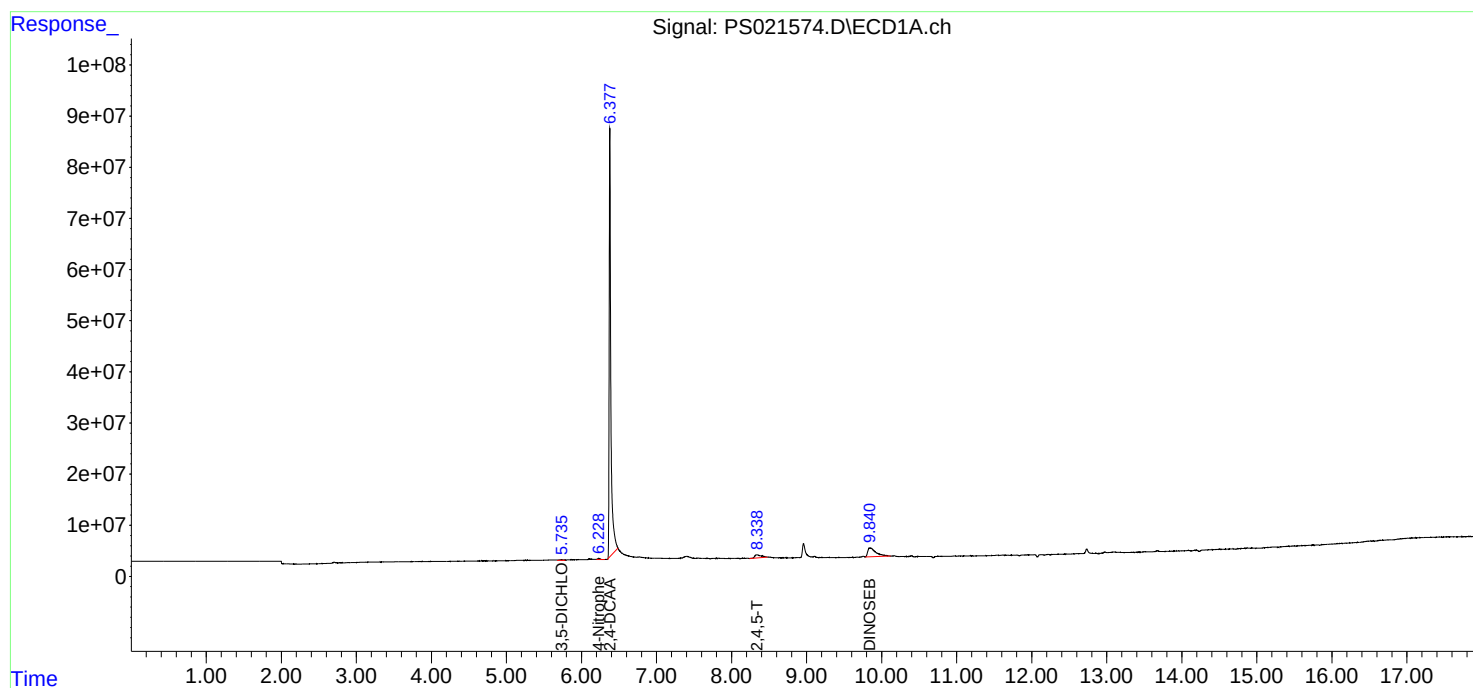


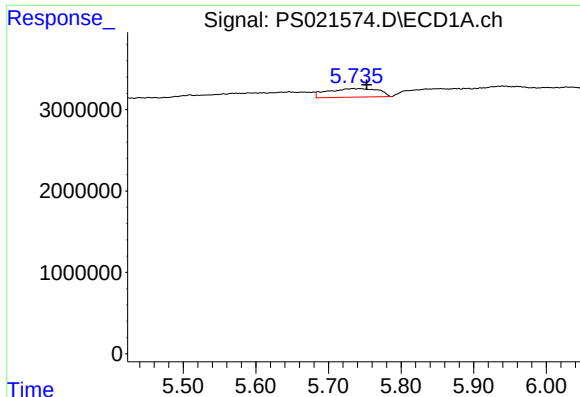

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.734 min
Delta R.T.: -0.018 min
Response: 5141761
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

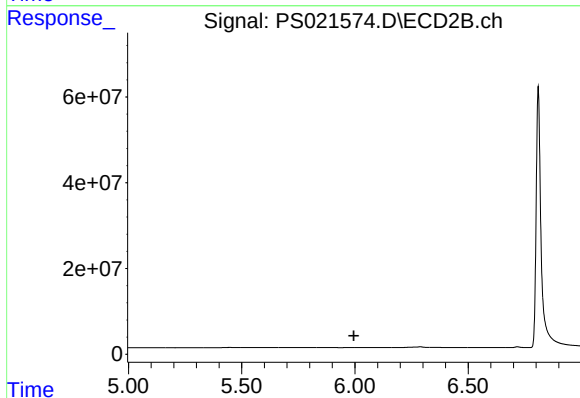


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

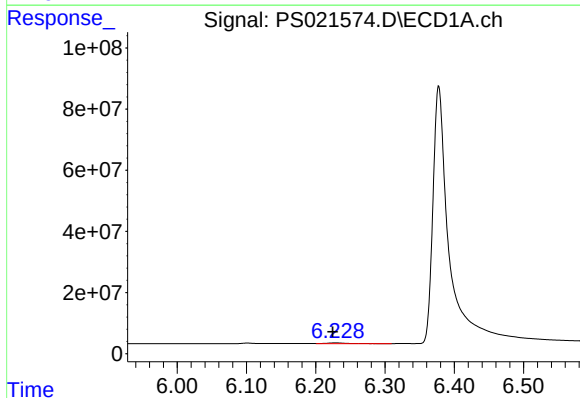


#3 4-Nitrophenol

R.T.: 6.228 min
Delta R.T.: 0.004 min
Response: 5002548
Conc: 2.78 ng/ml

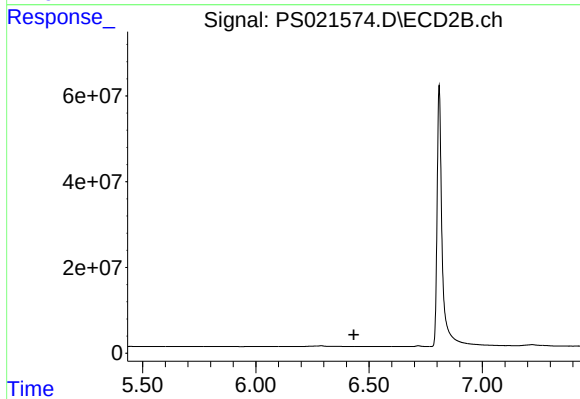

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

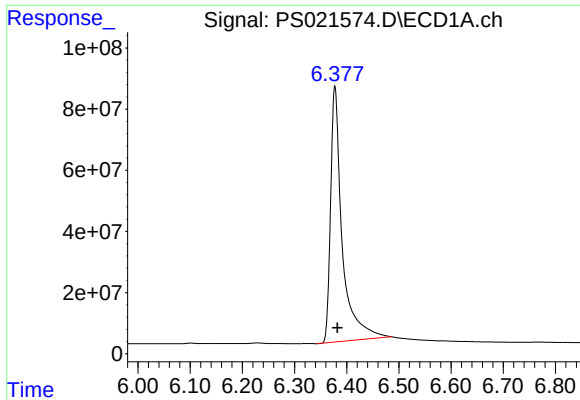

#4 2,4-DCAA


R.T.: 6.378 min
Delta R.T.: -0.004 min
Response: 1290585116
Conc: 444.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

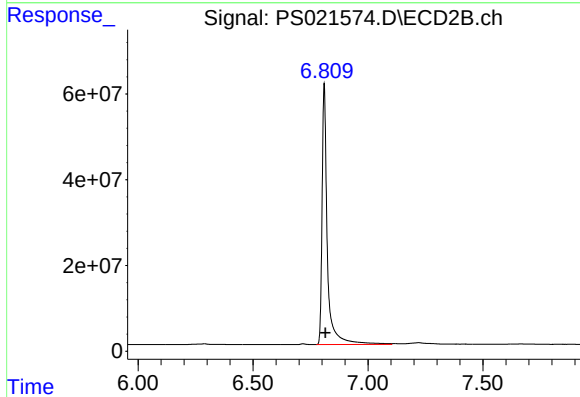


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.006 min
Response: 977862891
Conc: 567.21 ng/ml

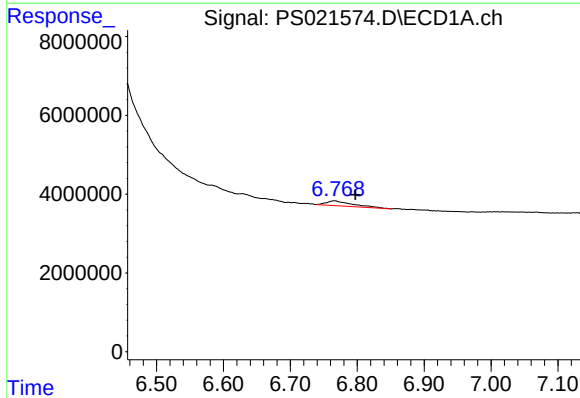


#7 MCPA

R.T.: 6.766 min
Delta R.T.: -0.032 min
Response: 3392428
Conc: N.D.

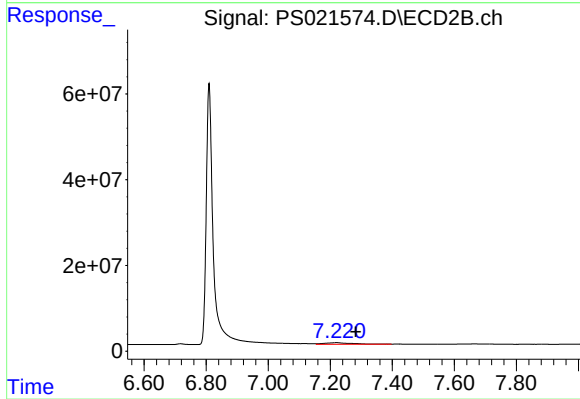

#7 MCPA


R.T.: 7.220 min
Delta R.T.: -0.063 min
Response: 20778683
Conc: 2.35 ug/ml

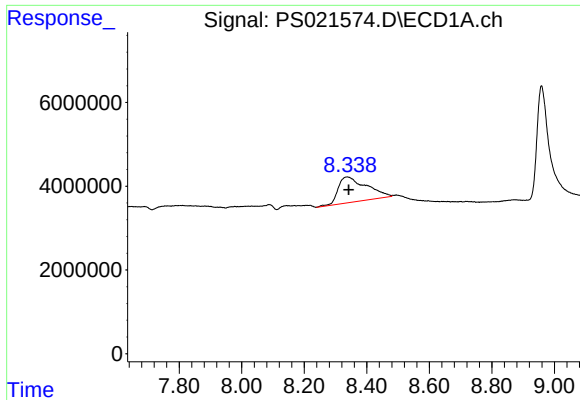

#12 2,4,5-T


R.T.: 8.337 min
Delta R.T.: -0.005 min
Response: 38073294
Conc: 2.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

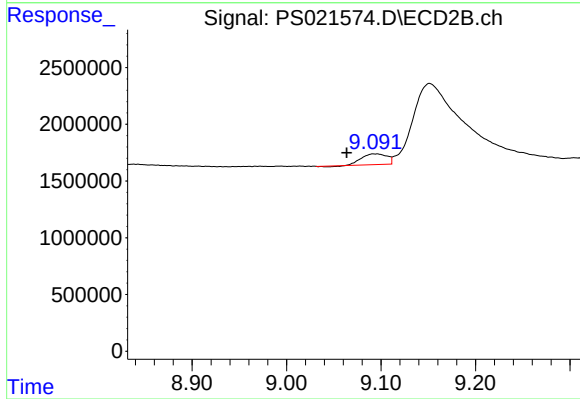


#12 2,4,5-T

R.T.: 9.092 min
Delta R.T.: 0.028 min
Response: 1727473
Conc: N.D.

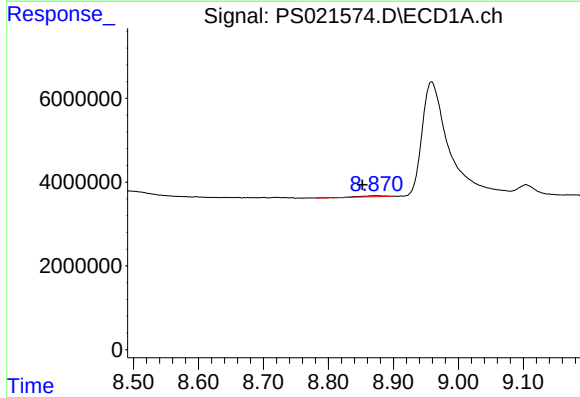


#13 2,4-DB

R.T.: 8.872 min
Delta R.T.: 0.020 min
Response: 579930
Conc: N.D.

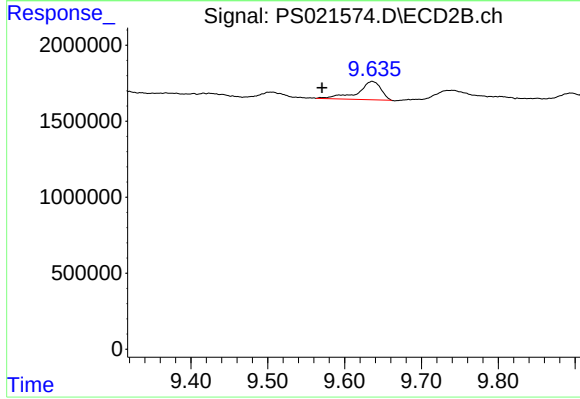

#13 2,4-DB


R.T.: 9.636 min
Delta R.T.: 0.065 min
Response: 2531640
Conc: 1.76 ng/ml

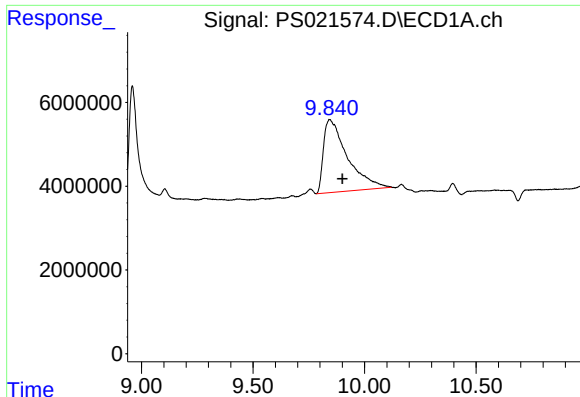

#14 DINOSEB


R.T.: 9.843 min
Delta R.T.: -0.058 min
Response: 129392644
Conc: 8.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

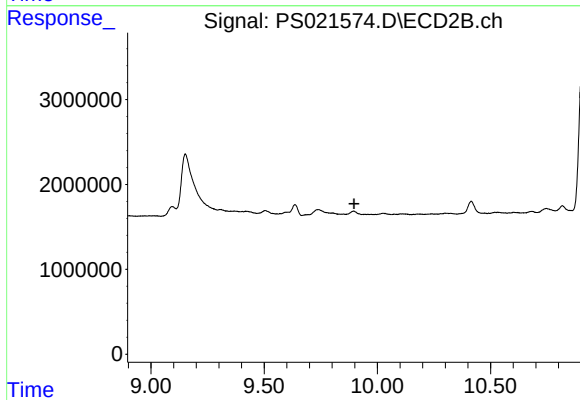


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.897 min
Response: 0
Conc: N.D.

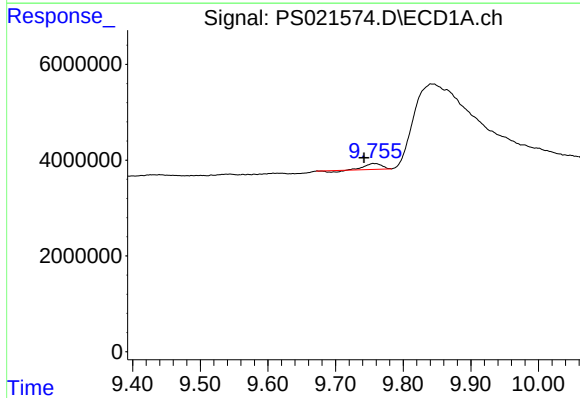

#15 Picloram

R.T.: 9.757 min
Delta R.T.: 0.015 min
Response: 1772146
Conc: N.D.

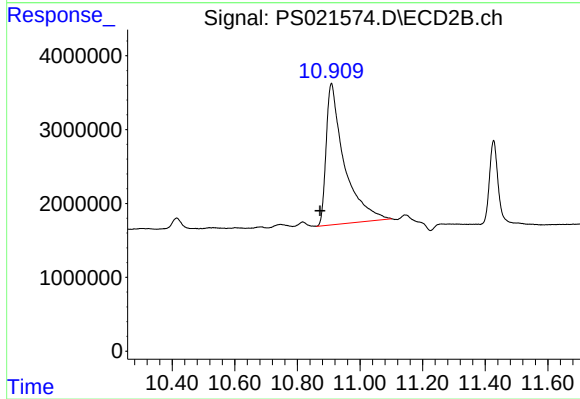

#15 Picloram

R.T.: 10.909 min
Delta R.T.: 0.037 min
Response: 76841190
Conc: 4.73 ng/ml