

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122822\
 Data File : PS021582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2022 19:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 21:04:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.375	6.809	1380.2E6	962.6E6	475.025	558.339
Target Compounds							
2) T	3,5-DICHL...	5.729	0.000	11180764	0	2.813	N.D. #
3) T	4-Nitroph...	6.222	0.000	6766437	0	3.763	N.D. #
5) T	DICAMBA	0.000	6.968	0	13817145	N.D.	1.809
6) T	MCP	6.703	7.122f	-1147779	4129856	N.D.	<MDL
7) T	MCPA	6.752f	7.213f	5900471	34745258	<MDL	3.929 #
8) T	DICHLORPROP	7.129	7.638	458412	4662502	<MDL	2.367 #
9) T	2,4-D	0.000	7.938f	0	1031559	N.D.	<MDL
10) T	Pentachlo...	7.545	0.000	2058889	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.083	8.683	29424678	3005279	1.591	<MDL #
12) T	2,4,5-T	8.384f	9.076	24866214	6196696	1.318	<MDL #
13) T	2,4-DB	8.825	9.585	633688	1703217	<MDL	1.185 #
14) T	DINOSEB	9.895	9.891	9675952	5315607	<MDL	<MDL #
15) T	Picloram	9.751	10.906	2305667	6413016	<MDL	<MDL #
16) T	DCPA	10.162	10.816	7738801	3040335	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122822\
Data File : PS021582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2022 19:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 21:04:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

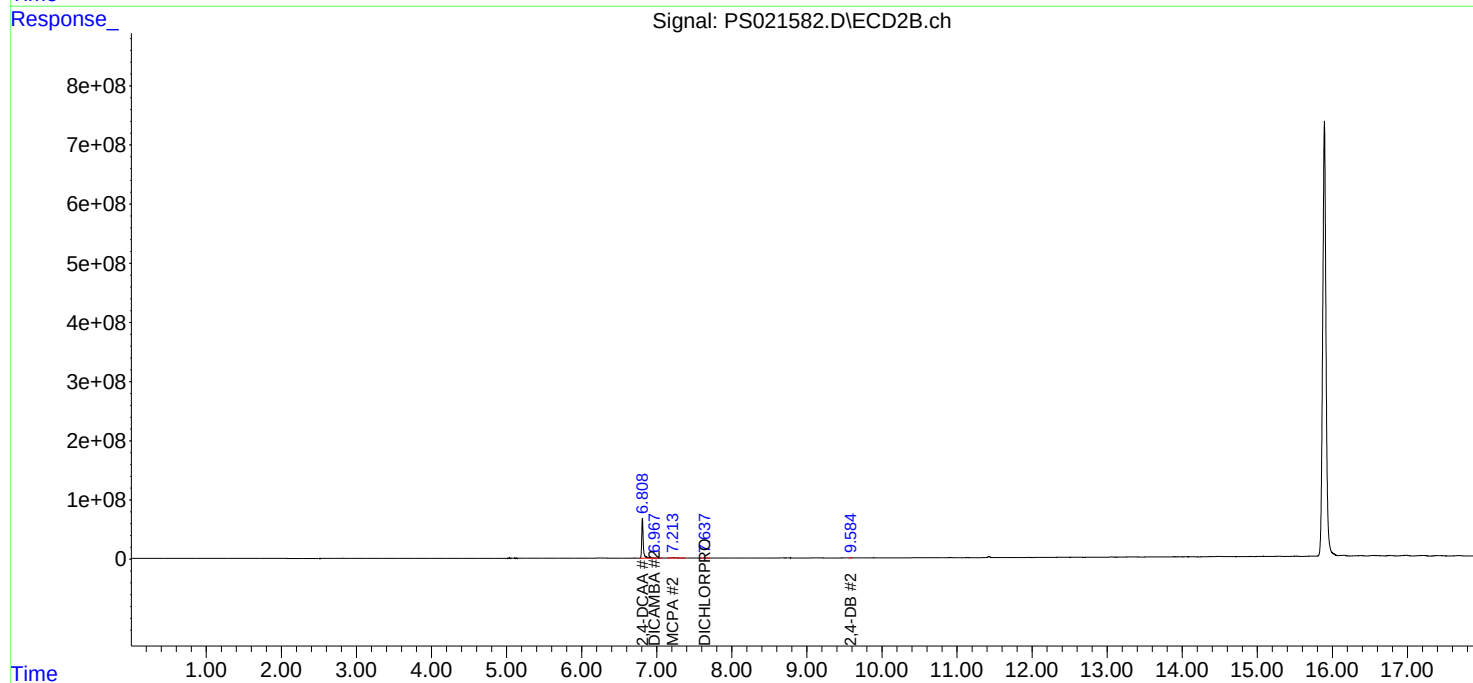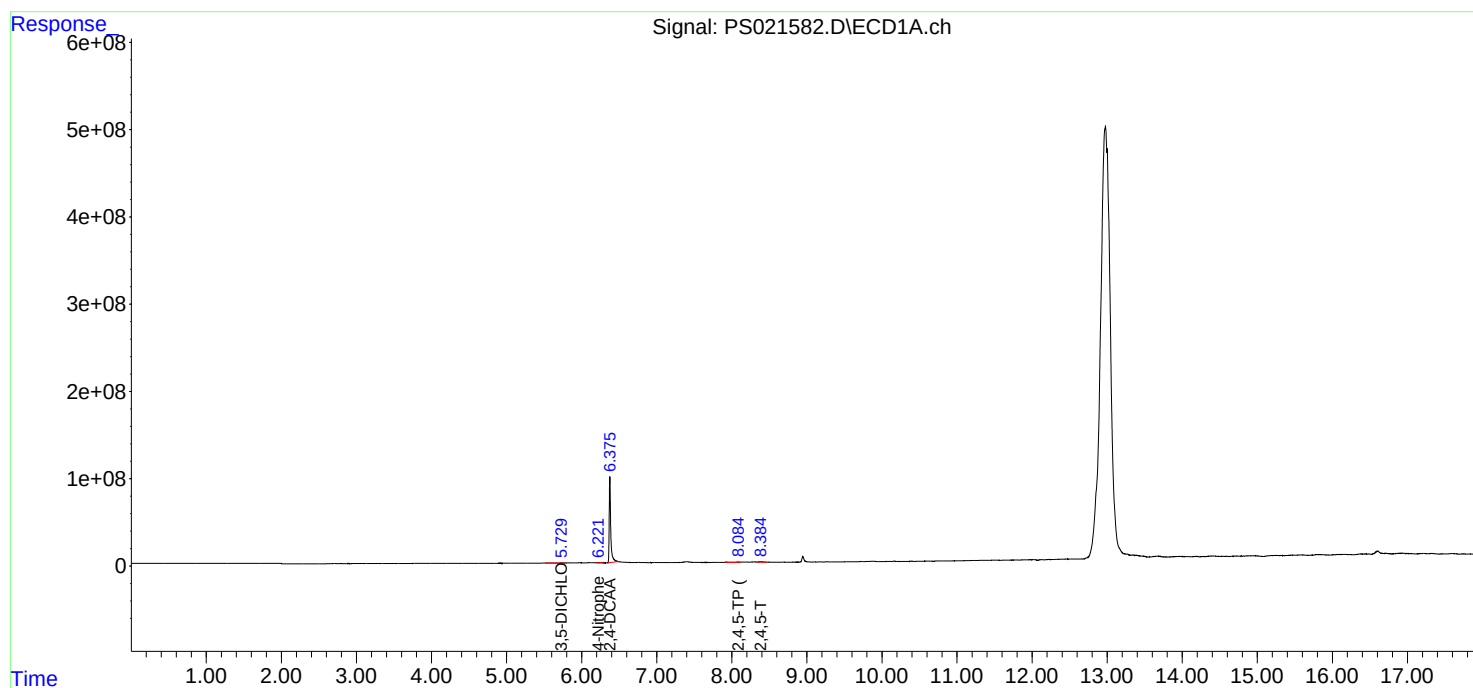


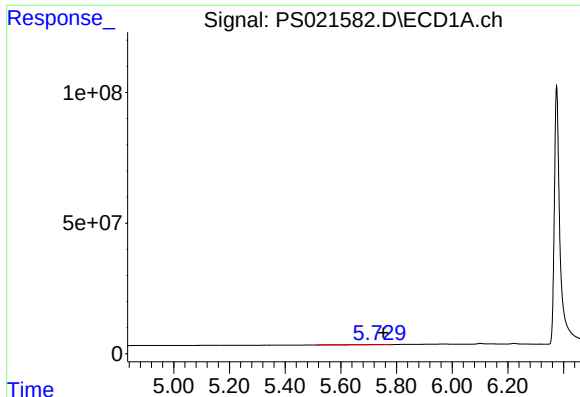

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.729 min
Delta R.T.: -0.024 min
Response: 11180764
Conc: 2.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

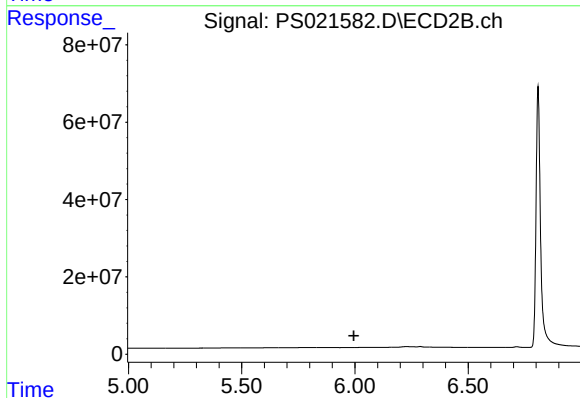


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

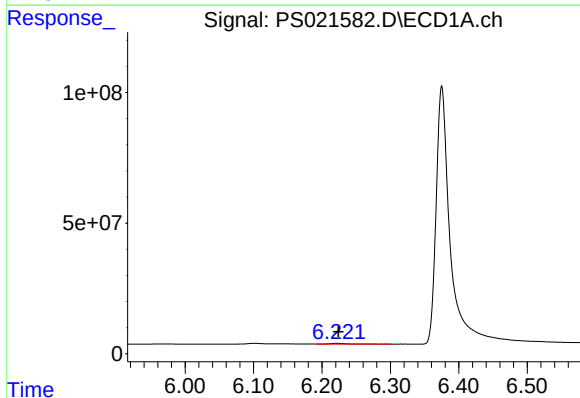


#3 4-Nitrophenol

R.T.: 6.222 min
Delta R.T.: -0.002 min
Response: 6766437
Conc: 3.76 ng/ml

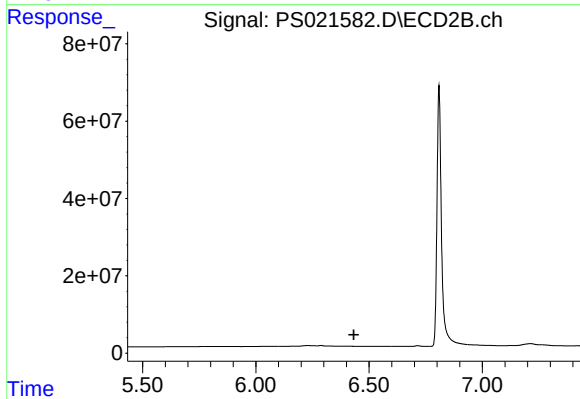

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

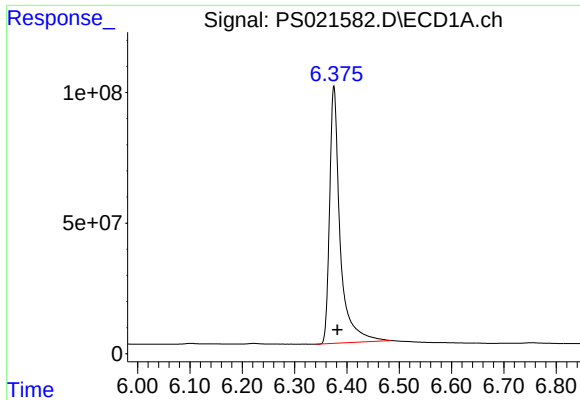

#4 2,4-DCAA


R.T.: 6.375 min
Delta R.T.: -0.007 min
Response: 1380182781
Conc: 475.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

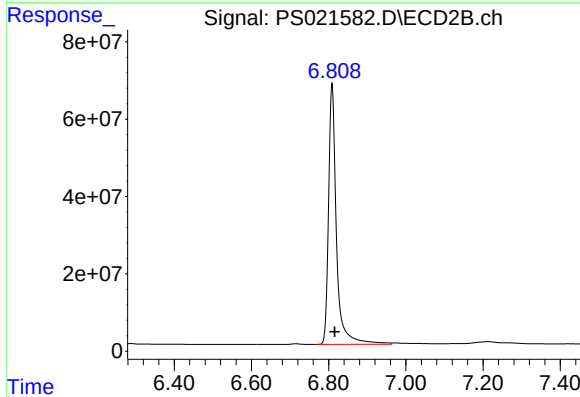


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.007 min
Response: 962573044
Conc: 558.34 ng/ml

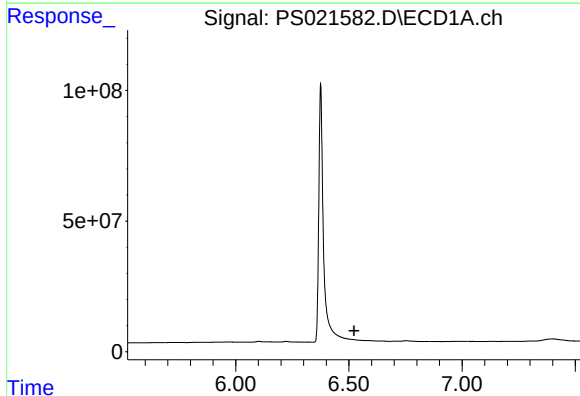


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

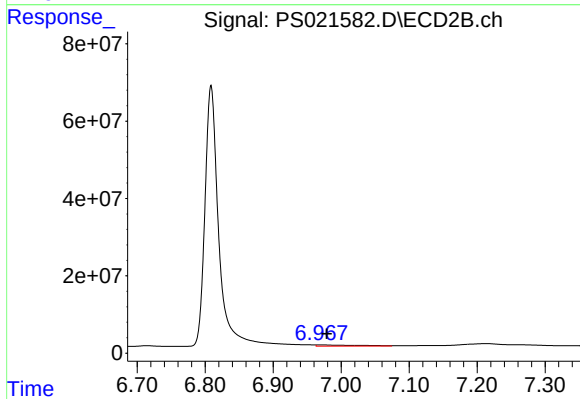

#5 DICAMBA


R.T.: 6.968 min
Delta R.T.: -0.011 min
Response: 13817145
Conc: 1.81 ng/ml

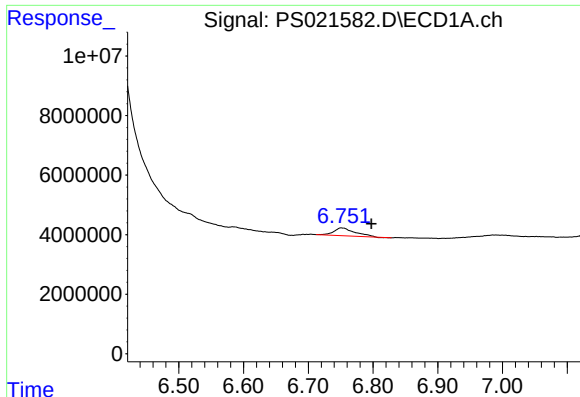

#7 MCPA


R.T.: 6.752 min
Delta R.T.: -0.045 min
Response: 5900471
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

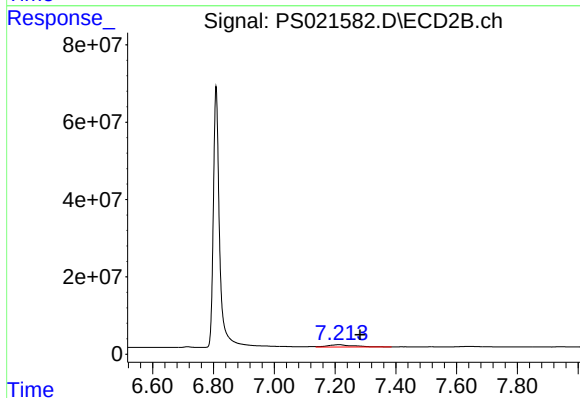


#7 MCPA

R.T.: 7.213 min
Delta R.T.: -0.070 min
Response: 34745258
Conc: 3.93 ug/ml

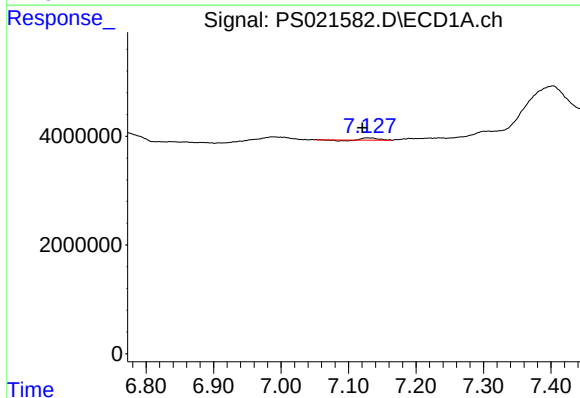


#8 DICHLORPROP

R.T.: 7.129 min
Delta R.T.: 0.009 min
Response: 458412
Conc: N.D.

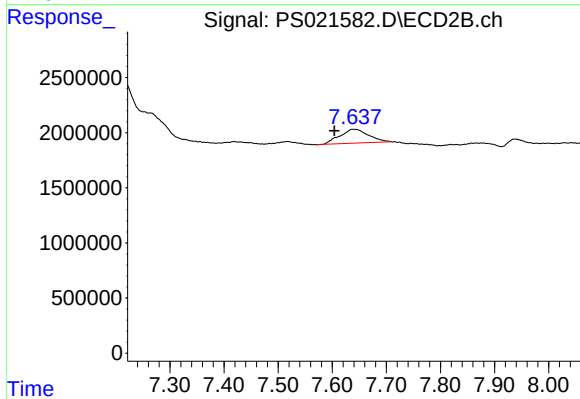

#8 DICHLORPROP


R.T.: 7.638 min
Delta R.T.: 0.034 min
Response: 4662502
Conc: 2.37 ng/ml

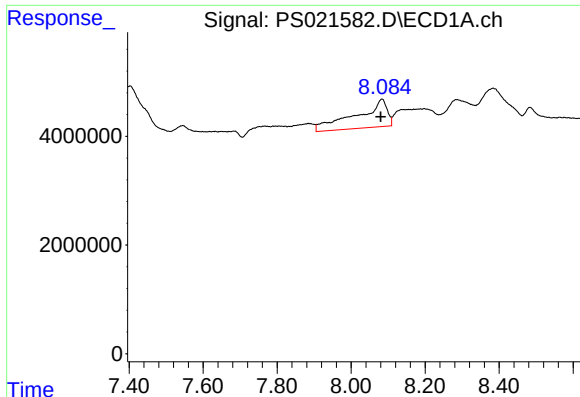

#11 2,4,5-TP (SILVEX)


R.T.: 8.083 min
Delta R.T.: 0.004 min
Response: 29424678
Conc: 1.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

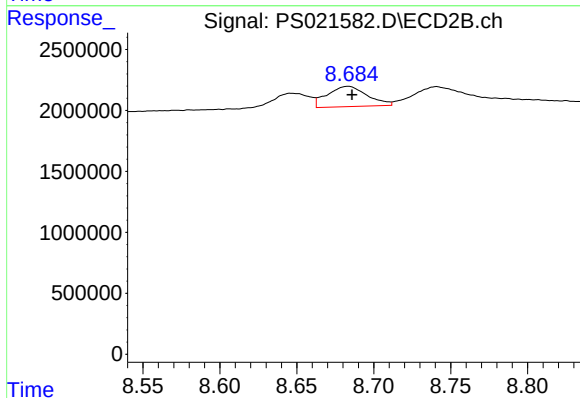


#11 2,4,5-TP (SILVEX)

R.T.: 8.683 min
Delta R.T.: -0.003 min
Response: 3005279
Conc: N.D.

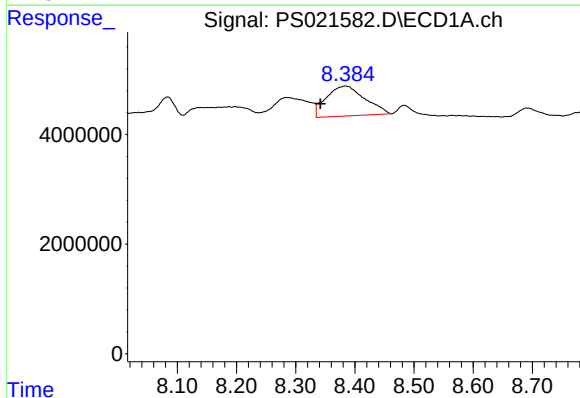


#12 2,4,5-T

R.T.: 8.384 min
Delta R.T.: 0.042 min
Response: 24866214
Conc: 1.32 ng/ml

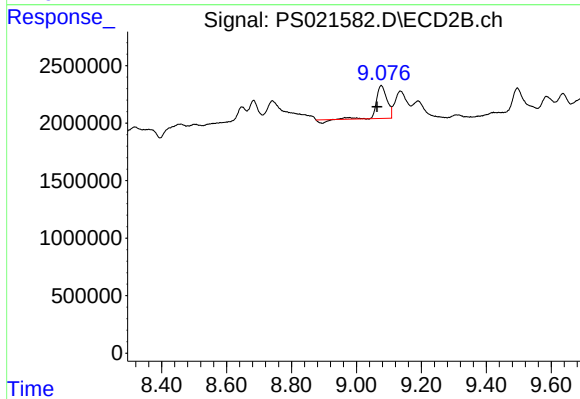

#12 2,4,5-T


R.T.: 9.076 min
Delta R.T.: 0.013 min
Response: 6196696
Conc: N.D.

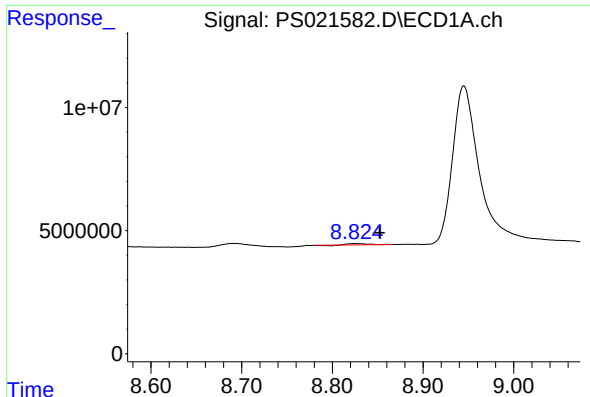

#13 2,4-DB

R.T.: 8.825 min
Delta R.T.: -0.027 min
Response: 633688
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

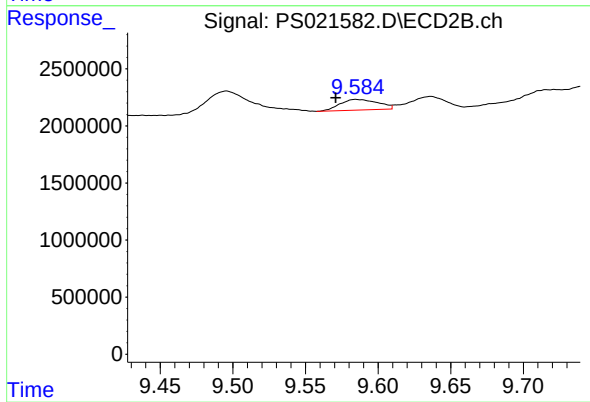

#13 2,4-DB

R.T.: 9.585 min
Delta R.T.: 0.014 min
Response: 1703217
Conc: 1.18 ng/ml