

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
 Data File : PS025255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 16:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 23:50:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.352	6.763	1196.5E6	377.3E6	533.967	531.571
Target Compounds							
1) T	Dalapon	2.508f	2.562	14563846	6202326	4.706	5.397
2) T	3,5-DICHL...	5.694	0.000	104031	0	<MDL	N.D. #
3) T	4-Nitroph...	0.000	6.361	0	588683	N.D.	1.185
5) T	DICAMBA	0.000	6.923	0	953933	N.D.	<MDL
6) T	MCP	0.000	6.962f	0	1233004	N.D.	<MDL
7) T	MCPA	6.712f	7.155f	5779316	13103305	<MDL	4.169 #
8) T	DICHLORPROP	0.000	7.546	0	1070548	N.D.	1.384
10) T	Pentachlo...	7.505	8.240	10700875	3320282	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.599	0	1173615	N.D.	<MDL
12) T	2,4,5-T	0.000	8.973	0	1620379	N.D.	<MDL
13) T	2,4-DB	0.000	9.469	0	1016717	N.D.	1.853
14) T	DINOSEB	0.000	9.798	0	1128862	N.D.	<MDL
15) T	Picloram	9.690	10.757	98799194	29641882	4.729	4.351
16) T	DCPA	0.000	10.757	0	29641882	N.D.	5.551



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
Data File : PS025255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 16:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 23:50:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

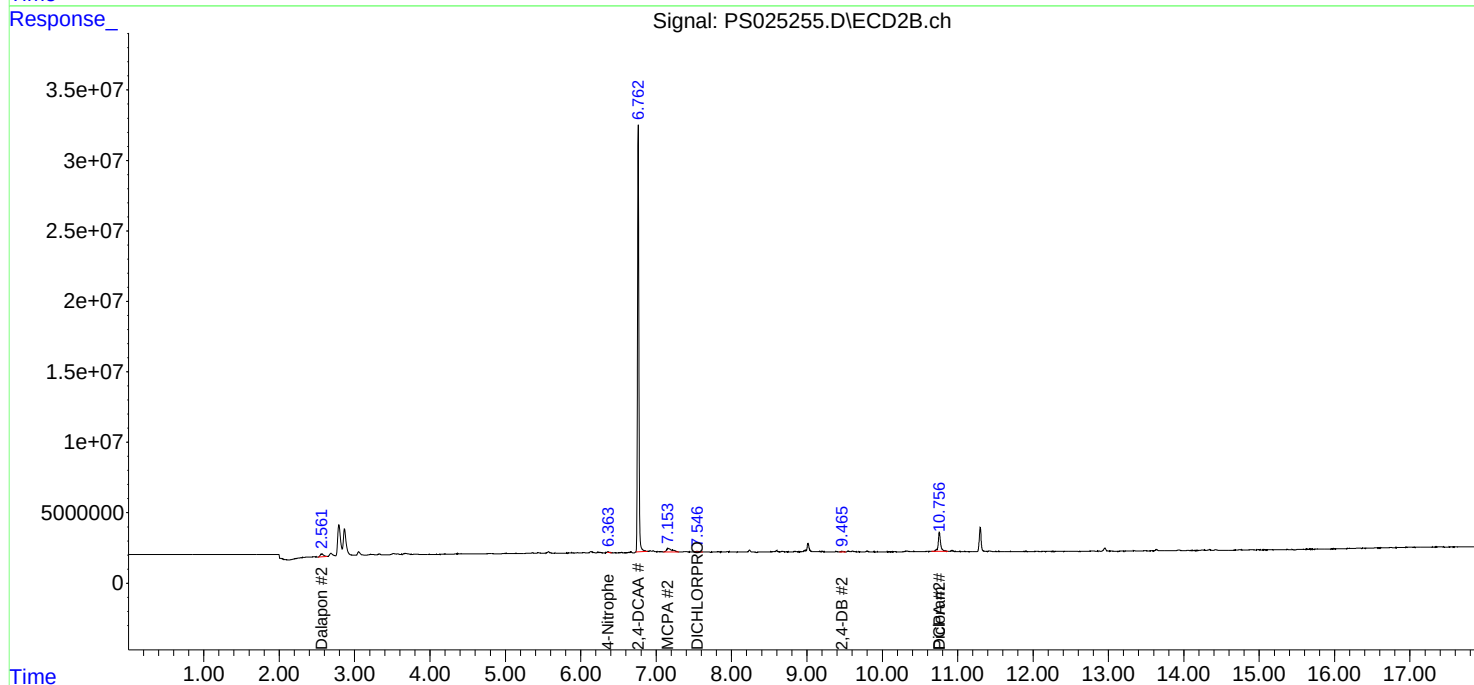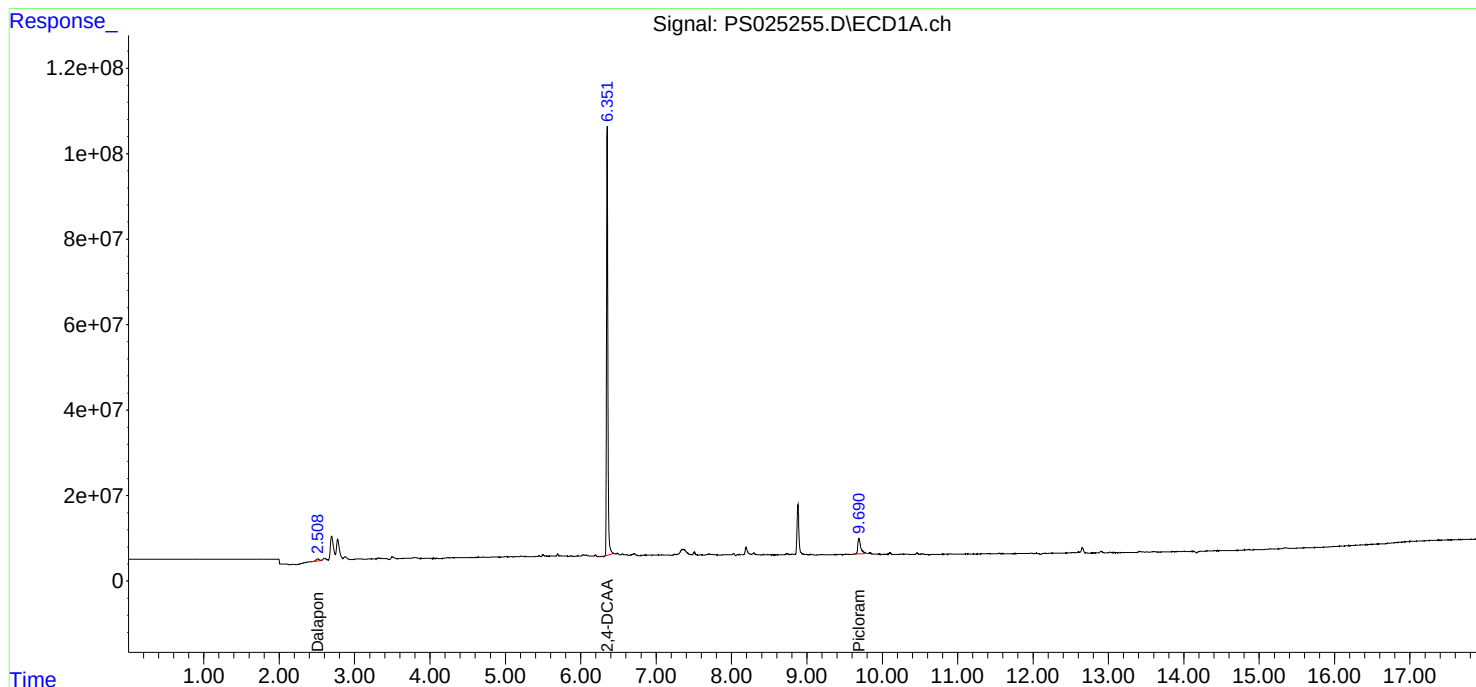


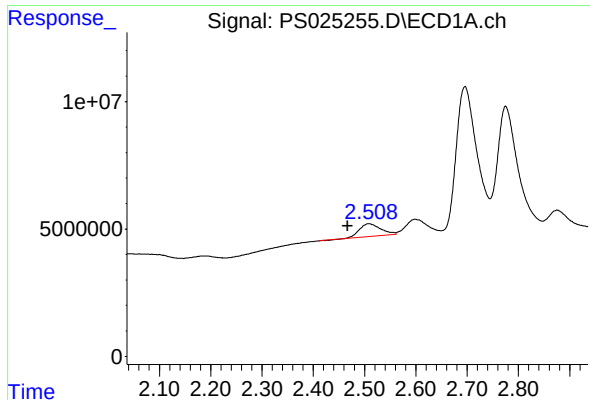

#1 Dalapon


R.T.: 2.508 min
Delta R.T.: 0.041 min
Response: 14563846
Conc: 4.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

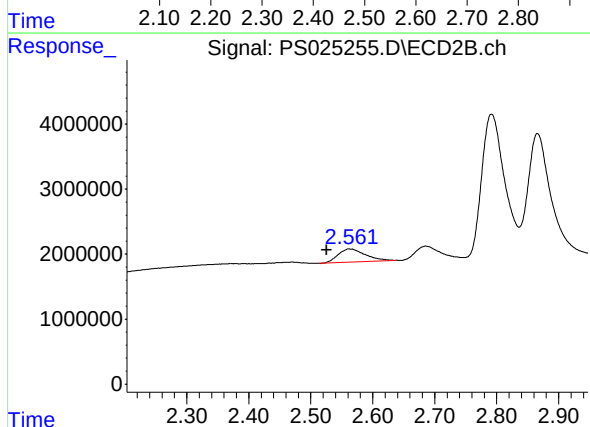


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.036 min
Response: 6202326
Conc: 5.40 ng/ml

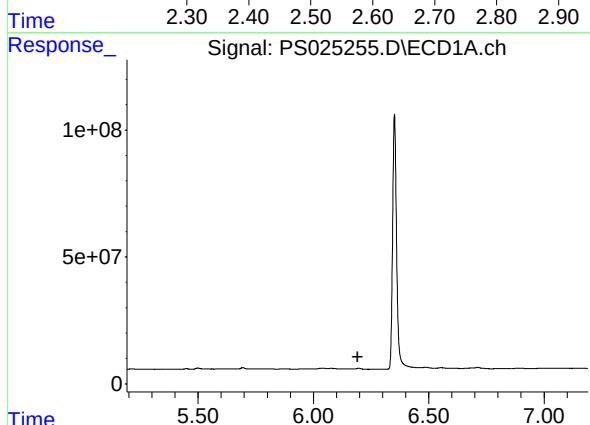


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

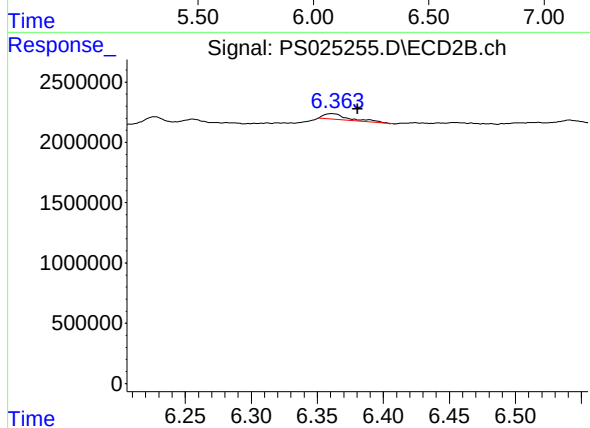

#3 4-Nitrophenol


R.T.: 6.361 min
Delta R.T.: -0.020 min
Response: 588683
Conc: 1.19 ng/ml

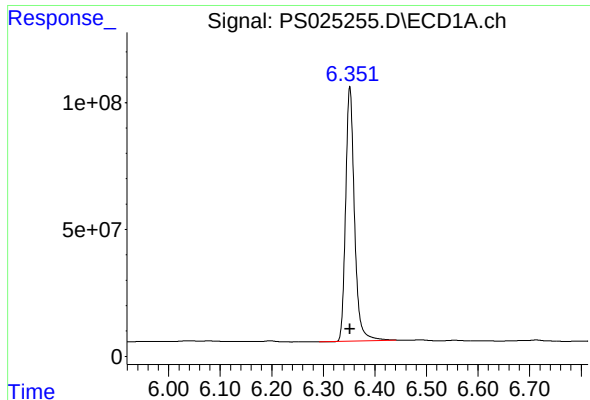

#4 2,4-DCAA


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 1196514718
Conc: 533.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

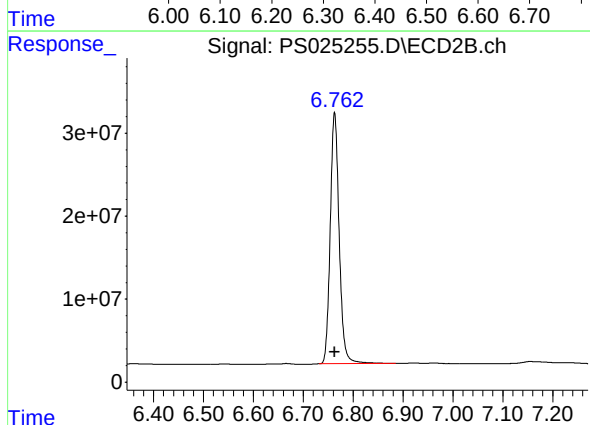


#4 2,4-DCAA

R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 377294970
Conc: 531.57 ng/ml

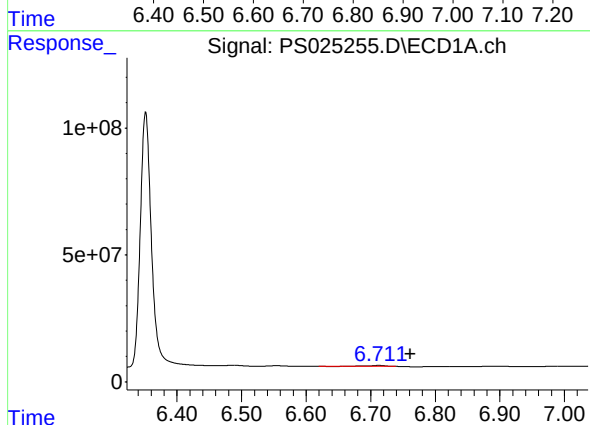


#7 MCPA

R.T.: 6.712 min
Delta R.T.: -0.049 min
Response: 5779316
Conc: N.D.

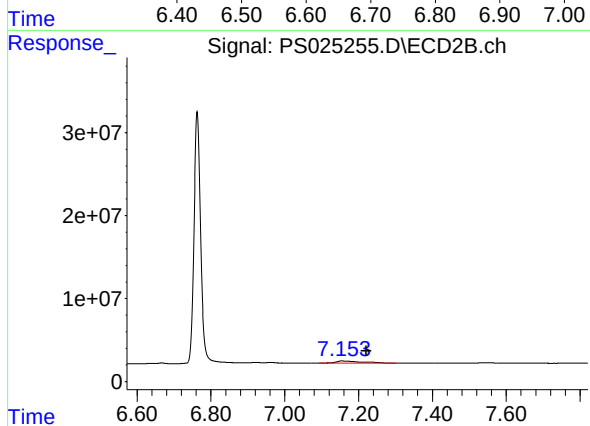

#7 MCPA


R.T.: 7.155 min
Delta R.T.: -0.066 min
Response: 13103305
Conc: 4.17 ug/ml

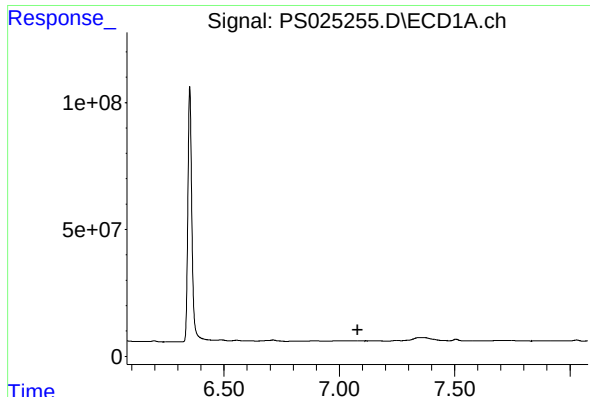

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

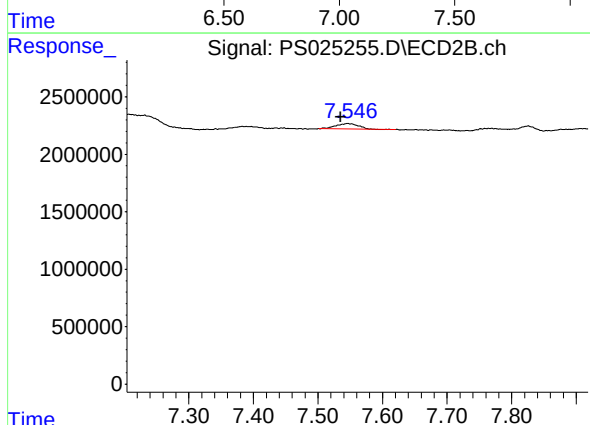


#8 DICHLORPROP

R.T.: 7.546 min
Delta R.T.: 0.011 min
Response: 1070548
Conc: 1.38 ng/ml

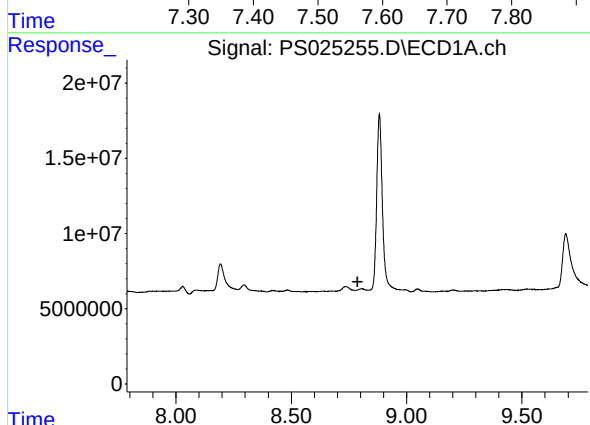


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.787 min
Response: 0
Conc: N.D.

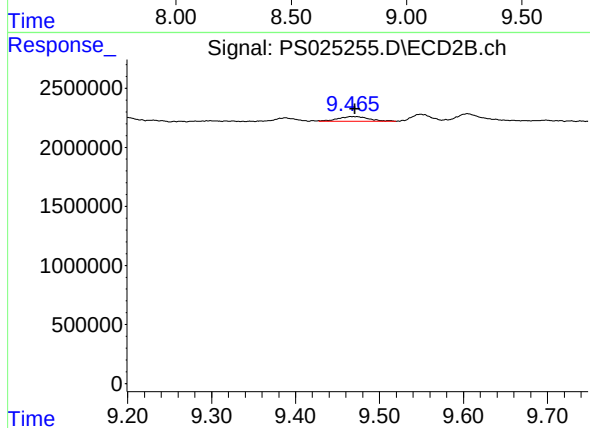

#13 2,4-DB


R.T.: 9.469 min
Delta R.T.: -0.001 min
Response: 1016717
Conc: 1.85 ng/ml

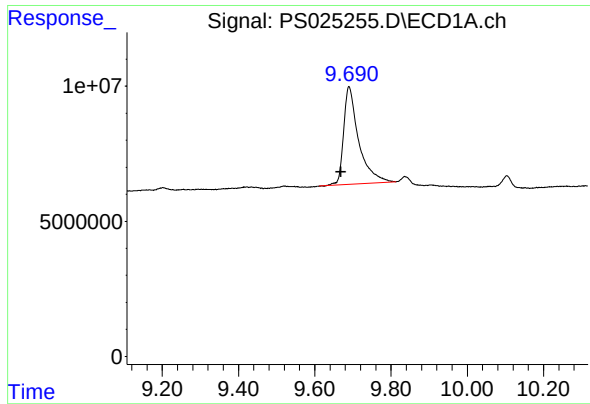

#15 Picloram


R.T.: 9.690 min
Delta R.T.: 0.022 min
Response: 98799194
Conc: 4.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

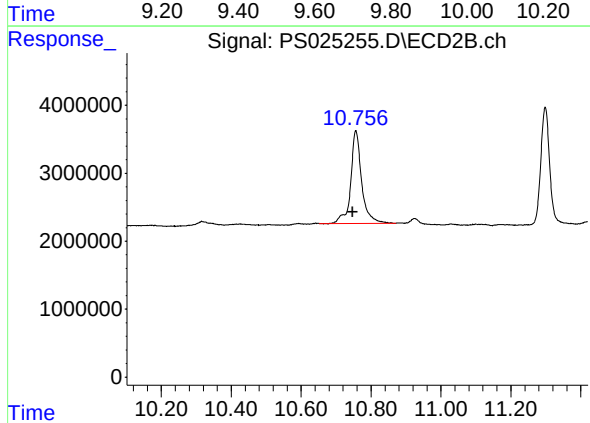


#15 Picloram

R.T.: 10.757 min
Delta R.T.: 0.009 min
Response: 29641882
Conc: 4.35 ng/ml

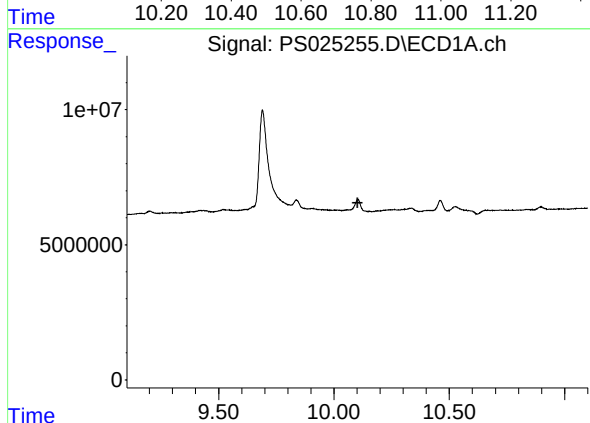

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.102 min
Response: 0
Conc: N.D.

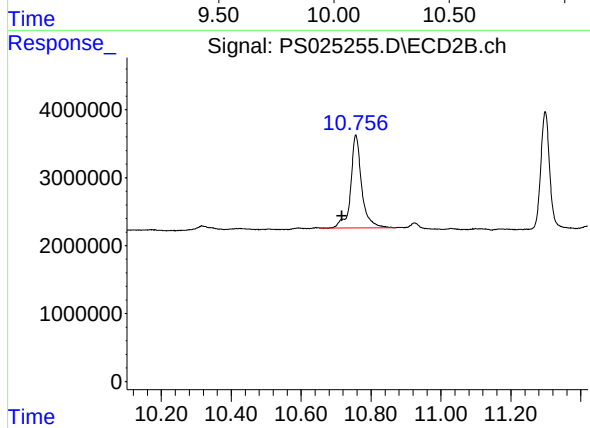

#16 DCPA

R.T.: 10.757 min
Delta R.T.: 0.039 min
Response: 29641882
Conc: 5.55 ng/ml