

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
 Data File : PS025279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2023 03:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 04:26:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.351	6.762	1205.1E6	380.9E6	537.812	536.661
Target Compounds						
1) T Dalapon	2.504	2.561	9899694	4387660	3.199	3.818
3) T 4-Nitroph...	0.000	6.359	0	657504	N.D.	1.324
5) T DICAMBA	0.000	6.913	0	402046	N.D.	<MDL
6) T MCPP	6.677	6.963f	1922415	966220	<MDL	<MDL #
7) T MCPA	0.000	7.227	0	2800633	N.D.	<MDL
8) T DICHLORPROP	0.000	7.548	0	3703883	N.D.	4.788
10) T Pentachlo...	0.000	8.295f	0	1782819	N.D.	<MDL
12) T 2,4,5-T	0.000	8.967	0	242485	N.D.	<MDL
13) T 2,4-DB	0.000	9.461	0	803294	N.D.	1.464
15) T Picloram	0.000	10.755	0	2137385	N.D.	<MDL
16) T DCPA	0.000	10.755	0	2137385	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
Data File : PS025279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2023 03:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:26:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

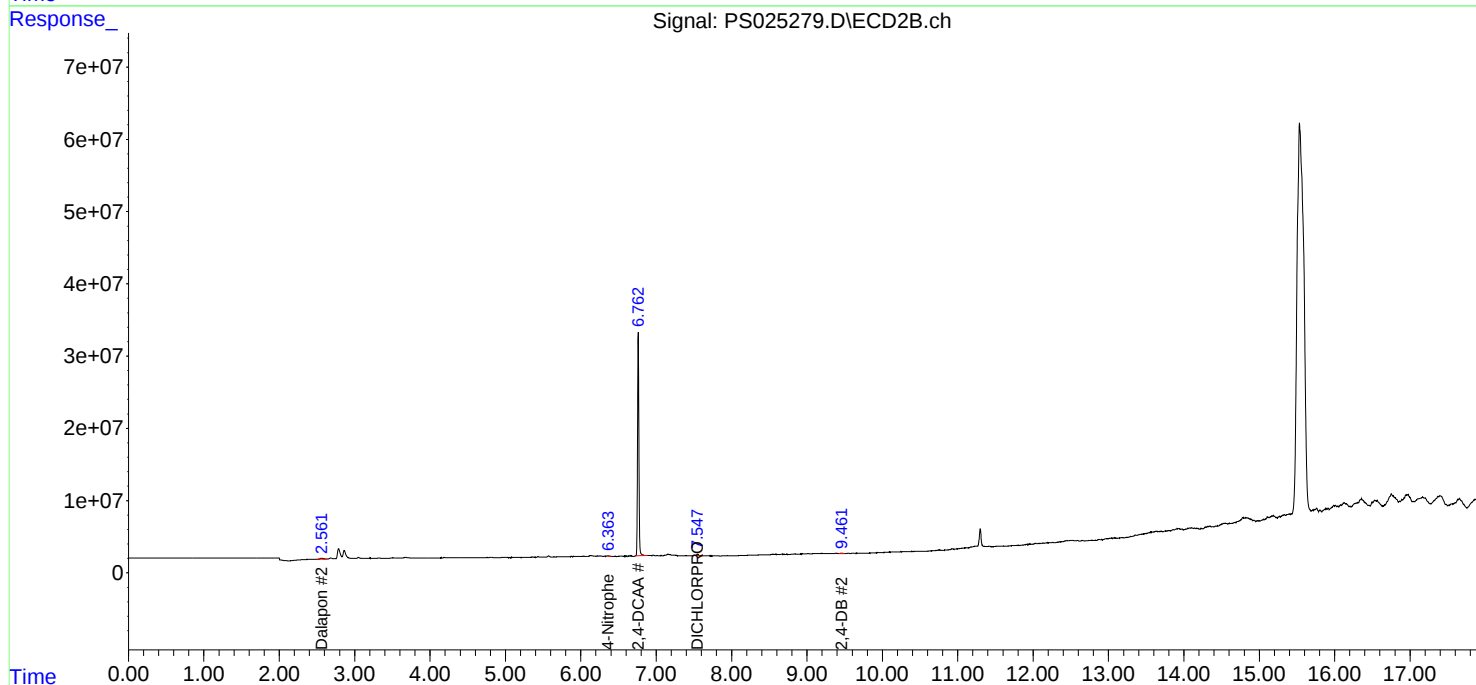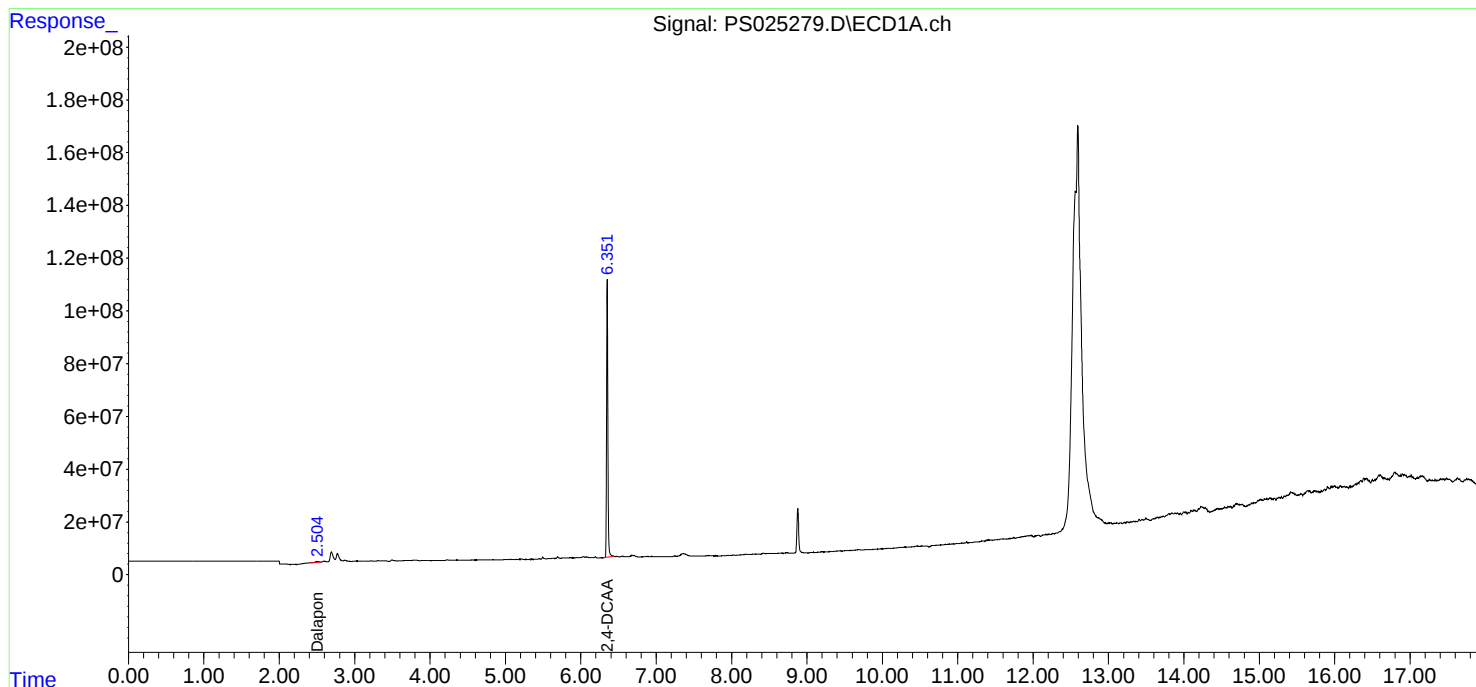


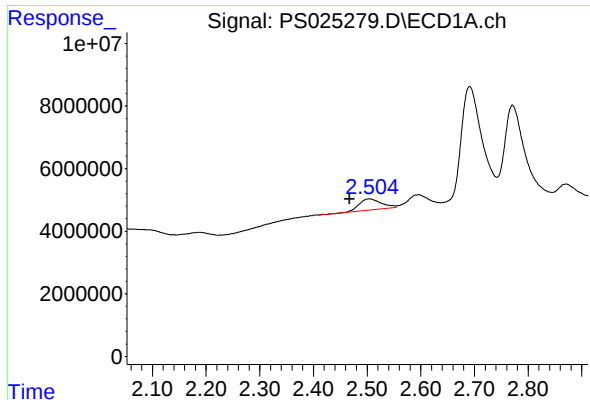

#1 Dalapon


R.T.: 2.504 min
Delta R.T.: 0.037 min
Response: 9899694
Conc: 3.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

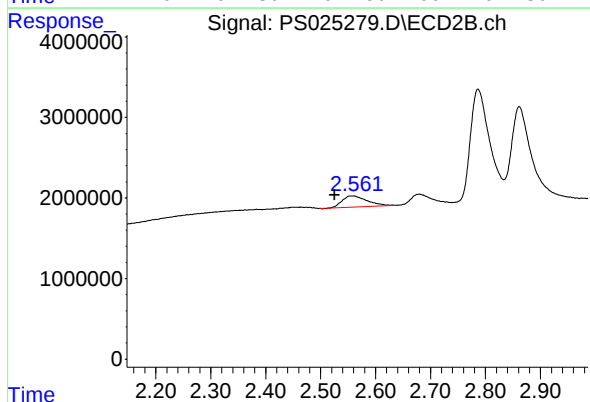


#1 Dalapon

R.T.: 2.561 min
Delta R.T.: 0.035 min
Response: 4387660
Conc: 3.82 ng/ml

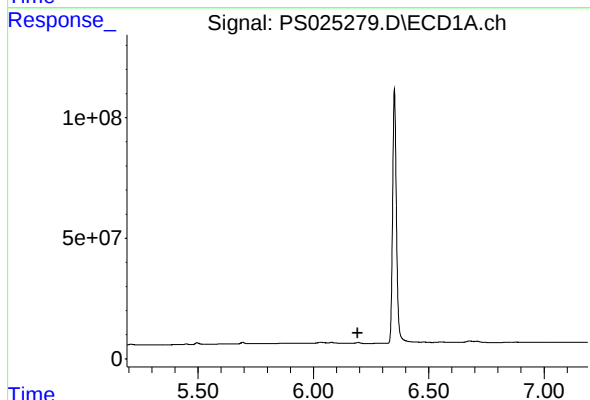


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

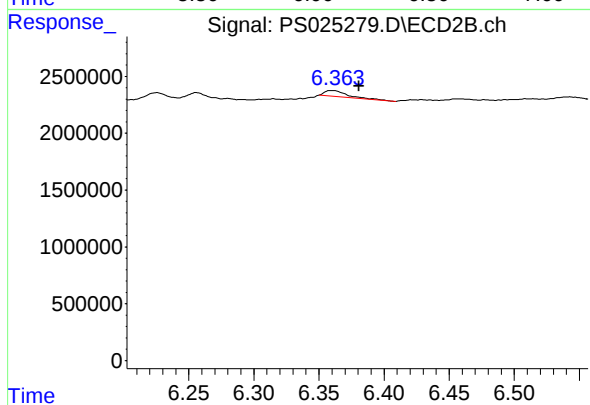

#3 4-Nitrophenol


R.T.: 6.359 min
Delta R.T.: -0.021 min
Response: 657504
Conc: 1.32 ng/ml

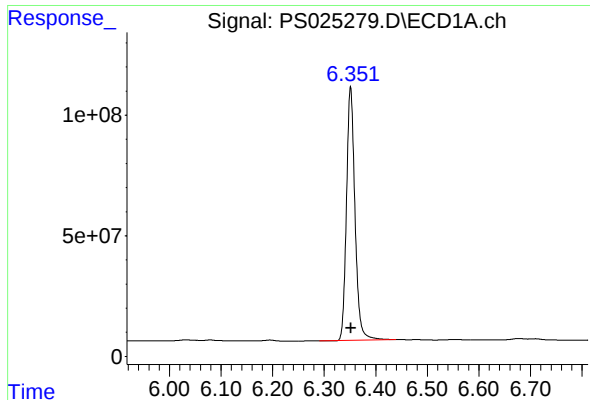

#4 2,4-DCAA


R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 1205131399
Conc: 537.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

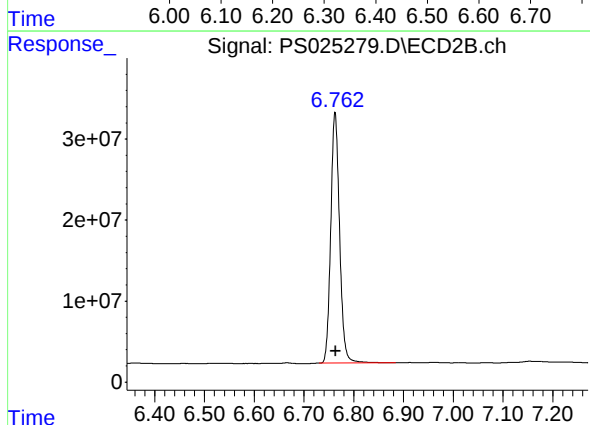


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 380907429
Conc: 536.66 ng/ml

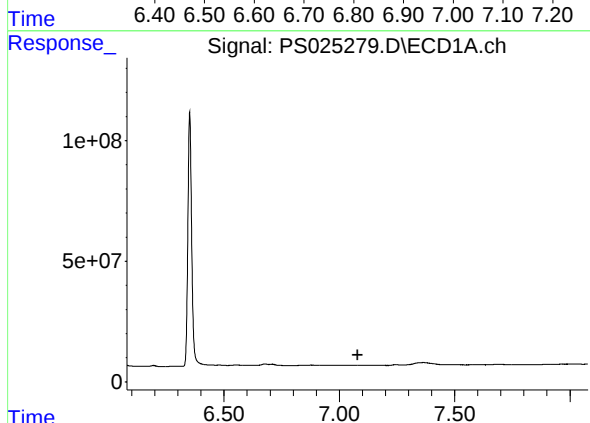


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

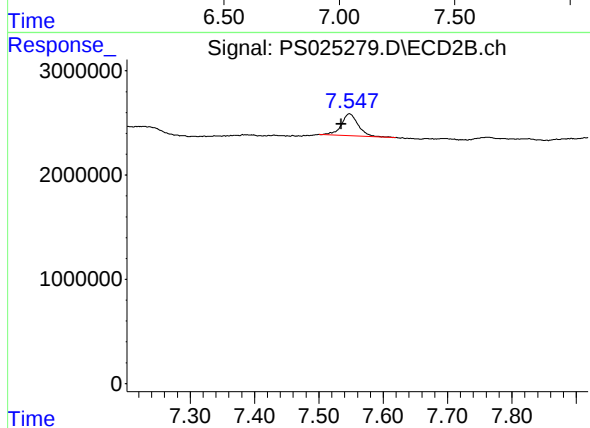

#8 DICHLORPROP


R.T.: 7.548 min
Delta R.T.: 0.013 min
Response: 3703883
Conc: 4.79 ng/ml

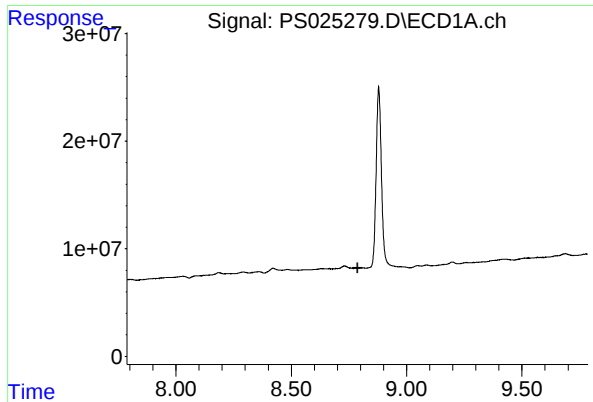

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

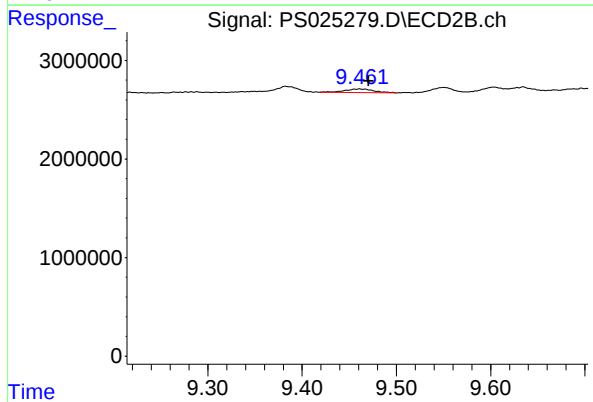

#13 2,4-DB

R.T.: 9.461 min
Delta R.T.: -0.009 min
Response: 803294
Conc: 1.46 ng/ml