

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
 Data File : PS025291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2023 07:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 23:34:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.350	6.762	1219.5E6	383.8E6	544.229	540.799
Target Compounds							
1) T	Dalapon	2.507	2.558	7701884	3662790	2.489	3.187 #
2) T	3,5-DICHL...	5.693	0.000	169303	0	<MDL	N.D. #
3) T	4-Nitroph...	0.000	6.360	0	504648	N.D.	1.016
5) T	DICAMBA	0.000	6.914	0	543609	N.D.	<MDL
6) T	MCP	6.676	6.961f	2940224	1762231	<MDL	<MDL #
7) T	MCPA	0.000	7.233	0	2678613	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.546	0	4342870	N.D.	5.614
9) T	2,4-D	7.242	7.764f	6328878	225392	2.043	<MDL #
12) T	2,4,5-T	0.000	8.968	0	364930	N.D.	<MDL
13) T	2,4-DB	0.000	9.457	0	987581	N.D.	1.800
14) T	DINOSEB	0.000	9.800	0	308317	N.D.	<MDL
15) T	Picloram	0.000	10.753	0	3030969	N.D.	<MDL
16) T	DCPA	0.000	10.753	0	3030969	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
Data File : PS025291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2023 07:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 23:34:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

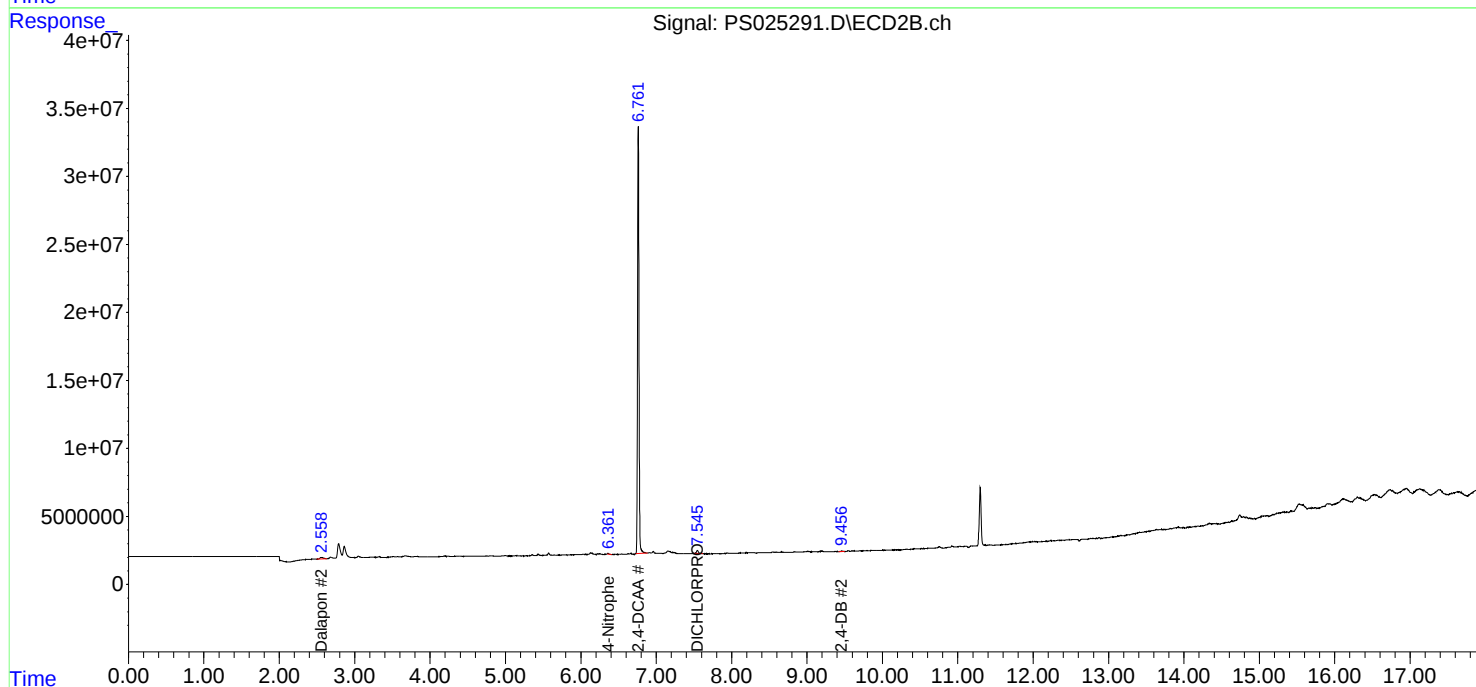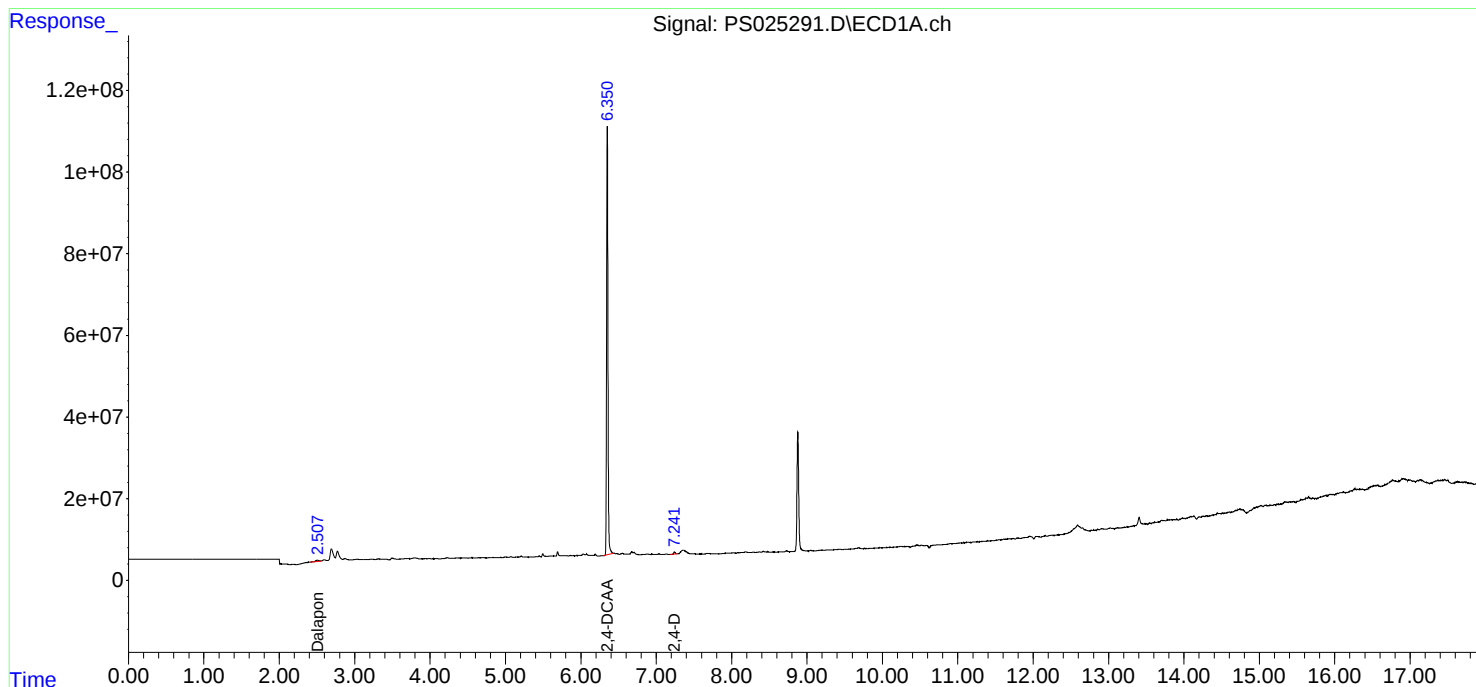


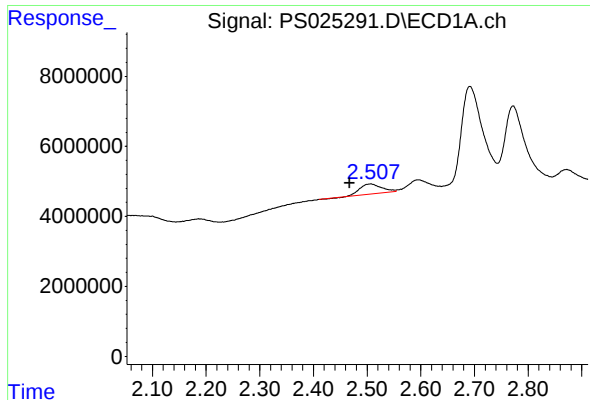

#1 Dalapon


R.T.: 2.507 min
Delta R.T.: 0.040 min
Response: 7701884
Conc: 2.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

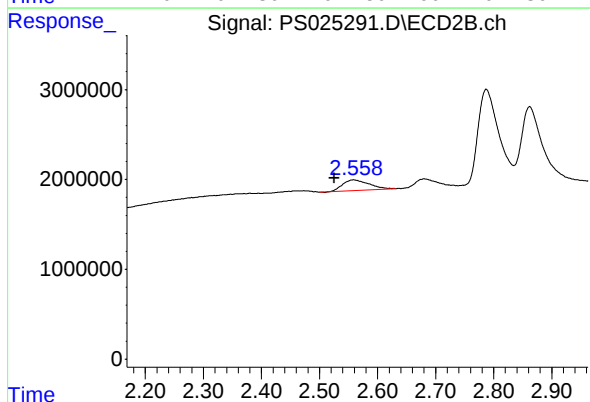


#1 Dalapon

R.T.: 2.558 min
Delta R.T.: 0.032 min
Response: 3662790
Conc: 3.19 ng/ml

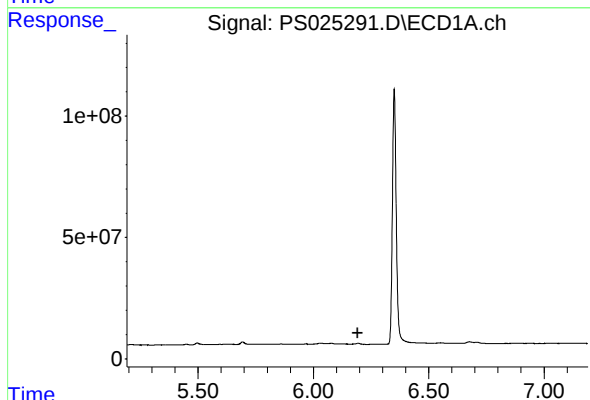


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

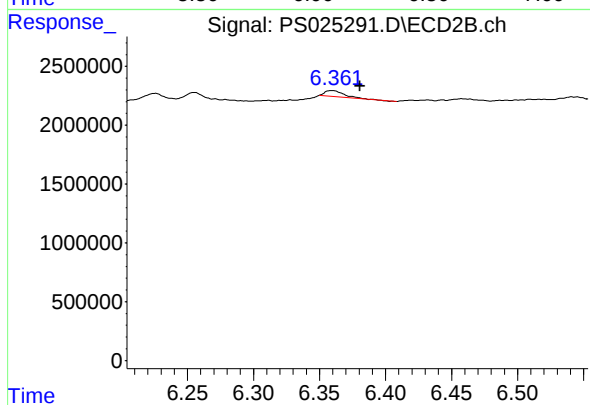

#3 4-Nitrophenol


R.T.: 6.360 min
Delta R.T.: -0.021 min
Response: 504648
Conc: 1.02 ng/ml

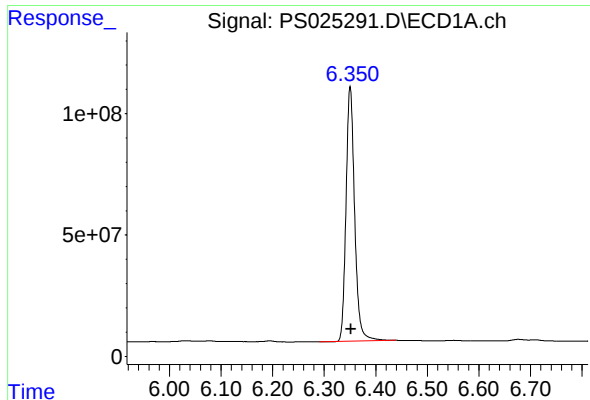

#4 2,4-DCAA


R.T.: 6.350 min
Delta R.T.: -0.002 min
Response: 1219510278
Conc: 544.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

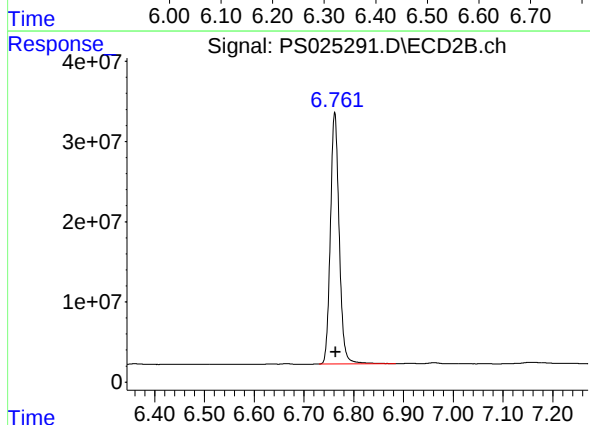


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.002 min
Response: 383844580
Conc: 540.80 ng/ml

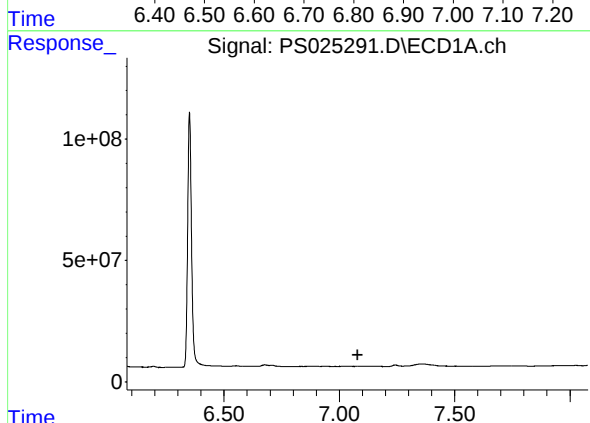


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

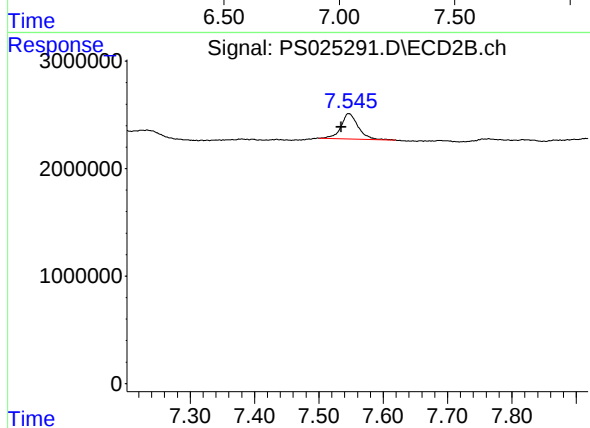

#8 DICHLORPROP


R.T.: 7.546 min
Delta R.T.: 0.011 min
Response: 4342870
Conc: 5.61 ng/ml

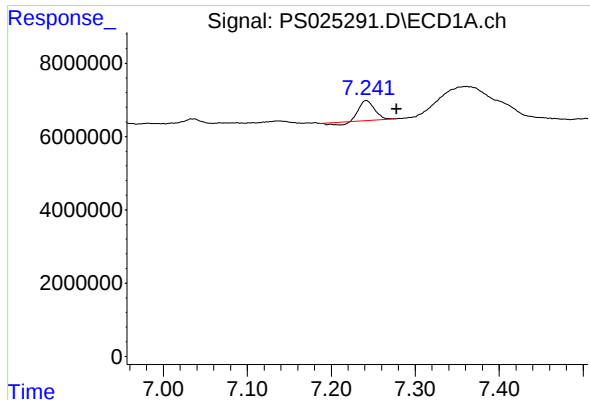

#9 2,4-D


R.T.: 7.242 min
Delta R.T.: -0.036 min
Response: 6328878
Conc: 2.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

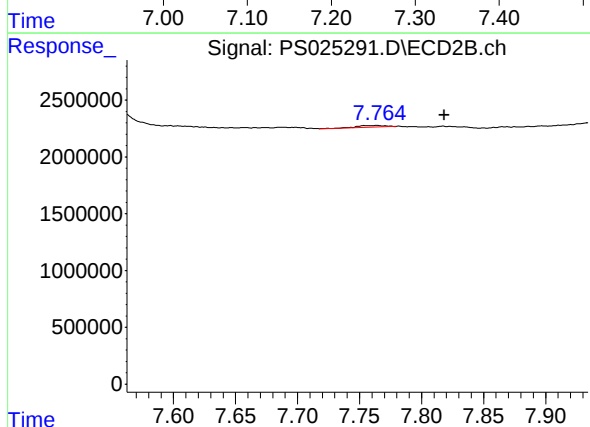


#9 2,4-D

R.T.: 7.764 min
Delta R.T.: -0.054 min
Response: 225392
Conc: N.D.

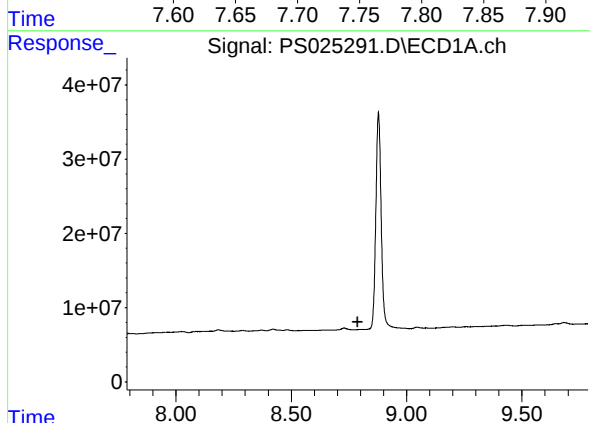

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.787 min
Response: 0
Conc: N.D.

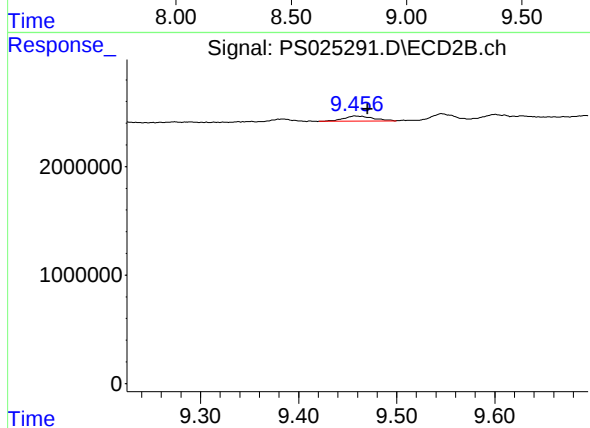

#13 2,4-DB

R.T.: 9.457 min
Delta R.T.: -0.013 min
Response: 987581
Conc: 1.80 ng/ml