

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
 Data File : PS025303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2023 12:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 23:37:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.352	6.763	1181.0E6	380.6E6	527.033	536.158
Target Compounds						
1) T Dalapon	0.000	2.557	0	3475511	N.D.	3.024
2) T 3,5-DICHL...	5.693	0.000	1409175	0	<MDL	N.D. #
3) T 4-Nitroph...	0.000	6.364	0	837941	N.D.	1.687
5) T DICAMBA	0.000	6.960	0	2740252	N.D.	<MDL
6) T MCPP	6.680f	6.960f	22229666	2740252	3.304	1.373 #
7) T MCPA	0.000	7.213	0	376682	N.D.	<MDL
8) T DICHLORPROP	0.000	7.549	0	7968273	N.D.	10.301
9) T 2,4-D	7.242	7.760f	22287945	46025	7.195	<MDL #
11) T 2,4,5-TP ...	0.000	8.549f	0	364571	N.D.	<MDL
15) T Picloram	0.000	10.773	0	2383719	N.D.	<MDL
16) T DCPA	0.000	10.773f	0	2383719	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
Data File : PS025303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2023 12:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 23:37:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

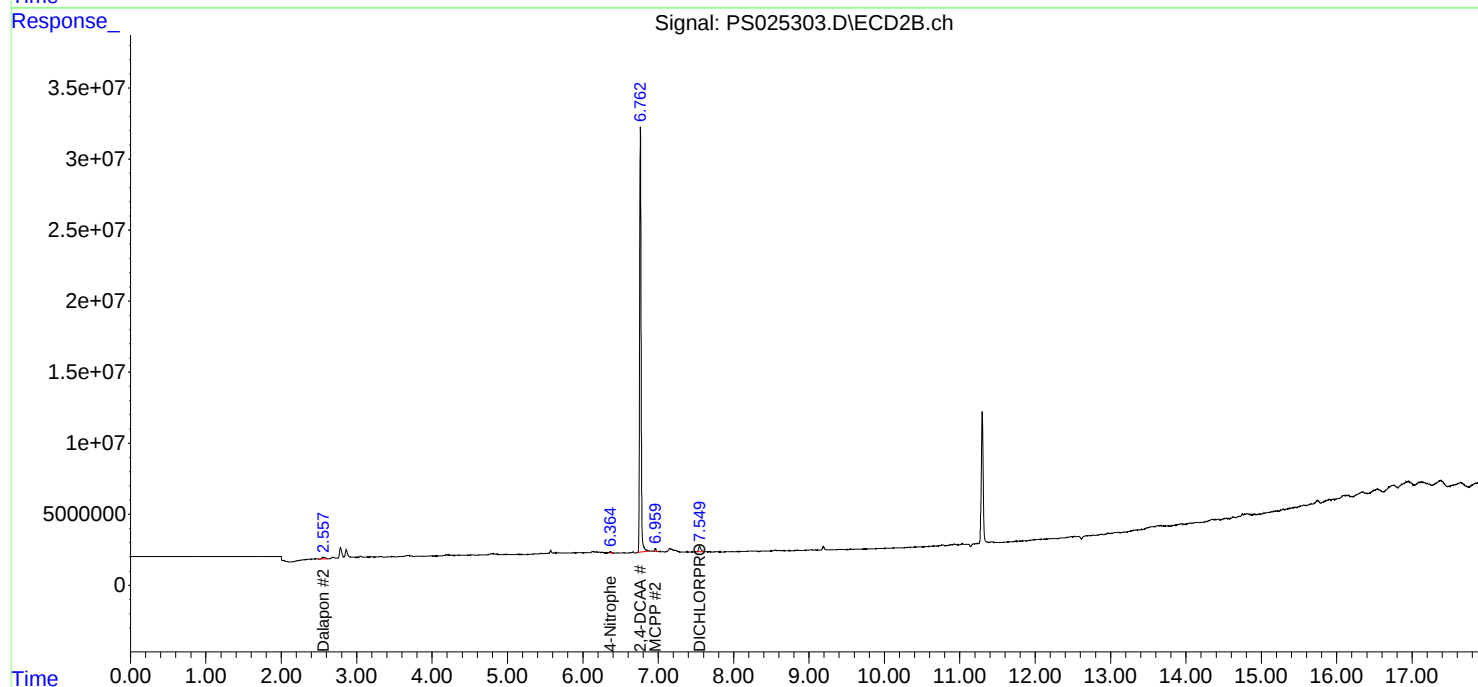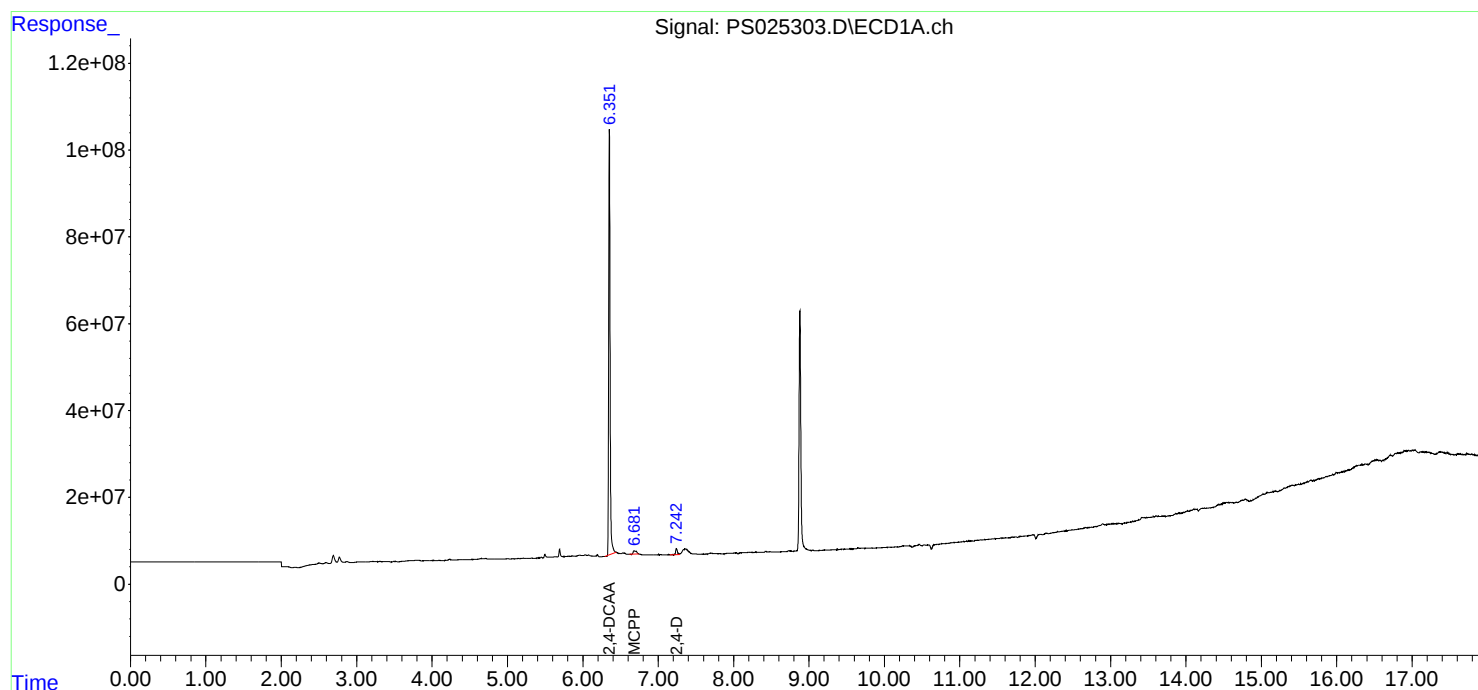


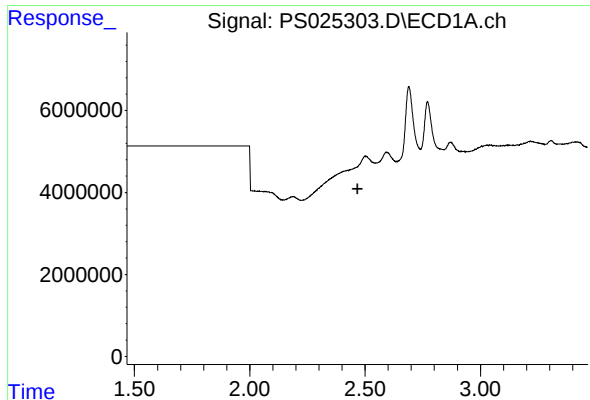

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

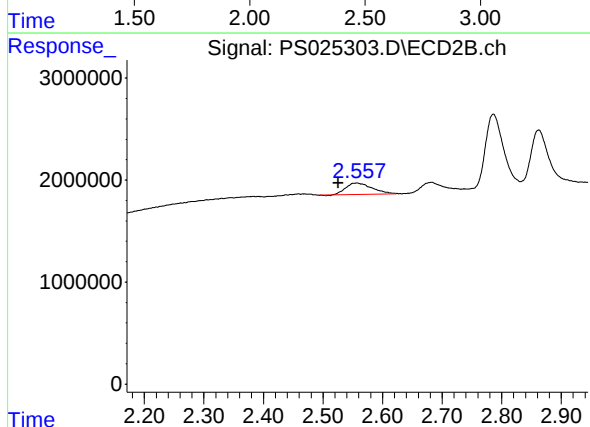


#1 Dalapon

R.T.: 2.557 min
Delta R.T.: 0.031 min
Response: 3475511
Conc: 3.02 ng/ml

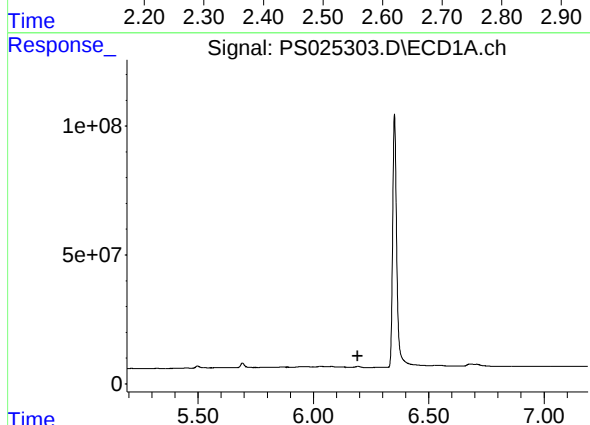


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

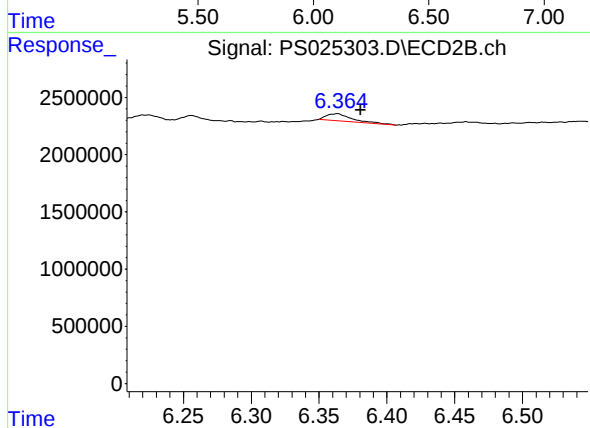

#3 4-Nitrophenol


R.T.: 6.364 min
Delta R.T.: -0.017 min
Response: 837941
Conc: 1.69 ng/ml

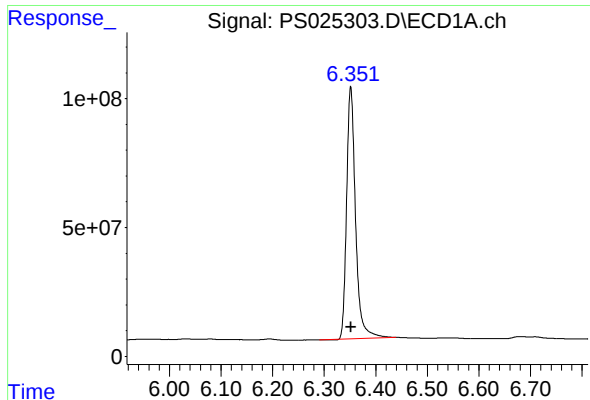

#4 2,4-DCAA


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 1180976576
Conc: 527.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

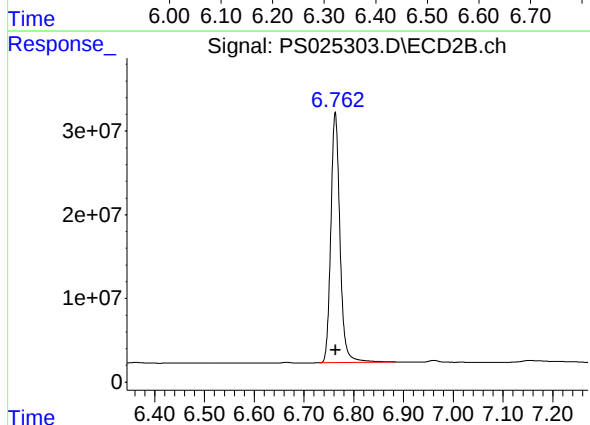


#4 2,4-DCAA

R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 380550381
Conc: 536.16 ng/ml

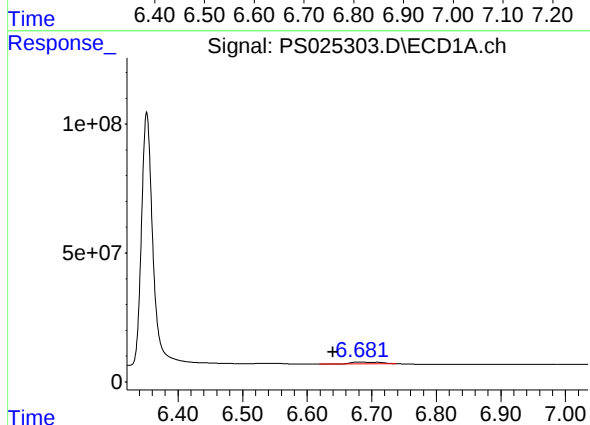


#6 MCPP

R.T.: 6.680 min
Delta R.T.: 0.040 min
Response: 22229666
Conc: 3.30 ug/ml

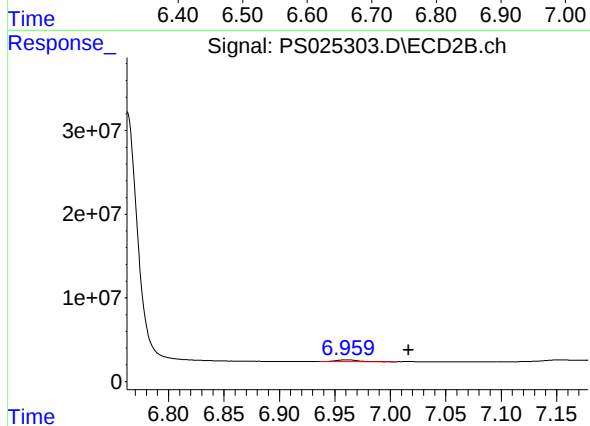

#6 MCPP


R.T.: 6.960 min
Delta R.T.: -0.056 min
Response: 2740252
Conc: 1.37 ug/ml

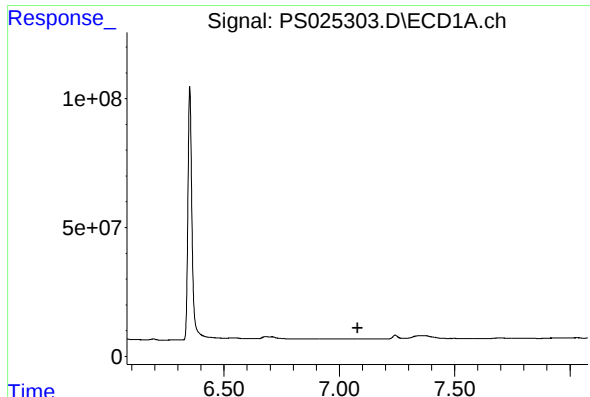

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

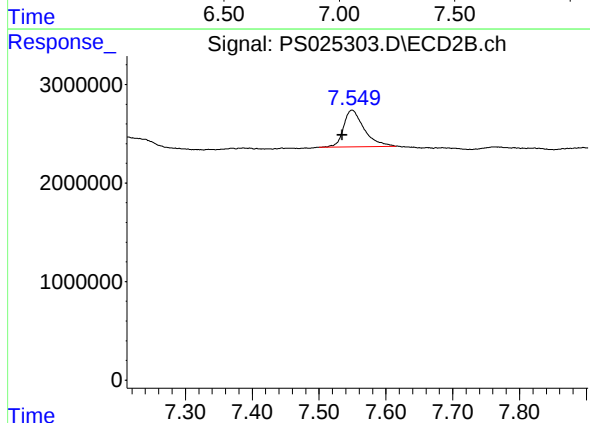


#8 DICHLORPROP

R.T.: 7.549 min
Delta R.T.: 0.014 min
Response: 7968273
Conc: 10.30 ng/ml

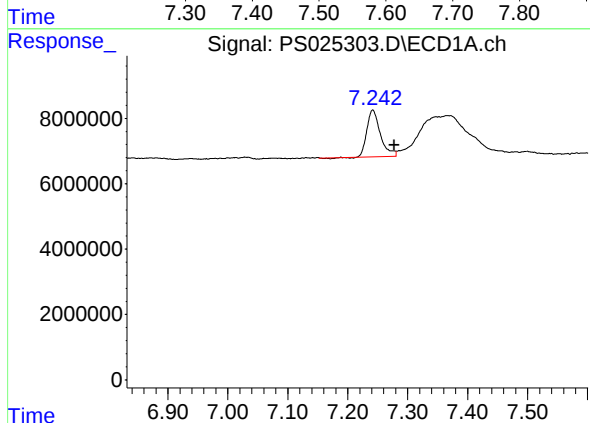

#9 2,4-D

R.T.: 7.242 min
Delta R.T.: -0.036 min
Response: 22287945
Conc: 7.19 ng/ml

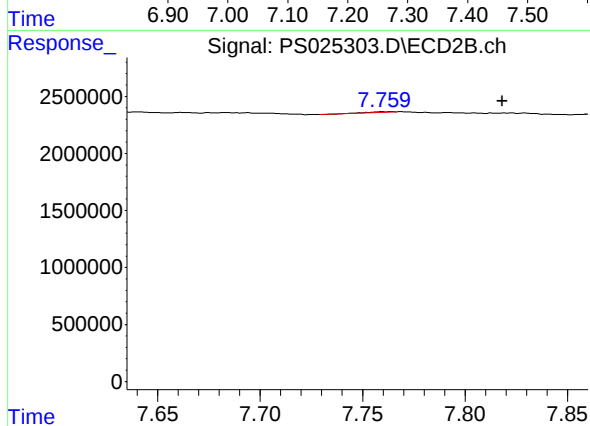

#9 2,4-D

R.T.: 7.760 min
Delta R.T.: -0.058 min
Response: 46025
Conc: N.D.