

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
 Data File : PS025266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 21:52
 Operator : AR\AJ
 Sample : 05906-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 GHL-SS-34

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/29/2023
 Supervised By :Ankita Jodhani 12/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 23:53:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.351 6.762 617.2E6 162.6E6 275.424m 229.063m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122823\
Data File : PS025266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 21:52
Operator : AR\AJ
Sample : 05906-06
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
GHL-SS-34


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/29/2023
Supervised By : Ankita Jodhani 12/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 23:53:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

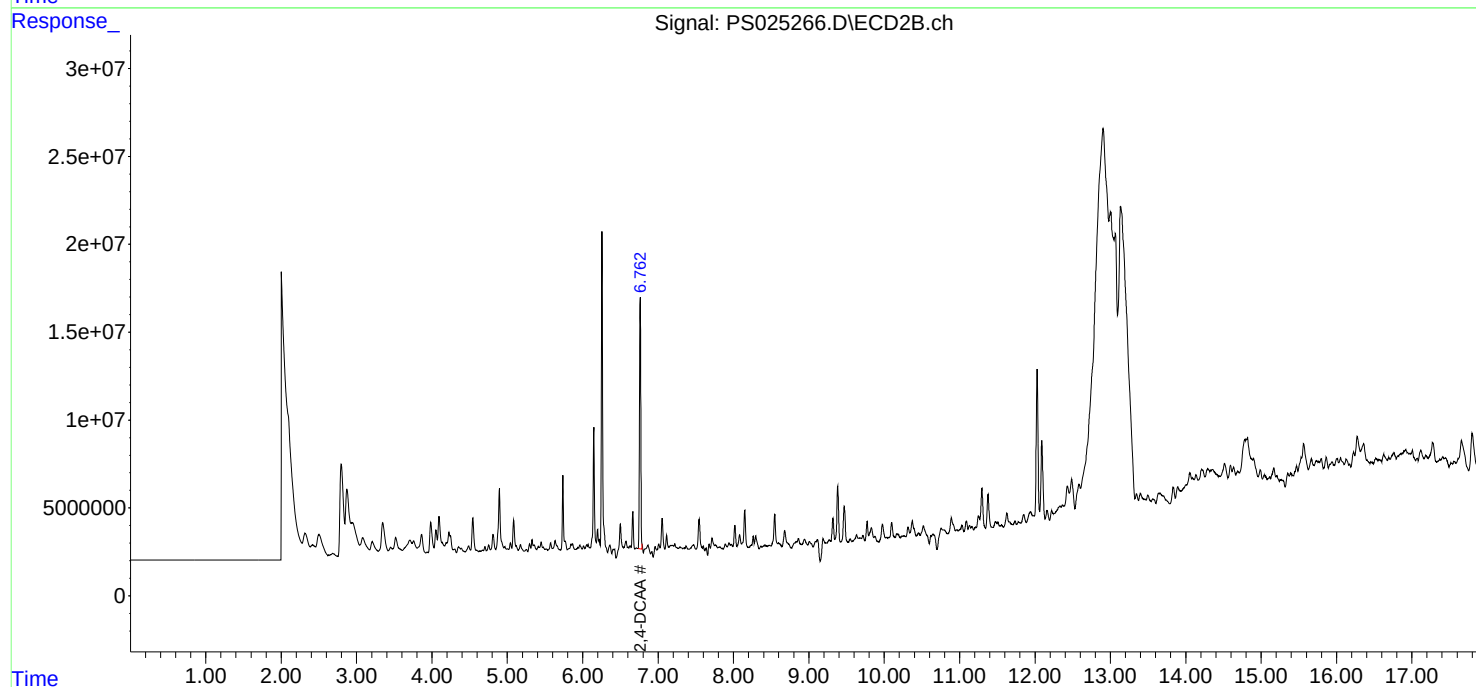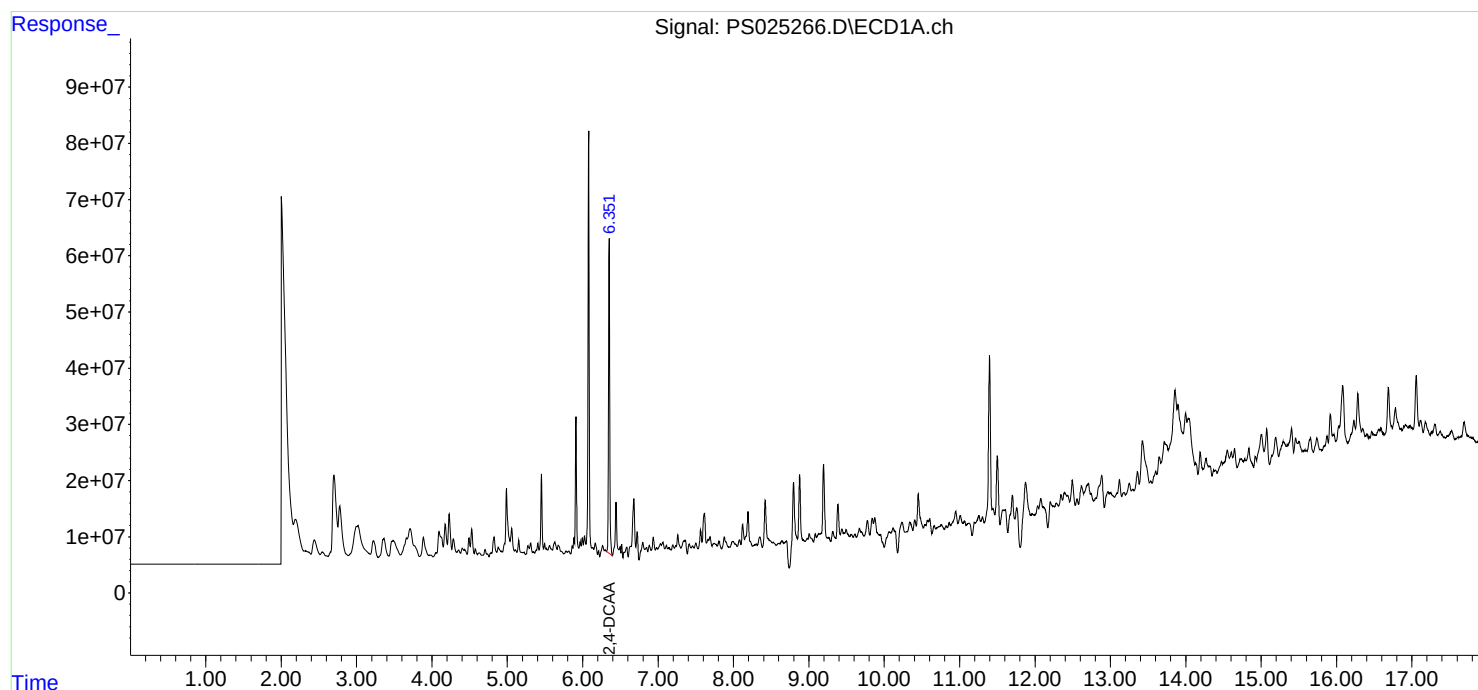

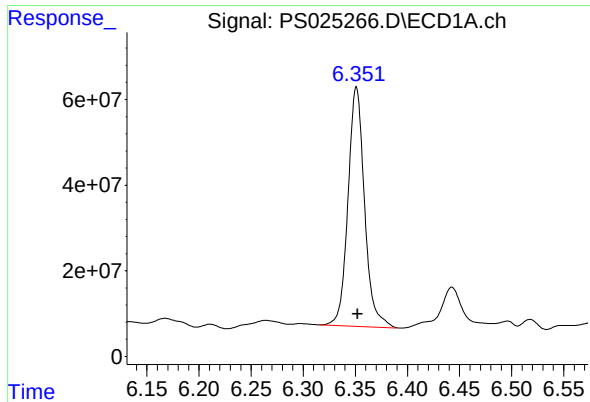


#4 2,4-DCAA

R.T.: 6.351 min
Delta R.T.: -0.001 min
Response: 617170054
Conc: 275.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
GHL-SS-34

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/29/2023
Supervised By :Ankita Jodhani 12/29/2023

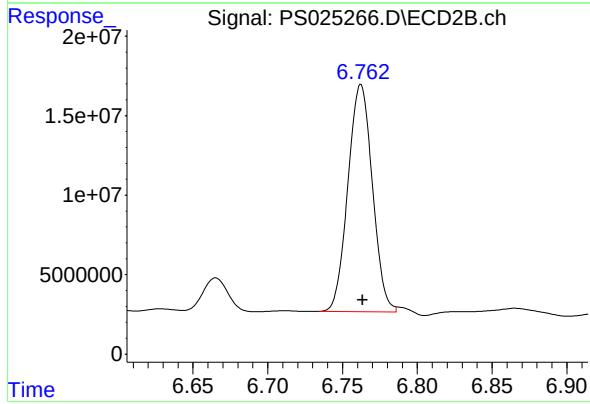

#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.002 min
Response: 162582573
Conc: 229.06 ng/ml