

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122922\
 Data File : PS021593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 08:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 03:23:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.377	6.809	1309.1E6	976.6E6	450.567	566.460 #
Target Compounds							
1) T	Dalapon	2.515	0.000	1001294	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.731	0.000	7122779	0	1.792	N.D. #
3) T	4-Nitroph...	6.227	0.000	4711048	0	2.620	N.D. #
6) T	MCP	0.000	7.120f	0	899780	N.D.	<MDL
7) T	MCPA	6.759	7.216f	3685374	11285105	<MDL	1.276 #
8) T	DICHLORPROP	7.131	7.656f	96354	1994833	<MDL	1.013 #
9) T	2,4-D	7.314	7.953f	2304365	53551	<MDL	<MDL #
10) T	Pentachlo...	7.547	0.000	2289627	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.087	8.687	3242812	2395251	<MDL	<MDL #
12) T	2,4,5-T	8.311	9.088	33128399	2521155	1.756	<MDL #
13) T	2,4-DB	8.846	9.635f	2060917	1936632	<MDL	1.347 #
14) T	DINOSEB	0.000	9.892	0	1011951	N.D.	<MDL
15) T	Picloram	9.753	10.902	3612912	78805760	<MDL	4.846 #
16) T	DCPA	10.165	10.816	3011264	1235108	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122922\
Data File : PS021593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 08:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 03:23:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

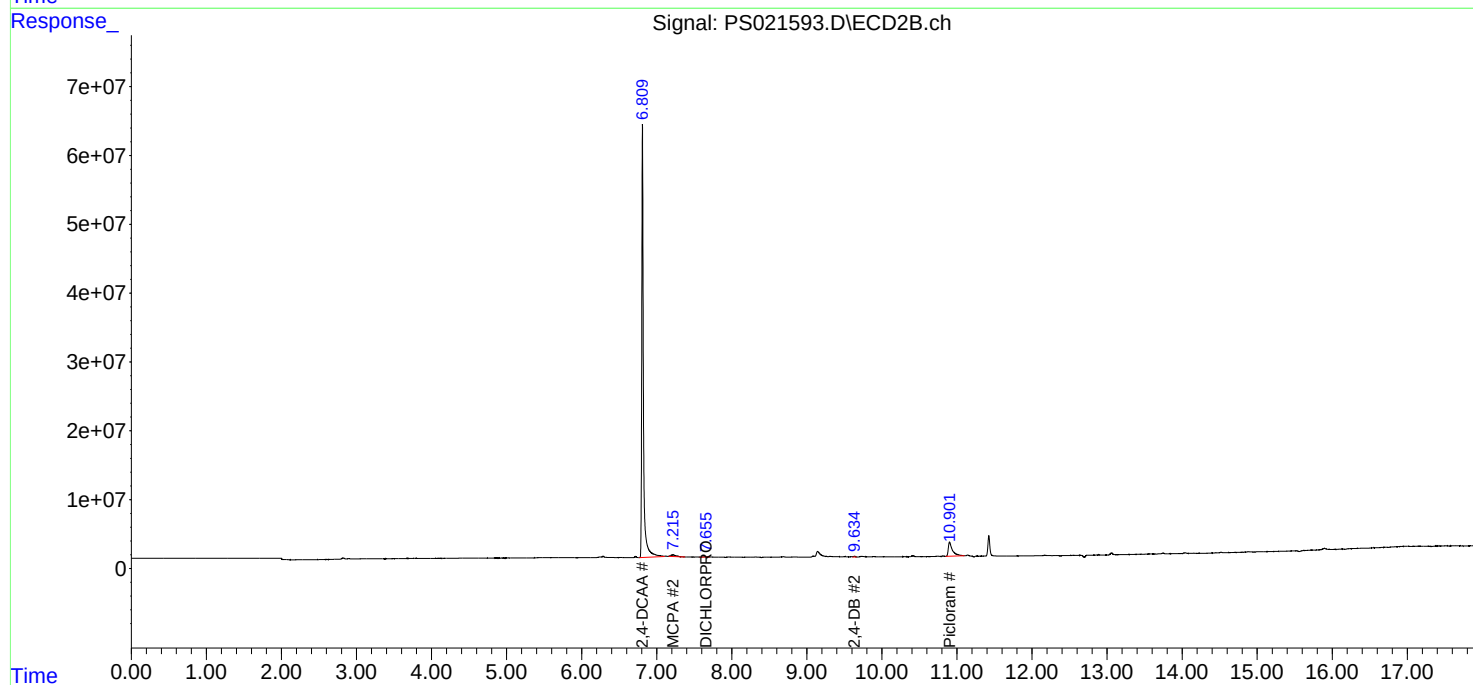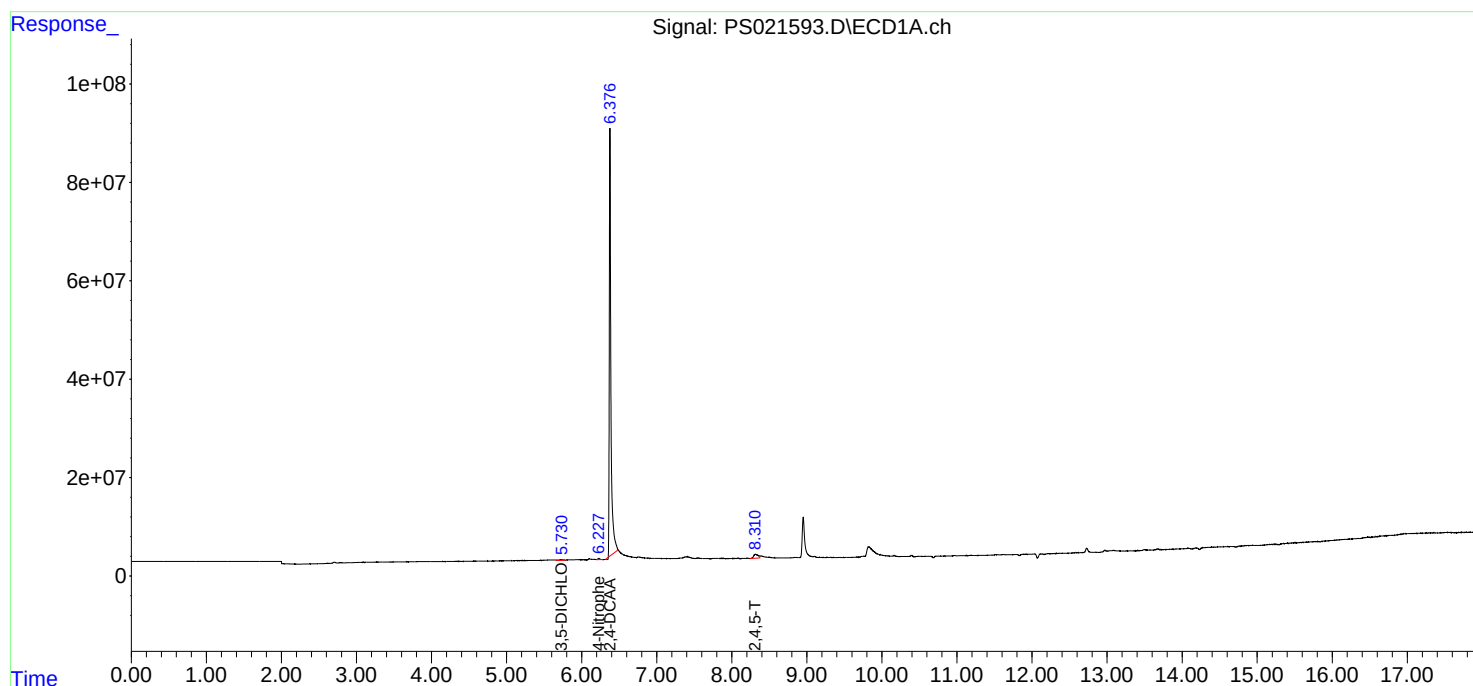


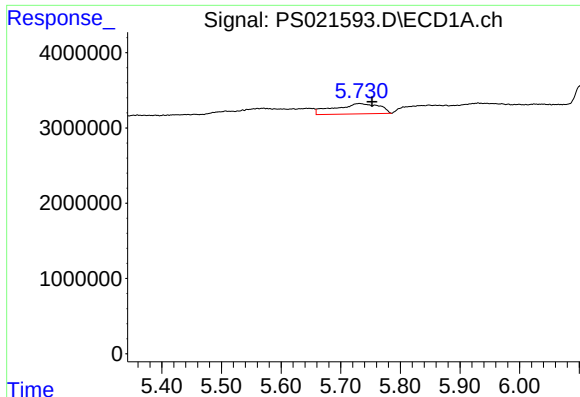

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.731 min
Delta R.T.: -0.021 min
Response: 7122779
Conc: 1.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

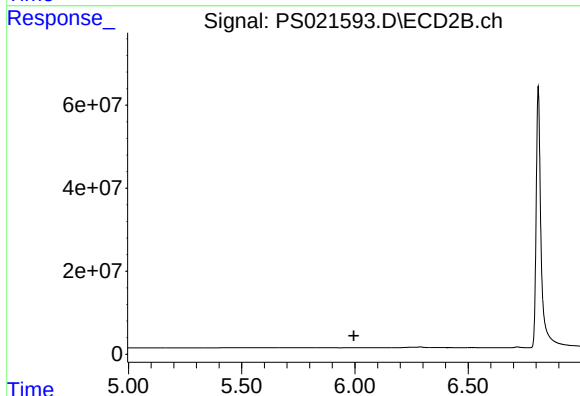


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

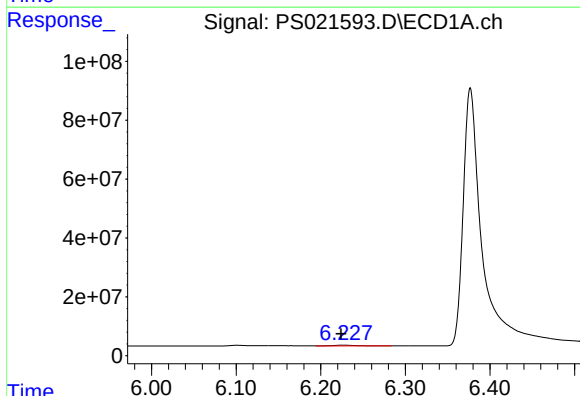


#3 4-Nitrophenol

R.T.: 6.227 min
Delta R.T.: 0.002 min
Response: 4711048
Conc: 2.62 ng/ml

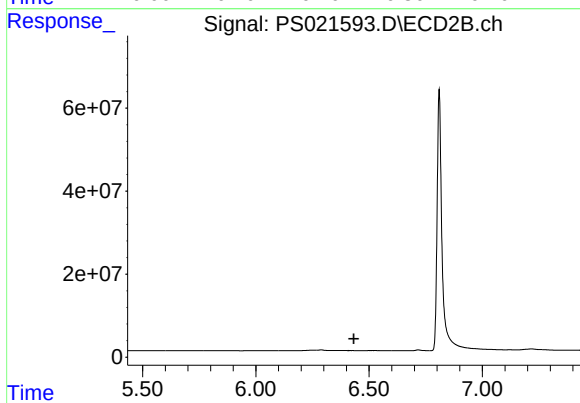

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

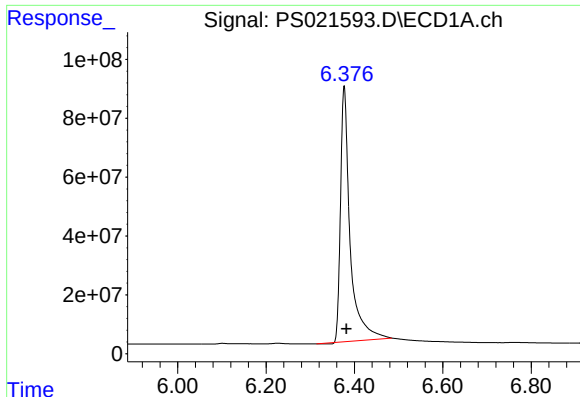

#4 2,4-DCAA


R.T.: 6.377 min
Delta R.T.: -0.005 min
Response: 1309121171
Conc: 450.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

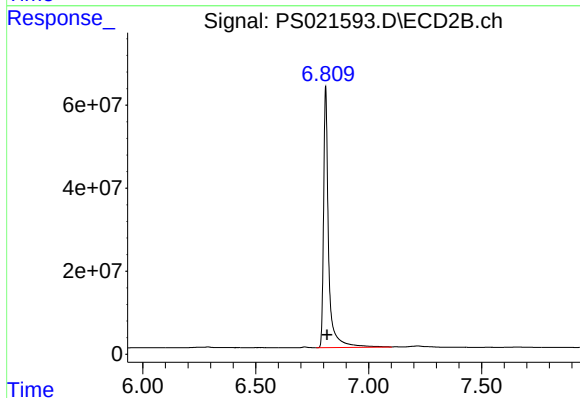


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.006 min
Response: 976572896
Conc: 566.46 ng/ml

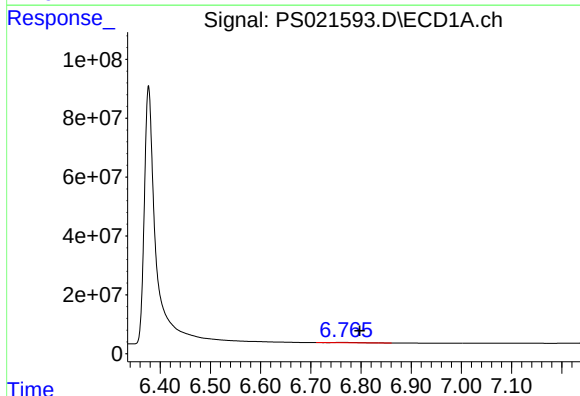


#7 MCPA

R.T.: 6.759 min
Delta R.T.: -0.038 min
Response: 3685374
Conc: N.D.

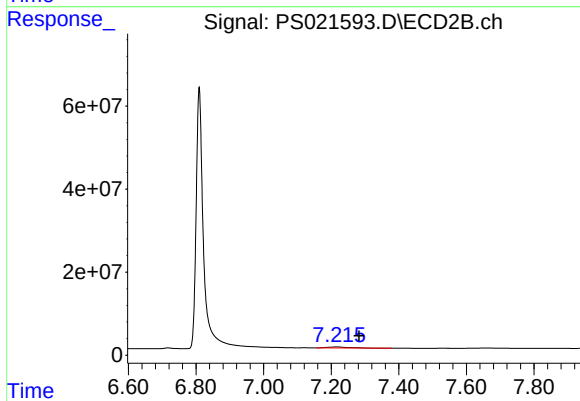

#7 MCPA


R.T.: 7.216 min
Delta R.T.: -0.066 min
Response: 11285105
Conc: 1.28 ug/ml

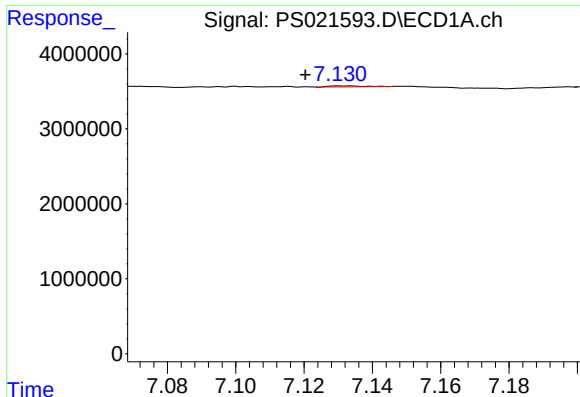

#8 DICHLORPROP


R.T.: 7.131 min
Delta R.T.: 0.011 min
Response: 96354
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

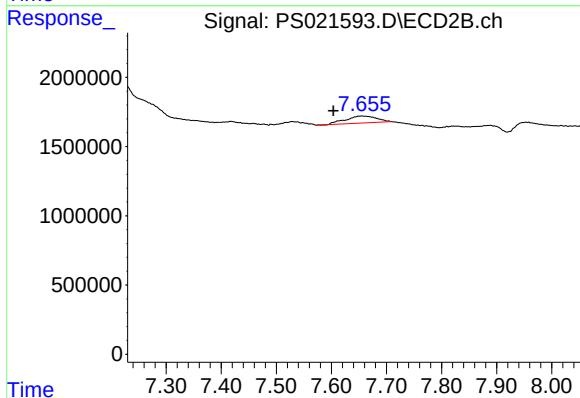


#8 DICHLORPROP

R.T.: 7.656 min
Delta R.T.: 0.052 min
Response: 1994833
Conc: 1.01 ng/ml

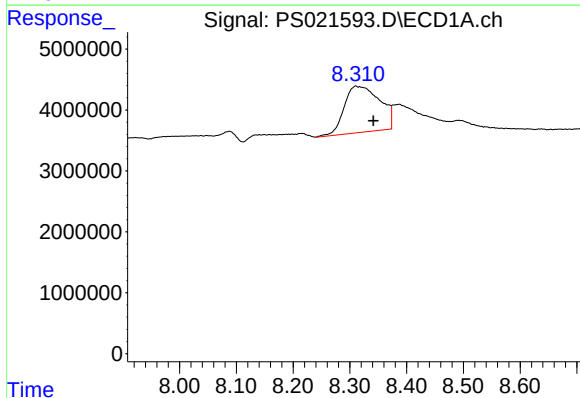


#12 2,4,5-T

R.T.: 8.311 min
Delta R.T.: -0.031 min
Response: 33128399
Conc: 1.76 ng/ml

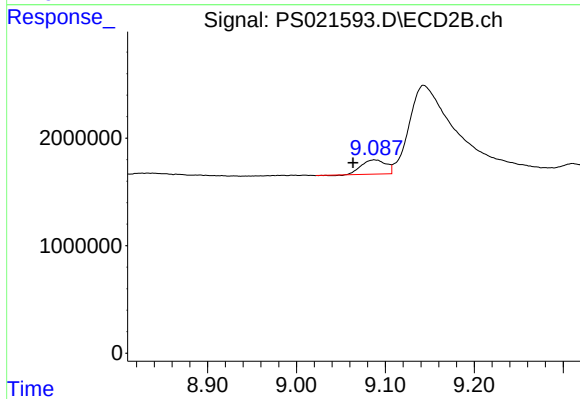

#12 2,4,5-T


R.T.: 9.088 min
Delta R.T.: 0.024 min
Response: 2521155
Conc: N.D.

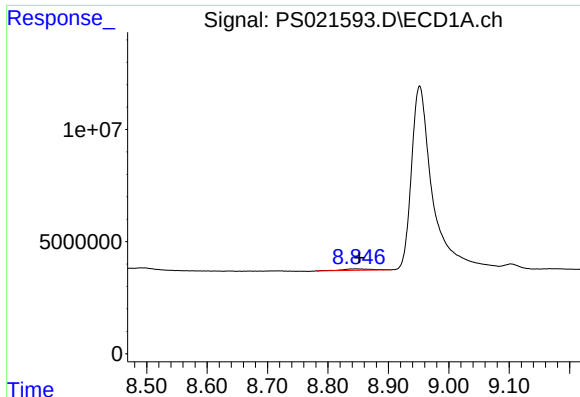

#13 2,4-DB


R.T.: 8.846 min
Delta R.T.: -0.006 min
Response: 2060917
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

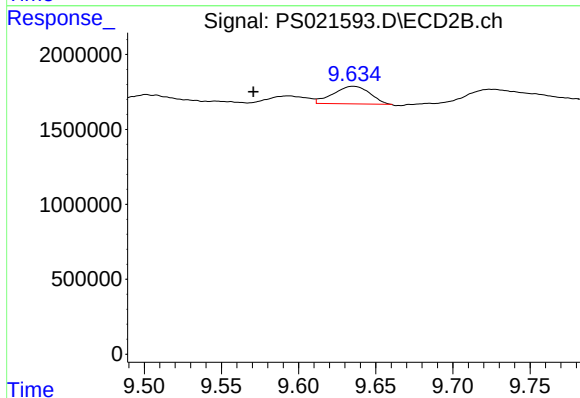


#13 2,4-DB

R.T.: 9.635 min
Delta R.T.: 0.065 min
Response: 1936632
Conc: 1.35 ng/ml

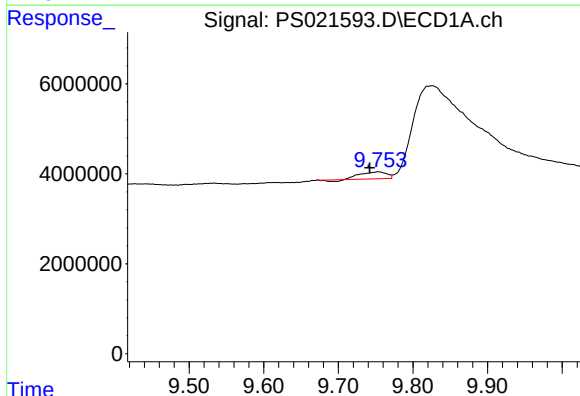

#15 Picloram

R.T.: 9.753 min
Delta R.T.: 0.011 min
Response: 3612912
Conc: N.D.

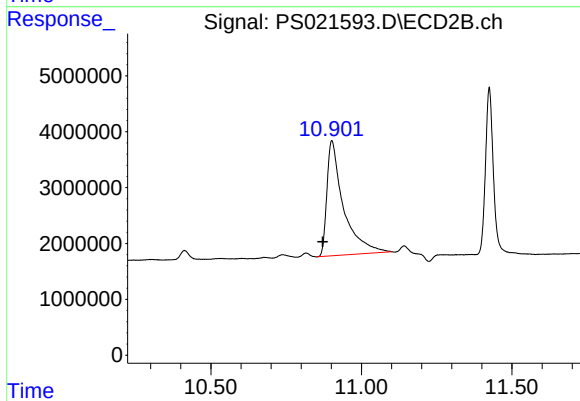

#15 Picloram

R.T.: 10.902 min
Delta R.T.: 0.030 min
Response: 78805760
Conc: 4.85 ng/ml