

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
 Data File : PS025306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2023 14:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 06:01:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.353	6.764	1181.9E6	383.1E6	527.464	539.804
Target Compounds						
1) T Dalapon	0.000	2.556	0	4022760	N.D.	3.500
2) T 3,5-DICHL...	5.693	5.886f	-566577	279387	N.D.	<MDL
3) T 4-Nitroph...	0.000	6.363	0	1034323	N.D.	2.082
5) T DICAMBA	0.000	6.962	0	3787617	N.D.	1.251
6) T MCPP	6.684f	6.962f	12048388	3787617	1.791	1.897
7) T MCPA	6.709f	7.230	11732860	2121929	1.237	<MDL #
8) T DICHLORPROP	0.000	7.552	0	10669567	N.D.	13.793
9) T 2,4-D	7.244	7.763f	35987740	11747	11.617	<MDL #
12) T 2,4,5-T	0.000	9.027f	0	1279930	N.D.	<MDL
15) T Picloram	0.000	10.774	0	3792461	N.D.	<MDL
16) T DCPA	0.000	10.774f	0	3792461	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
Data File : PS025306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2023 14:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 06:01:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

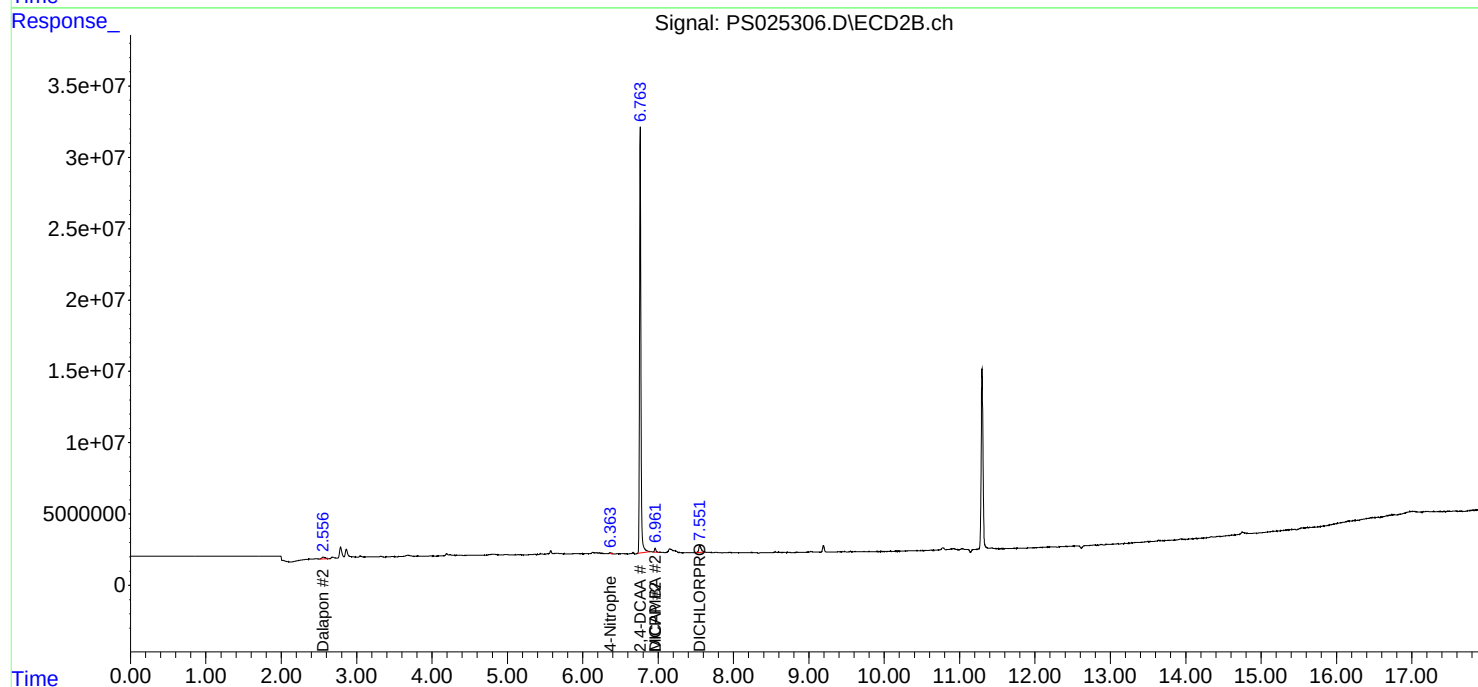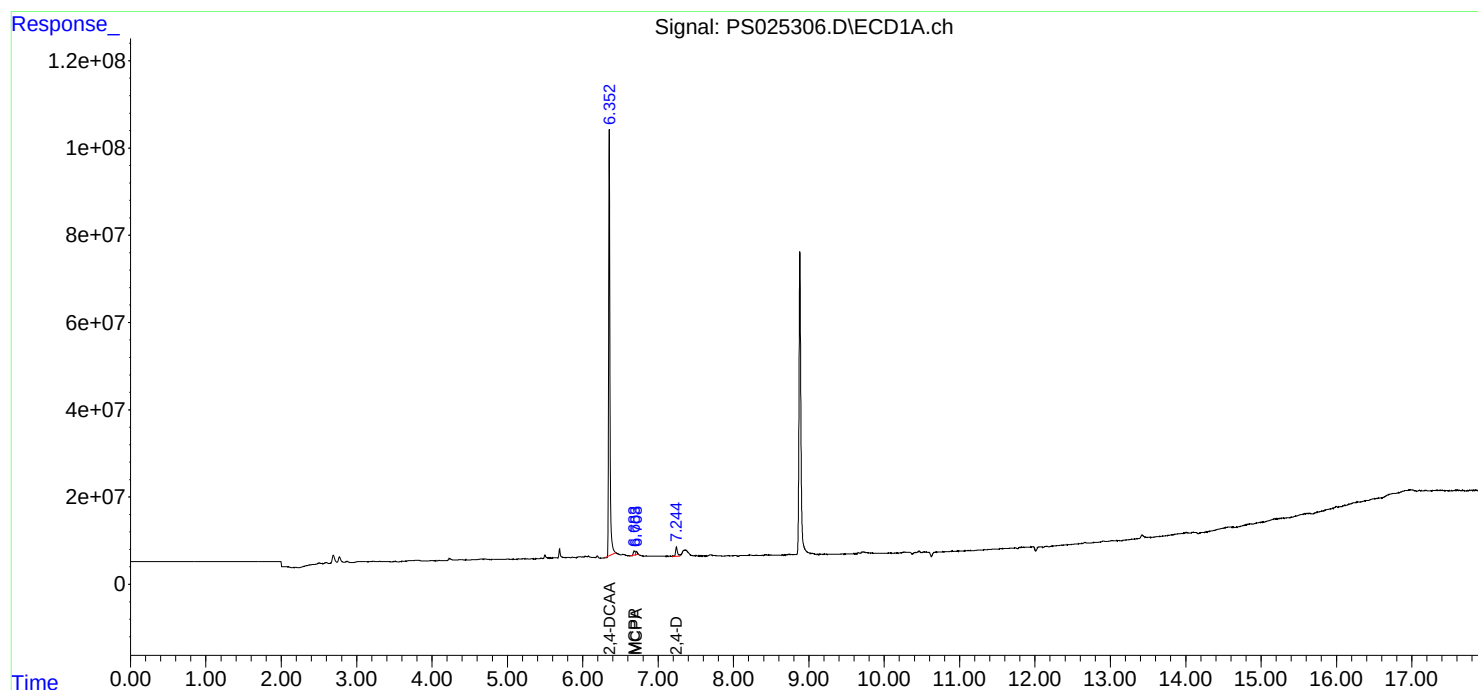


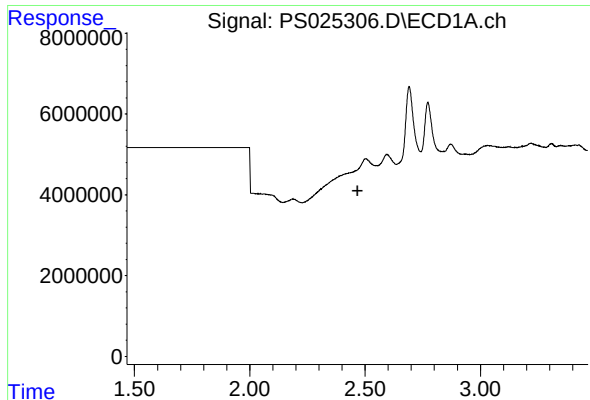

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

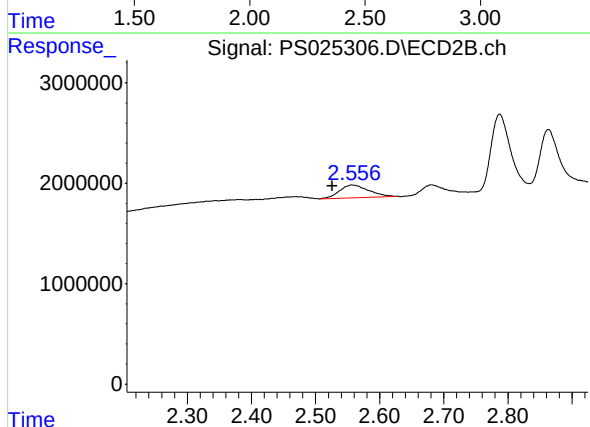


#1 Dalapon

R.T.: 2.556 min
Delta R.T.: 0.030 min
Response: 4022760
Conc: 3.50 ng/ml

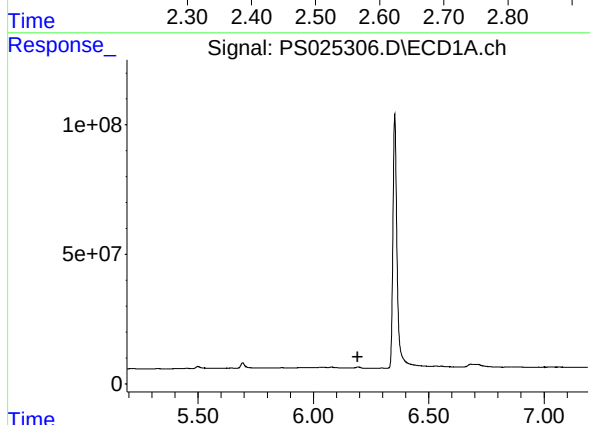


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

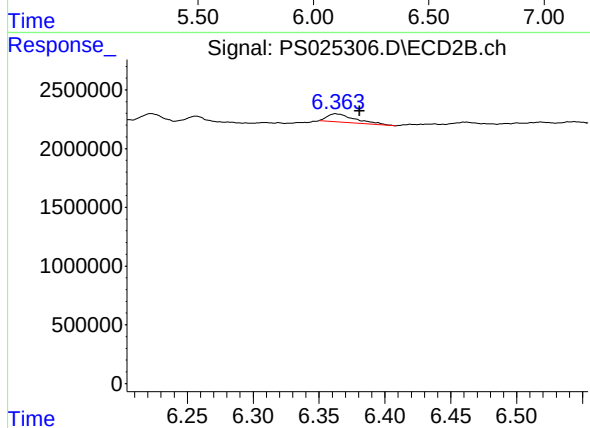

#3 4-Nitrophenol


R.T.: 6.363 min
Delta R.T.: -0.018 min
Response: 1034323
Conc: 2.08 ng/ml

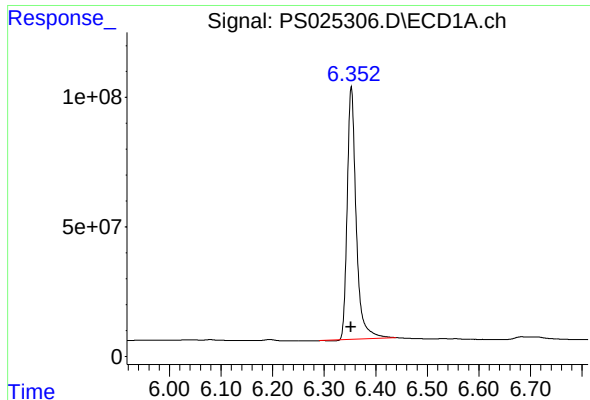

#4 2,4-DCAA


R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 1181942790
Conc: 527.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

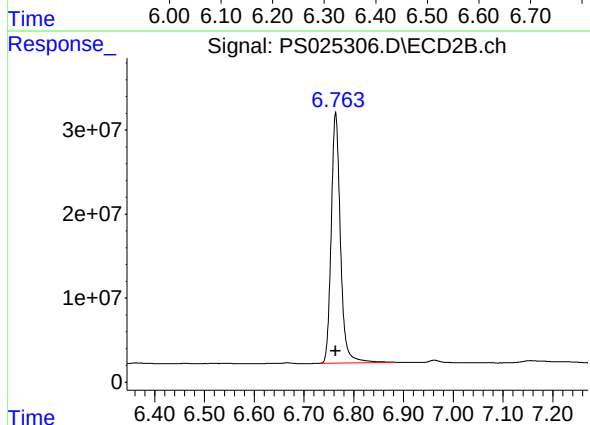


#4 2,4-DCAA

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 383138691
Conc: 539.80 ng/ml

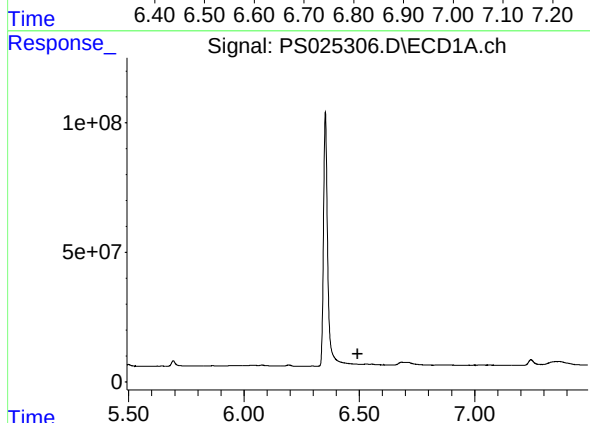


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

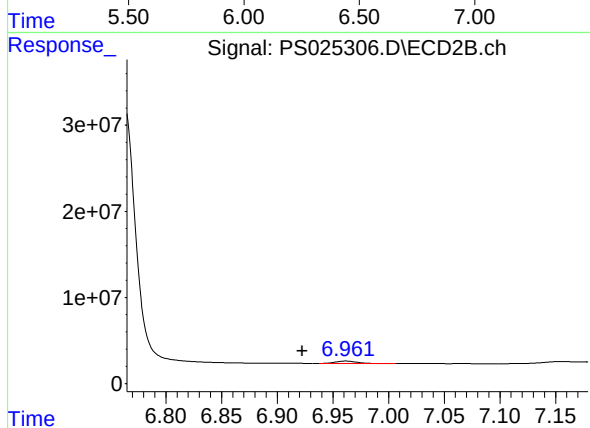

#5 DICAMBA


R.T.: 6.962 min
Delta R.T.: 0.039 min
Response: 3787617
Conc: 1.25 ng/ml

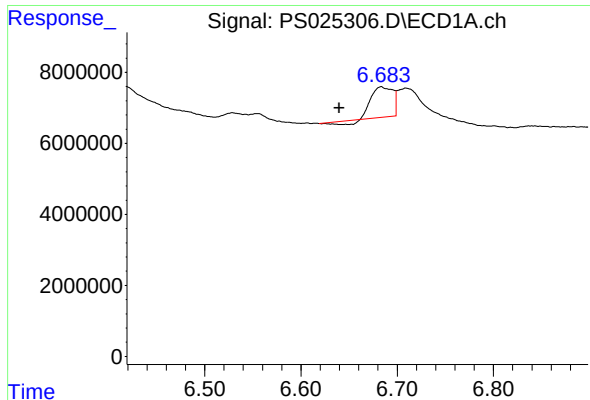

#6 MCPP


R.T.: 6.684 min
Delta R.T.: 0.044 min
Response: 12048388
Conc: 1.79 ug/ml

Instrument :
ECD_S
ClientSampleId :

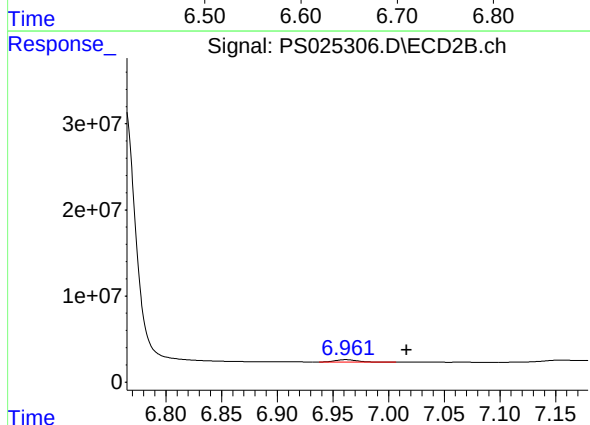


#6 MCPP

R.T.: 6.962 min
Delta R.T.: -0.055 min
Response: 3787617
Conc: 1.90 ug/ml

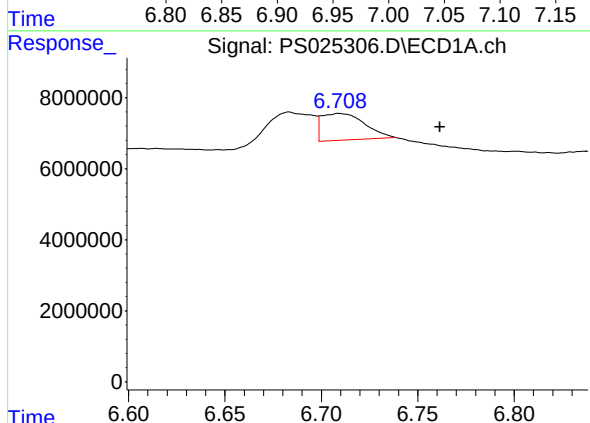


#7 MCPA

R.T.: 6.709 min
Delta R.T.: -0.052 min
Response: 11732860
Conc: 1.24 ug/ml

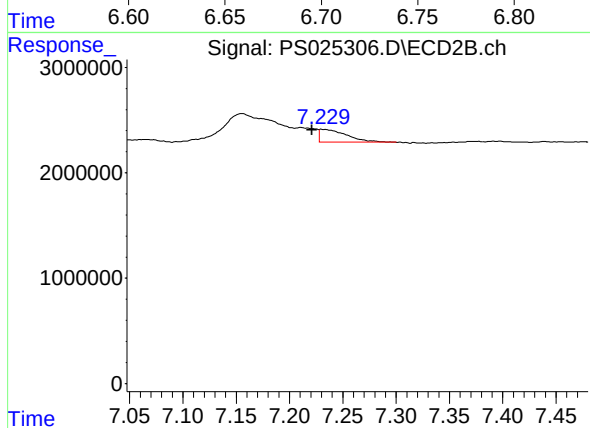

#7 MCPA


R.T.: 7.230 min
Delta R.T.: 0.009 min
Response: 2121929
Conc: N.D.

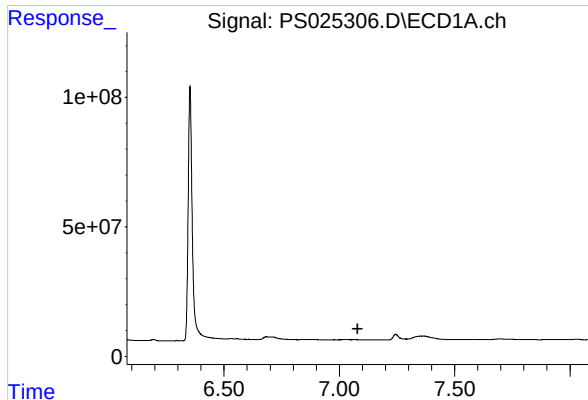

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

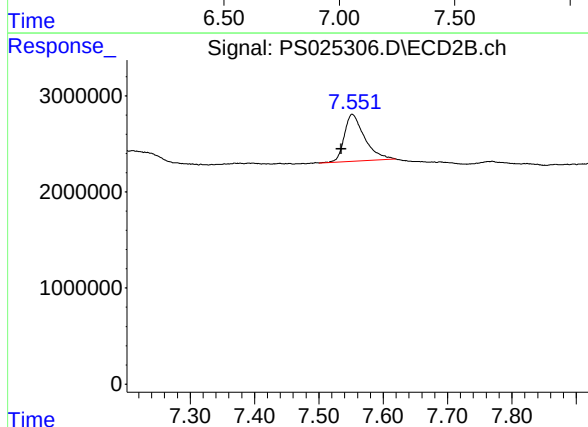


#8 DICHLORPROP

R.T.: 7.552 min
Delta R.T.: 0.017 min
Response: 10669567
Conc: 13.79 ng/ml

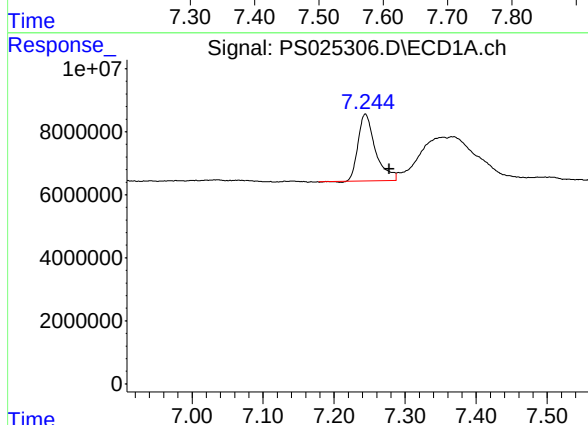

#9 2,4-D

R.T.: 7.244 min
Delta R.T.: -0.033 min
Response: 35987740
Conc: 11.62 ng/ml

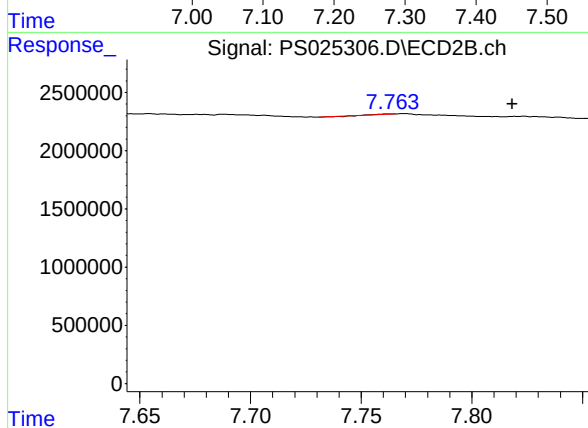

#9 2,4-D

R.T.: 7.763 min
Delta R.T.: -0.055 min
Response: 11747
Conc: N.D.