

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
 Data File : PS025318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2023 00:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 05:52:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.352	6.764	1206.2E6	384.9E6	538.287	542.242
Target Compounds							
1) T	Dalapon	0.000	2.552	0	4076762	N.D.	3.547
2) T	3,5-DICHL...	5.692	0.000	1514912	0	<MDL	N.D. #
3) T	4-Nitroph...	0.000	6.363	0	998249	N.D.	2.010
5) T	DICAMBA	0.000	6.962	0	3951703	N.D.	1.306
6) T	MCP	6.707f	7.066f	30704337	922469	4.564	<MDL #
7) T	MCPA	6.707f	7.155f	30704337	15327832	3.238	4.877 #
8) T	DICHLORPROP	0.000	7.554	0	13886557	N.D.	17.952
9) T	2,4-D	7.245	7.765f	33394083	151298	10.780	<MDL #
12) T	2,4,5-T	0.000	9.032f	0	688329	N.D.	<MDL
14) T	DINOSEB	0.000	9.729f	0	158368	N.D.	<MDL
15) T	Picloram	0.000	10.780	0	2721581	N.D.	<MDL
16) T	DCPA	0.000	10.780f	0	2721581	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
Data File : PS025318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2023 00:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 05:52:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

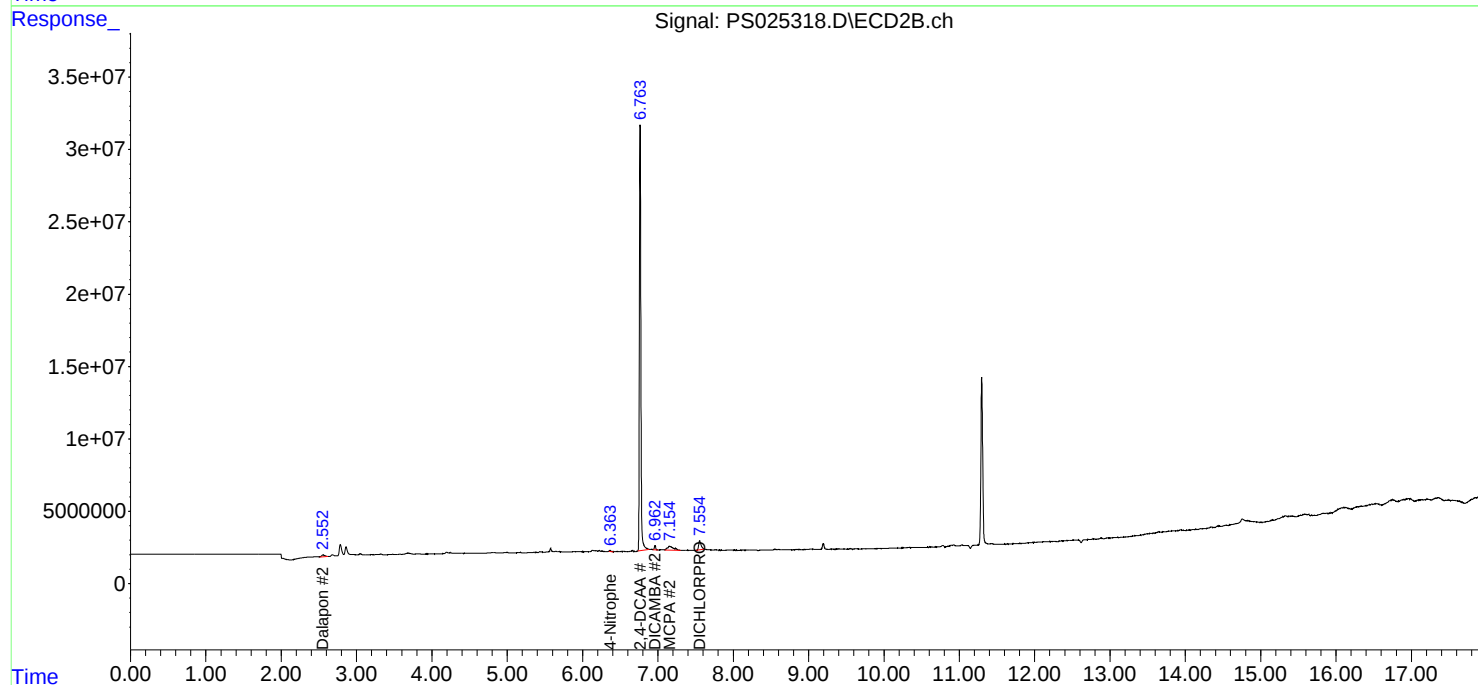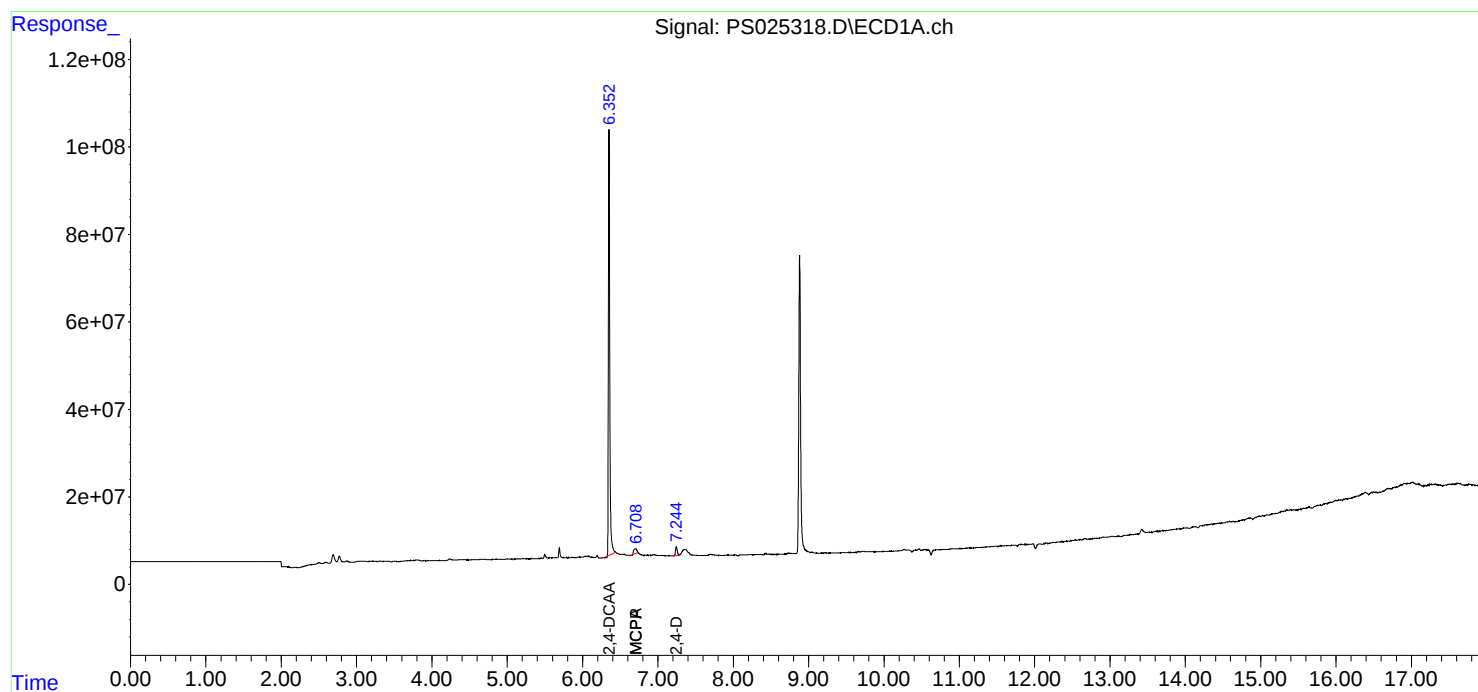


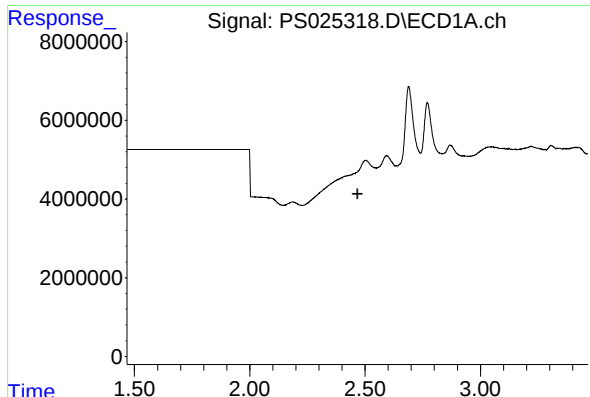

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

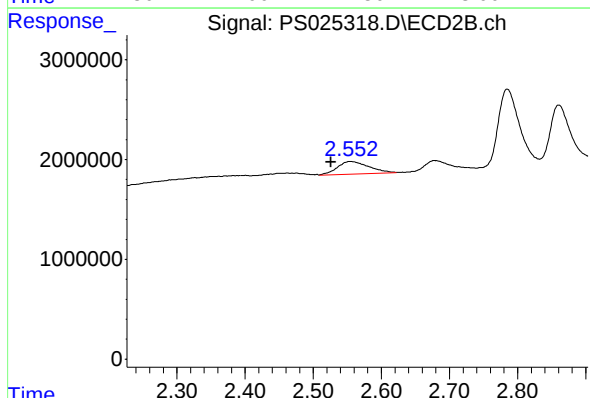


#1 Dalapon

R.T.: 2.552 min
Delta R.T.: 0.027 min
Response: 4076762
Conc: 3.55 ng/ml

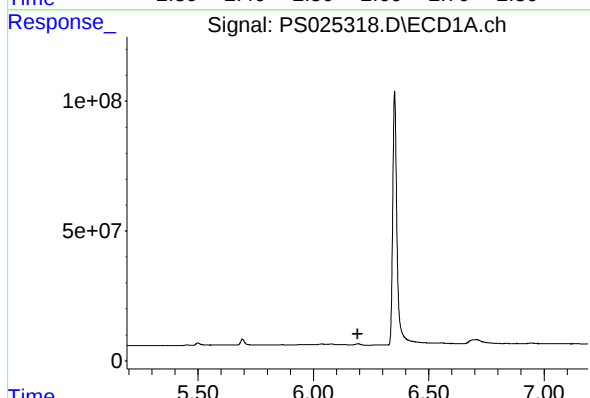


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

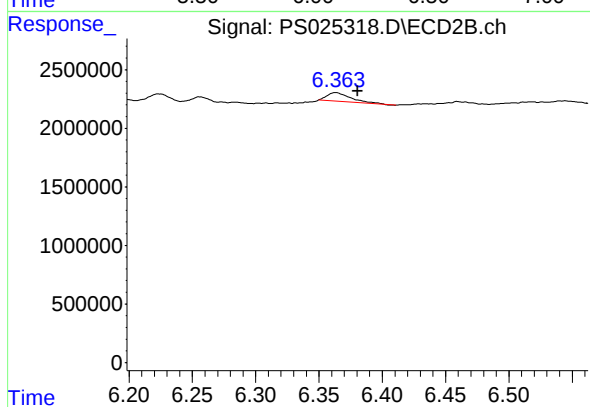

#3 4-Nitrophenol


R.T.: 6.363 min
Delta R.T.: -0.017 min
Response: 998249
Conc: 2.01 ng/ml

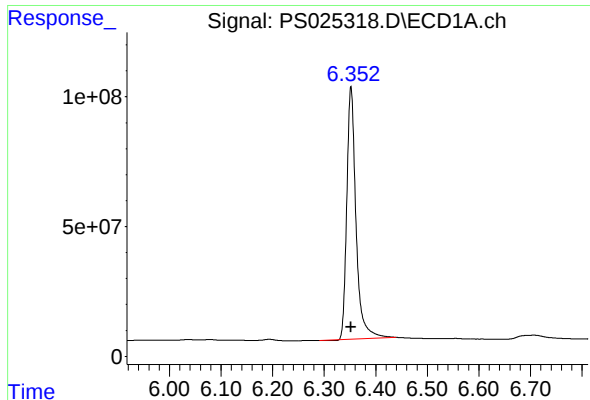

#4 2,4-DCAA


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 1206194233
Conc: 538.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

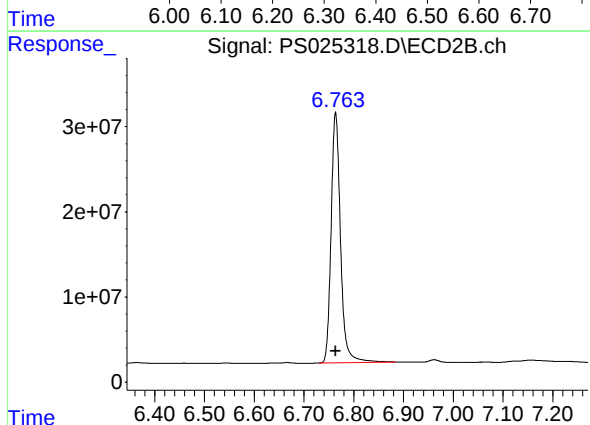


#4 2,4-DCAA

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 384868618
Conc: 542.24 ng/ml

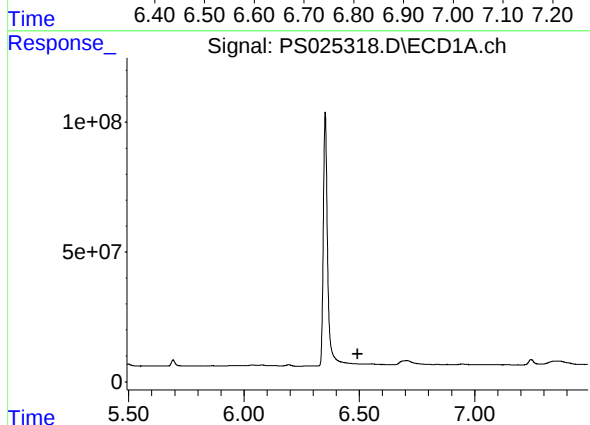


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

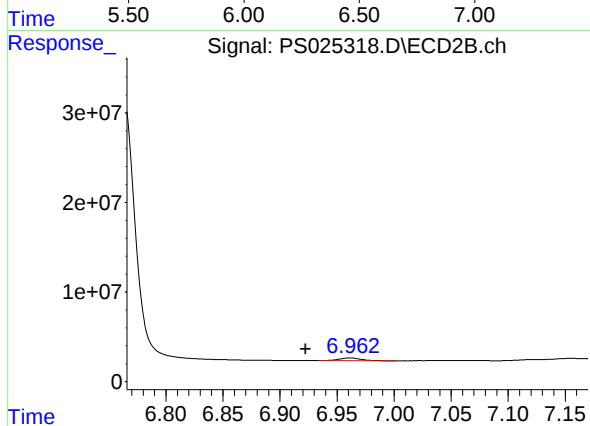

#5 DICAMBA


R.T.: 6.962 min
Delta R.T.: 0.039 min
Response: 3951703
Conc: 1.31 ng/ml

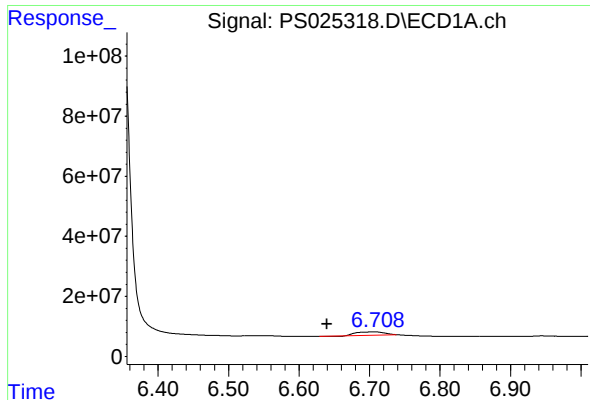

#6 MCPP


R.T.: 6.707 min
Delta R.T.: 0.067 min
Response: 30704337
Conc: 4.56 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

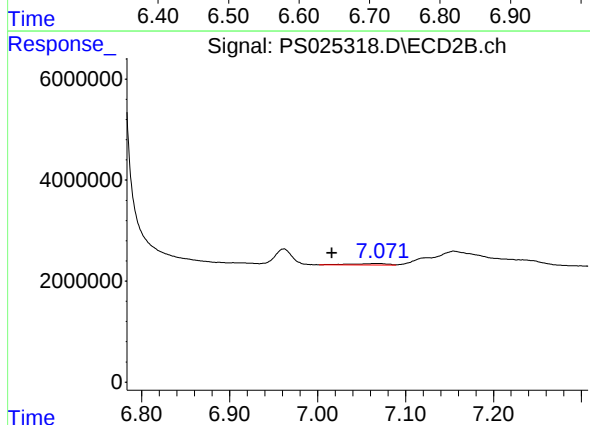


#6 MCPP

R.T.: 7.066 min
Delta R.T.: 0.049 min
Response: 922469
Conc: N.D.

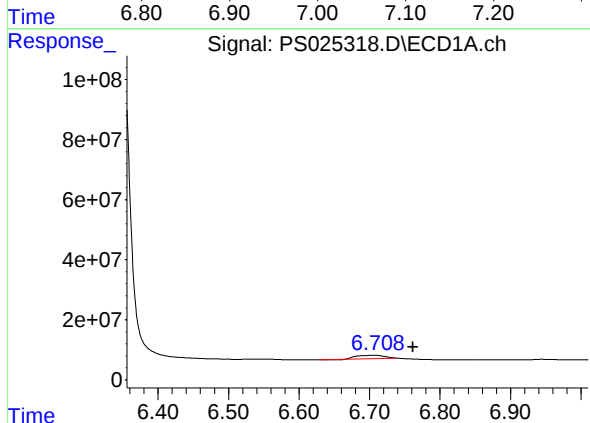


#7 MCPA

R.T.: 6.707 min
Delta R.T.: -0.055 min
Response: 30704337
Conc: 3.24 ug/ml

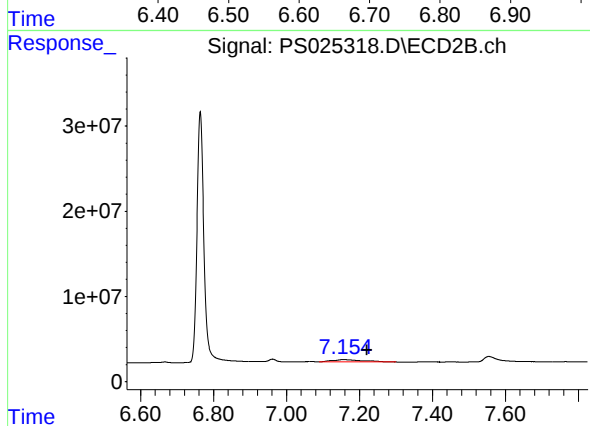

#7 MCPA


R.T.: 7.155 min
Delta R.T.: -0.066 min
Response: 15327832
Conc: 4.88 ug/ml

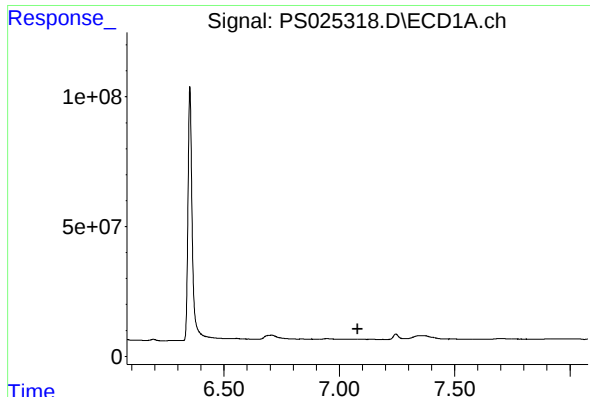

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

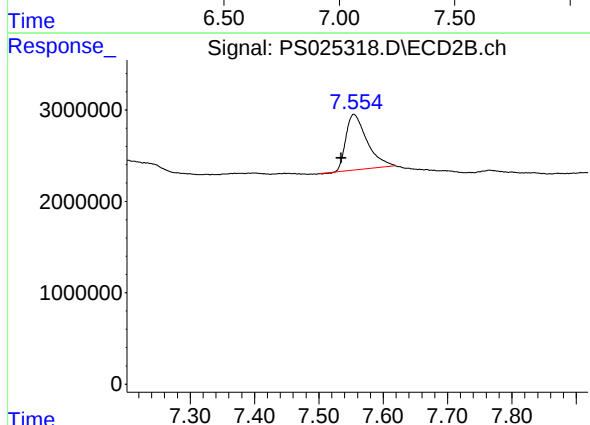


#8 DICHLORPROP

R.T.: 7.554 min
Delta R.T.: 0.019 min
Response: 1388657
Conc: 17.95 ng/ml

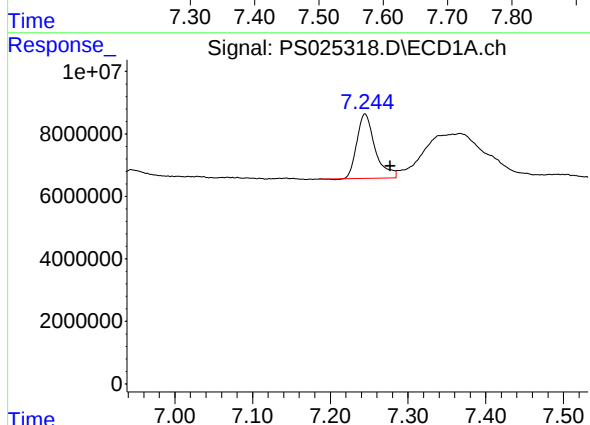

#9 2,4-D

R.T.: 7.245 min
Delta R.T.: -0.033 min
Response: 33394083
Conc: 10.78 ng/ml

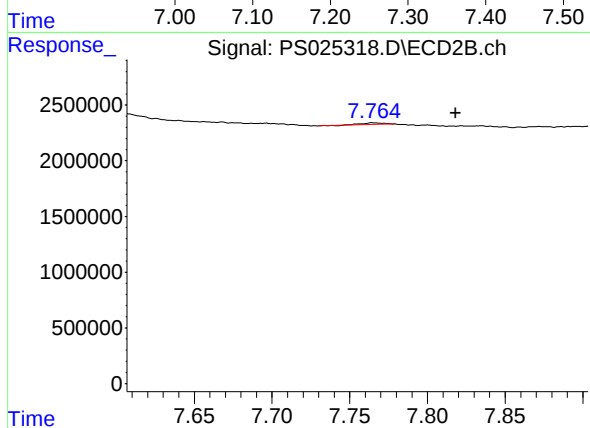

#9 2,4-D

R.T.: 7.765 min
Delta R.T.: -0.053 min
Response: 151298
Conc: N.D.