

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
 Data File : PS025330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2023 05:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 06:35:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.351	6.762	1222.8E6	386.3E6	545.713	544.261
------	----------	-------	-------	----------	---------	---------	---------

Target Compounds

1) T	Dalapon	0.000	2.554	0	3452000	N.D.	3.004
2) T	3,5-DICHL...	5.692	0.000	4784858	0	1.407	N.D. #
3) T	4-Nitroph...	6.192	6.364	11693114	1272423	7.548	2.562 #
5) T	DICAMBA	0.000	6.960	0	3575550	N.D.	1.181
6) T	MCP	6.682f	7.016	67436017	498124	10.023	<MDL #
7) T	MCPA	0.000	7.154f	0	12575834	N.D.	4.001
8) T	DICHLORPROP	0.000	7.550	0	24048583	N.D.	31.089
9) T	2,4-D	7.242	7.764f	31959654	239286	10.317	<MDL #
12) T	2,4,5-T	0.000	8.974	0	253679	N.D.	<MDL
13) T	2,4-DB	0.000	9.463	0	847390	N.D.	1.545
15) T	Picloram	0.000	10.767	0	3909499	N.D.	<MDL
16) T	DCPA	0.000	10.767f	0	3909499	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
Data File : PS025330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2023 05:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 06:35:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

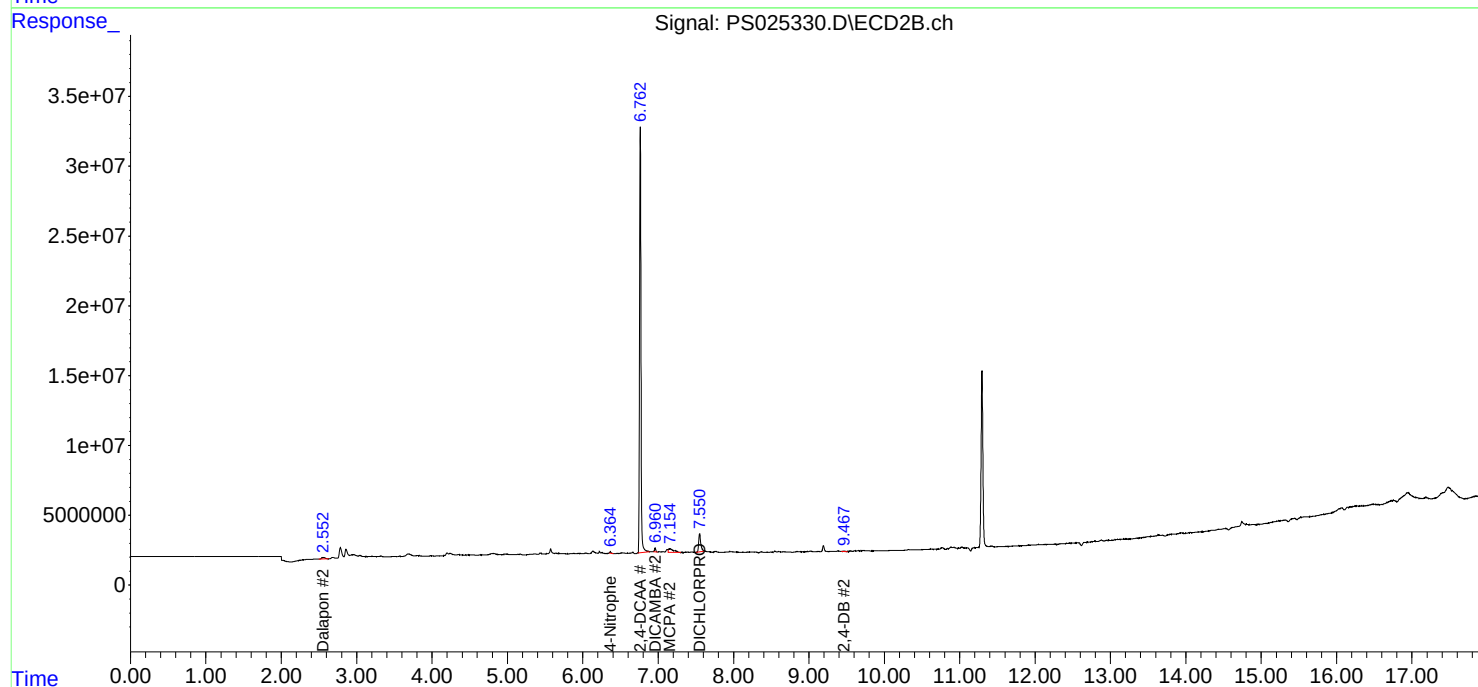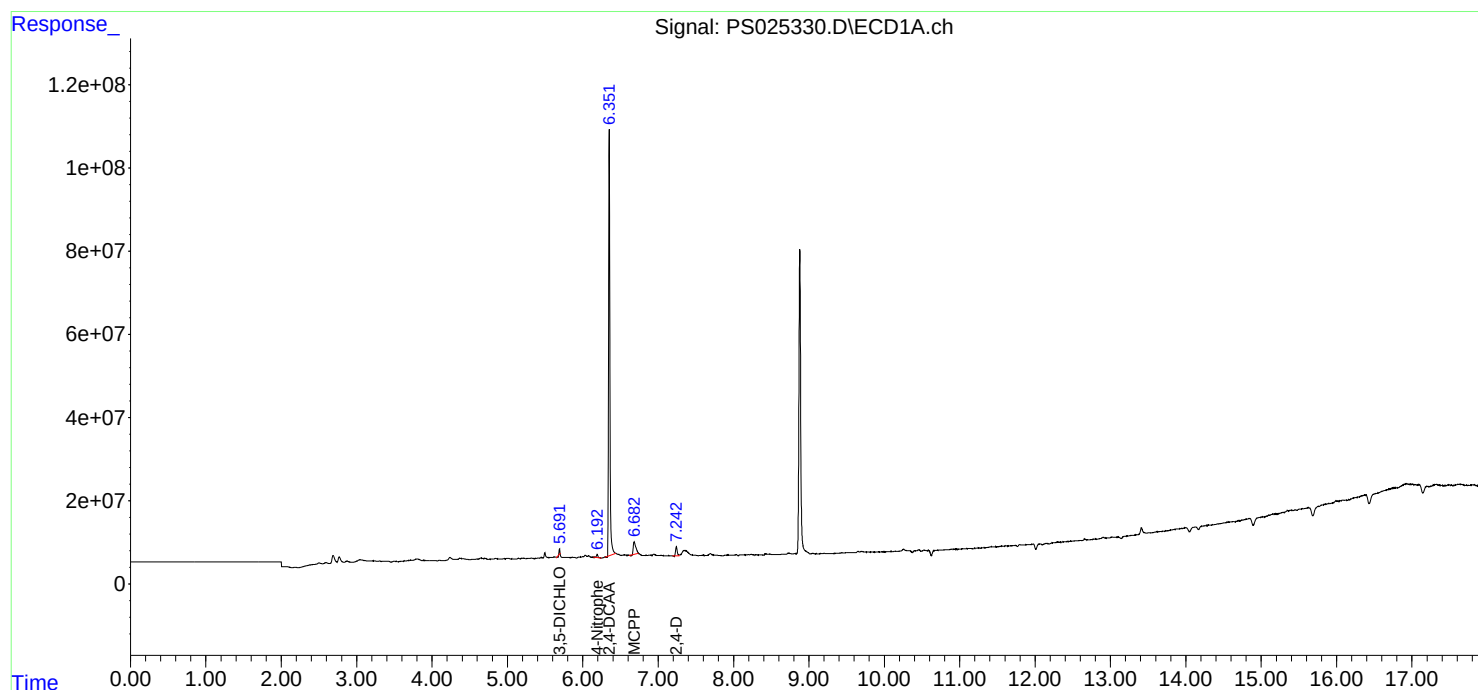


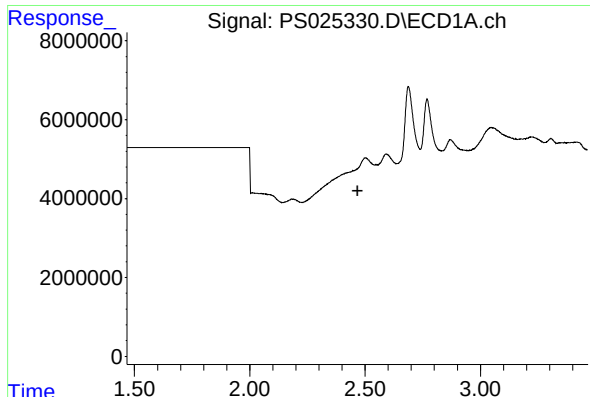

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

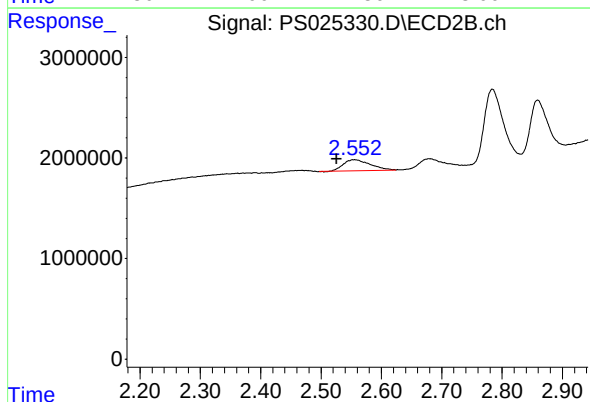


#1 Dalapon

R.T.: 2.554 min
Delta R.T.: 0.029 min
Response: 3452000
Conc: 3.00 ng/ml

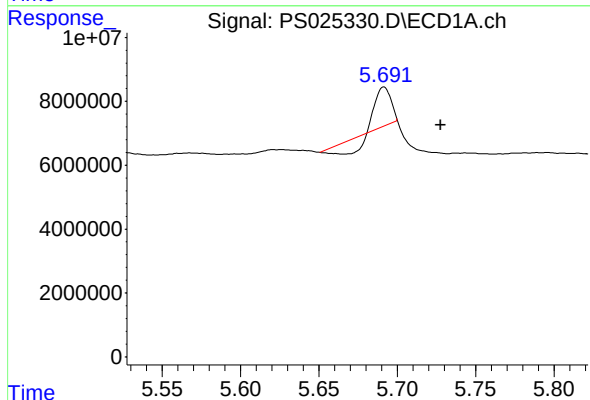


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.692 min
Delta R.T.: -0.036 min
Response: 4784858
Conc: 1.41 ng/ml

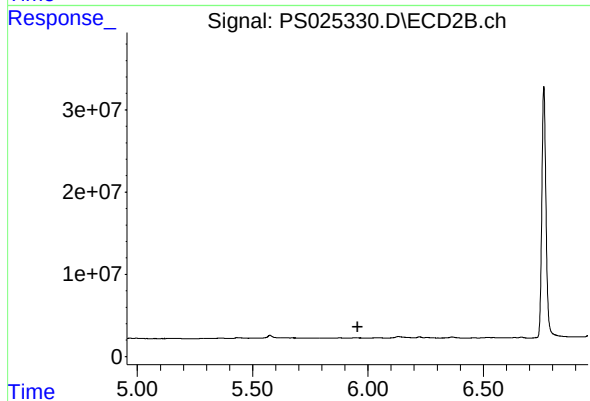

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

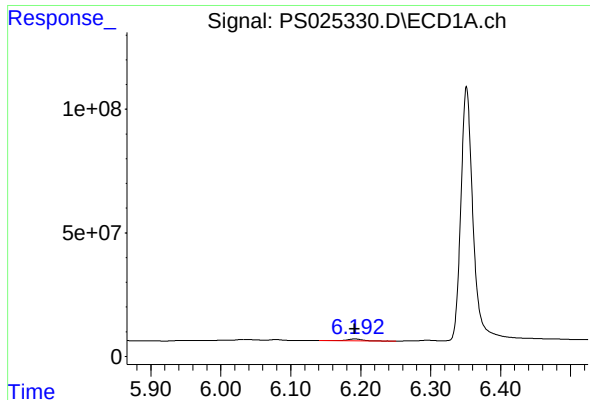

#3 4-Nitrophenol


R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 11693114
Conc: 7.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

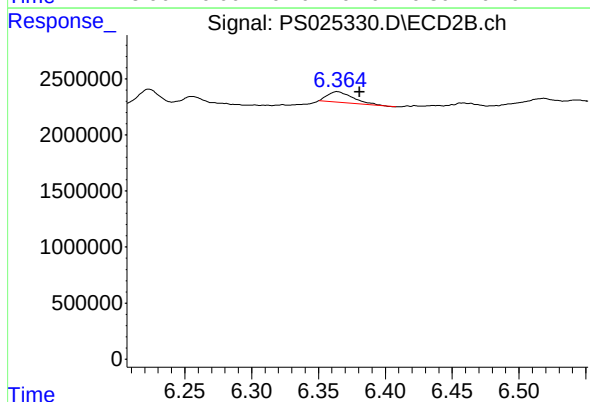


#3 4-Nitrophenol

R.T.: 6.364 min
Delta R.T.: -0.017 min
Response: 1272423
Conc: 2.56 ng/ml

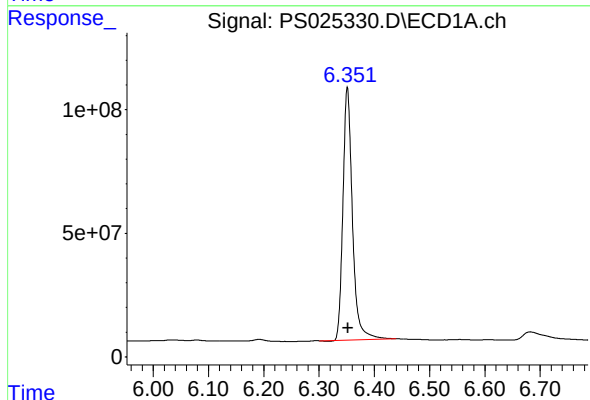


#4 2,4-DCAA

R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 1222835074
Conc: 545.71 ng/ml

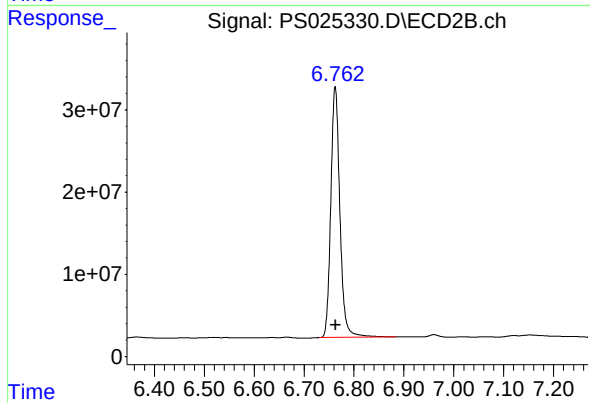

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 386301677
Conc: 544.26 ng/ml

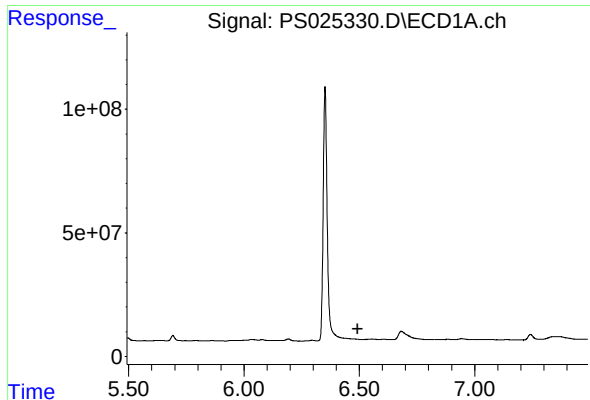

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

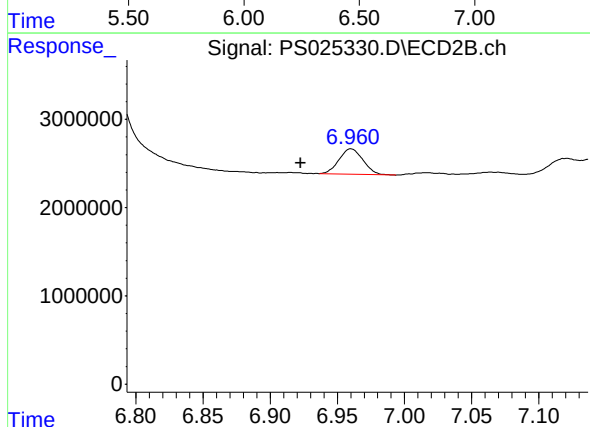


#5 DICAMBA

R.T.: 6.960 min
Delta R.T.: 0.038 min
Response: 3575550
Conc: 1.18 ng/ml

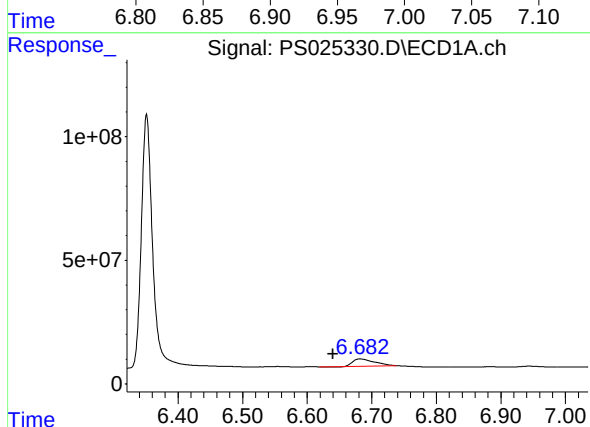


#6 MCPP

R.T.: 6.682 min
Delta R.T.: 0.042 min
Response: 67436017
Conc: 10.02 ug/ml

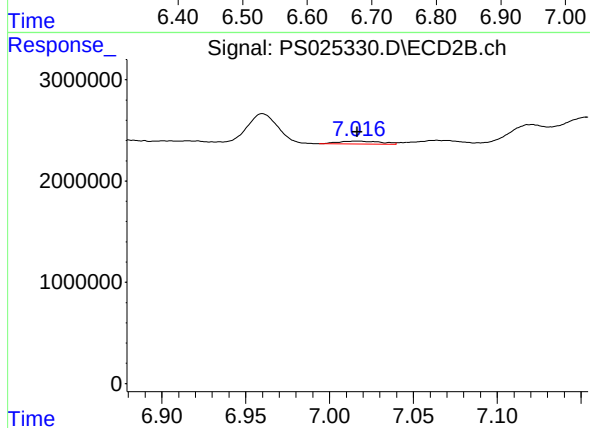

#6 MCPP


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 498124
Conc: N.D.

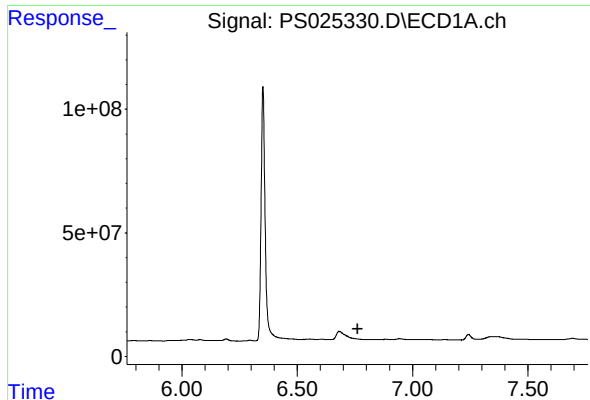

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

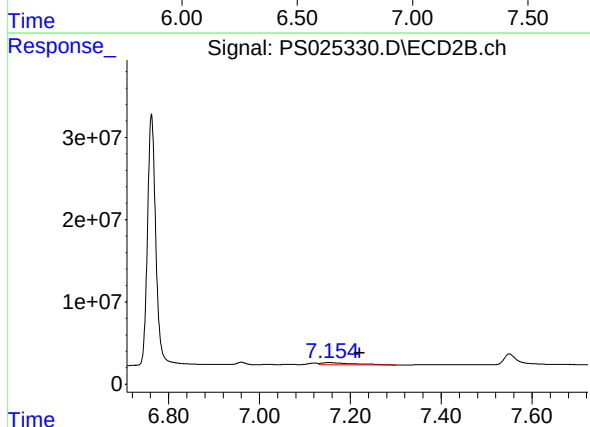


#7 MCPA

R.T.: 7.154 min
Delta R.T.: -0.067 min
Response: 12575834
Conc: 4.00 ug/ml

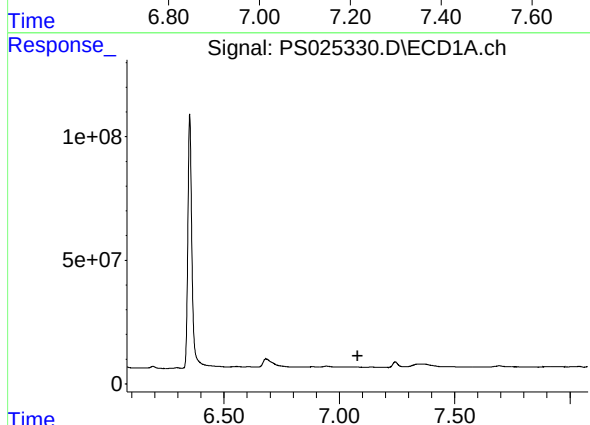


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

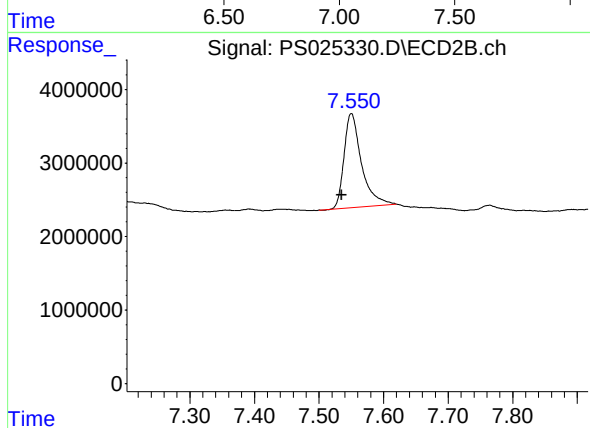

#8 DICHLORPROP


R.T.: 7.550 min
Delta R.T.: 0.015 min
Response: 24048583
Conc: 31.09 ng/ml

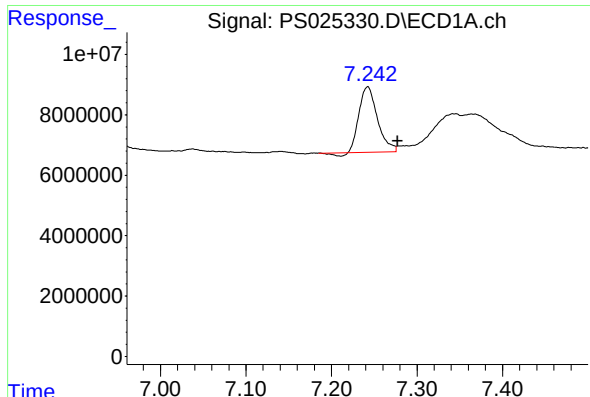

#9 2,4-D


R.T.: 7.242 min
Delta R.T.: -0.035 min
Response: 31959654
Conc: 10.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

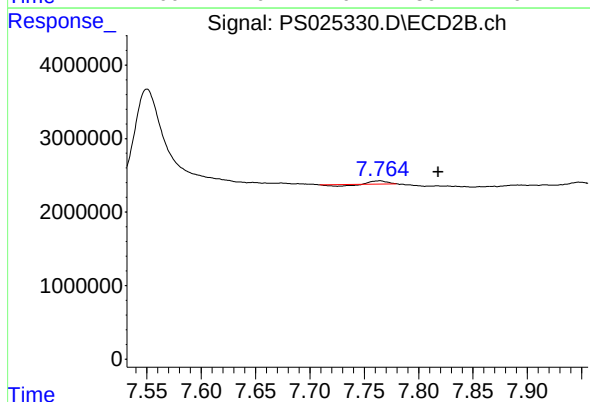


#9 2,4-D

R.T.: 7.764 min
Delta R.T.: -0.054 min
Response: 239286
Conc: N.D.

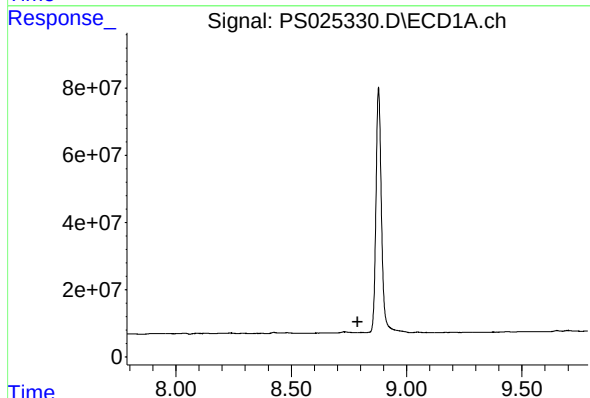

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.787 min
Response: 0
Conc: N.D.

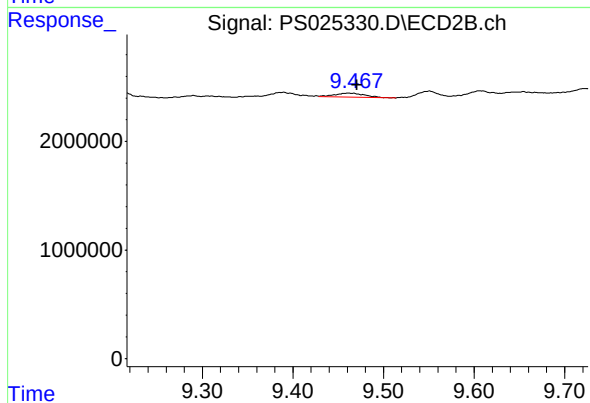

#13 2,4-DB

R.T.: 9.463 min
Delta R.T.: -0.007 min
Response: 847390
Conc: 1.54 ng/ml