

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
 Data File : PS025362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2023 19:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:20:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.351	6.762	1225.8E6	391.6E6	547.026	551.755
Target Compounds						
1) T Dalapon	0.000	2.555	0	3615230	N.D.	3.146
2) T 3,5-DICHL...	5.691	0.000	5775526	0	1.698	N.D. #
3) T 4-Nitroph...	6.191	6.365	17718624	1371367	11.438	2.761 #
5) T DICAMBA	0.000	6.960	0	4511928	N.D.	1.491
6) T MCPP	6.681f	7.025	52825086	624452	7.852	<MDL #
7) T MCPA	0.000	7.154f	0	11595422	N.D.	3.689
8) T DICHLORPROP	0.000	7.549	0	18279958	N.D.	23.632
9) T 2,4-D	7.243	7.763f	49477634	1435950	15.971	1.497 #
12) T 2,4,5-T	0.000	8.972	0	258336	N.D.	<MDL
13) T 2,4-DB	0.000	9.463	0	822815	N.D.	1.500
14) T DINOSEB	9.778f	0.000	20968762	0	1.824	N.D. #
15) T Picloram	9.651	10.764	6290181	5747767	<MDL	<MDL #
16) T DCPA	0.000	10.727	0	460076	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
Data File : PS025362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2023 19:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:20:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

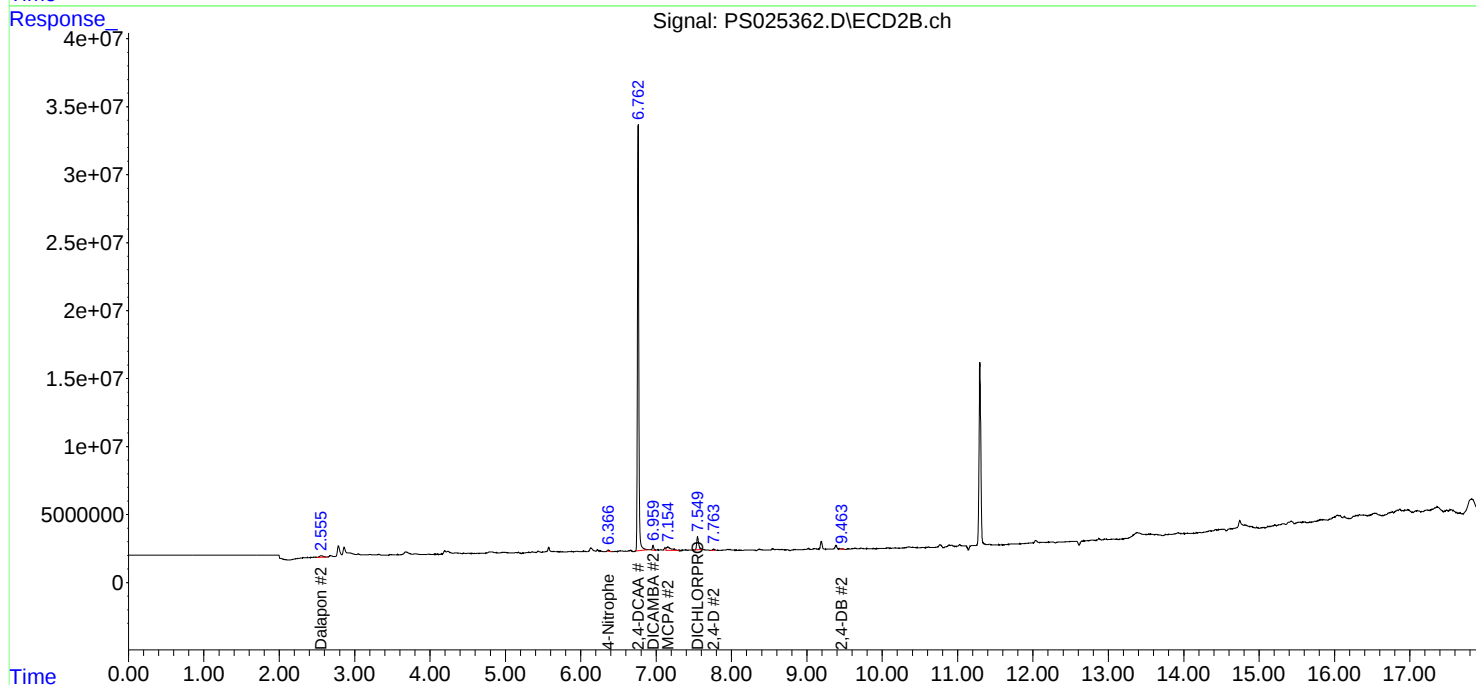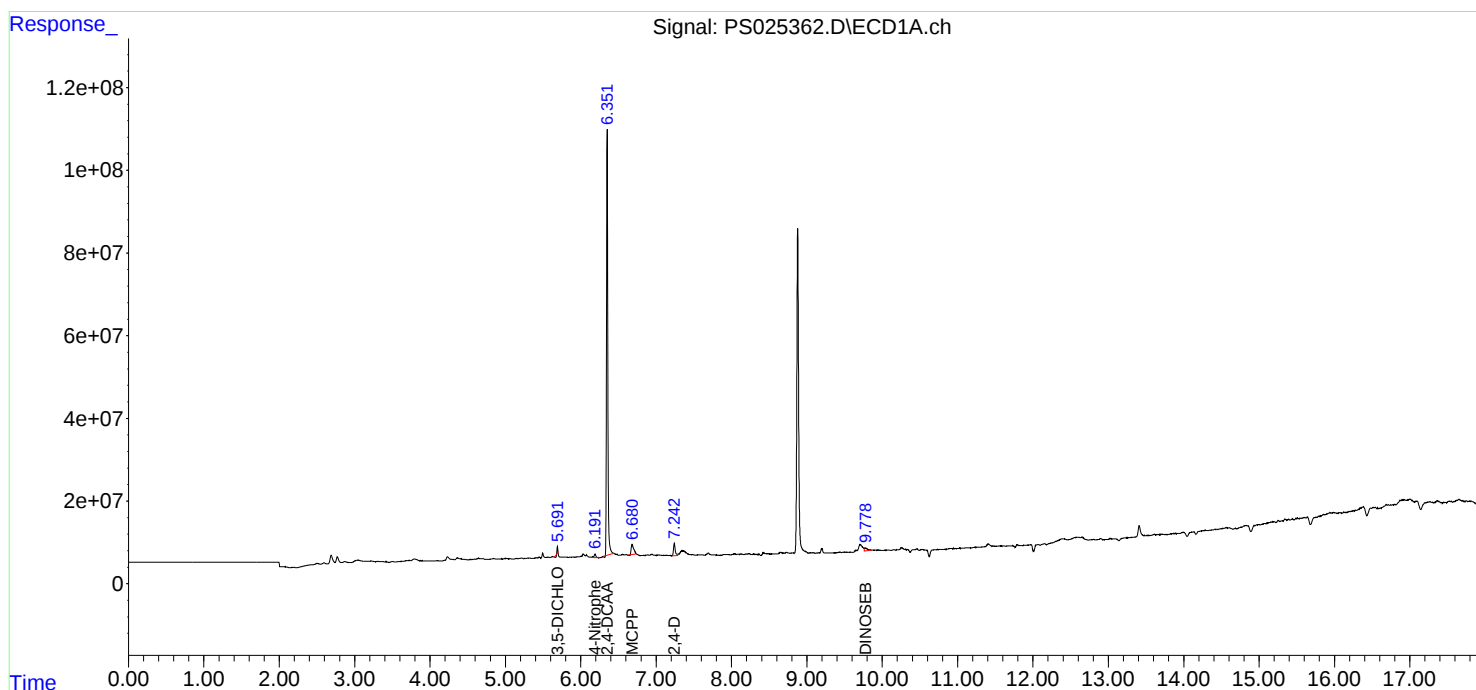


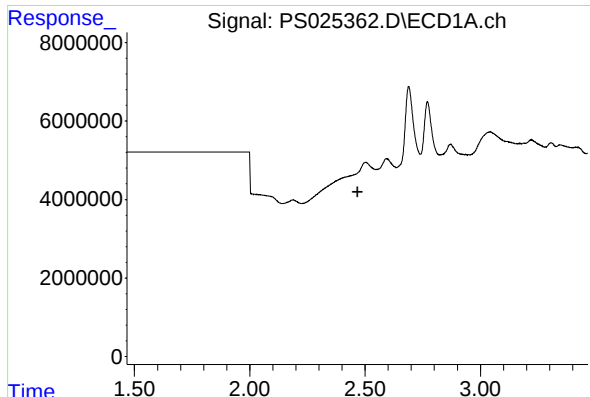

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

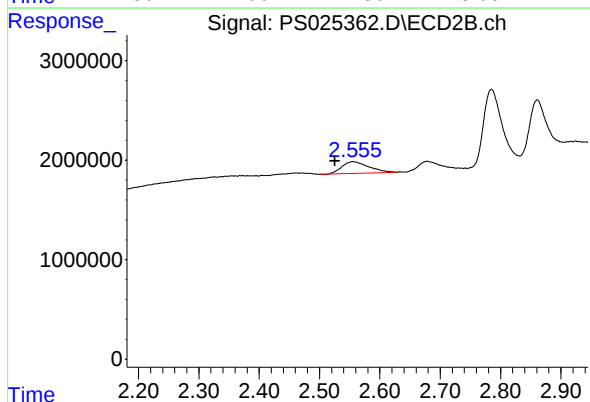


#1 Dalapon

R.T.: 2.555 min
Delta R.T.: 0.029 min
Response: 3615230
Conc: 3.15 ng/ml

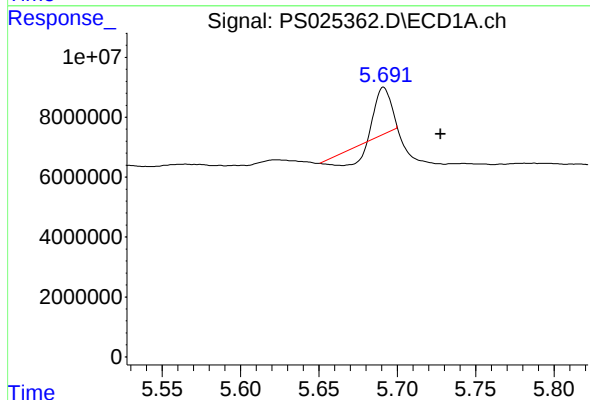


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.036 min
Response: 5775526
Conc: 1.70 ng/ml

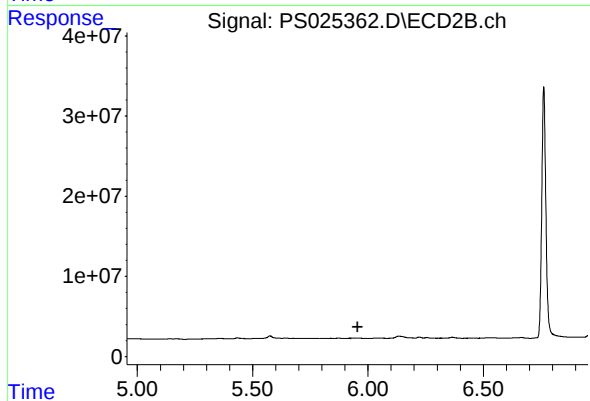

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

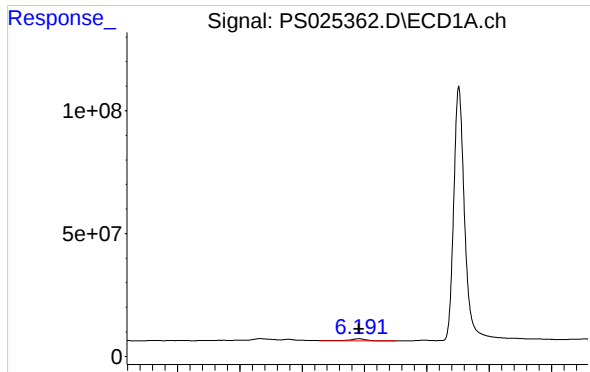

#3 4-Nitrophenol


R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 17718624
Conc: 11.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

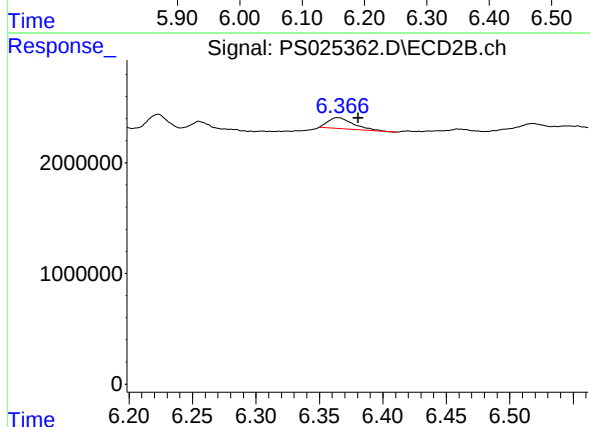


#3 4-Nitrophenol

R.T.: 6.365 min
Delta R.T.: -0.016 min
Response: 1371367
Conc: 2.76 ng/ml

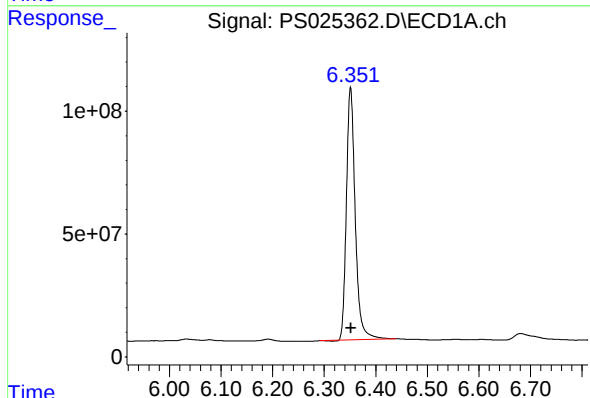


#4 2,4-DCAA

R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 1225777973
Conc: 547.03 ng/ml

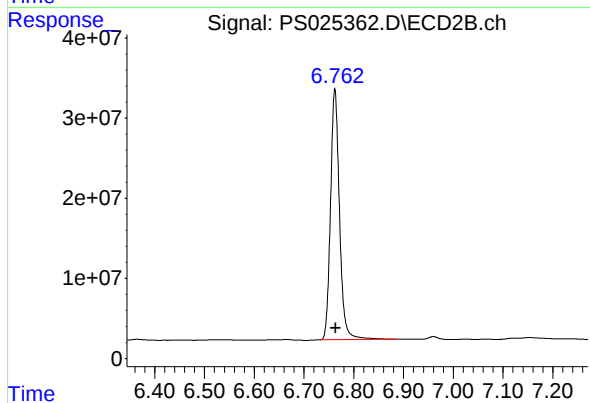

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 391621051
Conc: 551.76 ng/ml

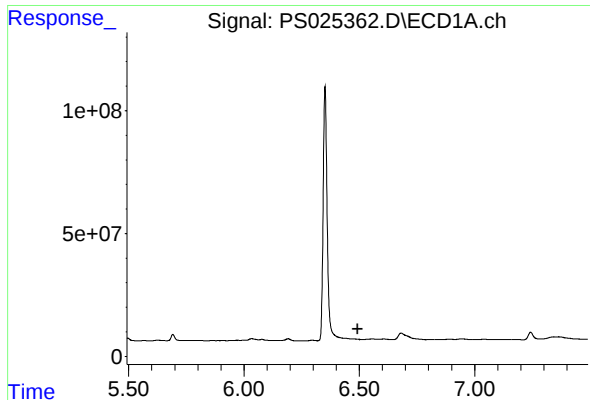

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

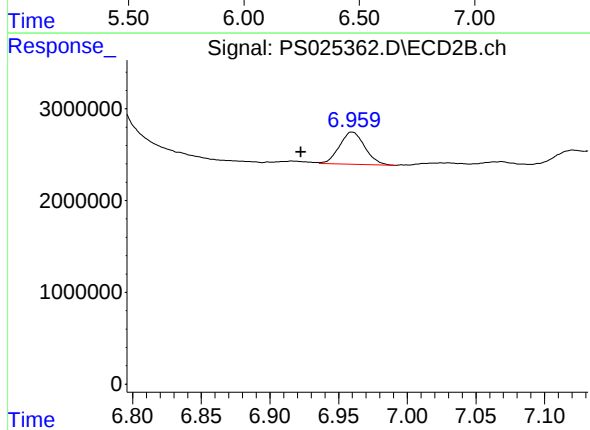


#5 DICAMBA

R.T.: 6.960 min
Delta R.T.: 0.037 min
Response: 4511928
Conc: 1.49 ng/ml

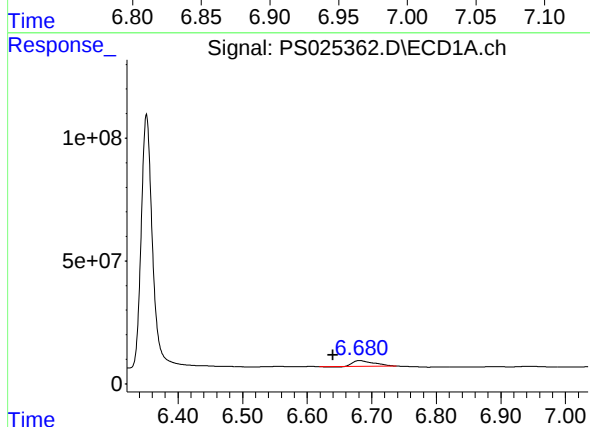


#6 MCPP

R.T.: 6.681 min
Delta R.T.: 0.041 min
Response: 52825086
Conc: 7.85 ug/ml

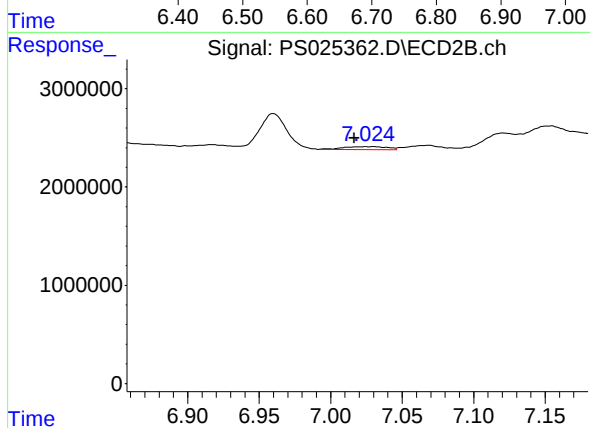

#6 MCPP


R.T.: 7.025 min
Delta R.T.: 0.009 min
Response: 624452
Conc: N.D.

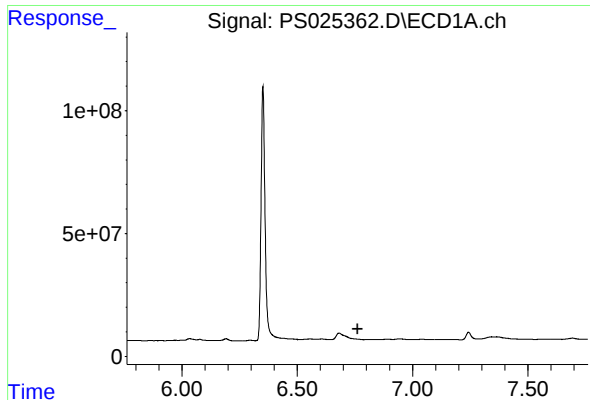

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

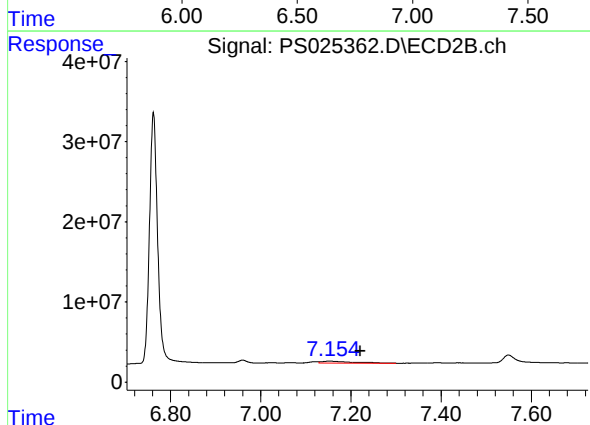


#7 MCPA

R.T.: 7.154 min
Delta R.T.: -0.067 min
Response: 11595422
Conc: 3.69 ug/ml

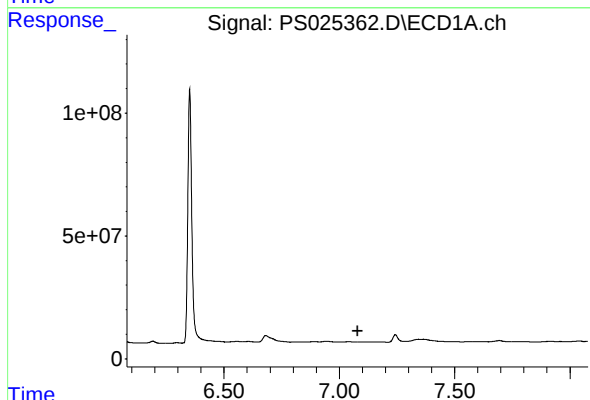


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

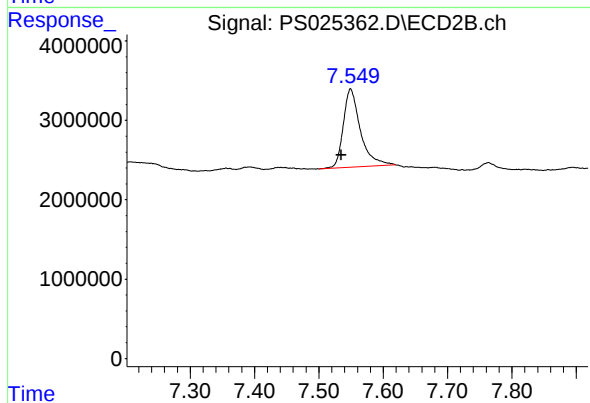

#8 DICHLORPROP


R.T.: 7.549 min
Delta R.T.: 0.014 min
Response: 18279958
Conc: 23.63 ng/ml

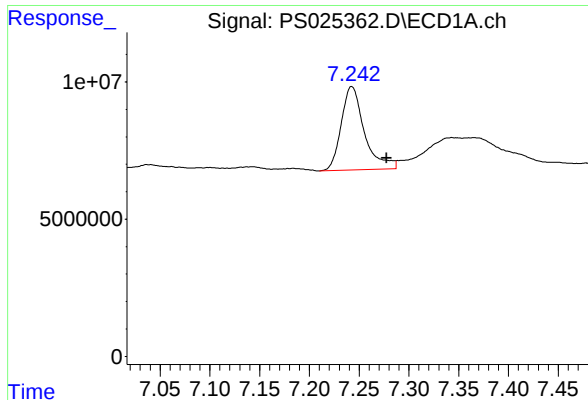

#9 2,4-D


R.T.: 7.243 min
Delta R.T.: -0.035 min
Response: 49477634
Conc: 15.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

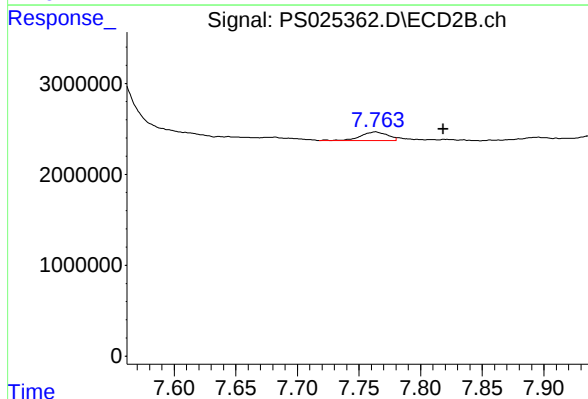


#9 2,4-D

R.T.: 7.763 min
Delta R.T.: -0.055 min
Response: 1435950
Conc: 1.50 ng/ml

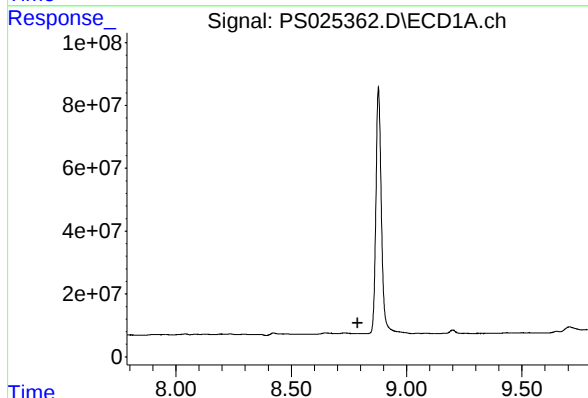


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.787 min
Response: 0
Conc: N.D.

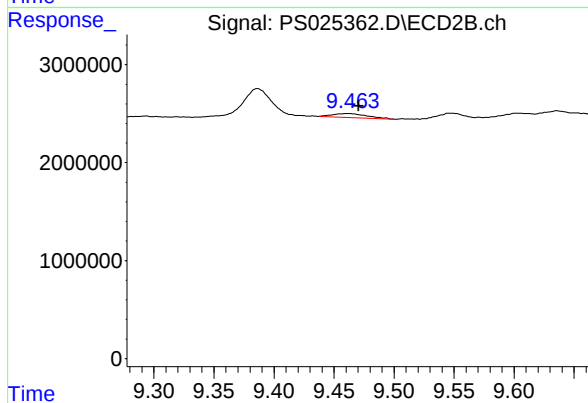

#13 2,4-DB


R.T.: 9.463 min
Delta R.T.: -0.008 min
Response: 822815
Conc: 1.50 ng/ml

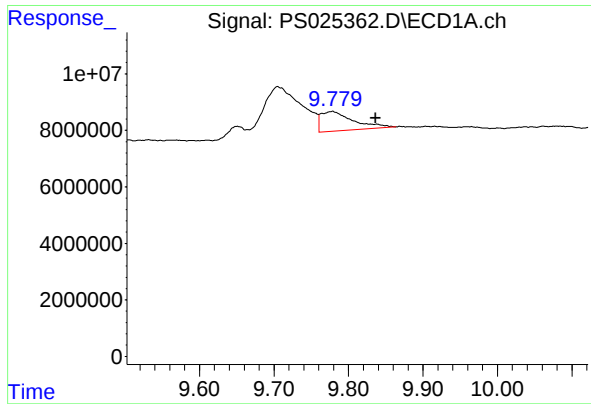

#14 DINOSEB

R.T.: 9.778 min
Delta R.T.: -0.059 min
Response: 20968762
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

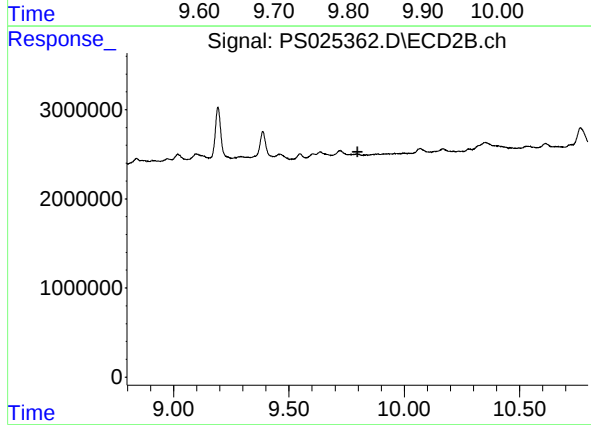

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.797 min
Response: 0
Conc: N.D.