

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
 Data File : PS025384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2023 05:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:25:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.351	6.762	1258.3E6	396.6E6	561.546	558.795
Target Compounds							
1) T	Dalapon	0.000	2.552	0	2875462	N.D.	2.502
2) T	3,5-DICHL...	5.691	0.000	11349925	0	3.337	N.D. #
3) T	4-Nitroph...	6.191	6.362	8594974	805357	5.548	1.621 #
5) T	DICAMBA	0.000	6.961	0	4945232	N.D.	1.634
6) T	MCP	6.678	7.066f	33591121	1342795	4.993	<MDL #
7) T	MCPA	0.000	7.209	0	3175663	N.D.	1.010
8) T	DICHLORPROP	0.000	7.548	0	11050431	N.D.	14.286
9) T	2,4-D	7.241	7.761f	51362362	877806	16.580	<MDL #
10) T	Pentachlo...	0.000	8.296f	0	1332908	N.D.	<MDL
12) T	2,4,5-T	0.000	8.966	0	282573	N.D.	<MDL
13) T	2,4-DB	8.729f	9.473	2555361	980513	1.060	1.787 #
14) T	DINOSEB	9.776f	9.786	70262924	727172	6.113	<MDL #
15) T	Picloram	9.701	10.760	175.4E6	14727942	8.396	2.162 #
16) T	DCPA	0.000	10.760f	0	14727942	N.D.	2.758



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
Data File : PS025384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2023 05:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:25:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

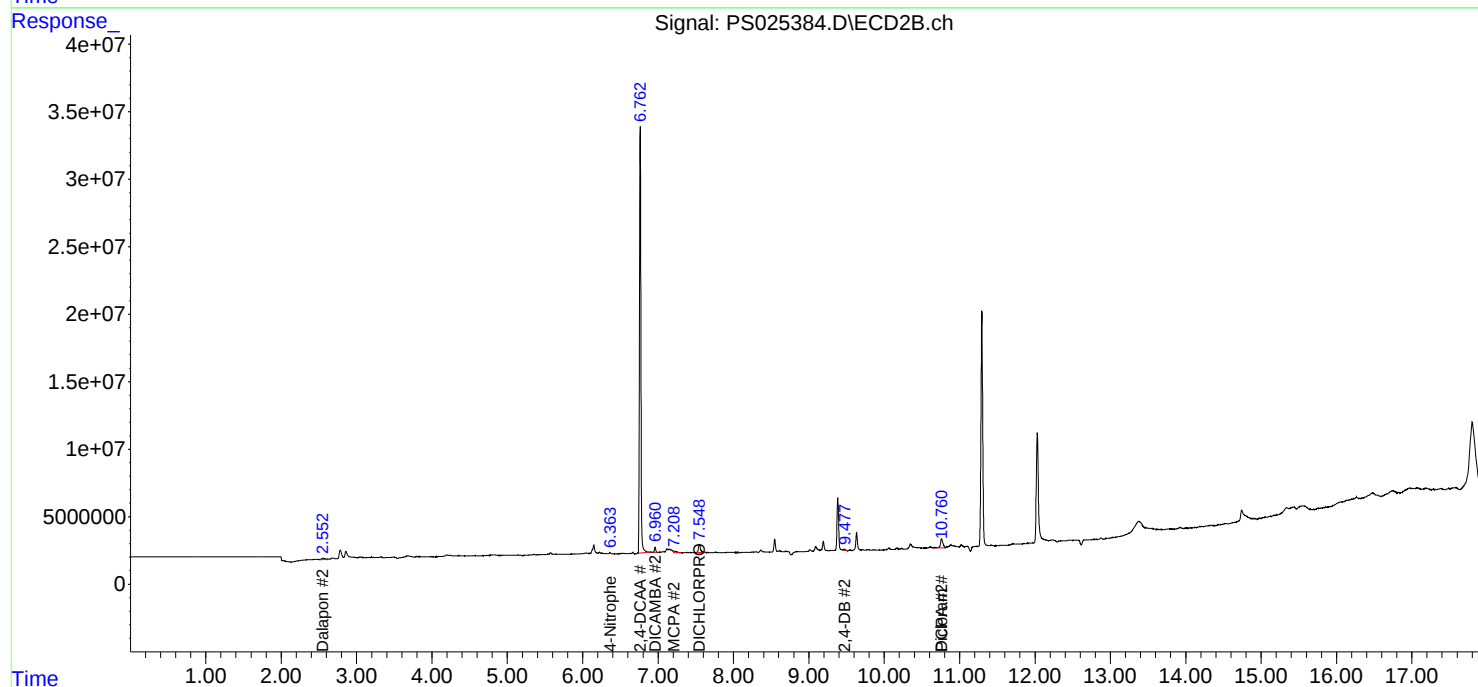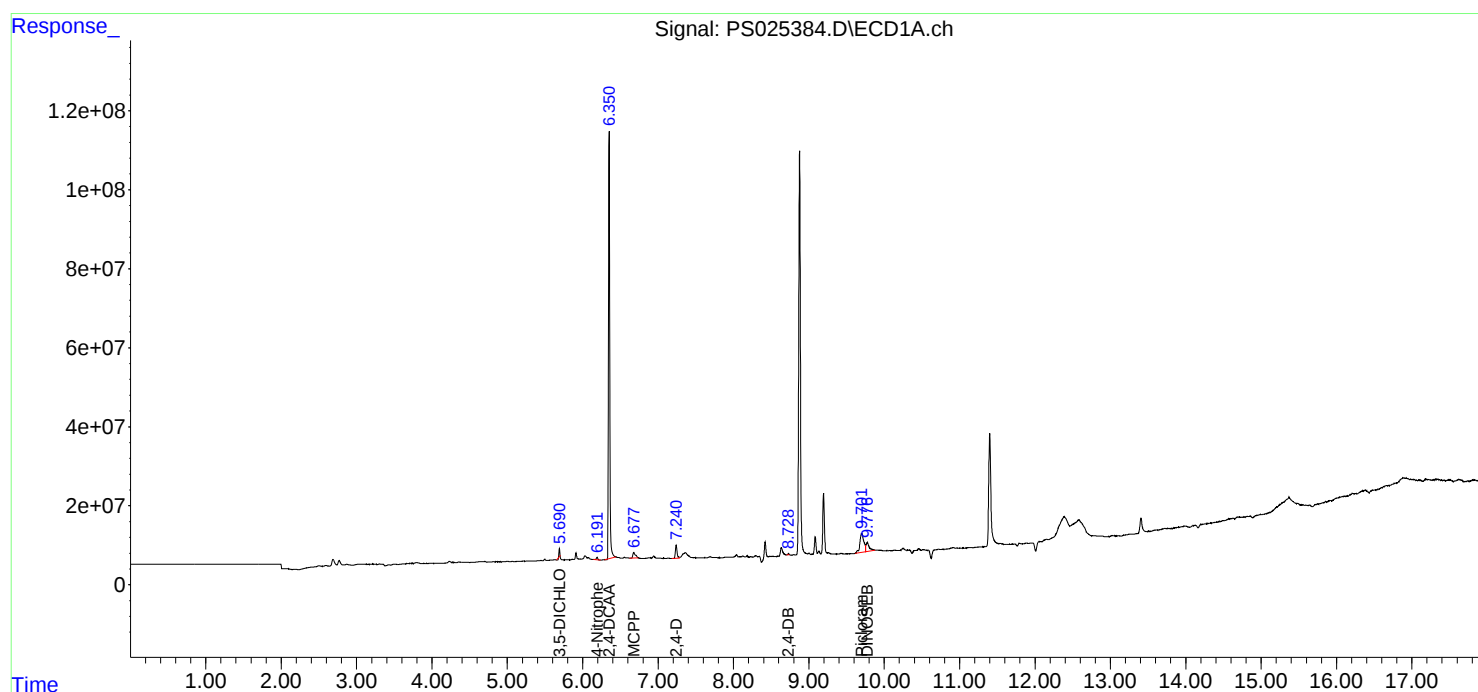


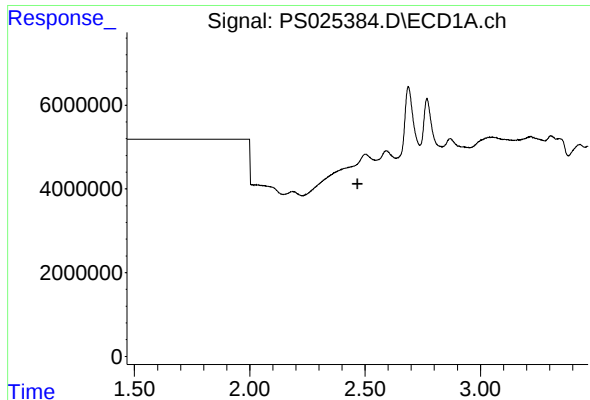

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

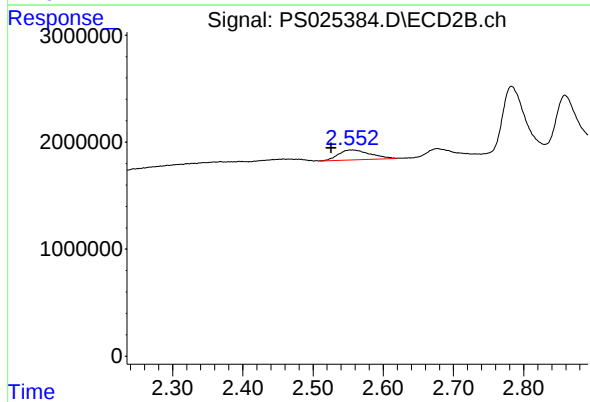


#1 Dalapon

R.T.: 2.552 min
Delta R.T.: 0.027 min
Response: 2875462
Conc: 2.50 ng/ml

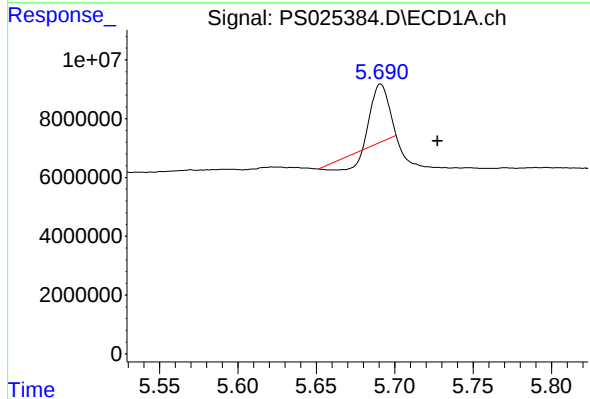


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.036 min
Response: 11349925
Conc: 3.34 ng/ml

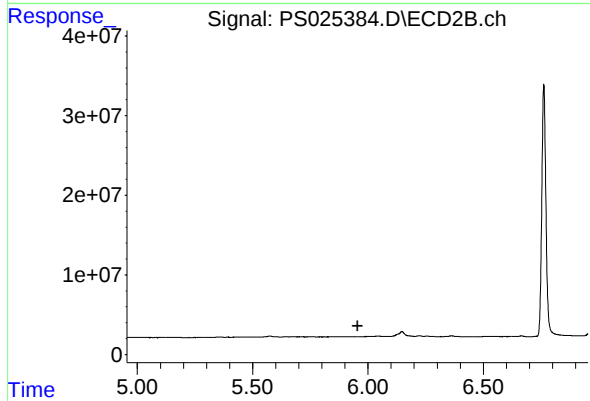

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

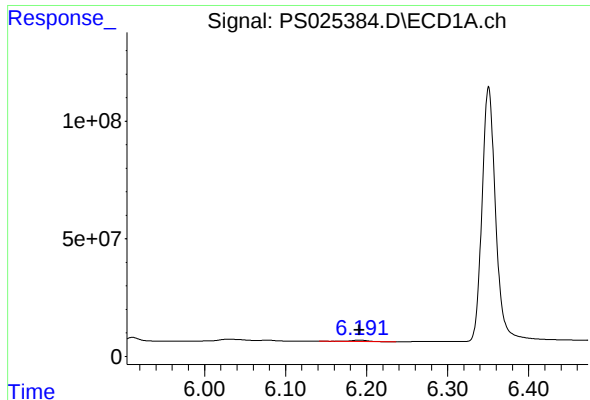

#3 4-Nitrophenol


R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 8594974
Conc: 5.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

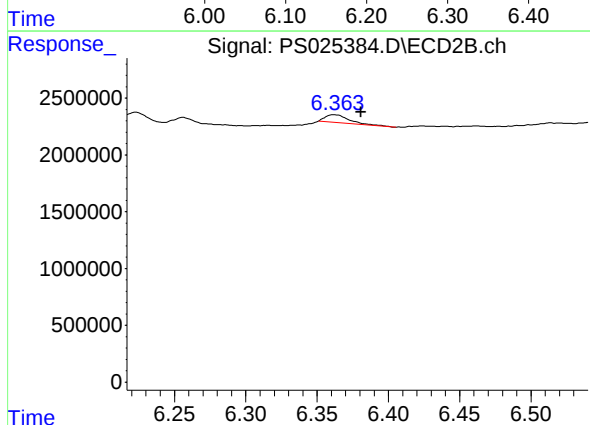


#3 4-Nitrophenol

R.T.: 6.362 min
Delta R.T.: -0.019 min
Response: 805357
Conc: 1.62 ng/ml

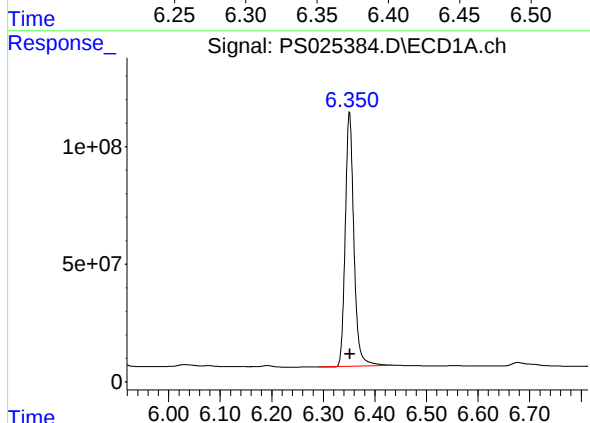


#4 2,4-DCAA

R.T.: 6.351 min
Delta R.T.: -0.001 min
Response: 1258313844
Conc: 561.55 ng/ml

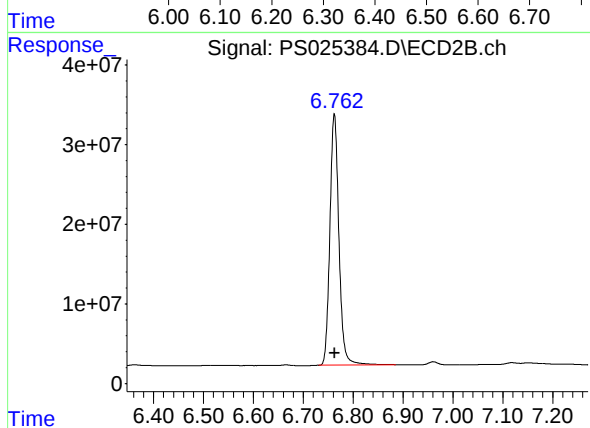

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 396617886
Conc: 558.80 ng/ml

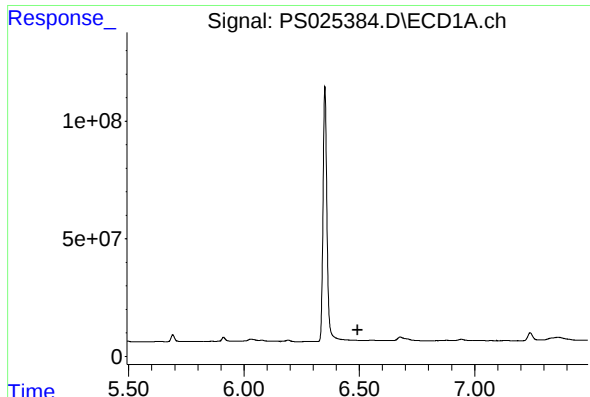

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

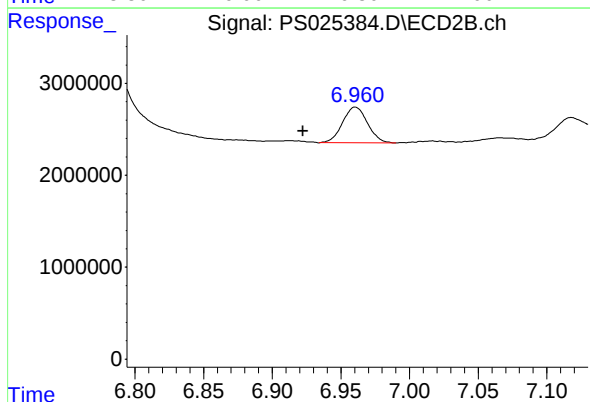


#5 DICAMBA

R.T.: 6.961 min
Delta R.T.: 0.038 min
Response: 4945232
Conc: 1.63 ng/ml

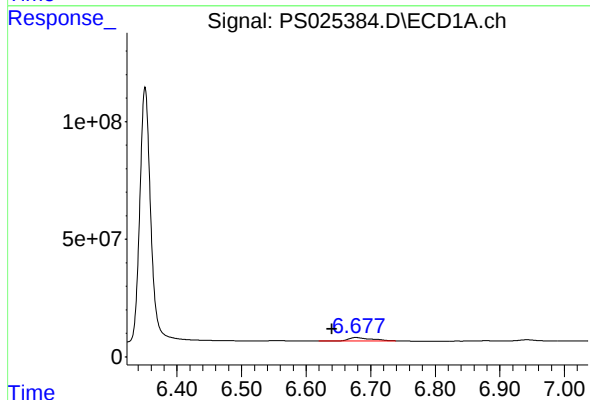


#6 MCPP

R.T.: 6.678 min
Delta R.T.: 0.038 min
Response: 33591121
Conc: 4.99 ug/ml

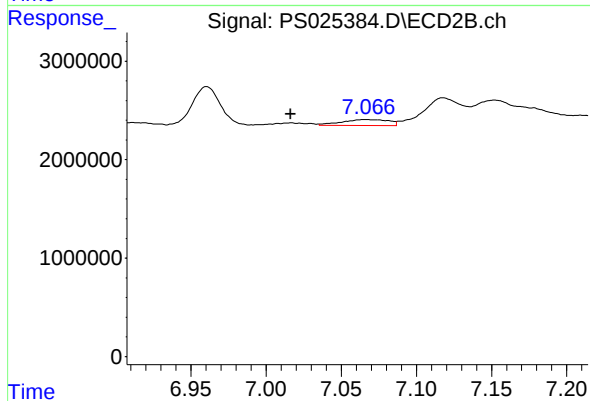

#6 MCPP


R.T.: 7.066 min
Delta R.T.: 0.050 min
Response: 1342795
Conc: N.D.

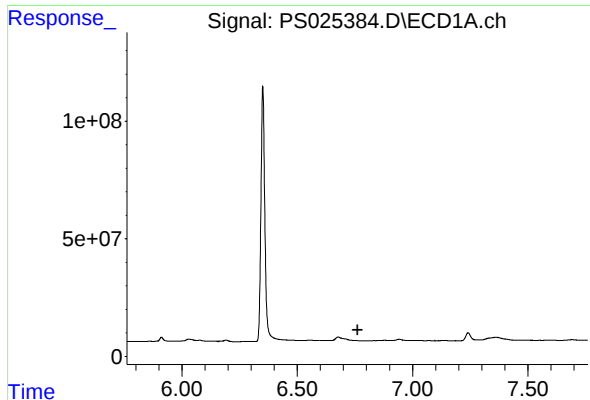

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

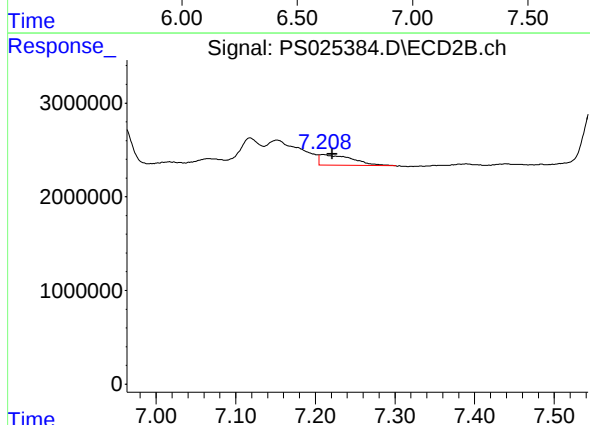


#7 MCPA

R.T.: 7.209 min
Delta R.T.: -0.012 min
Response: 3175663
Conc: 1.01 ug/ml

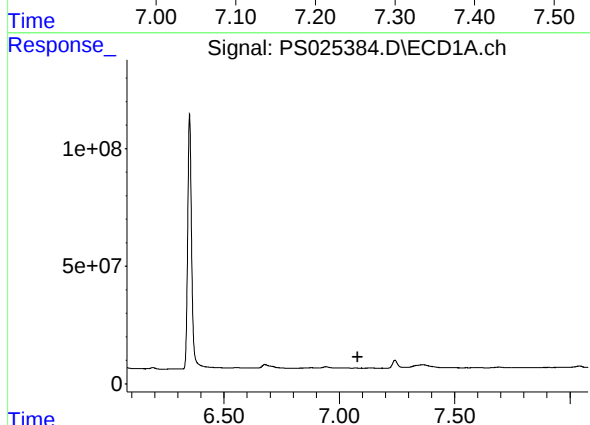


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

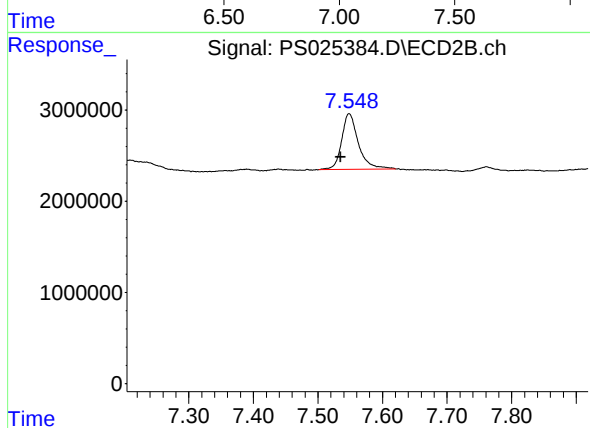

#8 DICHLORPROP


R.T.: 7.548 min
Delta R.T.: 0.013 min
Response: 11050431
Conc: 14.29 ng/ml

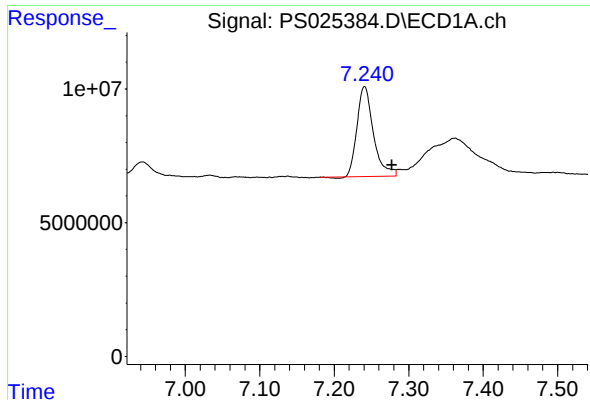

#9 2,4-D


R.T.: 7.241 min
Delta R.T.: -0.037 min
Response: 51362362
Conc: 16.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

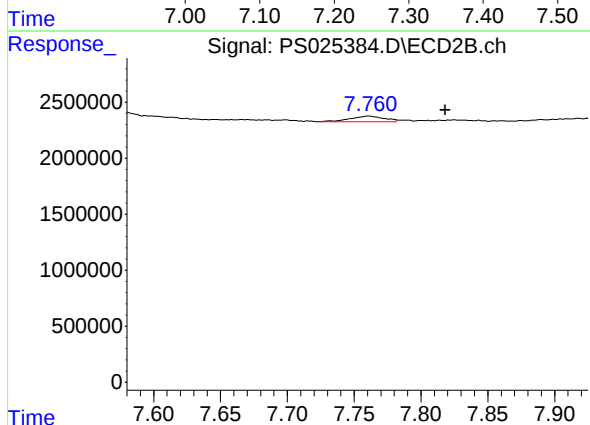


#9 2,4-D

R.T.: 7.761 min
Delta R.T.: -0.057 min
Response: 877806
Conc: N.D.

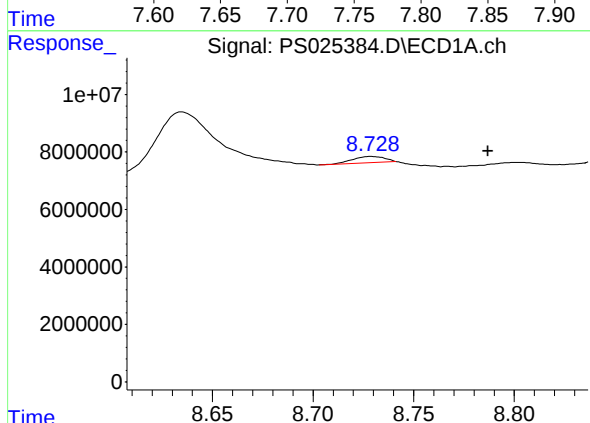


#13 2,4-DB

R.T.: 8.729 min
Delta R.T.: -0.058 min
Response: 2555361
Conc: 1.06 ng/ml

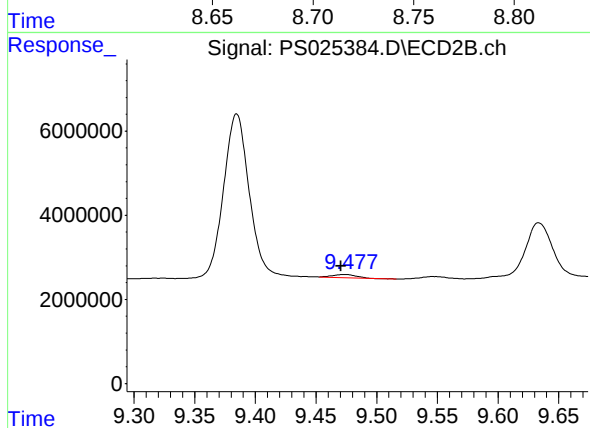

#13 2,4-DB


R.T.: 9.473 min
Delta R.T.: 0.003 min
Response: 980513
Conc: 1.79 ng/ml

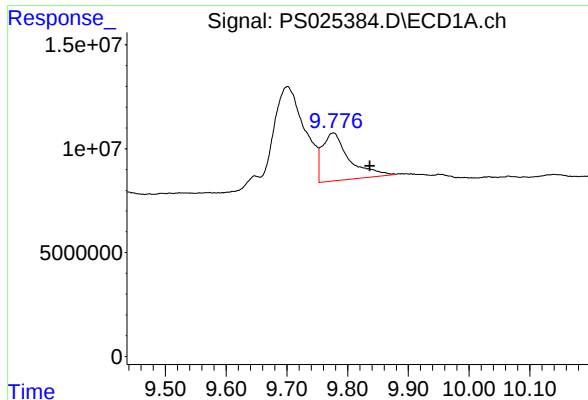

#14 DINOSEB


R.T.: 9.776 min
Delta R.T.: -0.060 min
Response: 70262924
Conc: 6.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

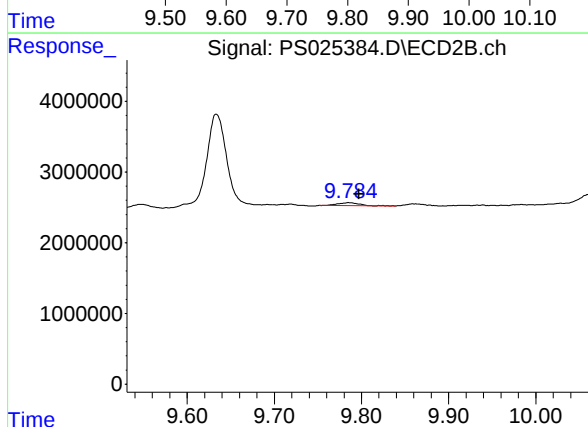


#14 DINOSEB

R.T.: 9.786 min
Delta R.T.: -0.011 min
Response: 727172
Conc: N.D.

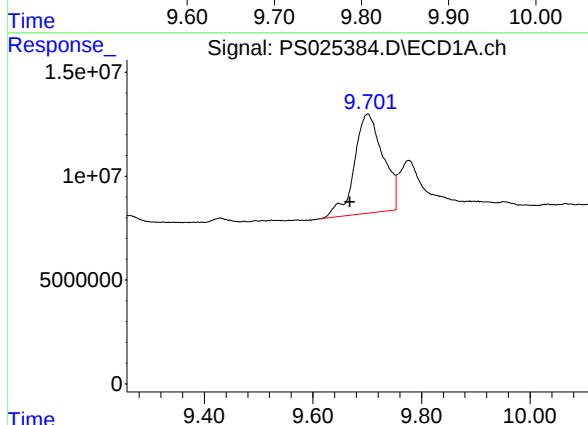


#15 Picloram

R.T.: 9.701 min
Delta R.T.: 0.032 min
Response: 175416352
Conc: 8.40 ng/ml

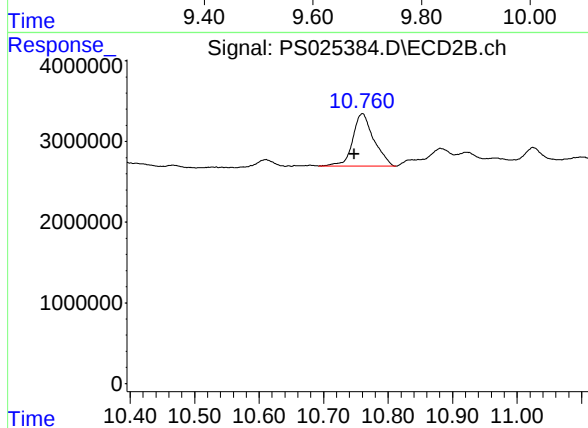

#15 Picloram


R.T.: 10.760 min
Delta R.T.: 0.012 min
Response: 14727942
Conc: 2.16 ng/ml

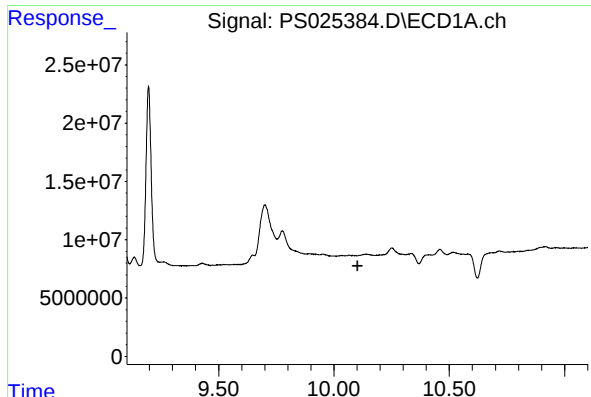

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

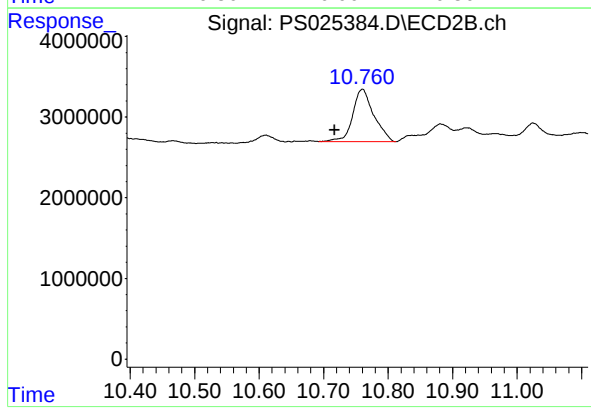

#16 DCPA

R.T.: 10.760 min
Delta R.T.: 0.043 min
Response: 14727942
Conc: 2.76 ng/ml