

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
 Data File : PS025346.D
 Signal(s) : ECD2B.ch
 Acq On : 30 Dec 23 12:33 pm
 Operator : AR\AJ
 Sample : 06015-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 O6016-06

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/02/2024
 Supervised By : Ankita Jodhani 01/02/2024

Integration File: autoint1.e
 Quant Time: Jan 01 00:16:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.349	6.761	1085.5E6	342.0E6	484.404m	481.849m
Target Compounds						
13) T 2,4-DB	8.800	9.475	4049.3E6	1343.3E6	1679.273m	2448.807m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
Data File : PS025346.D
Signal(s) : ECD2B.ch
Acq On : 30 Dec 23 12:33 pm
Operator : AR\AJ
Sample : 06015-06
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
ECD_S
ClientSampleId :
O6016-06


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/02/2024
Supervised By : Ankita Jodhani 01/02/2024

Integration File: autoint1.e
Quant Time: Jan 01 00:16:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

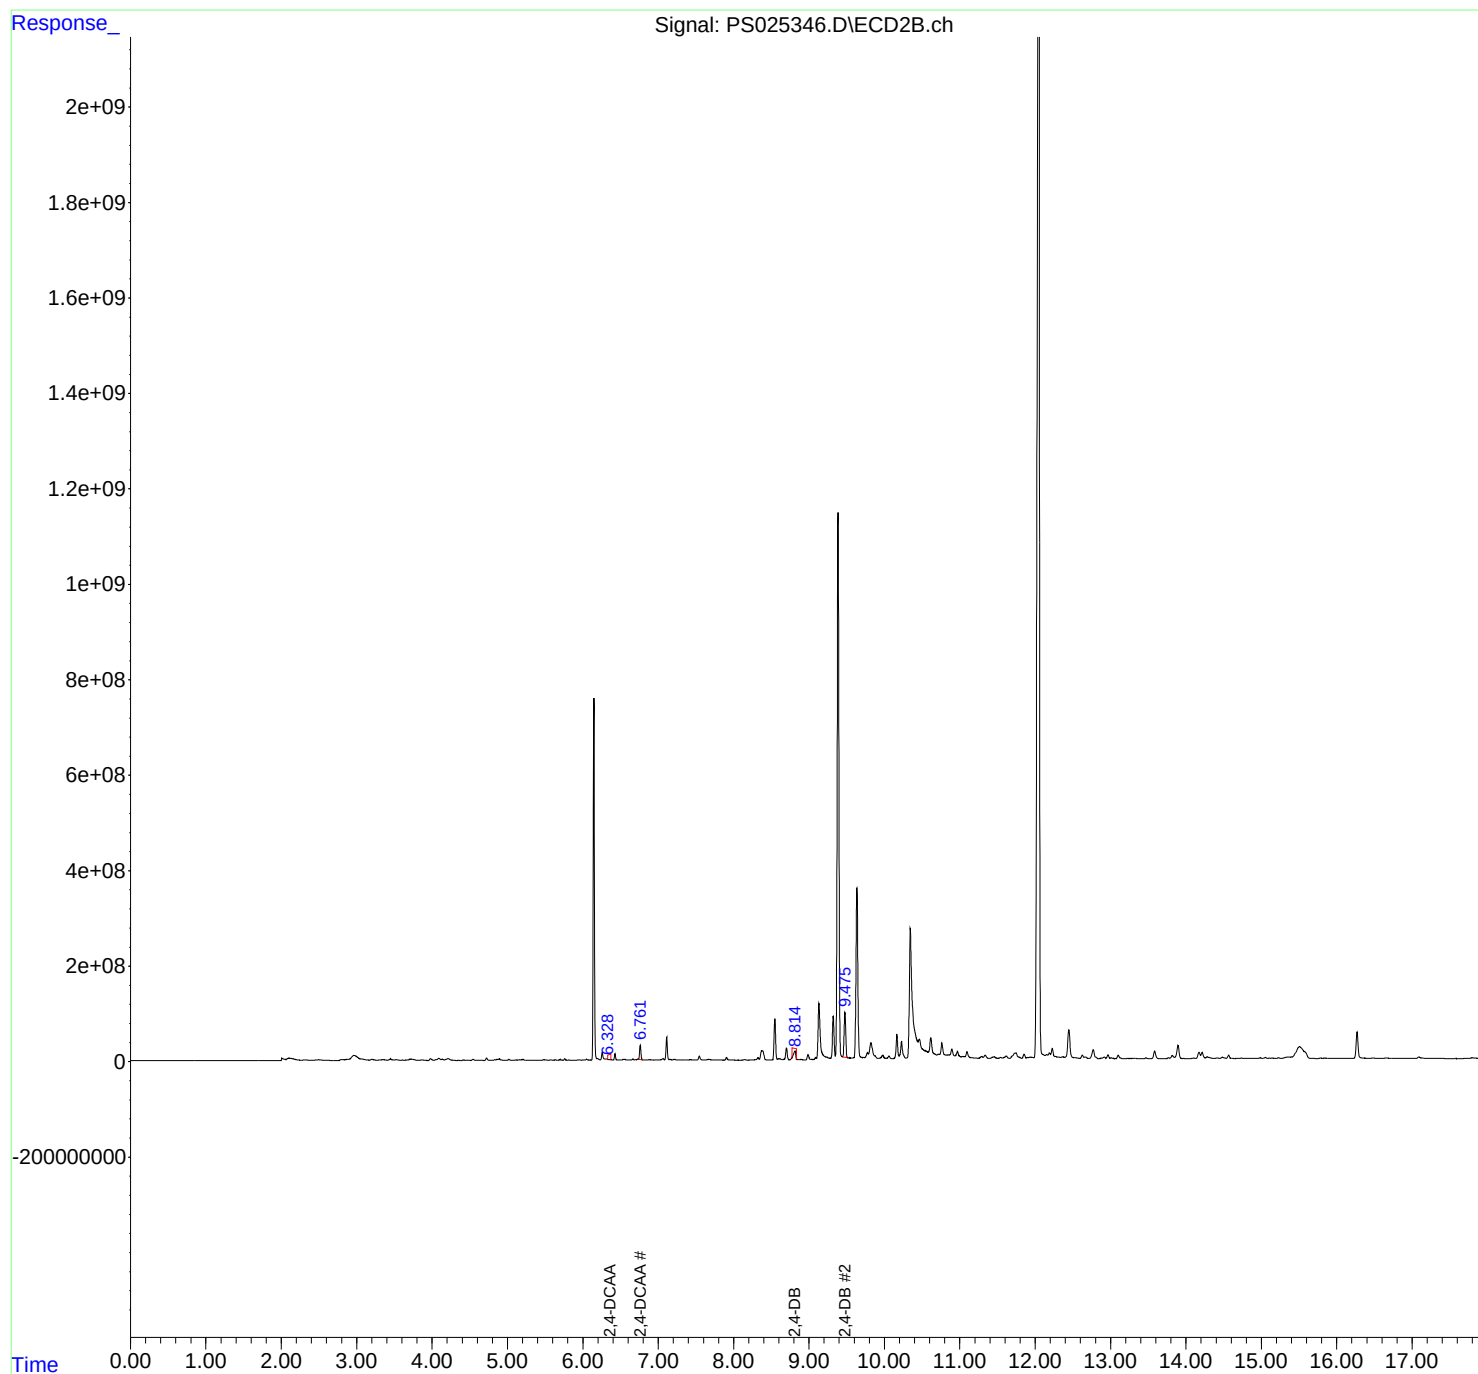

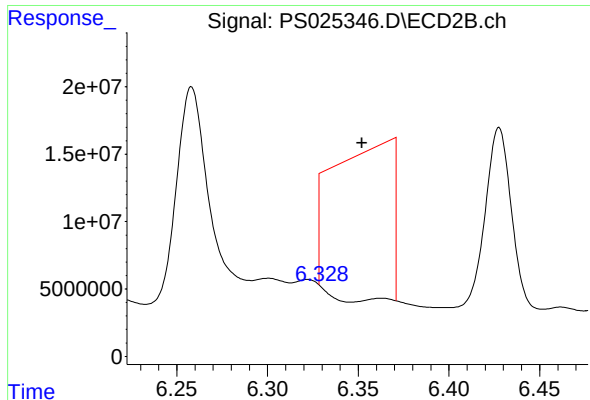


#4 2,4-DCAA

R.T.: 6.349 min
Delta R.T.: -0.003 min
Response: 1085454484
Conc: 484.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
O6016-06


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/02/2024
Supervised By :Ankita Jodhani 01/02/2024

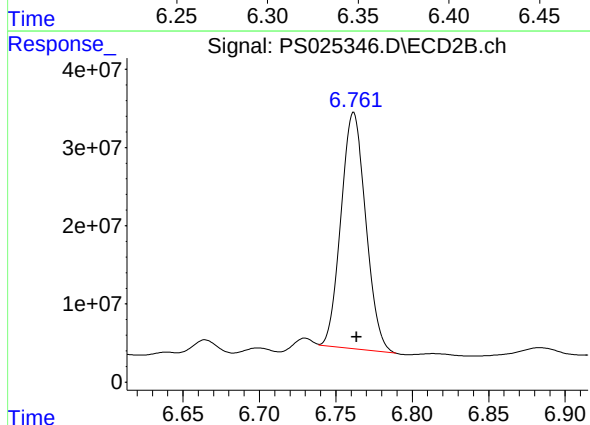


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: -0.002 min
Response: 342003931
Conc: 481.85 ng/ml

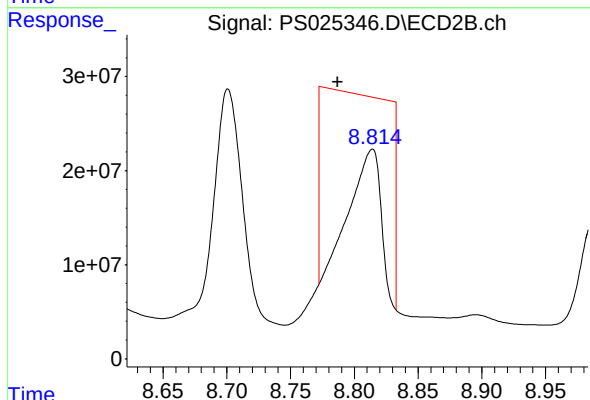

#13 2,4-DB

R.T.: 8.800 min
Delta R.T.: 0.013 min
Response: 4049315951
Conc: 1679.27 ng/ml

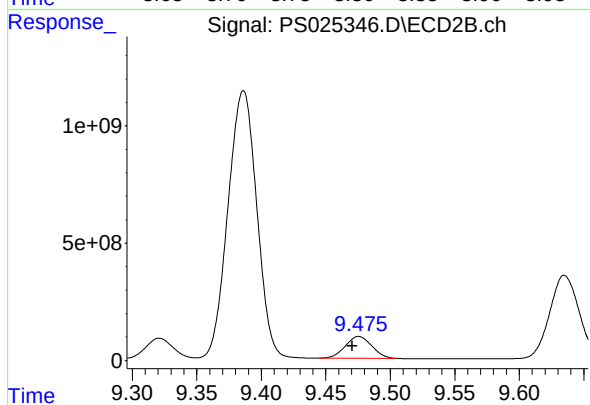

#13 2,4-DB

R.T.: 9.475 min
Delta R.T.: 0.004 min
Response: 1343325281
Conc: 2448.81 ng/ml