

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
 Data File : PS025365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2023 20:59
 Operator : AR\AJ
 Sample : 05907-04
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 GHL-SS-14-2-4

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/02/2024
 Supervised By :Ankita Jodhani 01/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 00:21:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

	System Monitoring Compounds						
4) S	2,4-DCAA	6.350	6.761	770.3E6	162.8E6	343.743	229.384 #
	Target Compounds						
13) T	2,4-DB	8.799	9.475	3217.8E6	1625.0E6	1334.441m	2962.372m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122923\
Data File : PS025365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2023 20:59
Operator : AR\AJ
Sample : 05907-04
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
GHL-SS-14-2-4


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/02/2024
Supervised By : Ankita Jodhani 01/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 00:21:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

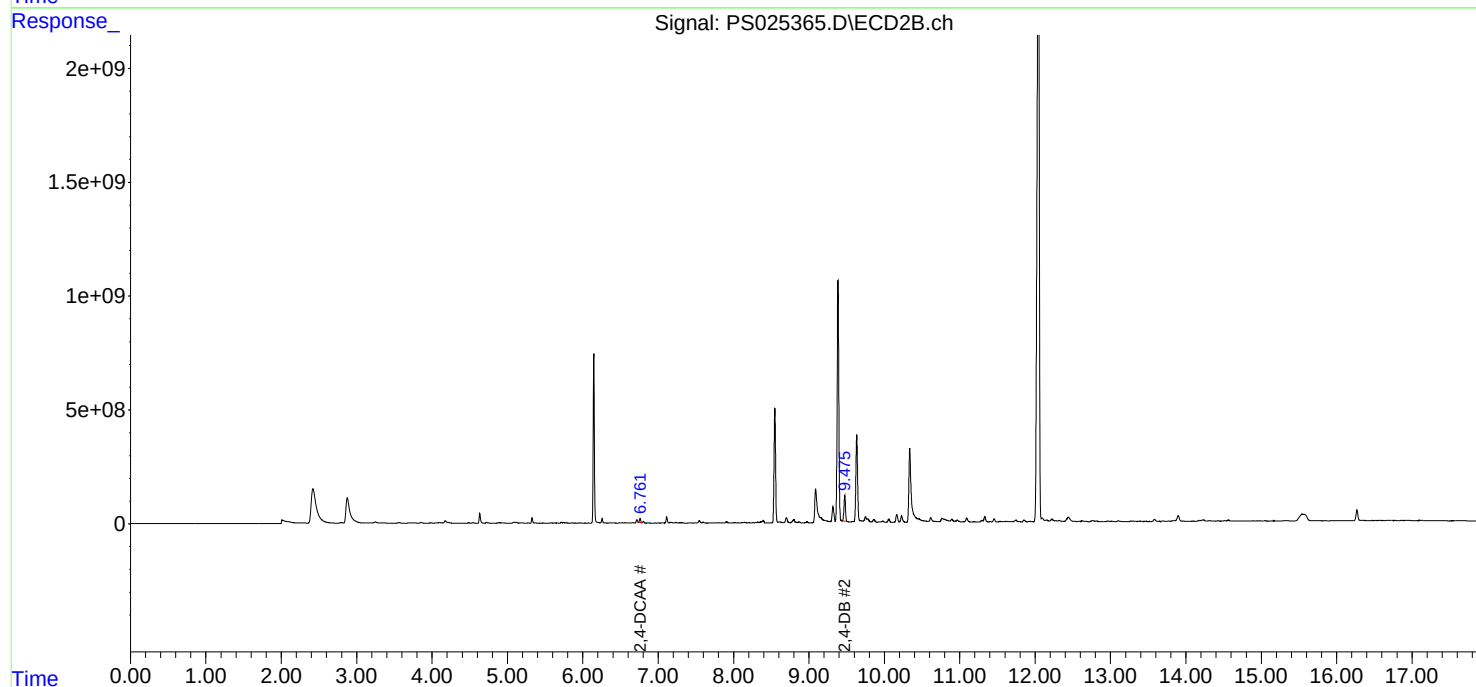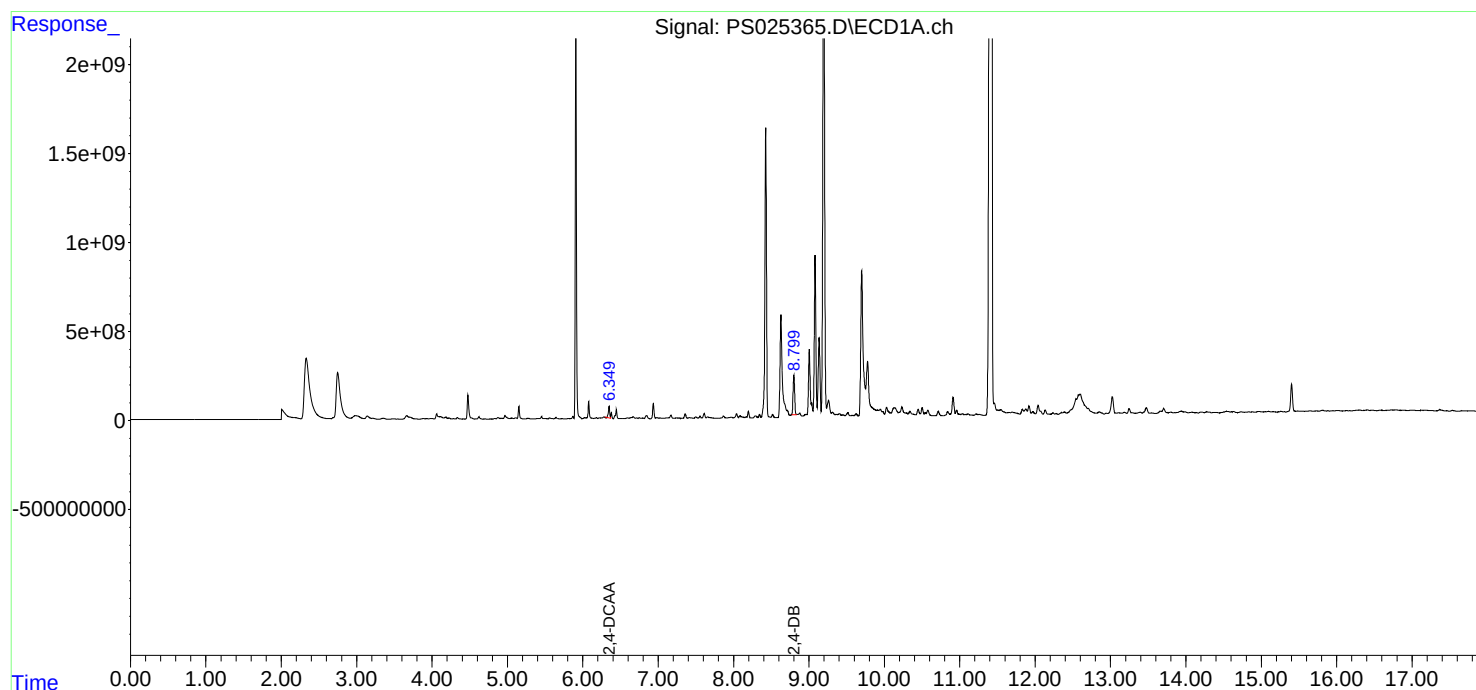

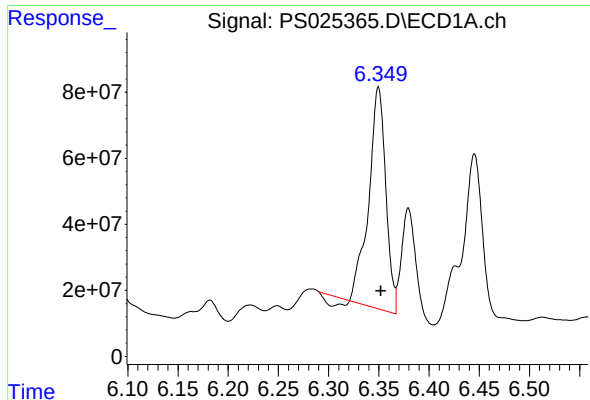


#4 2,4-DCAA

R.T.: 6.350 min
Delta R.T.: -0.002 min
Response: 770259861
Conc: 343.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
GHL-SS-14-2-4


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/02/2024
Supervised By :Ankita Jodhani 01/02/2024

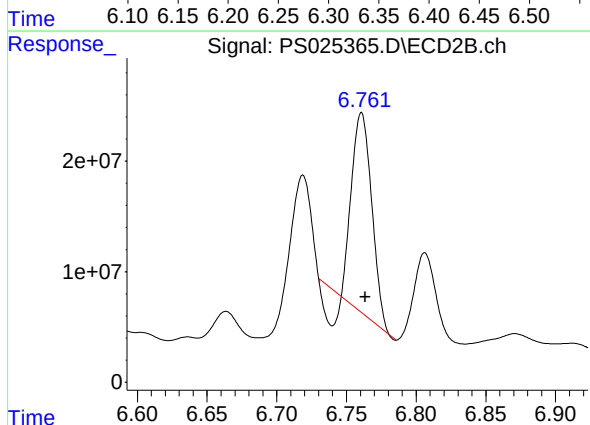


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: -0.003 min
Response: 162810917
Conc: 229.38 ng/ml

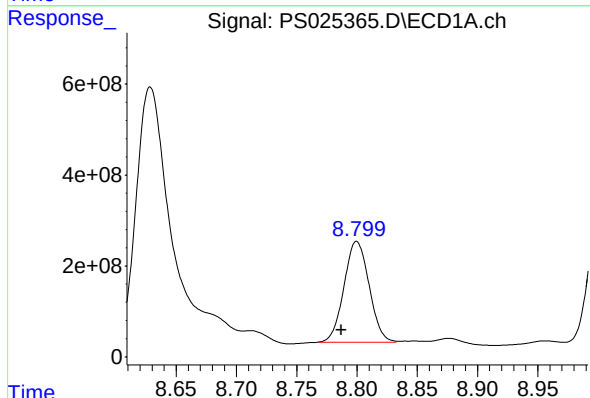

#13 2,4-DB

R.T.: 8.799 min
Delta R.T.: 0.012 min
Response: 3217805511
Conc: 1334.44 ng/ml m

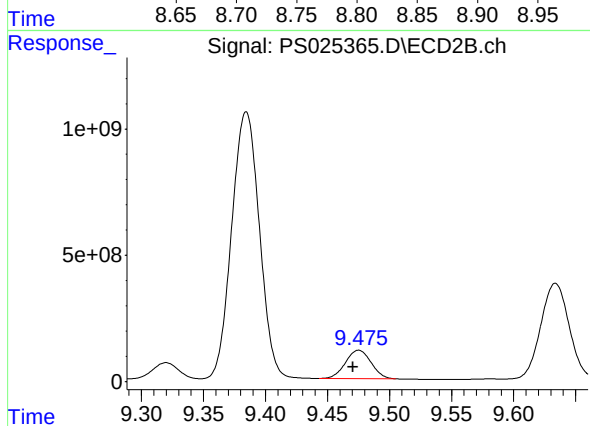

#13 2,4-DB

R.T.: 9.475 min
Delta R.T.: 0.004 min
Response: 1625048401
Conc: 2962.37 ng/ml m