

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123019\
 Data File : PS008245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2019 08:44
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 13:44:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.361	5.108	892.4E6	419.3E6	441.708	468.250
Target Compounds							
9) T	2,4-D	6.398	0.000	61088807	0	37.226	N.D. #
12) T	2,4,5-T	7.342	7.149	36863039	46382453	3.068	11.097 #
15) T	Picloram	8.867	8.822	404.9E6	174.8E6	164.033	26.778 #
16) T	DCPA	0.000	8.822	0	174.8E6	N.D.	26.199



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123019\
Data File : PS008245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2019 08:44
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 13:44:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

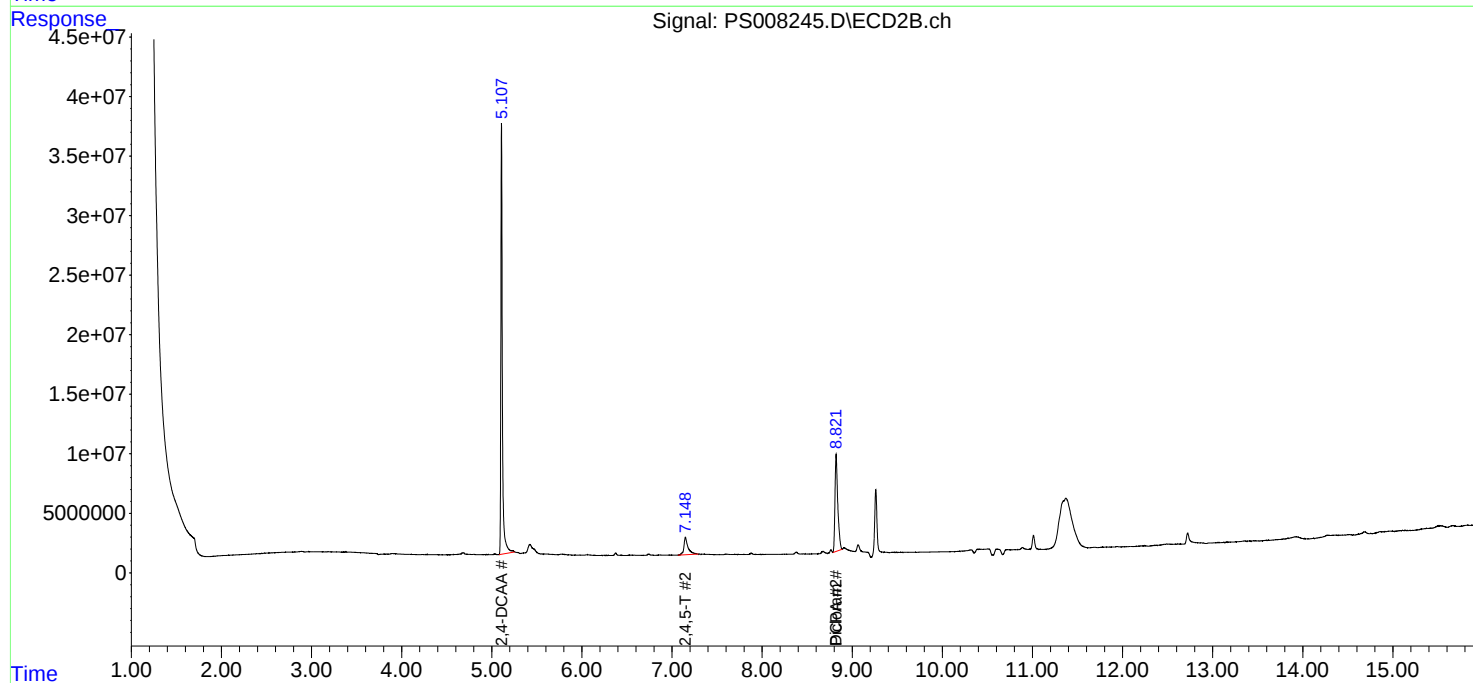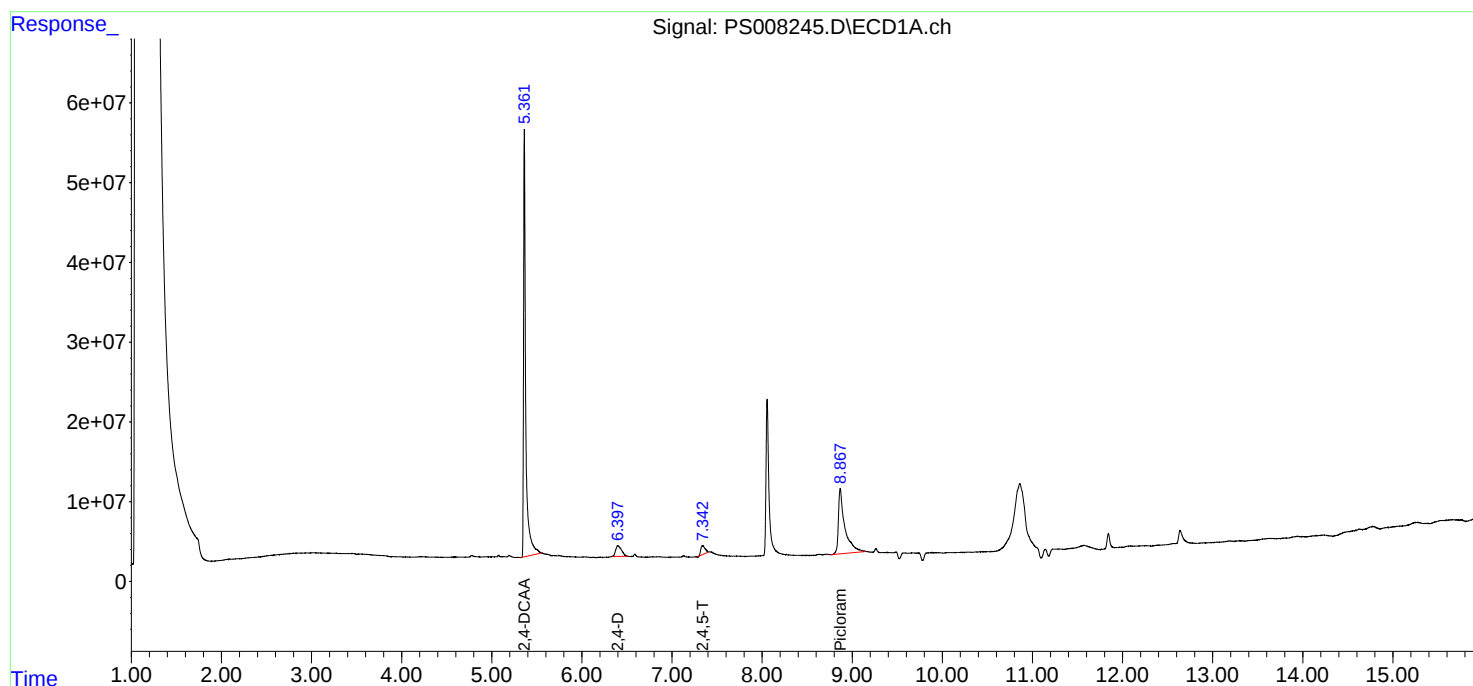


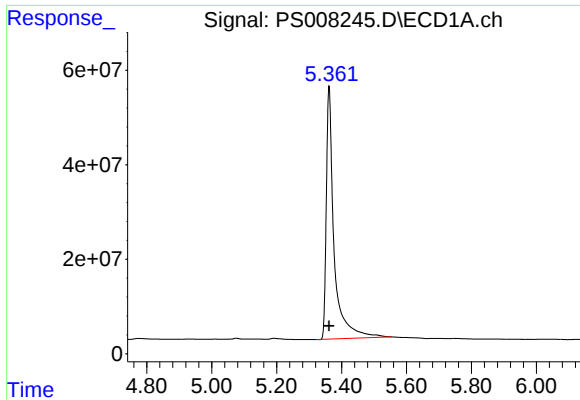

#4 2,4-DCAA


R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 892401136
Conc: 441.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

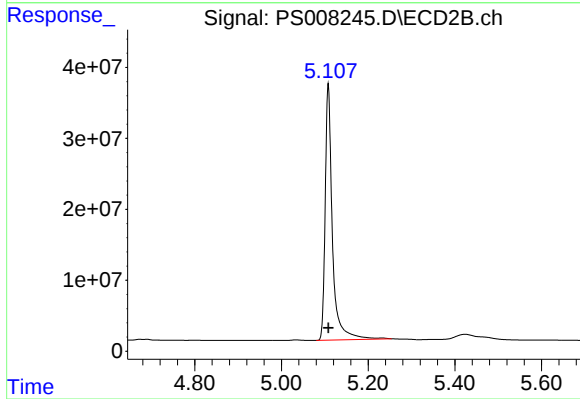


#4 2,4-DCAA

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 419262587
Conc: 468.25 ng/ml

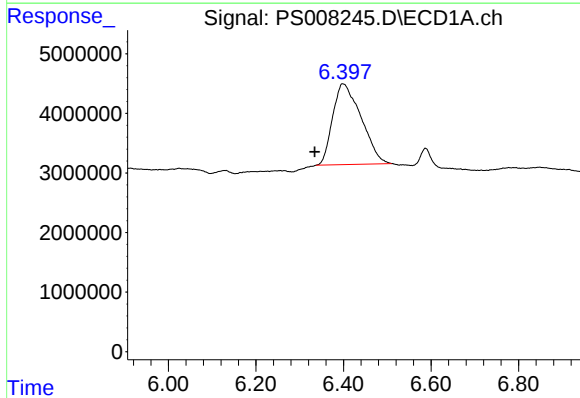


#9 2,4-D

R.T.: 6.398 min
Delta R.T.: 0.064 min
Response: 61088807
Conc: 37.23 ng/ml

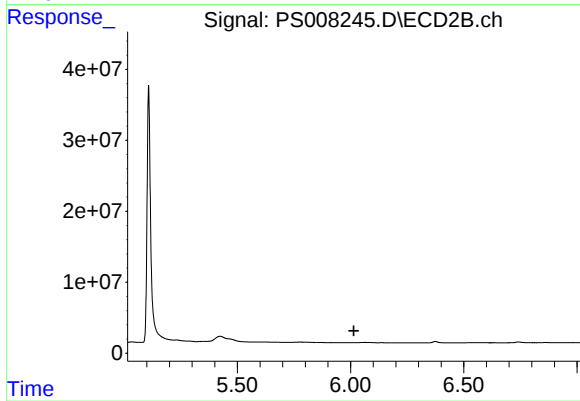

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

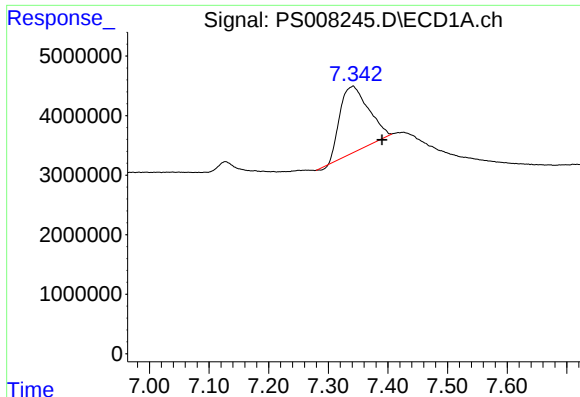

#12 2,4,5-T


R.T.: 7.342 min
Delta R.T.: -0.048 min
Response: 36863039
Conc: 3.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

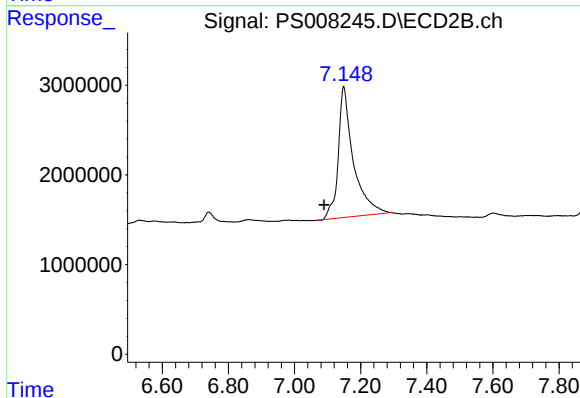


#12 2,4,5-T

R.T.: 7.149 min
Delta R.T.: 0.059 min
Response: 46382453
Conc: 11.10 ng/ml

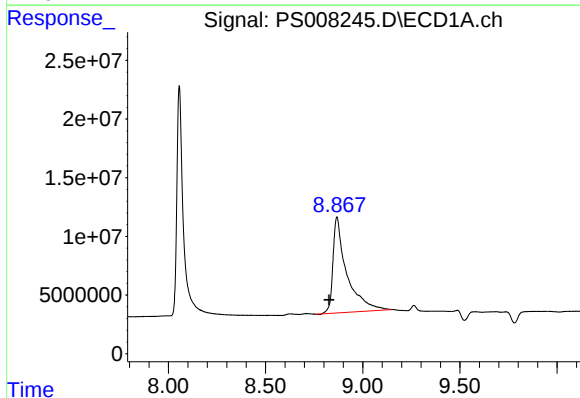


#15 Picloram

R.T.: 8.867 min
Delta R.T.: 0.041 min
Response: 404906568
Conc: 164.03 ng/ml

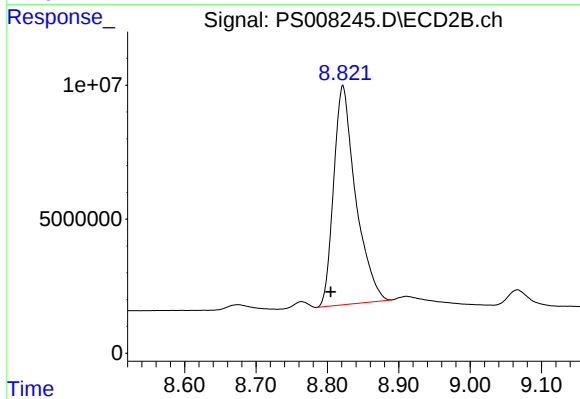

#15 Picloram


R.T.: 8.822 min
Delta R.T.: 0.017 min
Response: 174770457
Conc: 26.78 ng/ml

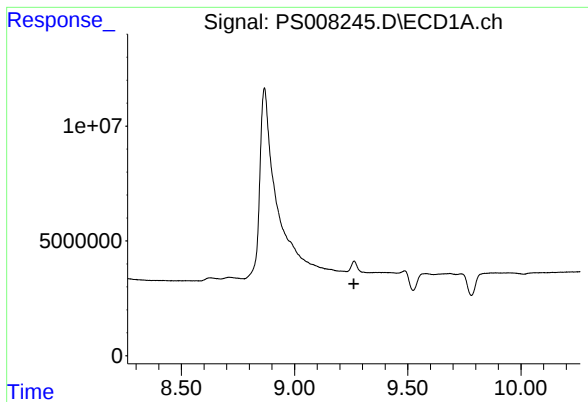

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.262 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

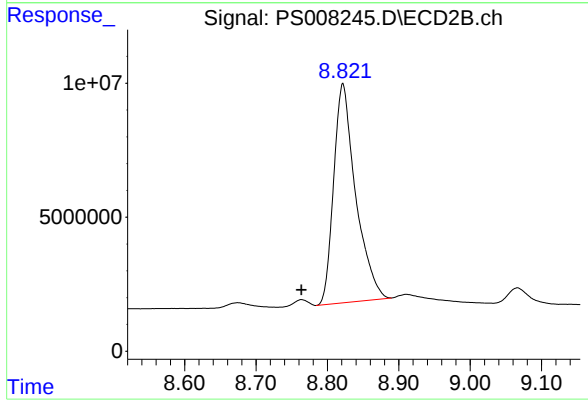

#16 DCPA

R.T.: 8.822 min
Delta R.T.: 0.058 min
Response: 174770457
Conc: 26.20 ng/ml