

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123019\
 Data File : PS008248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2019 11:15
 Operator : SM\AJ
 Sample : K6443-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 13:45:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.364	5.112	296.1E6	150.9E6	146.541	168.527
Target Compounds							
2) T	3,5-DICHL...	0.000	4.448	0	21531267	N.D.	18.491
5) T	DICAMBA	5.451	5.221	64009990	12363547	8.803	3.629 #
7) T	MCPA	5.818	5.473	38781295	30729704	5.071	8.077 #
9) T	2,4-D	6.395	6.001	65971253	6310959	40.202	6.216 #
10) T	Pentachlo...	0.000	6.432	0	5886292	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.693	0	21355691	N.D.	4.274
15) T	Picloram	0.000	8.830	0	26506092	N.D.	4.061
16) T	DCPA	0.000	8.725	0	20568951	N.D.	3.083



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS123019\
Data File : PS008248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2019 11:15
Operator : SM\AJ
Sample : K6443-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 13:45:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

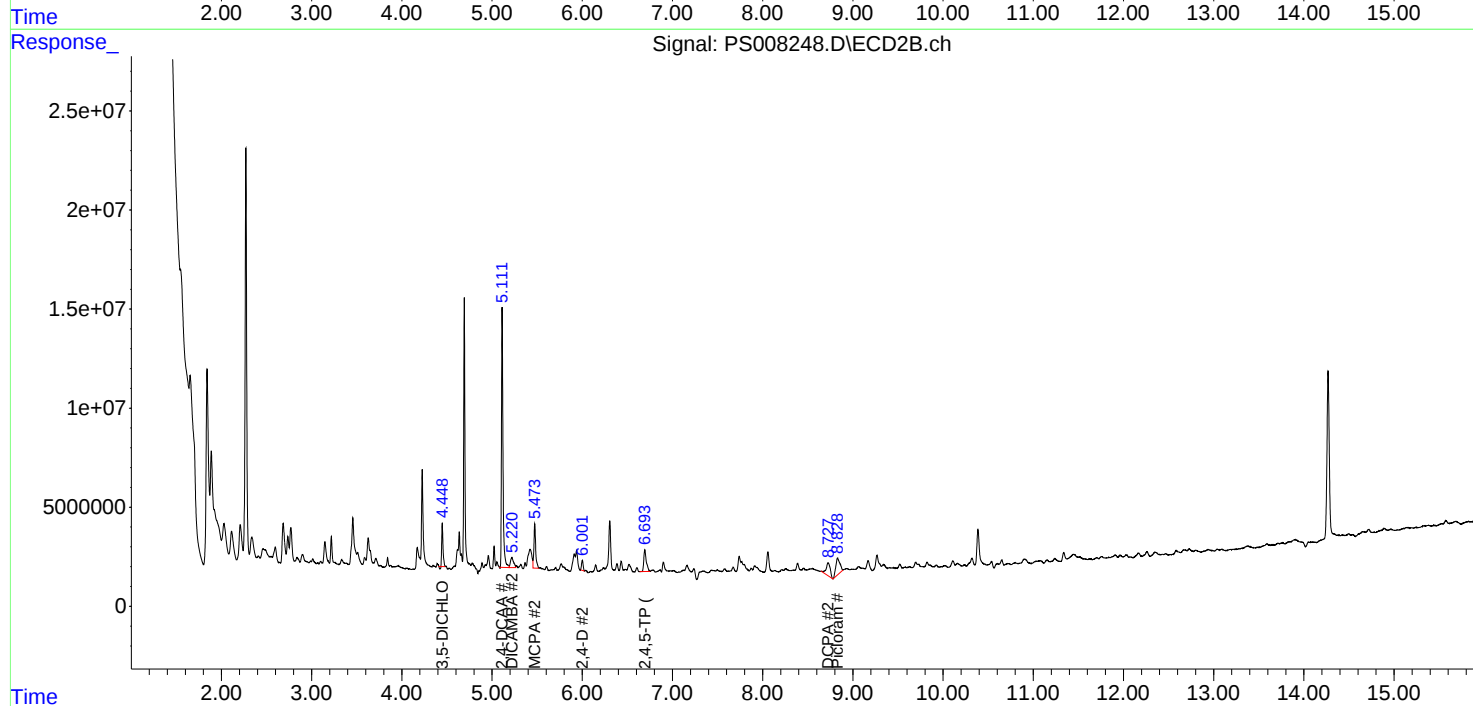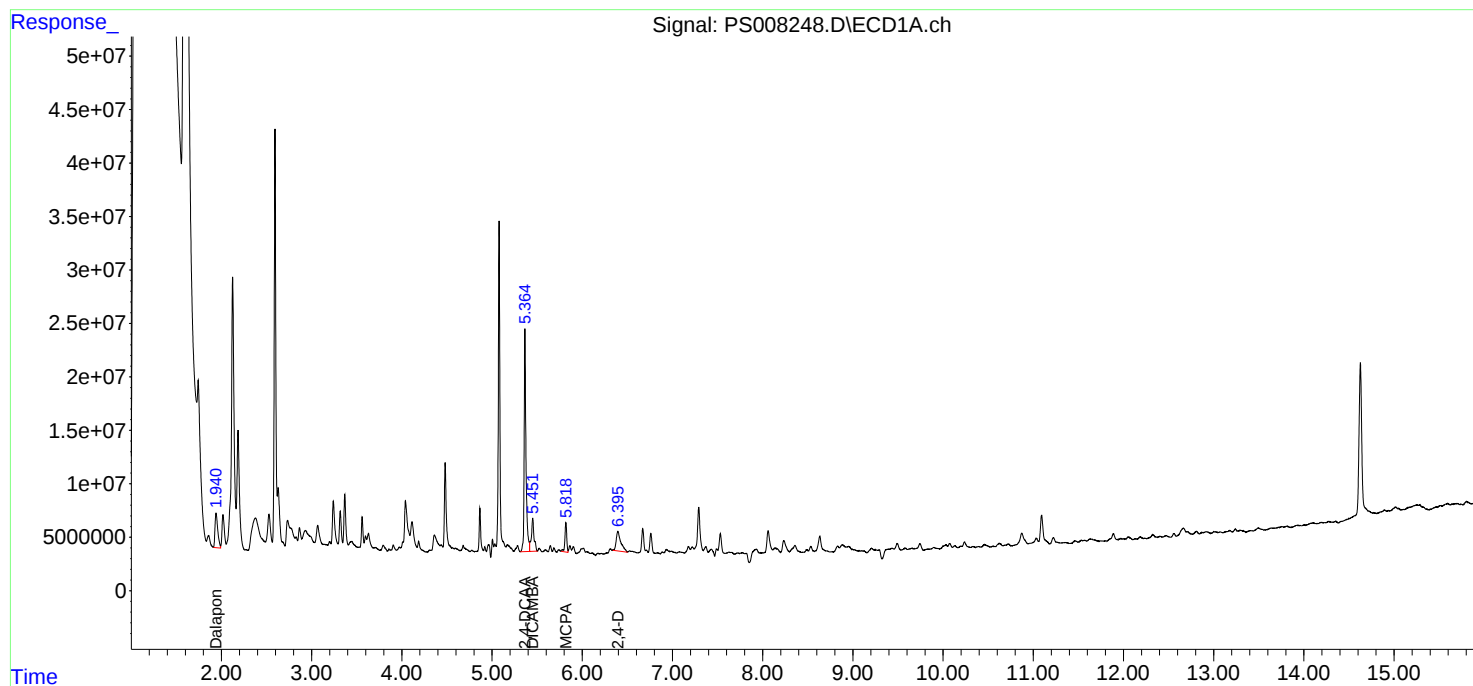


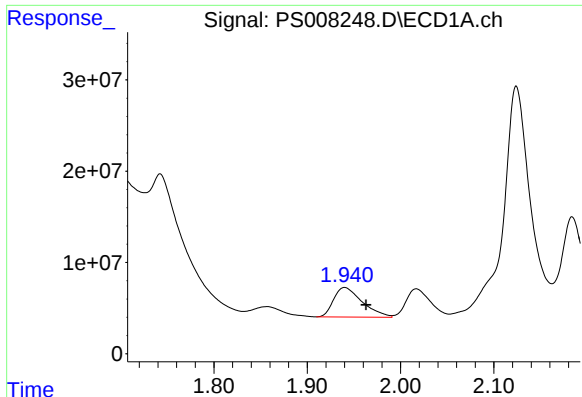

#1 Dalapon


R.T.: 1.940 min
Delta R.T.: -0.023 min
Response: 69054559
Conc: 28.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

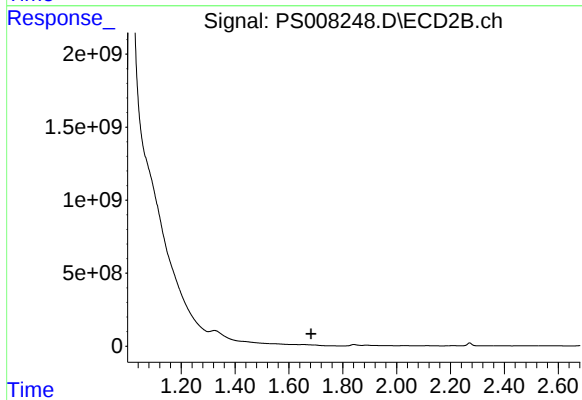


#1 Dalapon

R.T.: 1.653 min
Delta R.T.: -0.029 min
Response: -34988191
Conc: N.D.

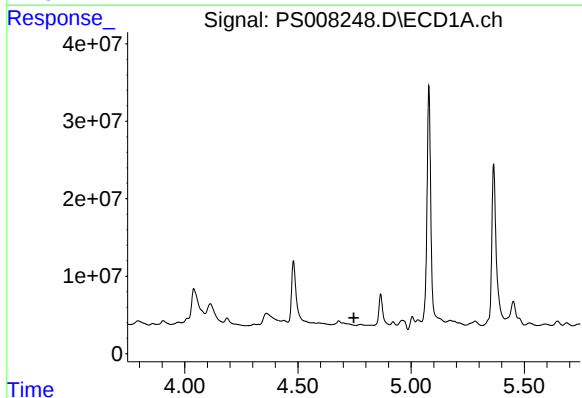


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

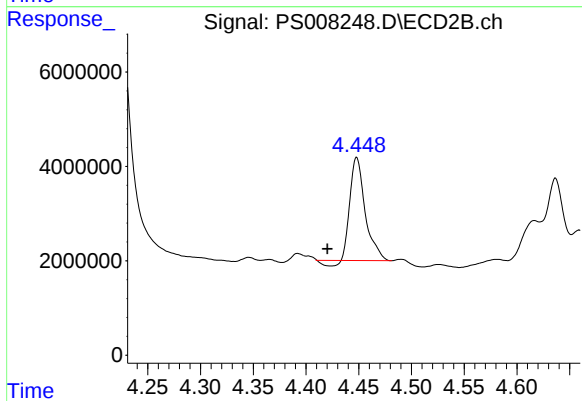

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.448 min
Delta R.T.: 0.028 min
Response: 21531267
Conc: 18.49 ng/ml

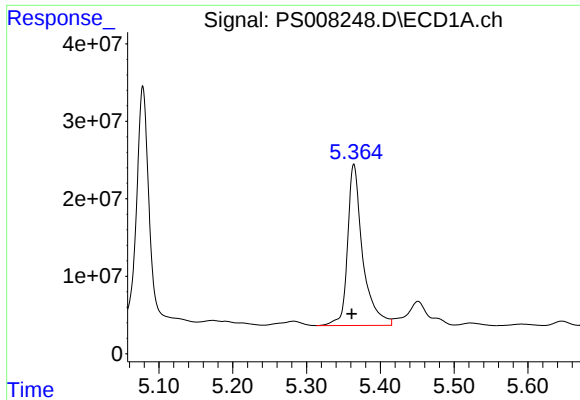

#4 2,4-DCAA


R.T.: 5.364 min
Delta R.T.: 0.003 min
Response: 296063497
Conc: 146.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

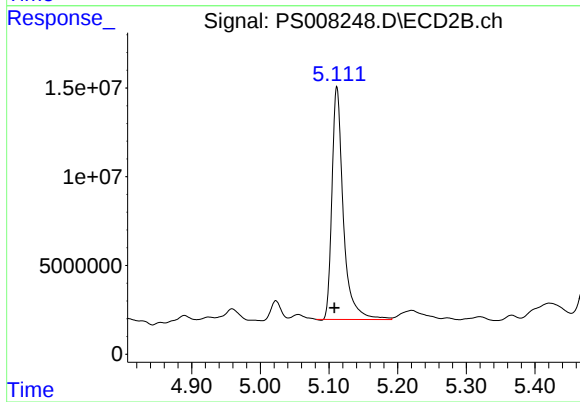


#4 2,4-DCAA

R.T.: 5.112 min
Delta R.T.: 0.003 min
Response: 150895802
Conc: 168.53 ng/ml

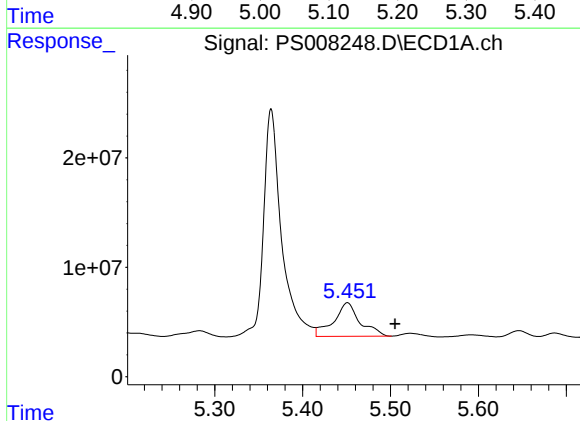


#5 DICAMBA

R.T.: 5.451 min
Delta R.T.: -0.054 min
Response: 64009990
Conc: 8.80 ng/ml

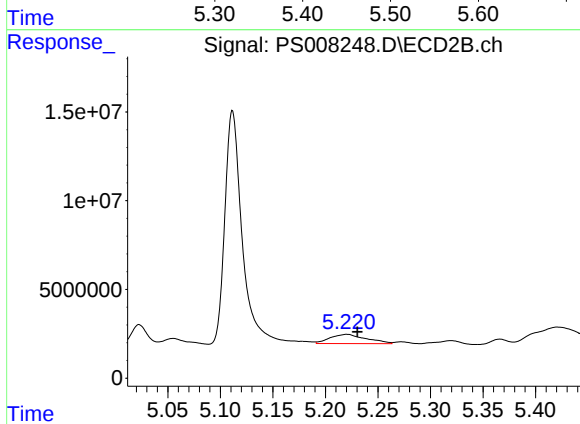

#5 DICAMBA


R.T.: 5.221 min
Delta R.T.: -0.010 min
Response: 12363547
Conc: 3.63 ng/ml

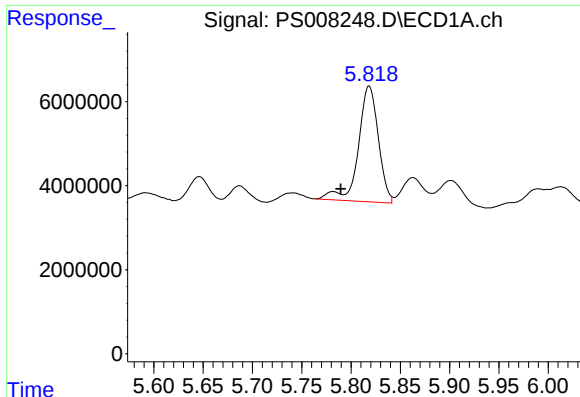

#7 MCPA


R.T.: 5.818 min
Delta R.T.: 0.029 min
Response: 38781295
Conc: 5.07 ug/ml

Instrument :
ECD_S
ClientSampleId :

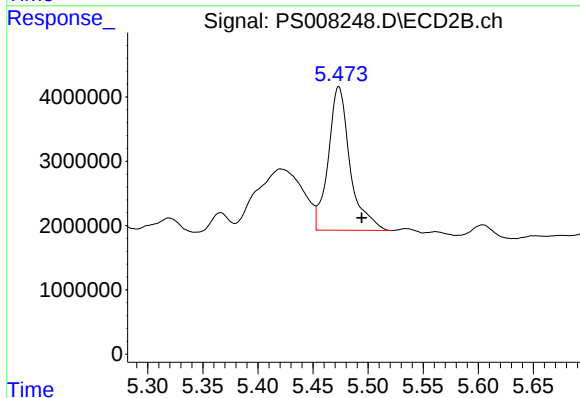


#7 MCPA

R.T.: 5.473 min
Delta R.T.: -0.021 min
Response: 30729704
Conc: 8.08 ug/ml

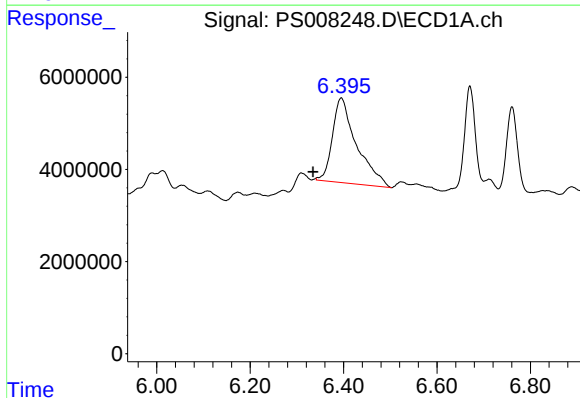


#9 2,4-D

R.T.: 6.395 min
Delta R.T.: 0.061 min
Response: 65971253
Conc: 40.20 ng/ml

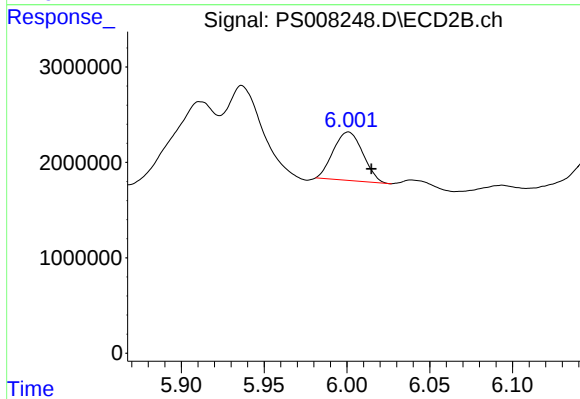

#9 2,4-D


R.T.: 6.001 min
Delta R.T.: -0.014 min
Response: 6310959
Conc: 6.22 ng/ml

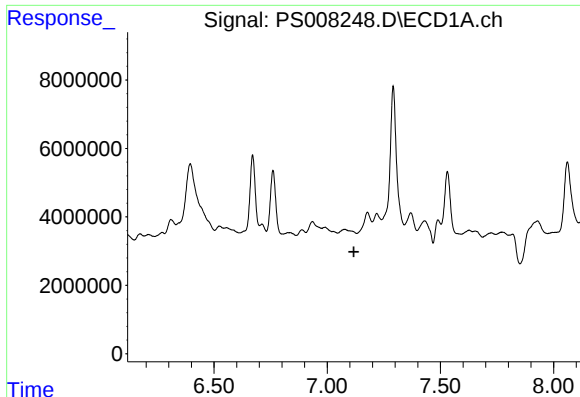

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

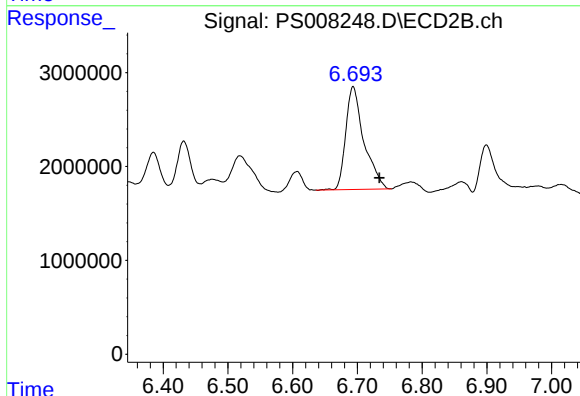


#11 2,4,5-TP (SILVEX)

R.T.: 6.693 min
Delta R.T.: -0.041 min
Response: 21355691
Conc: 4.27 ng/ml

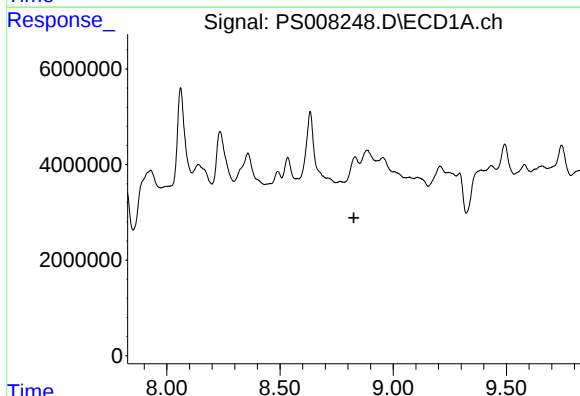


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.826 min
Response: 0
Conc: N.D.

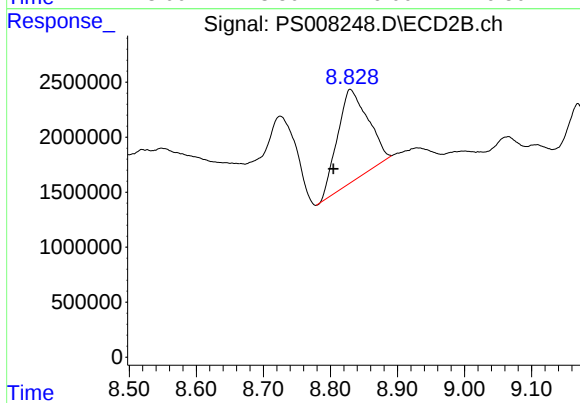

#15 Picloram


R.T.: 8.830 min
Delta R.T.: 0.025 min
Response: 26506092
Conc: 4.06 ng/ml

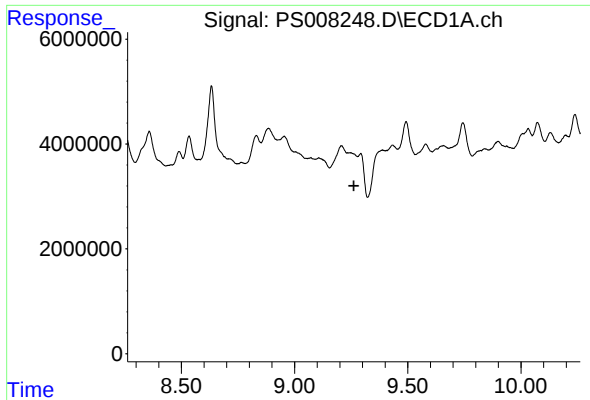

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.262 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

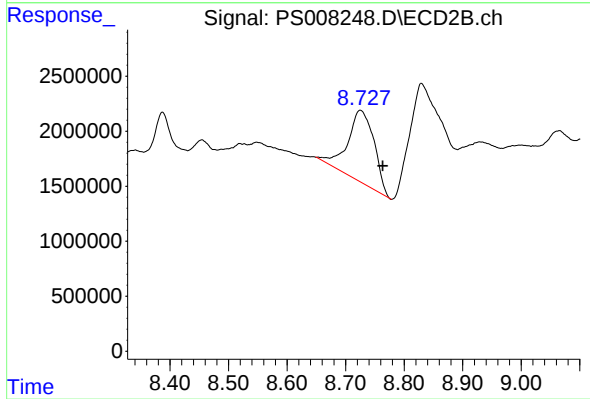

#16 DCPA

R.T.: 8.725 min
Delta R.T.: -0.039 min
Response: 20568951
Conc: 3.08 ng/ml